

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF080923\
 Data File : FF013165.D
 Signal(s) : FID2B.ch
 Acq On : 09 Aug 2023 10:49
 Operator : YP\AJ
 Sample : RT MARKER
 Misc :
 ALS Vial : 54 Sample Multiplier: 1

Instrument :
 FID_F
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Aug 09 23:54:06 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF080223.M
 Quant Title :
 QLast Update : Wed Aug 02 19:16:13 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
Target Compounds			
3) N-DODECANE	6.704	2706600	23.104 ug/ml
12) N-OCTACOSANE	17.160	2785084	22.537 ug/ml
13) N-TRIACONTANE	18.044	158481	1.305 ug/ml
14) N-DOTRIACONTANE	18.876	220393	1.956 ug/ml
15) N-TETRATRIACONTANE	19.658	171784	1.725 ug/ml
16) N-HEXATRIACONTANE	20.397	158316	1.771 ug/ml
17) N-OCTATRIACONTANE	21.127	62681	0.799 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF080923\
Data File : FF013165.D
Signal(s) : FID2B.ch
Acq On : 09 Aug 2023 10:49
Operator : YP\AJ
Sample : RT MARKER
Misc :
ALS Vial : 54 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Aug 09 23:54:06 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF080223.M
Quant Title :
QLast Update : Wed Aug 02 19:16:13 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

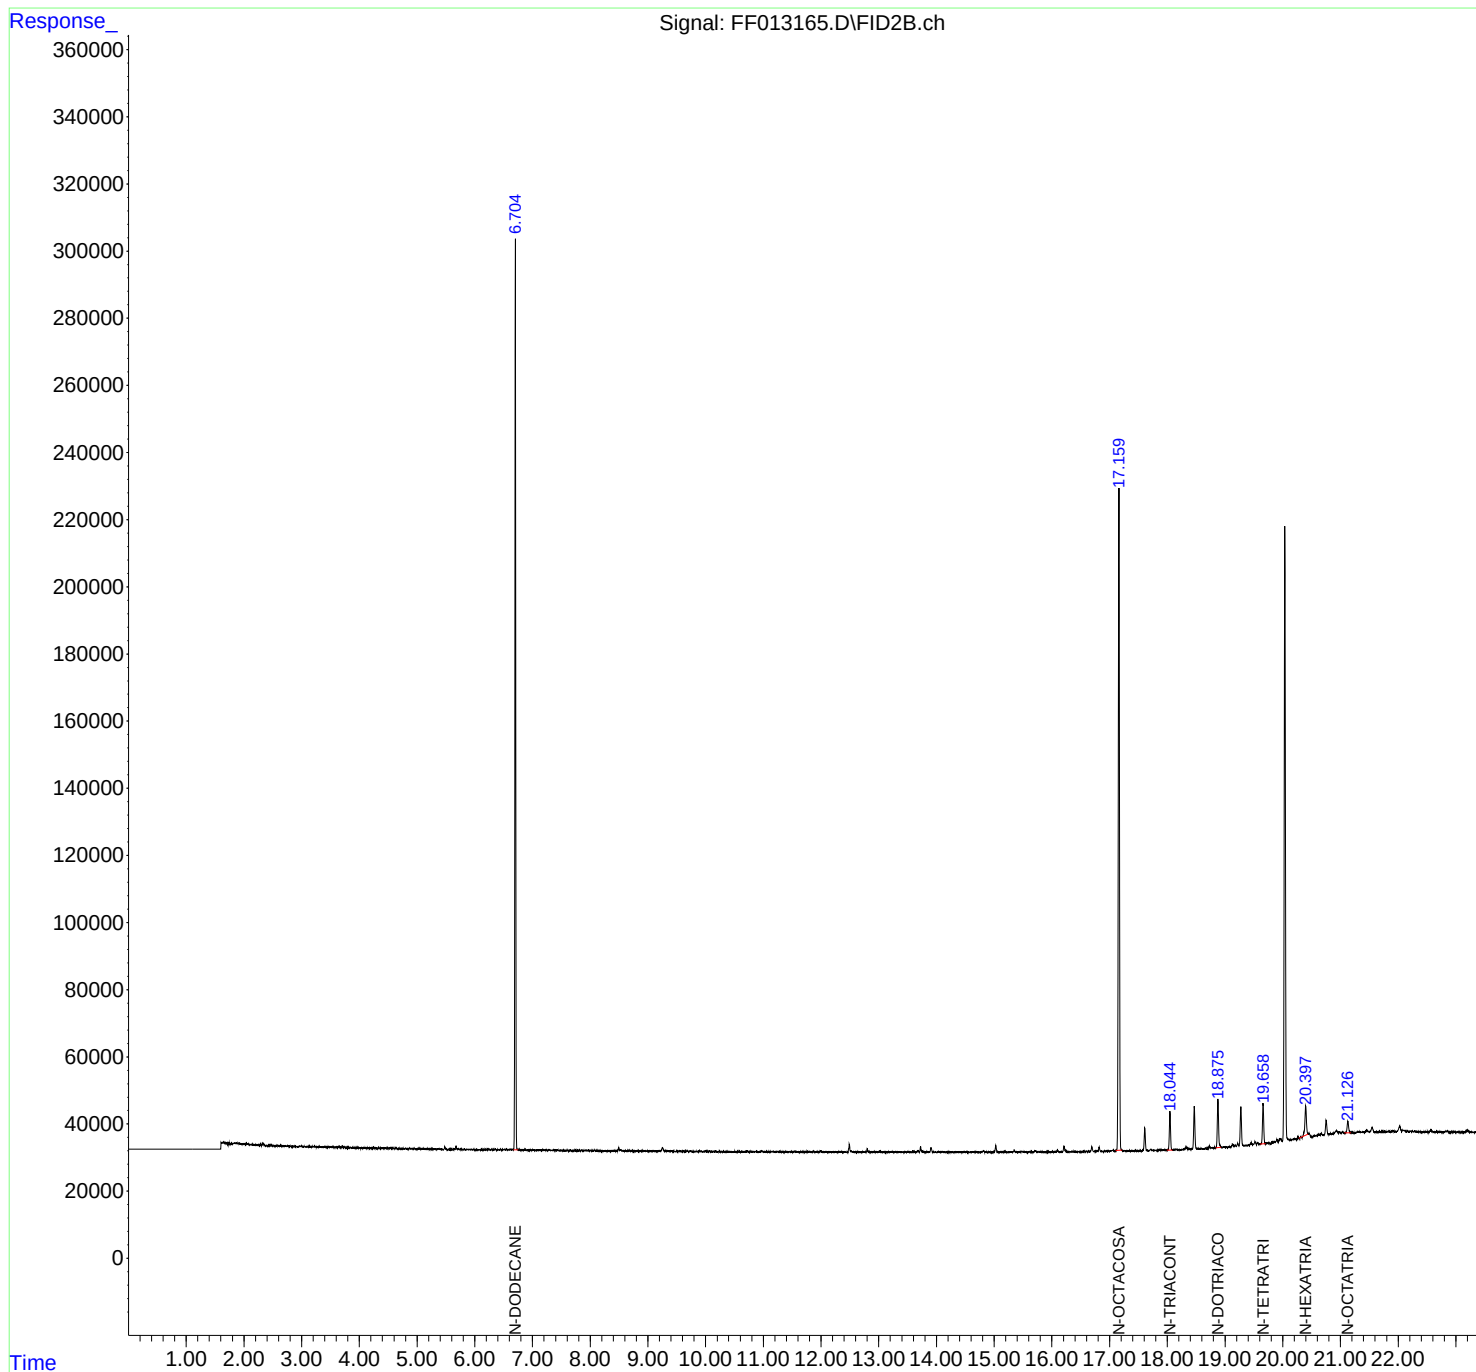


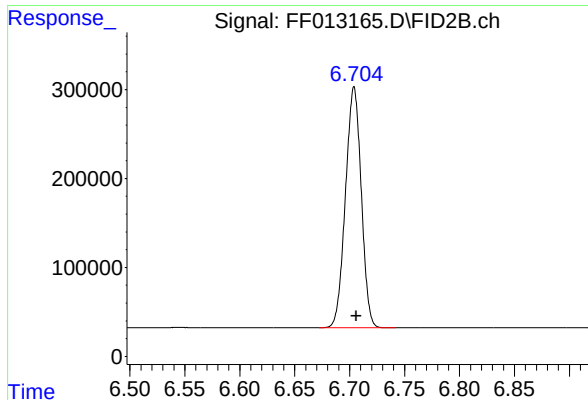

#3 N-DODECANE


R.T.: 6.704 min
Delta R.T.: -0.002 min
Response: 2706600
Conc: 23.10 ug/ml

Instrument :
FID_F
ClientSampleId :

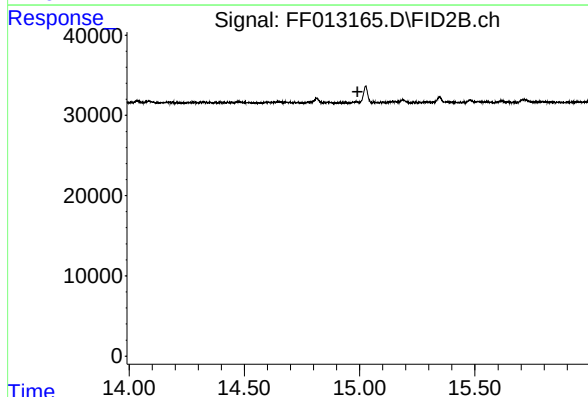


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 0.000 min
Exp R.T.: 14.991 min
Response: 0
Conc: N.D.

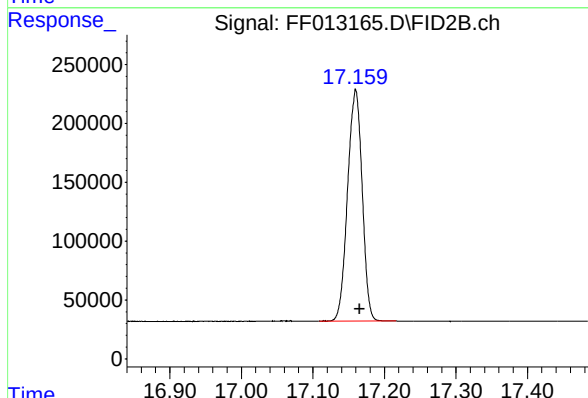


#12 N-OCTACOSANE

R.T.: 17.160 min
Delta R.T.: -0.006 min
Response: 2785084
Conc: 22.54 ug/ml

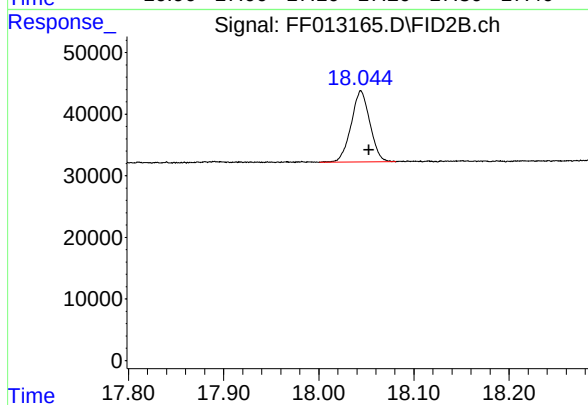

#13 N-TRIACONTANE

R.T.: 18.044 min
Delta R.T.: -0.009 min
Response: 158481
Conc: 1.31 ug/ml

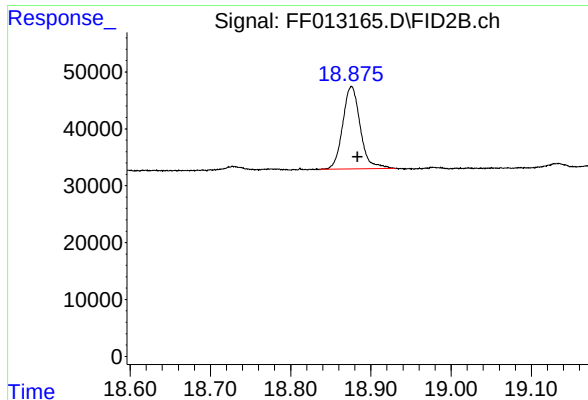


#14 N-DOTRIACONTANE

R.T.: 18.876 min
Delta R.T.: -0.008 min
Response: 220393
Conc: 1.96 ug/ml

Instrument :


FID_F

ClientSampleId :

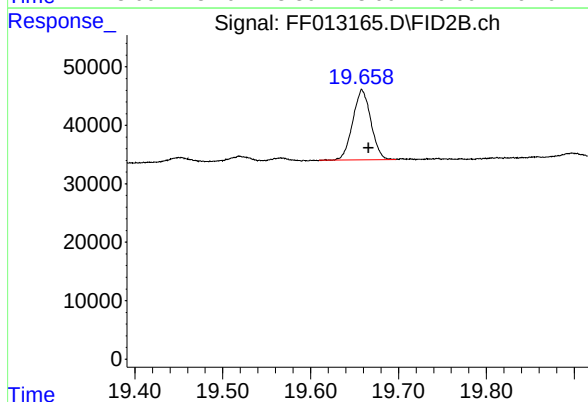


#15 N-TETRATRIACONTANE

R.T.: 19.658 min
Delta R.T.: -0.008 min
Response: 171784
Conc: 1.72 ug/ml

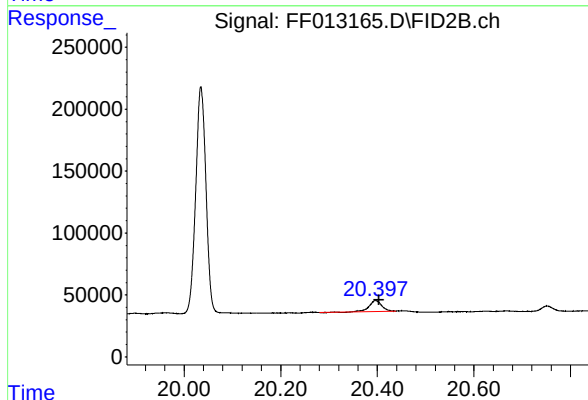

#16 N-HEXATRIACONTANE

R.T.: 20.397 min
Delta R.T.: -0.007 min
Response: 158316
Conc: 1.77 ug/ml

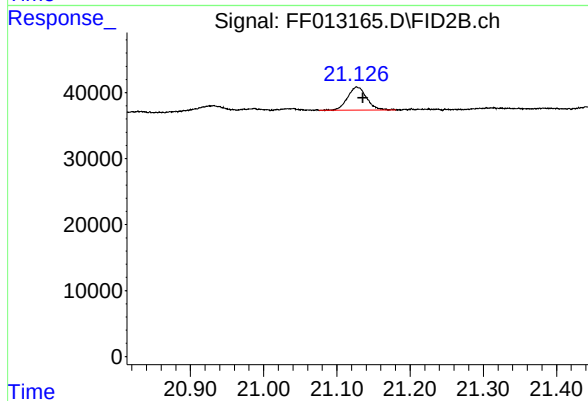

#17 N-OCTATRIACONTANE

R.T.: 21.127 min
Delta R.T.: -0.008 min
Response: 62681
Conc: 0.80 ug/ml