

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF081018\
Data File : FF001777.D
Signal(s) : FID2B.ch
Acq On : 10 Aug 2018 09:03
Operator : AJ\SJ
Sample : MECL2
Misc :
ALS Vial : 51 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Aug 10 13:10:02 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF073018.M
Quant Title :
QLast Update : Fri Aug 03 12:00:27 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

Compound		R.T.	Response	Conc Units

System Monitoring Compounds				
Target Compounds				
10)	N-TETRACOSANE	14.486	370251	2.595 ug/ml
13)	N-TRIACONTANE	17.376	121874	0.880 ug/ml
14)	N-DOTRIACONTANE	18.207	182184	1.396 ug/ml
15)	N-TETRATRIACONTANE	18.991	136590	1.130 ug/ml
16)	N-HEXATRIACONTANE	19.732	152940	1.375 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF081018\
Data File : FF001777.D
Signal(s) : FID2B.ch
Acq On : 10 Aug 2018 09:03
Operator : AJ\SJ
Sample : MECL2
Misc :
ALS Vial : 51 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Aug 10 13:10:02 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF073018.M
Quant Title :
QLast Update : Fri Aug 03 12:00:27 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

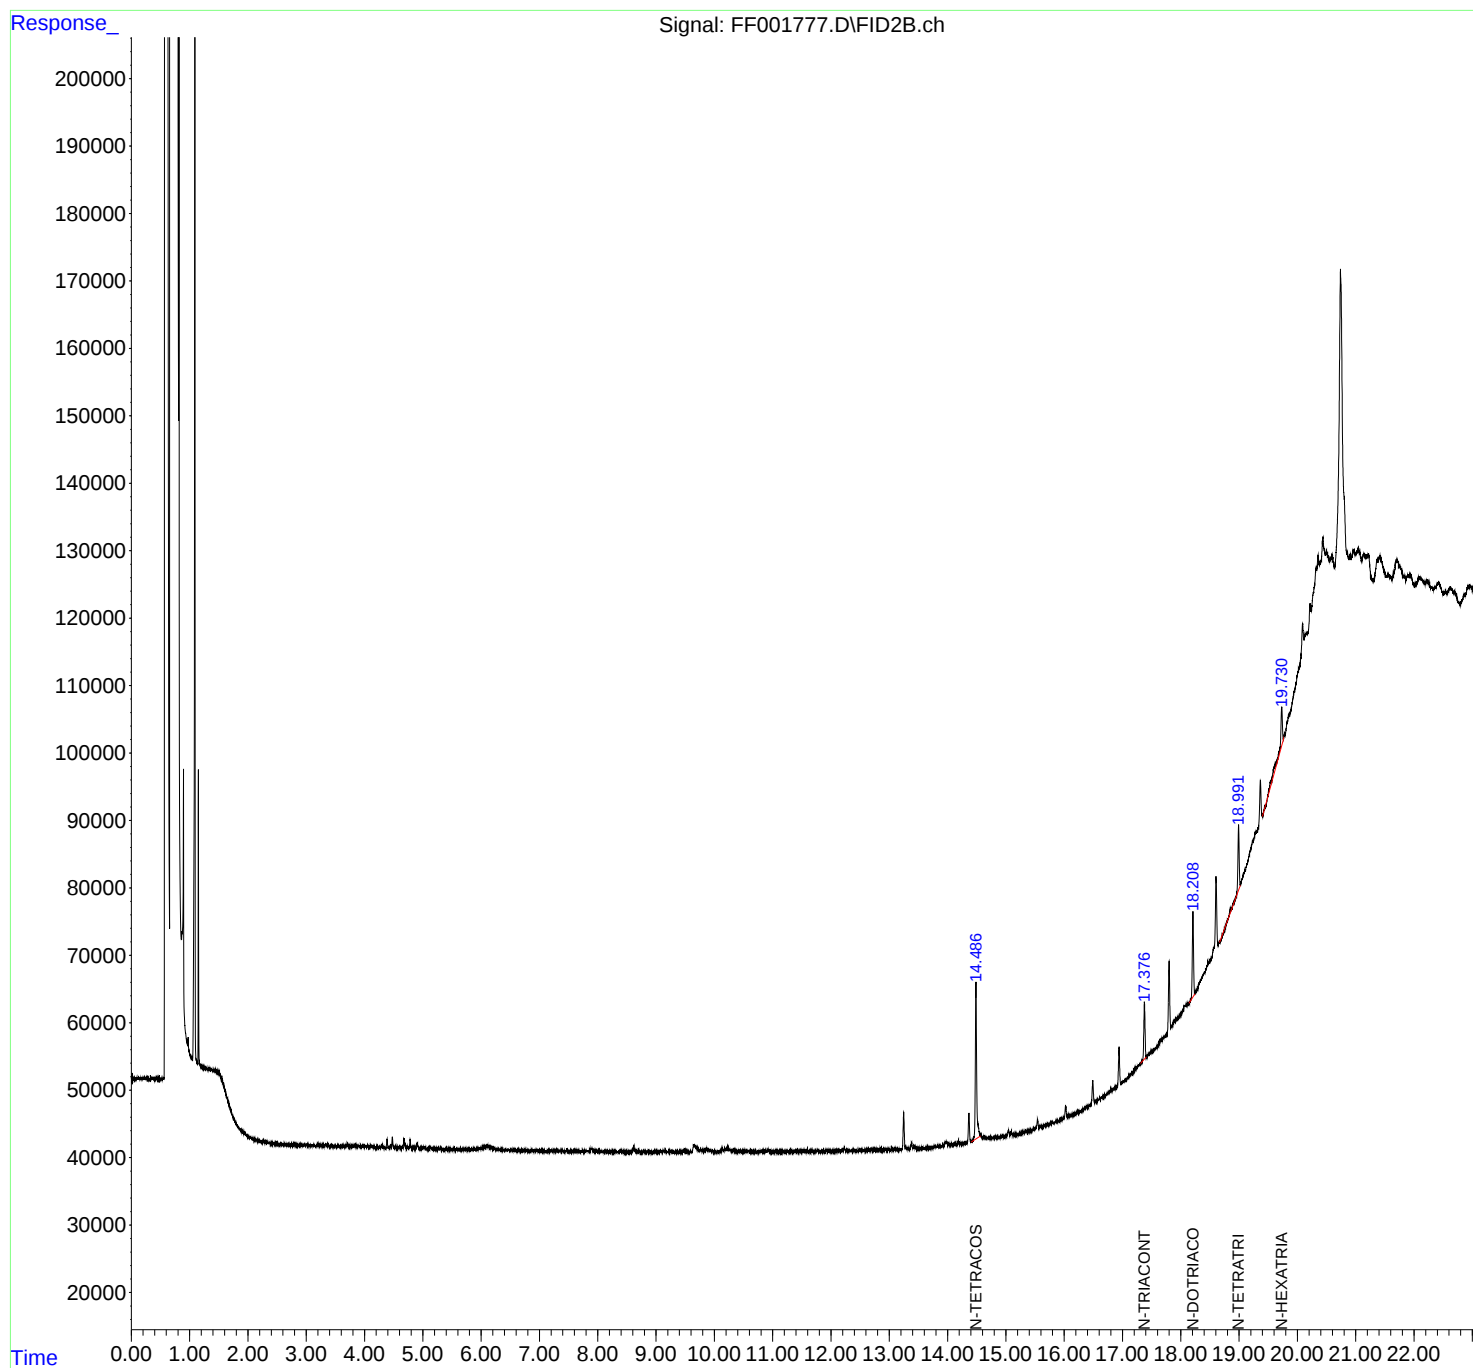


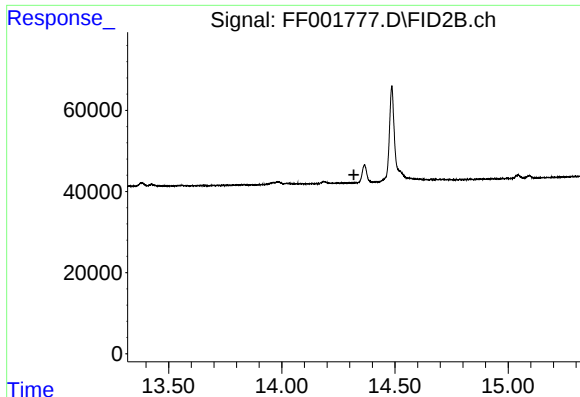

#9 TETRACOSANE-d50 (SURROGATE)


R.T.: 0.000 min
Exp R.T.: 14.318 min
Response: 0
Conc: N.D.

Instrument :
FID_F
ClientSampleId :

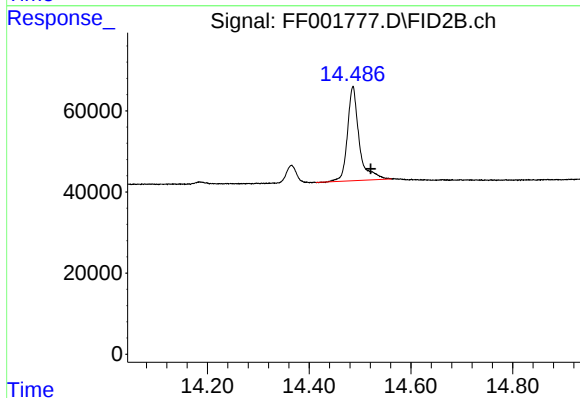


#10 N-TETRACOSANE

R.T.: 14.486 min
Delta R.T.: -0.035 min
Response: 370251
Conc: 2.60 ug/ml

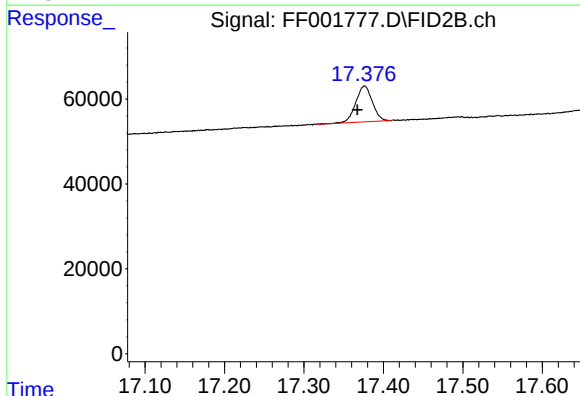


#13 N-TRIACONTANE

R.T.: 17.376 min
Delta R.T.: 0.009 min
Response: 121874
Conc: 0.88 ug/ml

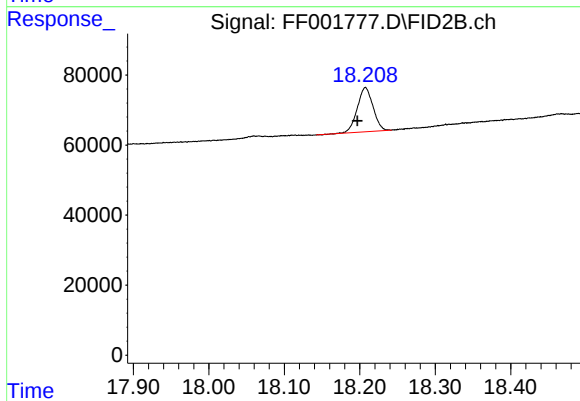

#14 N-DOTRIACONTANE


R.T.: 18.207 min
Delta R.T.: 0.011 min
Response: 182184
Conc: 1.40 ug/ml

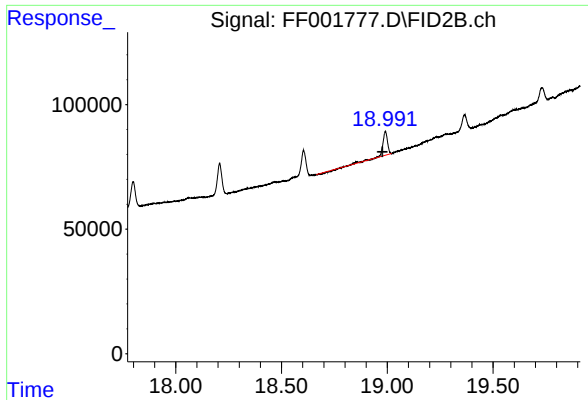

#15 N-TETRATRIACONTANE

R.T.: 18.991 min
Delta R.T.: 0.014 min
Response: 136590
Conc: 1.13 ug/ml

Instrument :
FID_F
ClientSampleId :

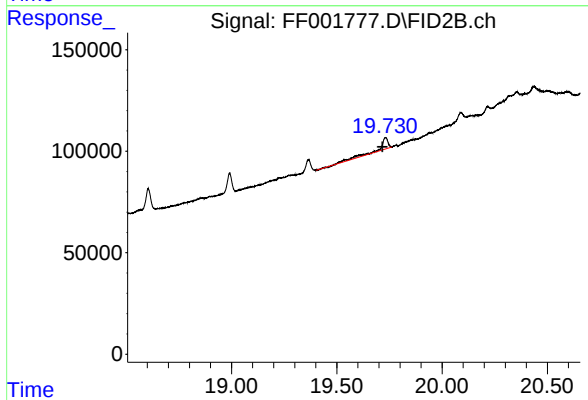

#16 N-HEXATRIACONTANE

R.T.: 19.732 min
Delta R.T.: 0.016 min
Response: 152940
Conc: 1.37 ug/ml