

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF081018\
 Data File : FF001781.D
 Signal(s) : FID2B.ch
 Acq On : 10 Aug 2018 11:37
 Operator : AJ\SJ
 Sample : J4276-01 10X
 Misc :
 ALS Vial : 55 Sample Multiplier: 1

Instrument :
 FID_F
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Aug 10 13:10:54 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF073018.M
 Quant Title :
 QLast Update : Fri Aug 03 12:00:27 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.322	351456	2.783 ug/ml
Target Compounds			
5) N-HEXADECANE	9.489	127462	0.851 ug/ml
6) N-OCTADECANE	10.924	169820	1.127 ug/ml
7) N-EICOSANE	12.230	335902	2.254 ug/ml
8) N-DOCOSANE	13.444	494149	3.383 ug/ml
10) N-TETRACOSANE	14.500	2101068	14.729 ug/ml
11) N-HEXACOSANE	15.543	138315	0.982 ug/ml
12) N-OCTACOSANE	16.491	235373	1.679 ug/ml
13) N-TRIACONTANE	17.379	376626	2.721 ug/ml
14) N-DOTRIACONTANE	18.206	568336	4.356 ug/ml
15) N-TETRATRIACONTANE	18.993	416634	3.447 ug/ml
16) N-HEXATRIACONTANE	19.736	412266	3.705 ug/ml
17) N-OCTATRIACONTANE	20.440	189184	1.898 ug/ml
18) N-TETRACONTANE	21.220	20267	0.203 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF081018\
Data File : FF001781.D
Signal(s) : FID2B.ch
Acq On : 10 Aug 2018 11:37
Operator : AJ\SJ
Sample : J4276-01 10X
Misc :
ALS Vial : 55 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Aug 10 13:10:54 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF073018.M
Quant Title :
QLast Update : Fri Aug 03 12:00:27 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

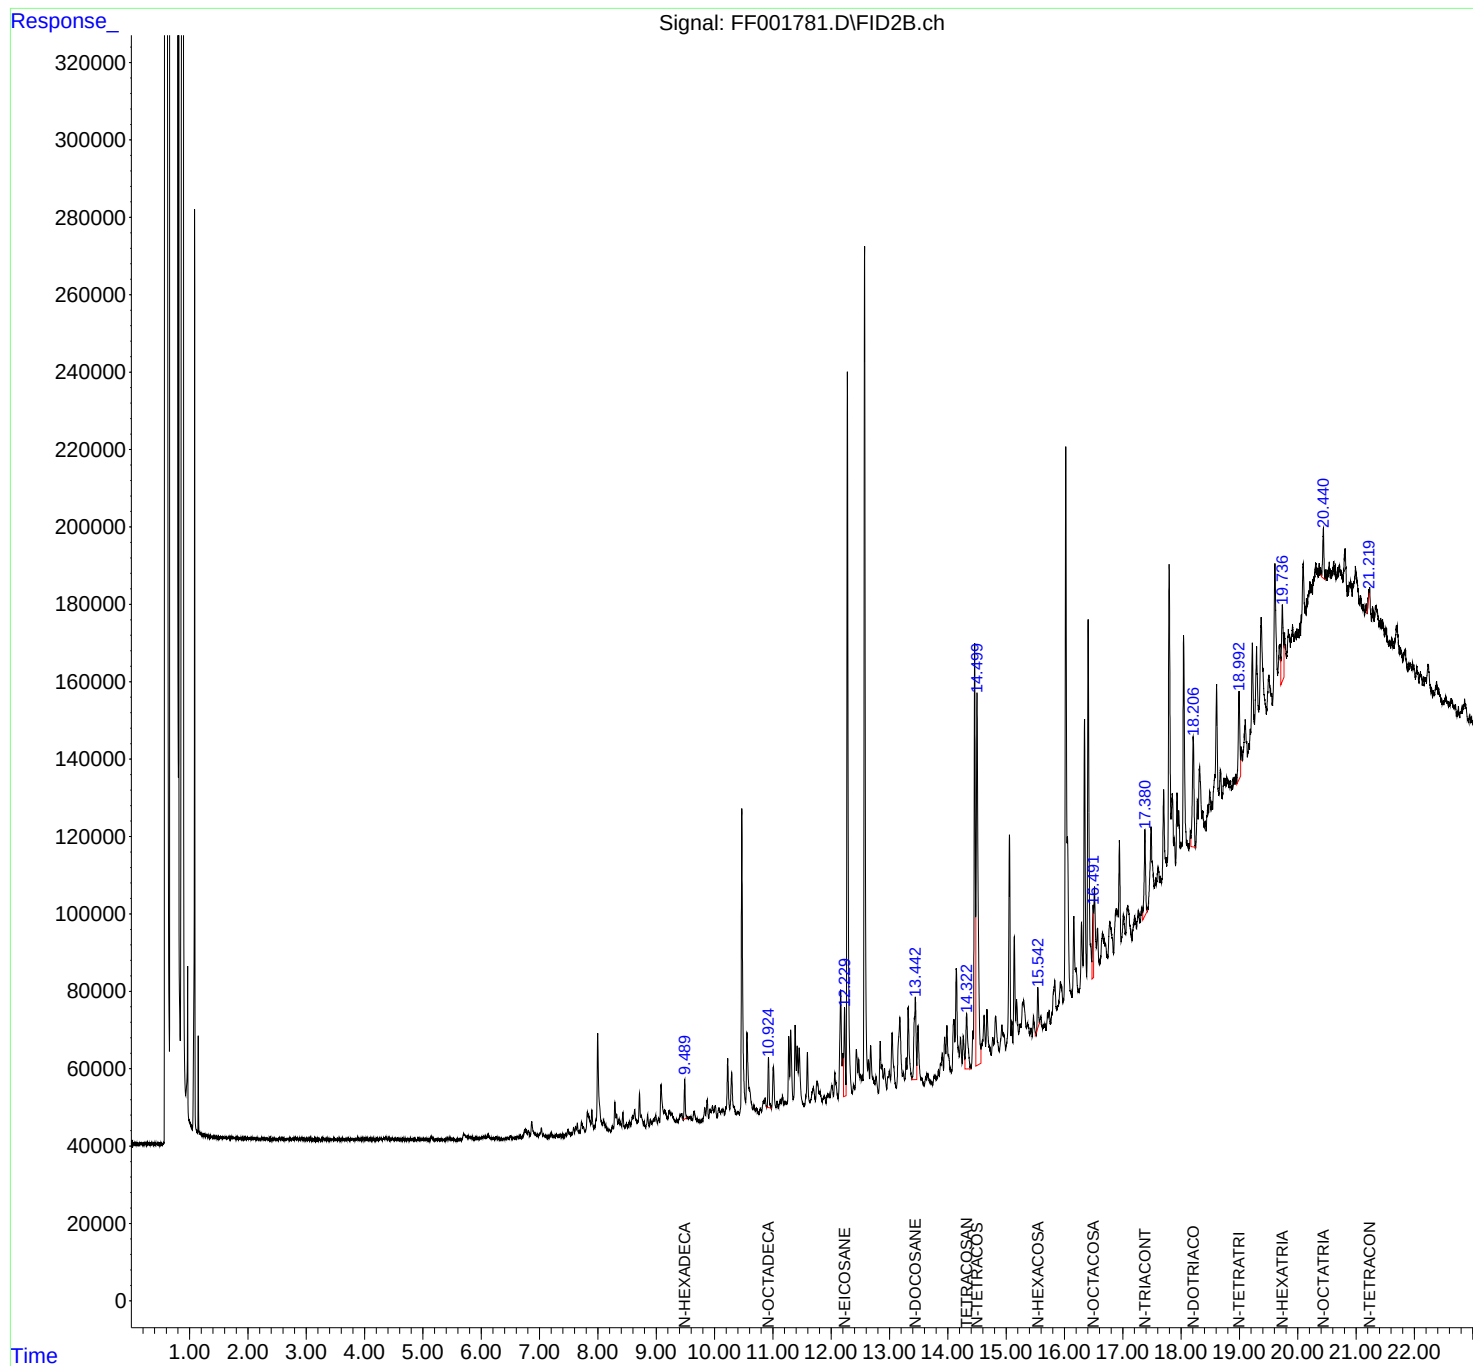


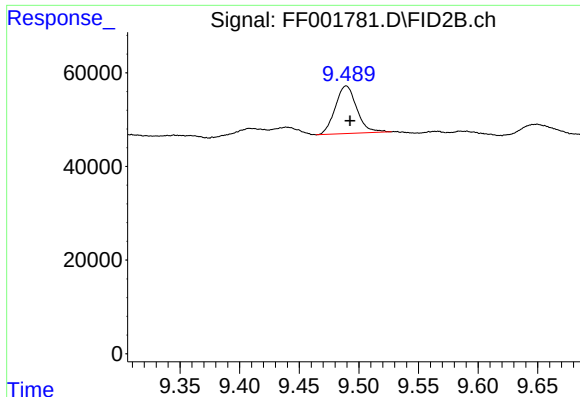

#5 N-HEXADECANE


R.T.: 9.489 min
Delta R.T.: -0.003 min
Response: 127462
Conc: 0.85 ug/ml

Instrument :
FID_F
ClientSampleId :

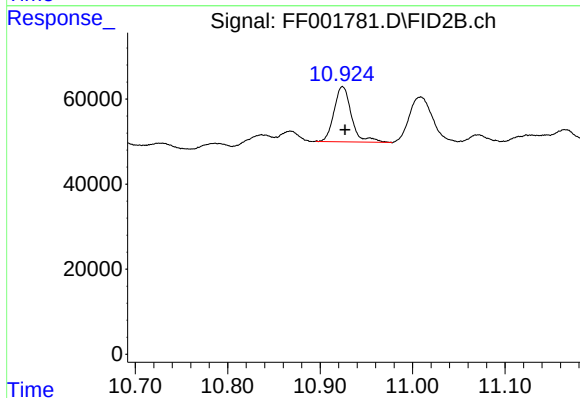


#6 N-OCTADECANE

R.T.: 10.924 min
Delta R.T.: -0.003 min
Response: 169820
Conc: 1.13 ug/ml

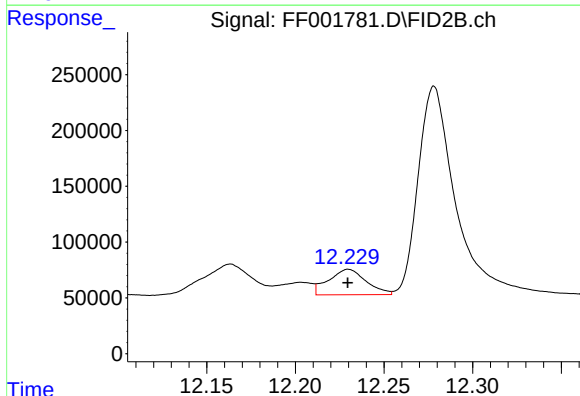


#7 N-EICOSANE

R.T.: 12.230 min
Delta R.T.: 0.000 min
Response: 335902
Conc: 2.25 ug/ml

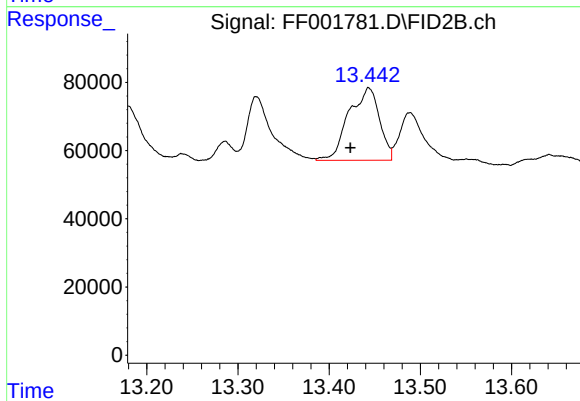

#8 N-DOCOSANE


R.T.: 13.444 min
Delta R.T.: 0.020 min
Response: 494149
Conc: 3.38 ug/ml

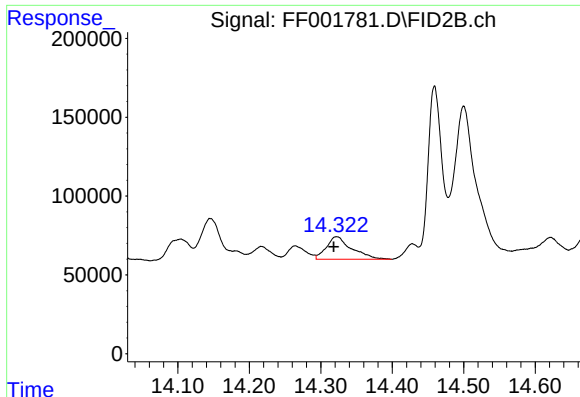

#9 TETRACOSANE-d50 (SURROGATE)


R.T.: 14.322 min
Delta R.T.: 0.004 min
Response: 351456
Conc: 2.78 ug/ml

Instrument :
FID_F
ClientSampleId :

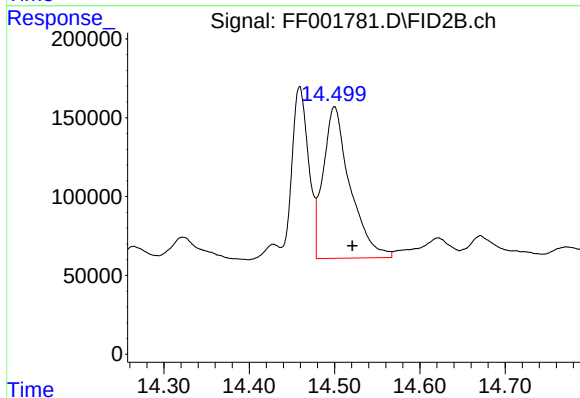


#10 N-TETRACOSANE

R.T.: 14.500 min
Delta R.T.: -0.021 min
Response: 2101068
Conc: 14.73 ug/ml

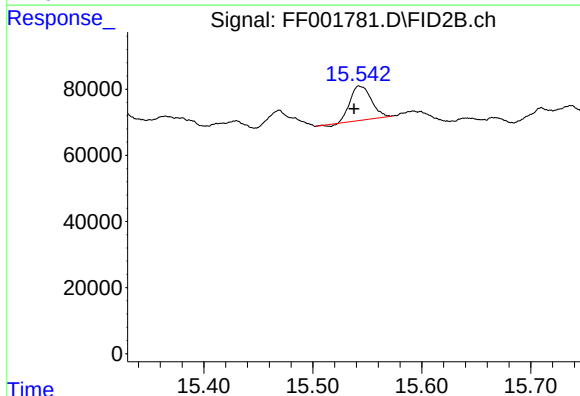


#11 N-HEXACOSANE

R.T.: 15.543 min
Delta R.T.: 0.005 min
Response: 138315
Conc: 0.98 ug/ml

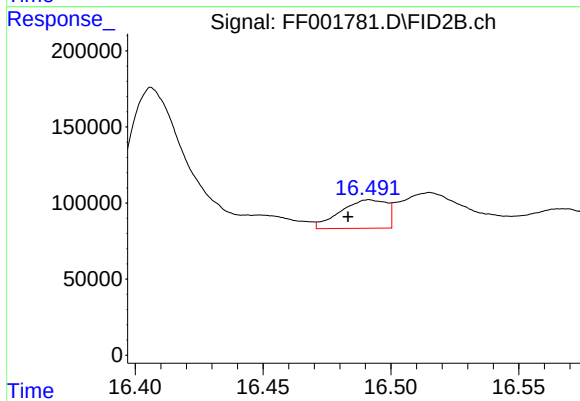

#12 N-OCTACOSANE


R.T.: 16.491 min
Delta R.T.: 0.008 min
Response: 235373
Conc: 1.68 ug/ml

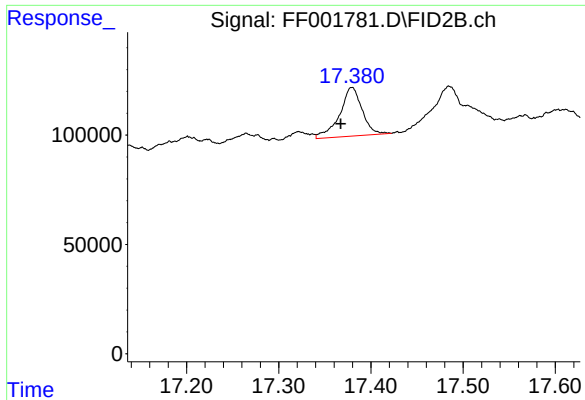

#13 N-TRIACONTANE


R.T.: 17.379 min
Delta R.T.: 0.012 min
Response: 376626
Conc: 2.72 ug/ml

Instrument :
FID_F
ClientSampleId :

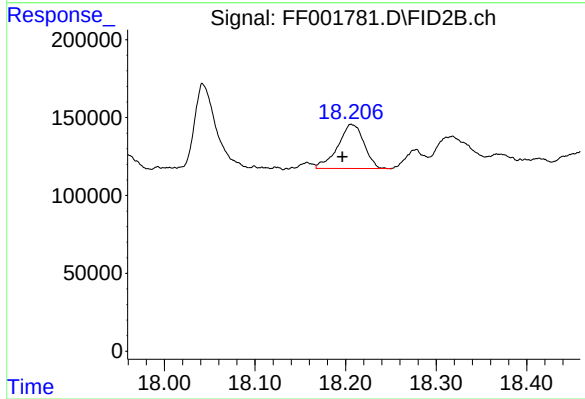


#14 N-DOTRIACONTANE

R.T.: 18.206 min
Delta R.T.: 0.010 min
Response: 568336
Conc: 4.36 ug/ml

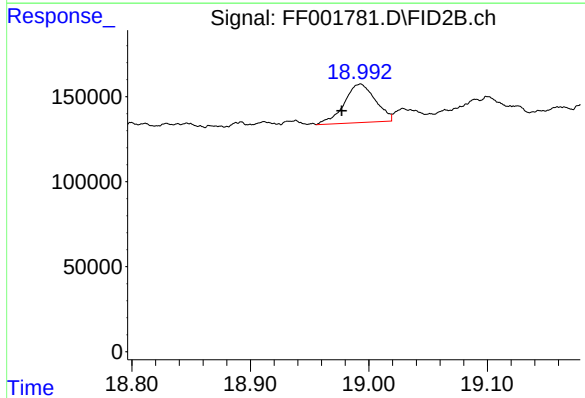


#15 N-TETRATRIACONTANE

R.T.: 18.993 min
Delta R.T.: 0.016 min
Response: 416634
Conc: 3.45 ug/ml

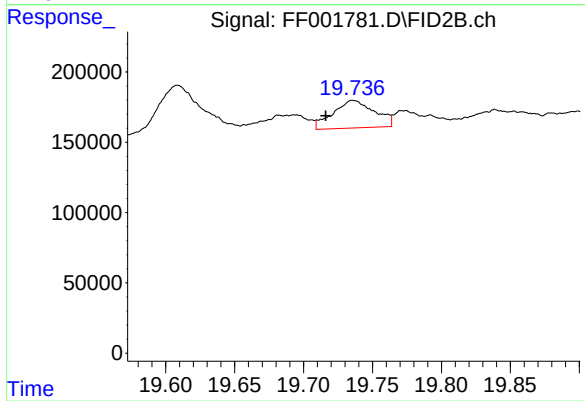

#16 N-HEXATRIACONTANE


R.T.: 19.736 min
Delta R.T.: 0.020 min
Response: 412266
Conc: 3.71 ug/ml

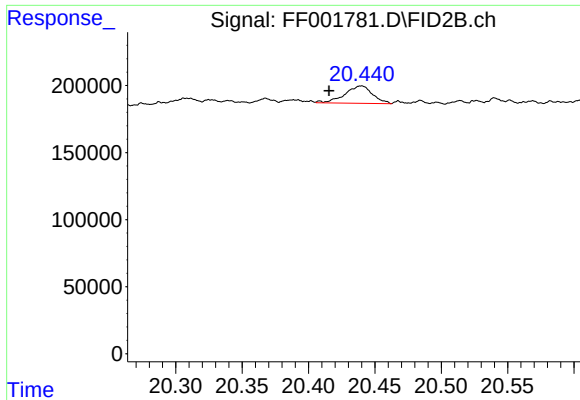

#17 N-OCTATRIACONTANE

R.T.: 20.440 min
Delta R.T.: 0.024 min
Response: 189184
Conc: 1.90 ug/ml

Instrument :
FID_F
ClientSampleId :

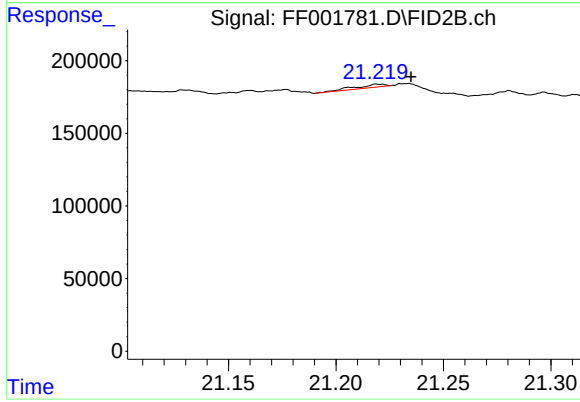

#18 N-TETRACONTANE

R.T.: 21.220 min
Delta R.T.: -0.015 min
Response: 20267
Conc: 0.20 ug/ml