

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF081018\
 Data File : FF001782.D
 Signal(s) : FID2B.ch
 Acq On : 10 Aug 2018 12:07
 Operator : AJ\SJ
 Sample : J4398-02
 Misc :
 ALS Vial : 56 Sample Multiplier: 1

Instrument :
 FID_F
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Aug 10 13:11:07 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF073018.M
 Quant Title :
 QLast Update : Fri Aug 03 12:00:27 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.324	2743018	21.718 ug/ml
Target Compounds			
4) N-TETRADECANE	7.959f	1548035	10.271 ug/ml
10) N-TETRACOSANE	14.486	276797	1.940 ug/ml
12) N-OCTACOSANE	16.490	78787	0.562 ug/ml
13) N-TRIACONTANE	17.375	150829	1.090 ug/ml
14) N-DOTRIACONTANE	18.203	290132	2.224 ug/ml
15) N-TETRATRIACONTANE	18.990	53121	0.439 ug/ml
16) N-HEXATRIACONTANE	19.729	162260	1.458 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF081018\
Data File : FF001782.D
Signal(s) : FID2B.ch
Acq On : 10 Aug 2018 12:07
Operator : AJ\SJ
Sample : J4398-02
Misc :
ALS Vial : 56 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Aug 10 13:11:07 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF073018.M
Quant Title :
QLast Update : Fri Aug 03 12:00:27 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

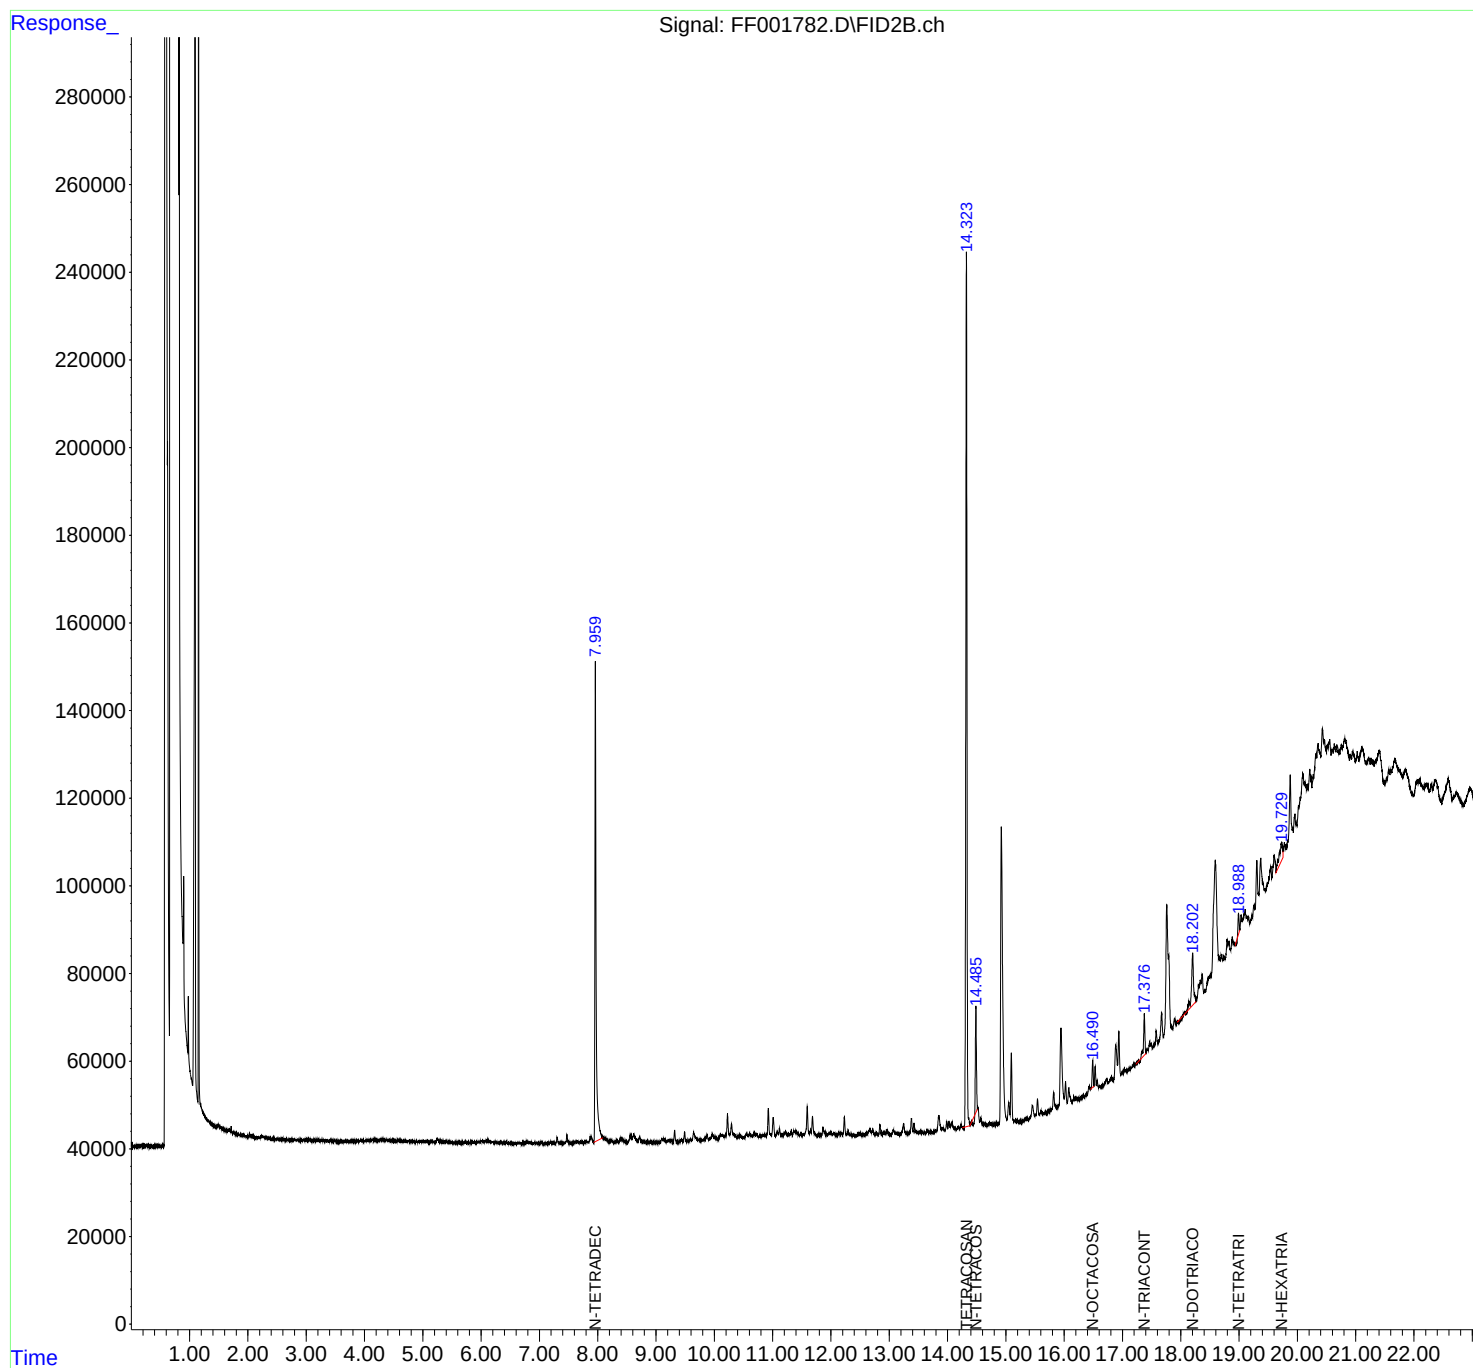


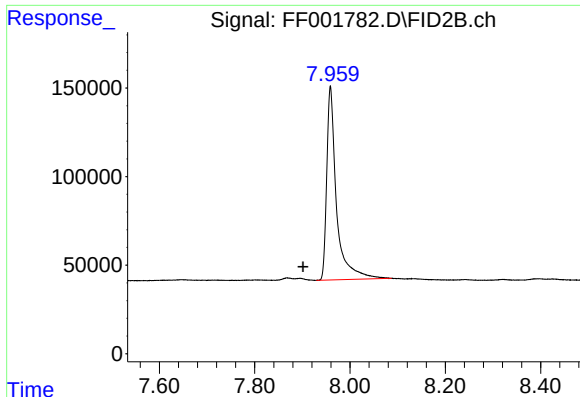

#4 N-TETRADECANE


R.T.: 7.959 min
Delta R.T.: 0.057 min
Response: 1548035
Conc: 10.27 ug/ml

Instrument :
FID_F
ClientSampleId :

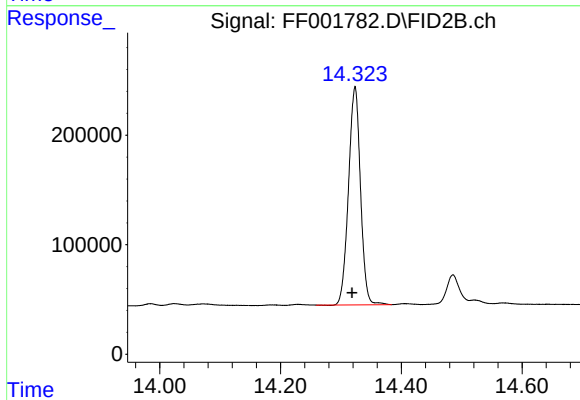


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.324 min
Delta R.T.: 0.005 min
Response: 2743018
Conc: 21.72 ug/ml

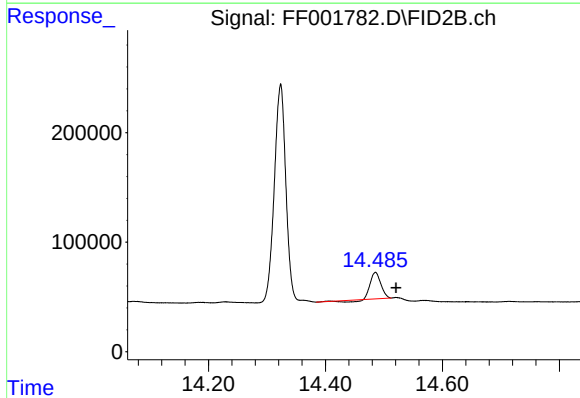


#10 N-TETRACOSANE

R.T.: 14.486 min
Delta R.T.: -0.035 min
Response: 276797
Conc: 1.94 ug/ml

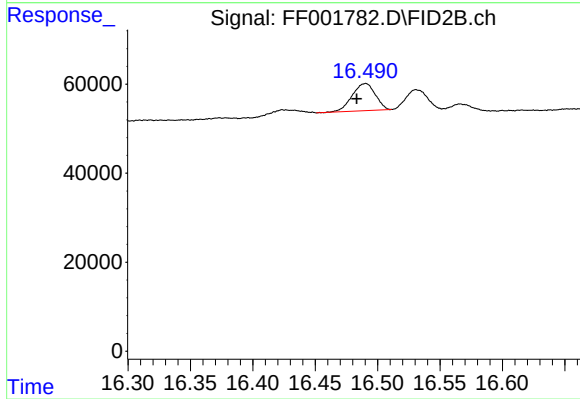

#12 N-OCTACOSANE


R.T.: 16.490 min
Delta R.T.: 0.007 min
Response: 78787
Conc: 0.56 ug/ml

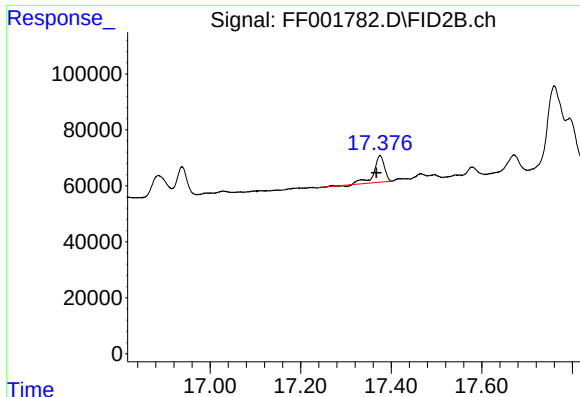

#13 N-TRIACONTANE


R.T.: 17.375 min
Delta R.T.: 0.008 min
Response: 150829
Conc: 1.09 ug/ml

Instrument :
FID_F
ClientSampleId :

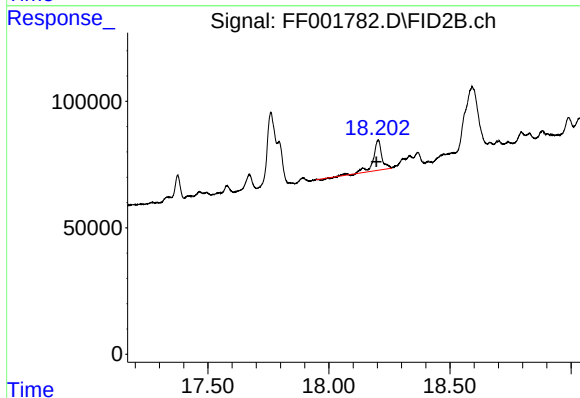


#14 N-DOTRIACONTANE

R.T.: 18.203 min
Delta R.T.: 0.006 min
Response: 290132
Conc: 2.22 ug/ml

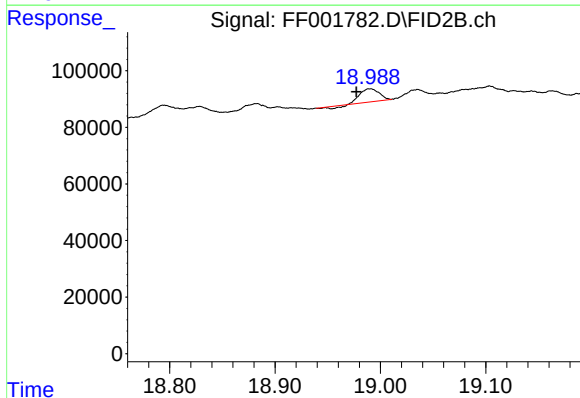

#15 N-TETRATRIACONTANE

R.T.: 18.990 min
Delta R.T.: 0.013 min
Response: 53121
Conc: 0.44 ug/ml

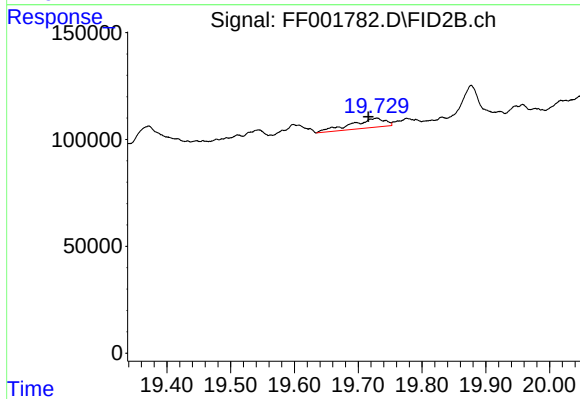

#16 N-HEXATRIACONTANE

R.T.: 19.729 min
Delta R.T.: 0.013 min
Response: 162260
Conc: 1.46 ug/ml