

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF081018\
 Data File : FF001783.D
 Signal(s) : FID2B.ch
 Acq On : 10 Aug 2018 12:38
 Operator : AJ\SJ
 Sample : J4398-03
 Misc :
 ALS Vial : 57 Sample Multiplier: 1

Instrument :
 FID_F
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Aug 10 13:11:18 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF073018.M
 Quant Title :
 QLast Update : Fri Aug 03 12:00:27 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.323	2792578	22.110 ug/ml
Target Compounds			
4) N-TETRADECANE	7.962f	453473	3.009 ug/ml
10) N-TETRACOSANE	14.486	231899	1.626 ug/ml
14) N-DOTRIACONTANE	18.204	129539	0.993 ug/ml
15) N-TETRATRIACONTANE	18.991	42706	0.353 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF081018\
Data File : FF001783.D
Signal(s) : FID2B.ch
Acq On : 10 Aug 2018 12:38
Operator : AJ\SJ
Sample : J4398-03
Misc :
ALS Vial : 57 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Aug 10 13:11:18 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF073018.M
Quant Title :
QLast Update : Fri Aug 03 12:00:27 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

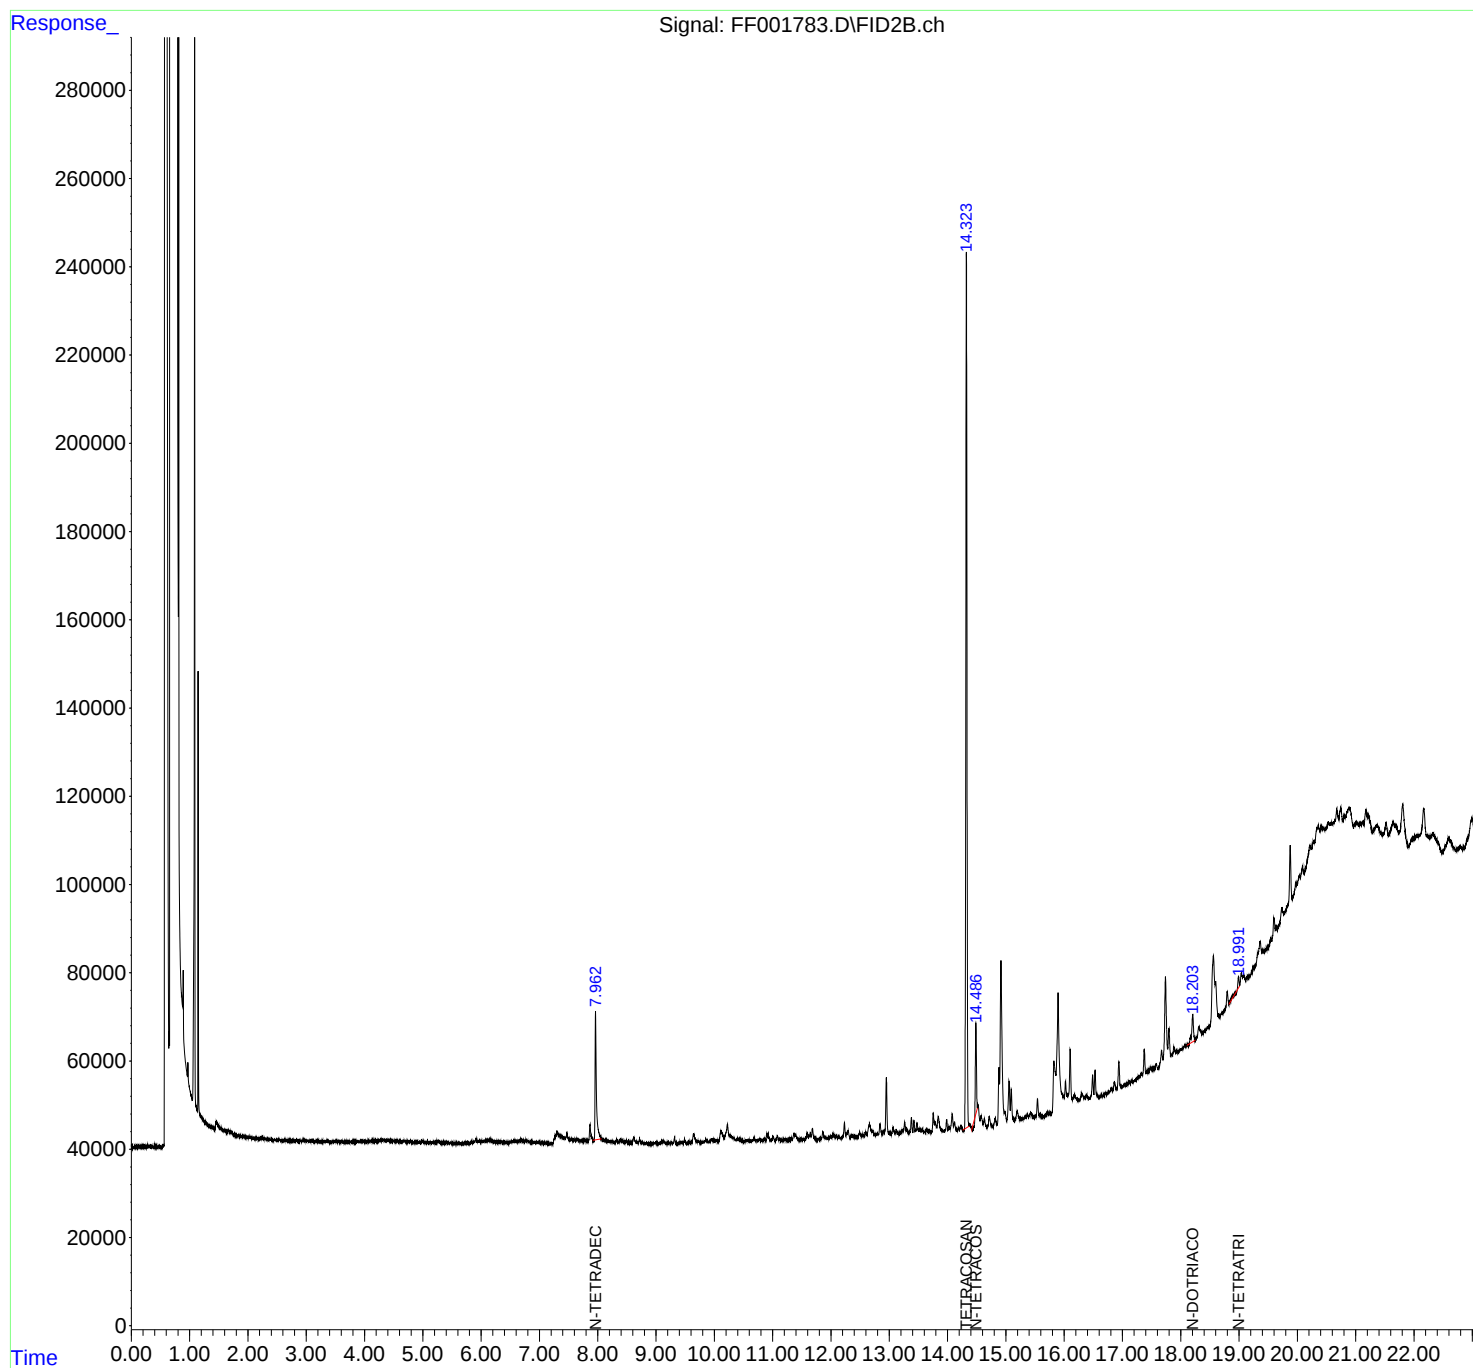


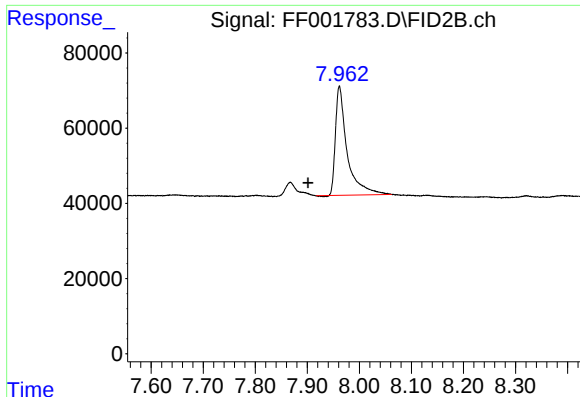

#4 N-TETRADECANE


R.T.: 7.962 min
Delta R.T.: 0.060 min
Response: 453473
Conc: 3.01 ug/ml

Instrument :
FID_F
ClientSampleId :

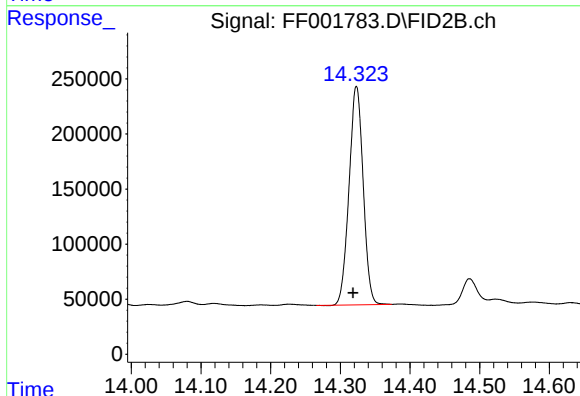


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.323 min
Delta R.T.: 0.005 min
Response: 2792578
Conc: 22.11 ug/ml

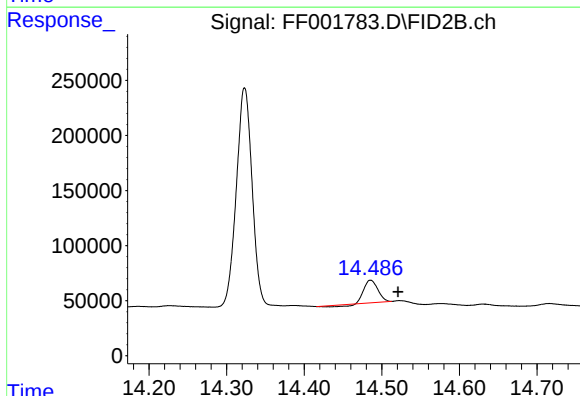


#10 N-TETRACOSANE

R.T.: 14.486 min
Delta R.T.: -0.035 min
Response: 231899
Conc: 1.63 ug/ml

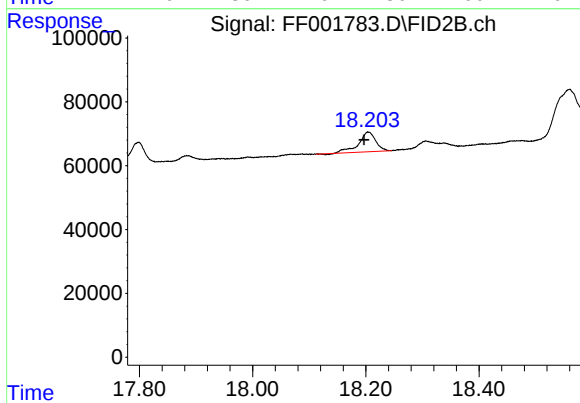

#14 N-DOTRIACONTANE

R.T.: 18.204 min
Delta R.T.: 0.008 min
Response: 129539
Conc: 0.99 ug/ml

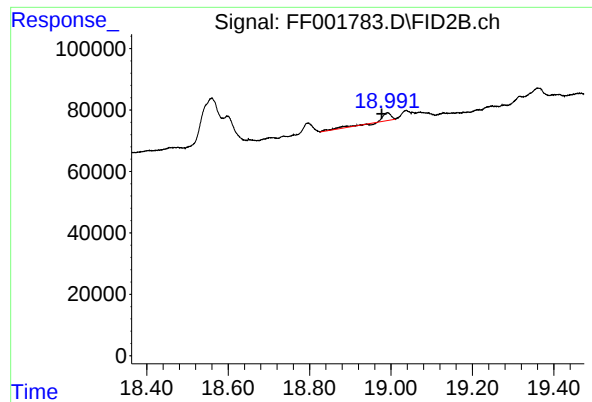

#15 N-TETRATRIACONTANE

R.T.: 18.991 min
Delta R.T.: 0.014 min
Response: 42706
Conc: 0.35 ug/ml

Instrument :
FID_F
ClientSampleId :