

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF081018\
 Data File : FF001787.D
 Signal(s) : FID2B.ch
 Acq On : 10 Aug 2018 14:41
 Operator : AJ\SJ
 Sample : J4272-05 10X
 Misc :
 ALS Vial : 61 Sample Multiplier: 1

Instrument :
 FID_F
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Aug 11 01:20:01 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF073018.M
 Quant Title :
 QLast Update : Fri Aug 03 12:00:27 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.324	281694	2.230 ug/ml
Target Compounds			
5) N-HEXADECANE	9.490	102224	0.683 ug/ml
6) N-OCTADECANE	10.926	79767	0.529 ug/ml
7) N-EICOSANE	12.232	181283	1.216 ug/ml
8) N-DOCOSANE	13.428	59471	0.407 ug/ml
10) N-TETRACOSANE	14.506	1439511	10.091 ug/ml
12) N-OCTACOSANE	16.491	94143	0.671 ug/ml
13) N-TRIACONTANE	17.380	168669	1.218 ug/ml
14) N-DOTRIACONTANE	18.207	323801	2.482 ug/ml
15) N-TETRATRIACONTANE	18.993	269993	2.234 ug/ml
16) N-HEXATRIACONTANE	19.706	233968	2.103 ug/ml
17) N-OCTATRIACONTANE	20.434	80803	0.811 ug/ml
18) N-TETRACONTANE	21.204	171875	1.725 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF081018\
Data File : FF001787.D
Signal(s) : FID2B.ch
Acq On : 10 Aug 2018 14:41
Operator : AJ\SJ
Sample : J4272-05 10X
Misc :
ALS Vial : 61 Sample Multiplier: 1

Instrument :
FID_F
ClientSampled :

Integration File: autoint1.e
Quant Time: Aug 11 01:20:01 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF073018.M
Quant Title :
QLast Update : Fri Aug 03 12:00:27 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

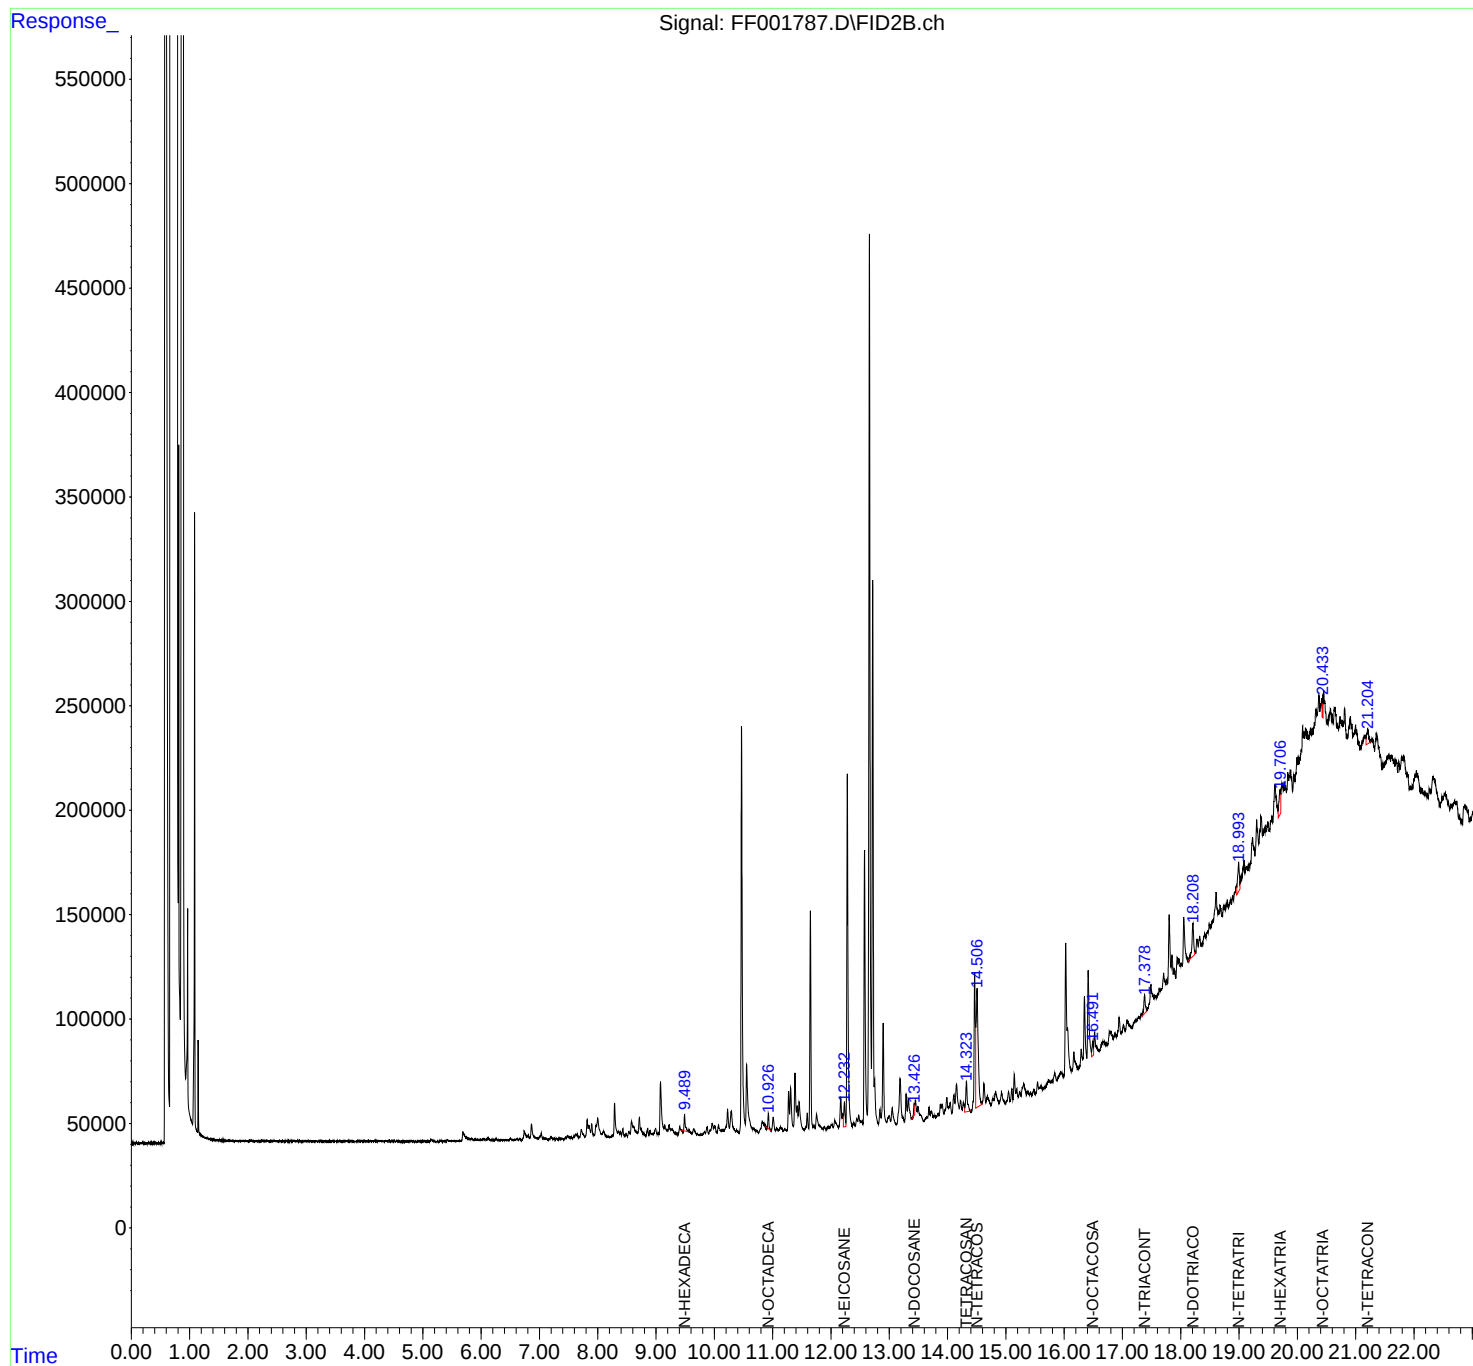


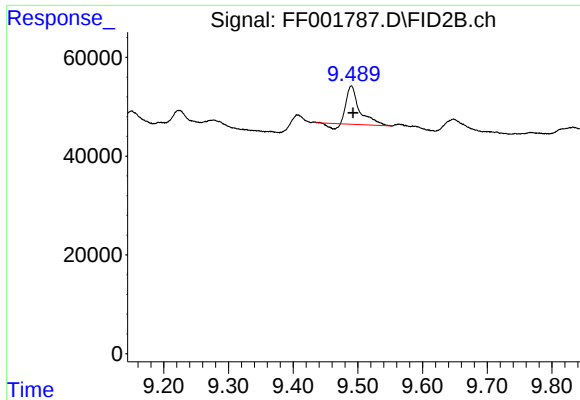

#5 N-HEXADECANE


R.T.: 9.490 min
Delta R.T.: -0.003 min
Response: 102224
Conc: 0.68 ug/ml

Instrument :
FID_F
ClientSampleId :

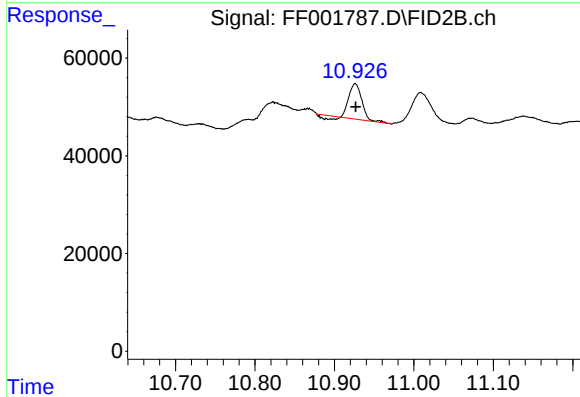


#6 N-OCTADECANE

R.T.: 10.926 min
Delta R.T.: 0.000 min
Response: 79767
Conc: 0.53 ug/ml

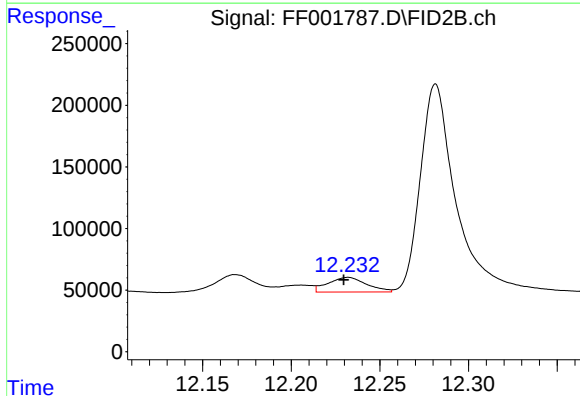


#7 N-EICOSANE

R.T.: 12.232 min
Delta R.T.: 0.003 min
Response: 181283
Conc: 1.22 ug/ml

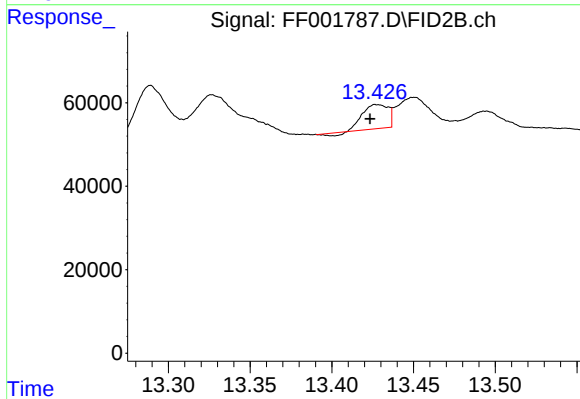

#8 N-DOCOSANE


R.T.: 13.428 min
Delta R.T.: 0.004 min
Response: 59471
Conc: 0.41 ug/ml

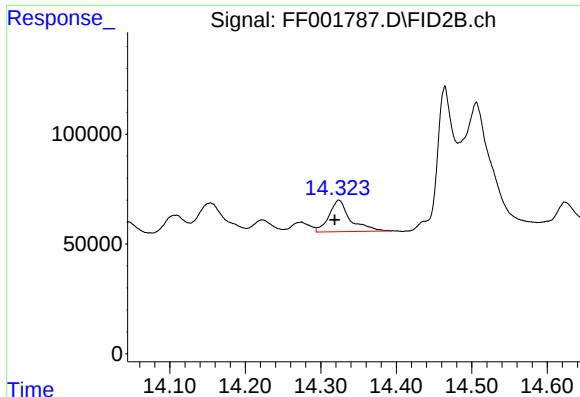

#9 TETRACOSANE-d50 (SURROGATE)


R.T.: 14.324 min
Delta R.T.: 0.006 min
Response: 281694
Conc: 2.23 ug/ml

Instrument :
FID_F
ClientSampleId :

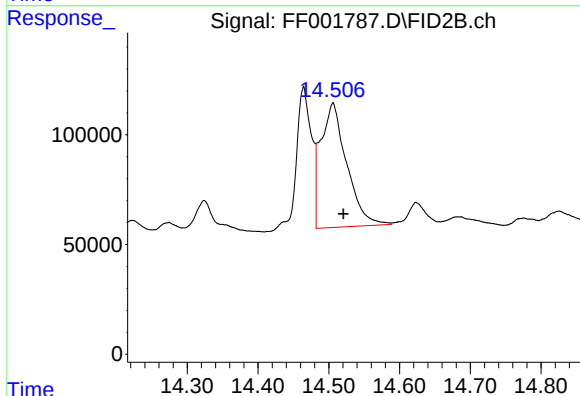


#10 N-TETRACOSANE

R.T.: 14.506 min
Delta R.T.: -0.015 min
Response: 1439511
Conc: 10.09 ug/ml

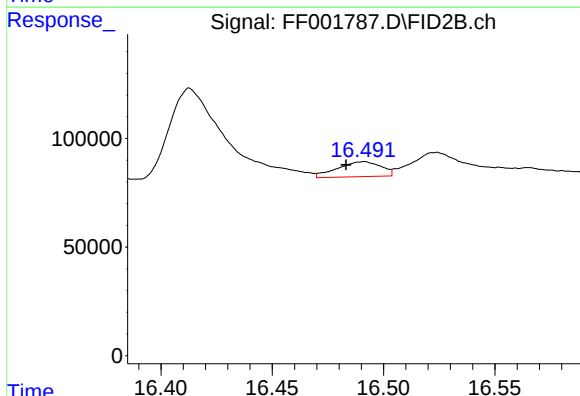


#12 N-OCTACOSANE

R.T.: 16.491 min
Delta R.T.: 0.008 min
Response: 94143
Conc: 0.67 ug/ml

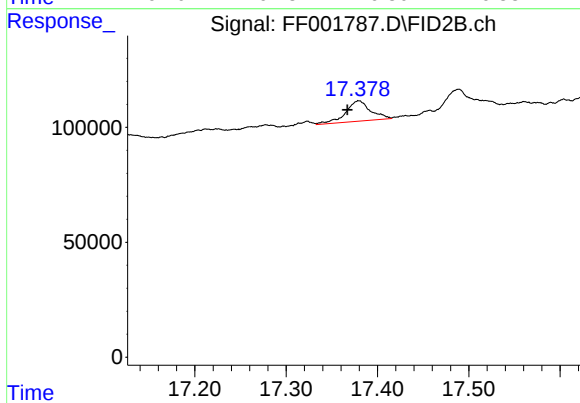

#13 N-TRIACONTANE


R.T.: 17.380 min
Delta R.T.: 0.012 min
Response: 168669
Conc: 1.22 ug/ml

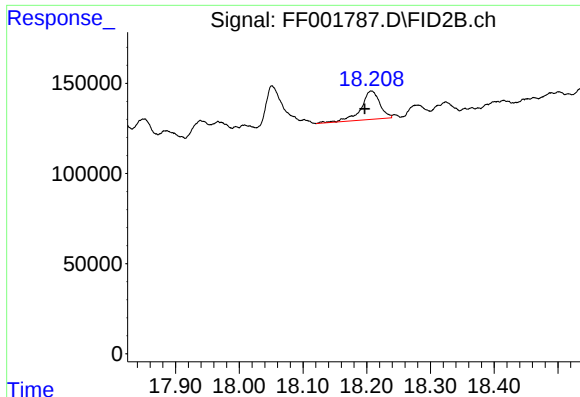

#14 N-DOTRIACONTANE


R.T.: 18.207 min
Delta R.T.: 0.011 min
Response: 323801
Conc: 2.48 ug/ml

Instrument :
FID_F
ClientSampleId :

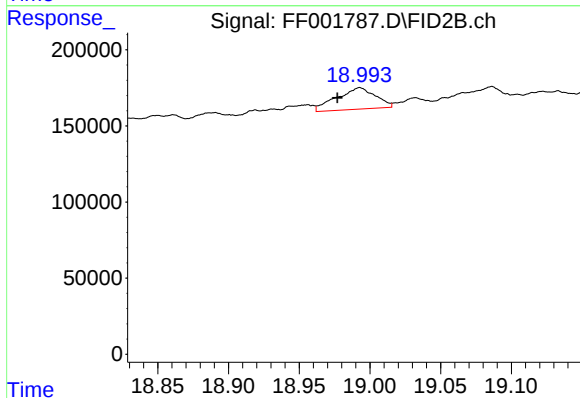


#15 N-TETRATRIACONTANE

R.T.: 18.993 min
Delta R.T.: 0.016 min
Response: 269993
Conc: 2.23 ug/ml

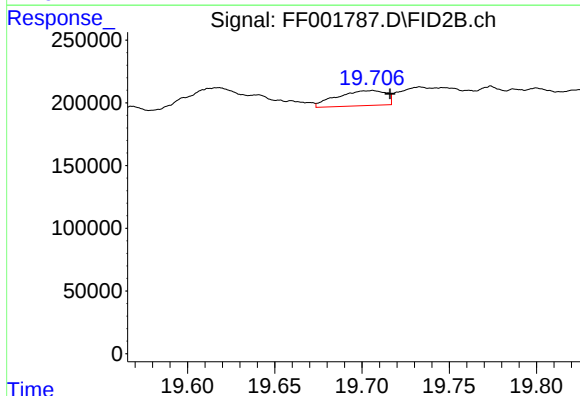


#16 N-HEXATRIACONTANE

R.T.: 19.706 min
Delta R.T.: -0.010 min
Response: 233968
Conc: 2.10 ug/ml

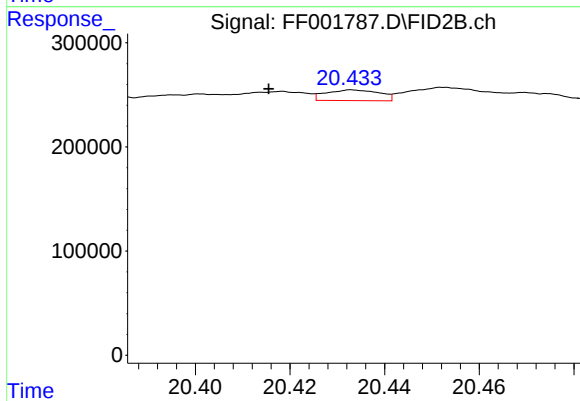

#17 N-OCTATRIACONTANE

R.T.: 20.434 min
Delta R.T.: 0.018 min
Response: 80803
Conc: 0.81 ug/ml

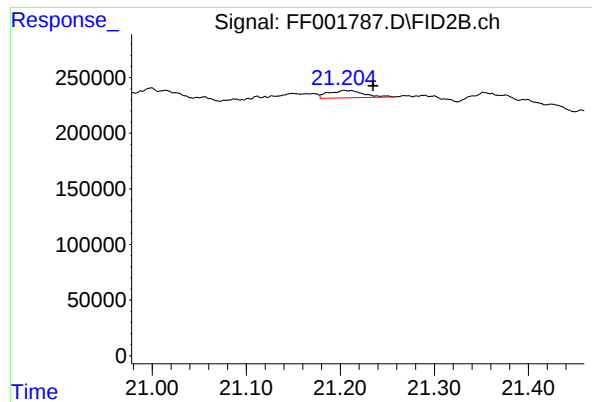

#18 N-TETRACONTANE

R.T.: 21.204 min
Delta R.T.: -0.031 min
Response: 171875
Conc: 1.73 ug/ml

Instrument :
FID_F
ClientSampleId :