

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF081018\
 Data File : FF001794.D
 Signal(s) : FID2B.ch
 Acq On : 10 Aug 2018 18:17
 Operator : AJ\SJ
 Sample : J4272-09
 Misc :
 ALS Vial : 66 Sample Multiplier: 1

Instrument :
 FID_F
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Aug 11 01:21:25 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF073018.M
 Quant Title :
 QLast Update : Fri Aug 03 12:00:27 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.324	2476272	19.606 ug/ml
Target Compounds			
4) N-TETRADECANE	7.846f	122859	0.815 ug/ml
5) N-HEXADECANE	9.501	269718	1.802 ug/ml
7) N-EICOSANE	12.231	380860	2.555 ug/ml
8) N-DOCOSANE	13.443	837310	5.732 ug/ml
10) N-TETRACOSANE	14.500	4526634	31.732 ug/ml
11) N-HEXACOSANE	15.552	150415	1.068 ug/ml
12) N-OCTACOSANE	16.511	1154002	8.230 ug/ml
13) N-TRIACONTANE	17.379	491553	3.551 ug/ml
14) N-DOTRIACONTANE	18.192	1216126	9.322 ug/ml
15) N-TETRATRIACONTANE	18.992	190173	1.573 ug/ml
16) N-HEXATRIACONTANE	19.739	327629	2.945 ug/ml
17) N-OCTATRIACONTANE	20.437	108950	1.093 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF081018\
Data File : FF001794.D
Signal(s) : FID2B.ch
Acq On : 10 Aug 2018 18:17
Operator : AJ\SJ
Sample : J4272-09
Misc :
ALS Vial : 66 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Aug 11 01:21:25 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF073018.M
Quant Title :
QLast Update : Fri Aug 03 12:00:27 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

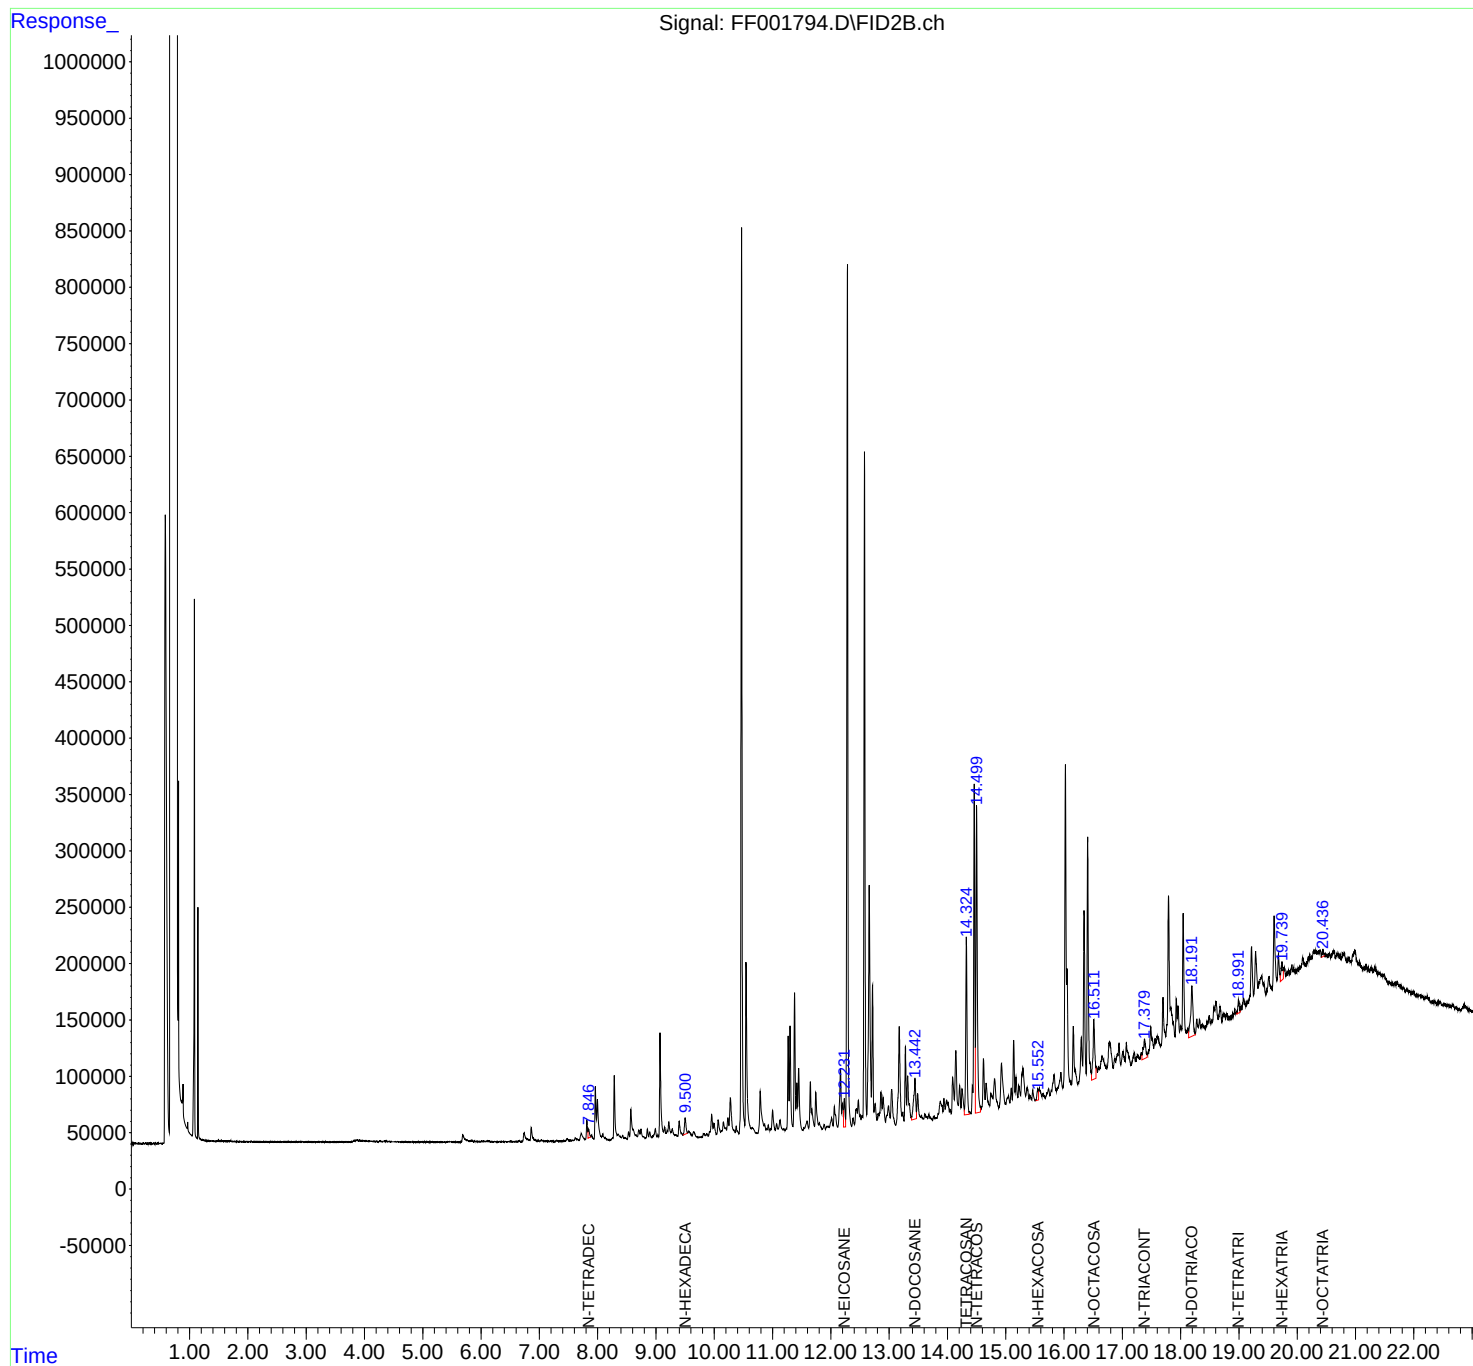


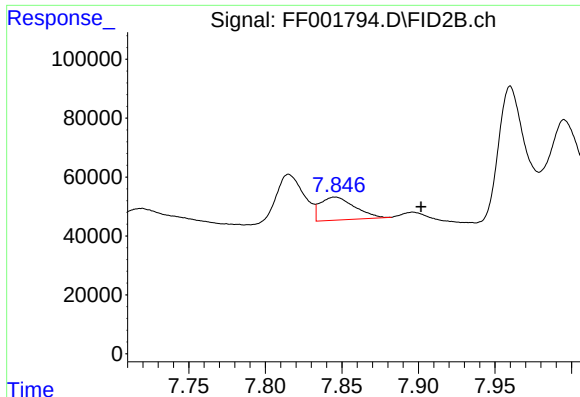

#4 N-TETRADECANE


R.T.: 7.846 min
Delta R.T.: -0.056 min
Response: 122859
Conc: 0.82 ug/ml

Instrument :
FID_F
ClientSampleId :

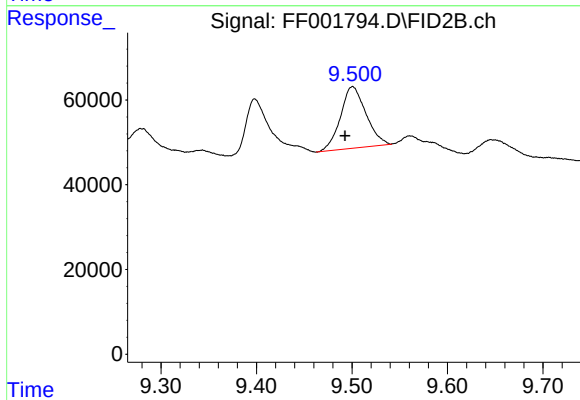


#5 N-HEXADECANE

R.T.: 9.501 min
Delta R.T.: 0.008 min
Response: 269718
Conc: 1.80 ug/ml

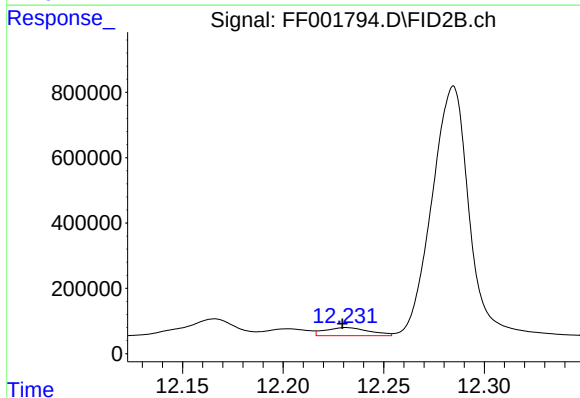


#7 N-EICOSANE

R.T.: 12.231 min
Delta R.T.: 0.002 min
Response: 380860
Conc: 2.56 ug/ml

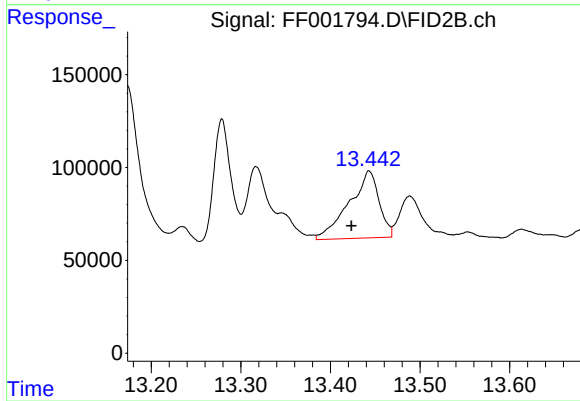

#8 N-DOCOSANE


R.T.: 13.443 min
Delta R.T.: 0.020 min
Response: 837310
Conc: 5.73 ug/ml

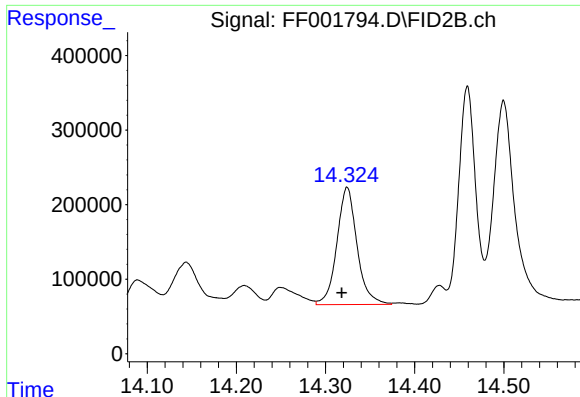

#9 TETRACOSANE-d50 (SURROGATE)


R.T.: 14.324 min
Delta R.T.: 0.006 min
Response: 2476272
Conc: 19.61 ug/ml

Instrument :
FID_F
ClientSampleId :

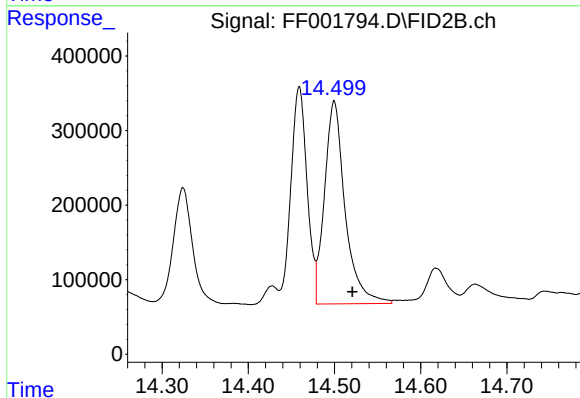


#10 N-TETRACOSANE

R.T.: 14.500 min
Delta R.T.: -0.021 min
Response: 4526634
Conc: 31.73 ug/ml

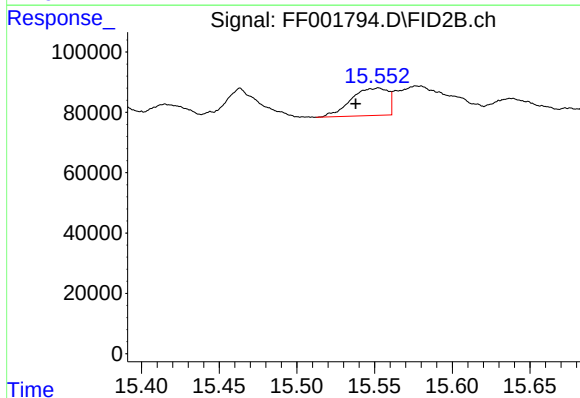


#11 N-HEXACOSANE

R.T.: 15.552 min
Delta R.T.: 0.015 min
Response: 150415
Conc: 1.07 ug/ml

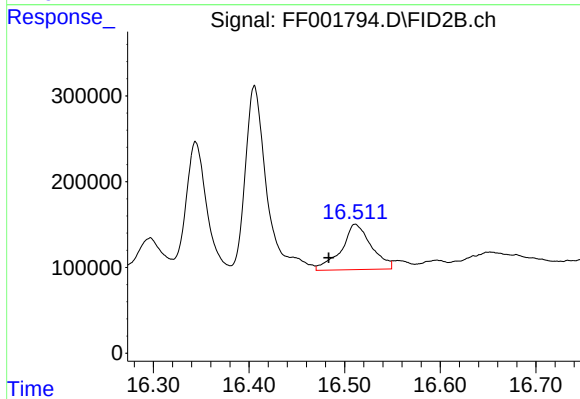

#12 N-OCTACOSANE


R.T.: 16.511 min
Delta R.T.: 0.028 min
Response: 1154002
Conc: 8.23 ug/ml

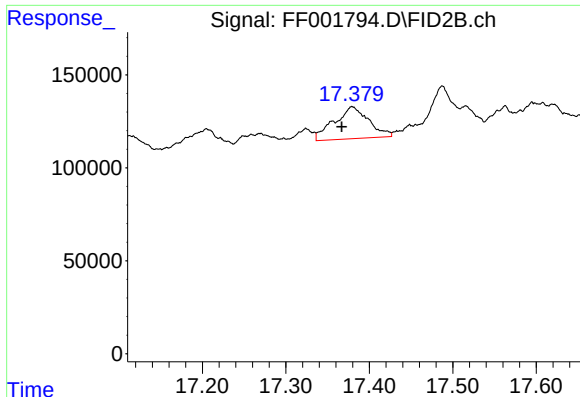

#13 N-TRIACONTANE


R.T.: 17.379 min
Delta R.T.: 0.012 min
Response: 491553
Conc: 3.55 ug/ml

Instrument :
FID_F
ClientSampleId :

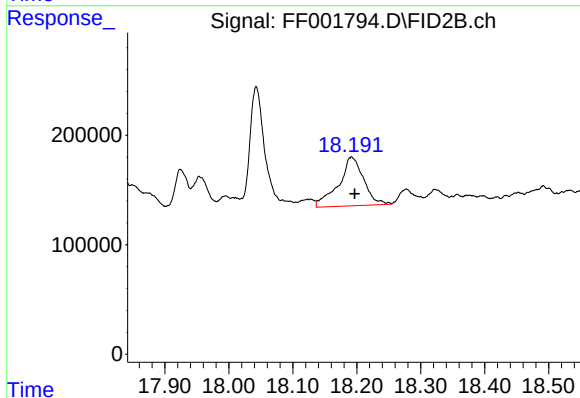


#14 N-DOTRIACONTANE

R.T.: 18.192 min
Delta R.T.: -0.005 min
Response: 1216126
Conc: 9.32 ug/ml

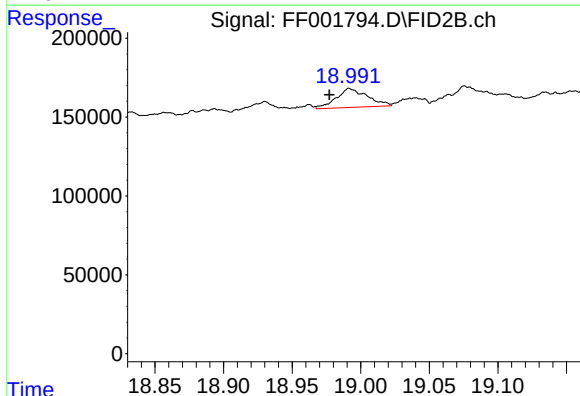


#15 N-TETRATRIACONTANE

R.T.: 18.992 min
Delta R.T.: 0.015 min
Response: 190173
Conc: 1.57 ug/ml

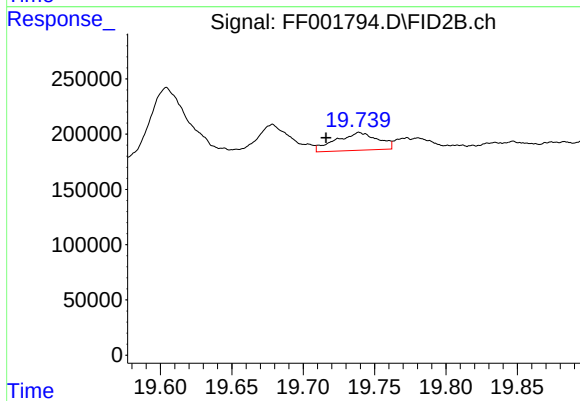

#16 N-HEXATRIACONTANE

R.T.: 19.739 min
Delta R.T.: 0.023 min
Response: 327629
Conc: 2.94 ug/ml

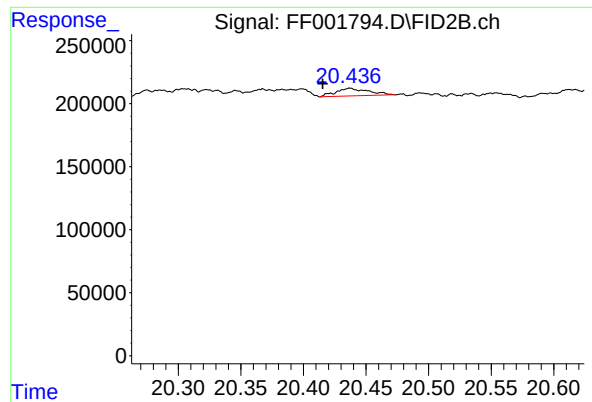

#17 N-OCTATRIACONTANE

R.T.: 20.437 min
Delta R.T.: 0.022 min
Response: 108950
Conc: 1.09 ug/ml

Instrument :
FID_F
ClientSampleId :