

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF081018\
 Data File : FF001795.D
 Signal(s) : FID2B.ch
 Acq On : 10 Aug 2018 18:48
 Operator : AJ\SJ
 Sample : J4272-15 10X
 Misc :
 ALS Vial : 67 Sample Multiplier: 1

Instrument :
 FID_F
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Aug 11 01:21:39 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF073018.M
 Quant Title :
 QLast Update : Fri Aug 03 12:00:27 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.322	199880	1.583 ug/ml
Target Compounds			
7) N-EICOSANE	12.291f	246635	1.655 ug/ml
10) N-TETRACOSANE	14.521	197036	1.381 ug/ml
12) N-OCTACOSANE	16.489	57697	0.411 ug/ml
13) N-TRIACONTANE	17.377	100586	0.727 ug/ml
14) N-DOTRIACONTANE	18.207	142347	1.091 ug/ml
15) N-TETRATRIACONTANE	18.990	135094	1.118 ug/ml
16) N-HEXATRIACONTANE	19.710	63834	0.574 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF081018\
Data File : FF001795.D
Signal(s) : FID2B.ch
Acq On : 10 Aug 2018 18:48
Operator : AJ\SJ
Sample : J4272-15 10X
Misc :
ALS Vial : 67 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Aug 11 01:21:39 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF073018.M
Quant Title :
QLast Update : Fri Aug 03 12:00:27 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

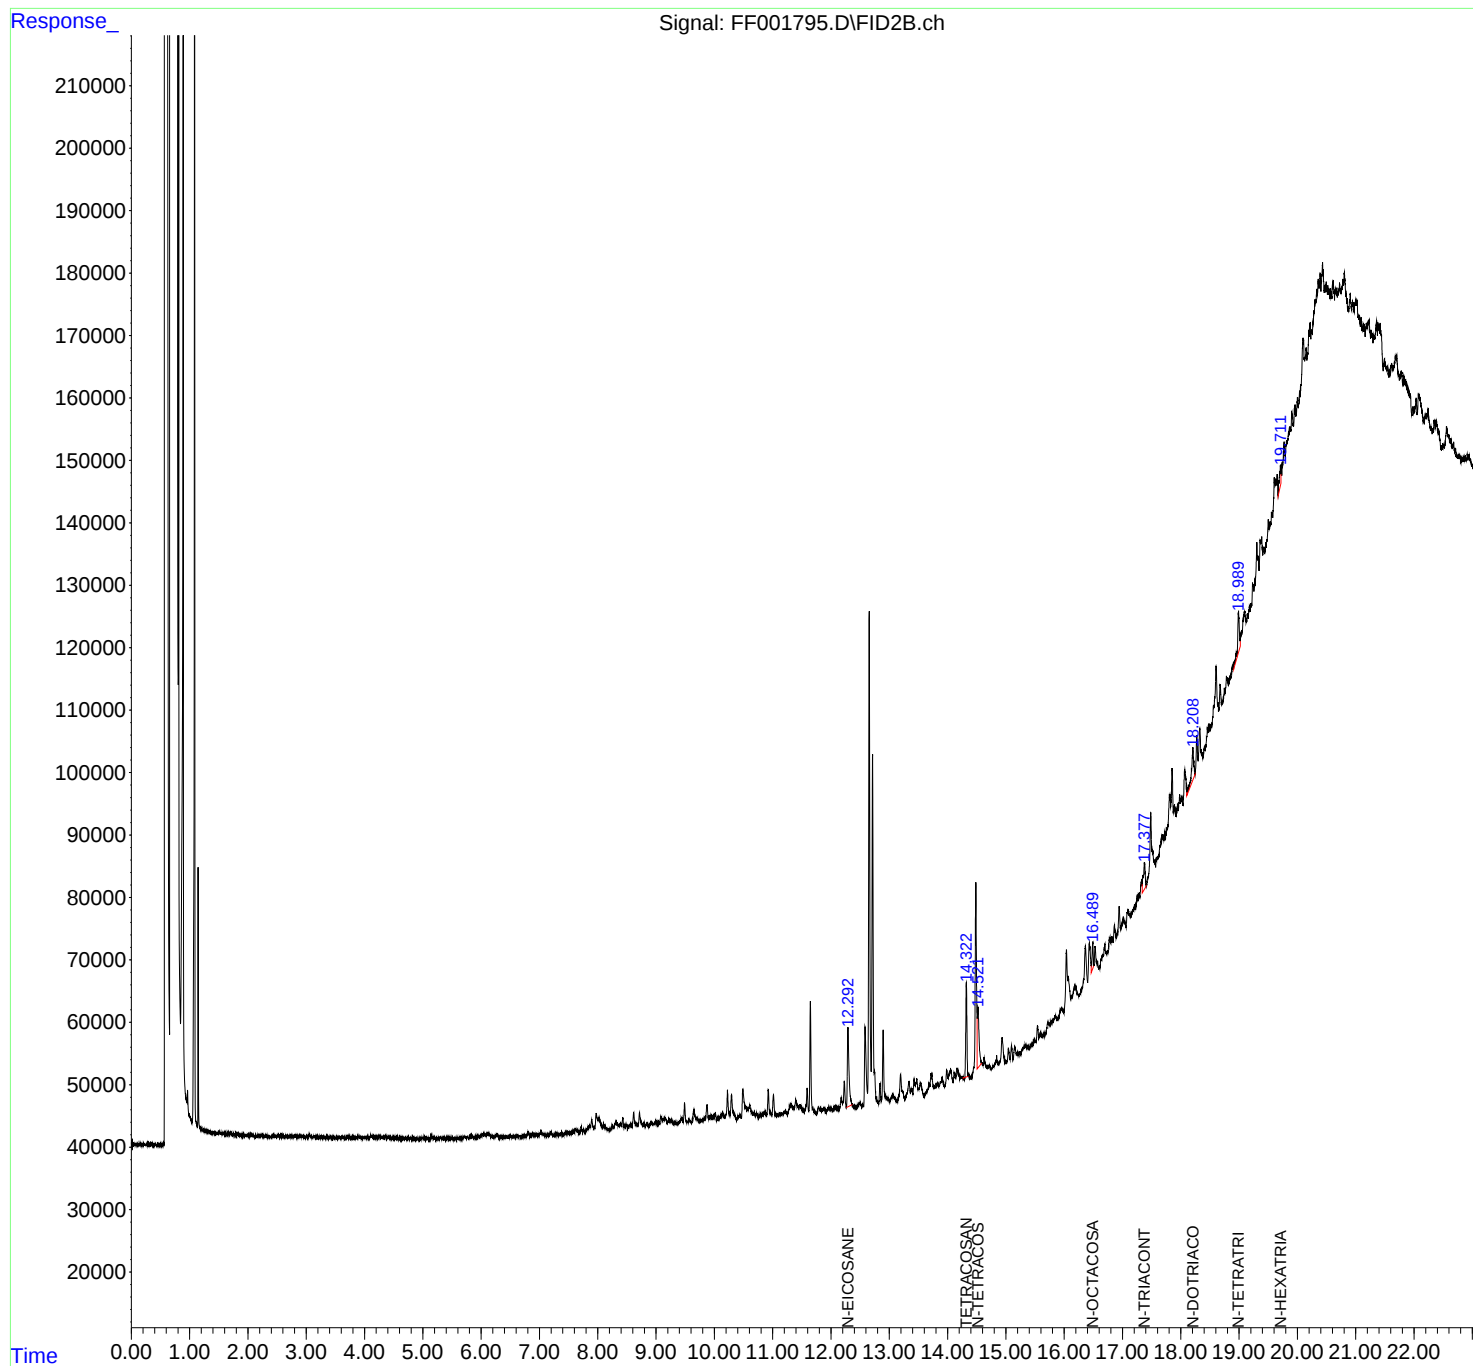


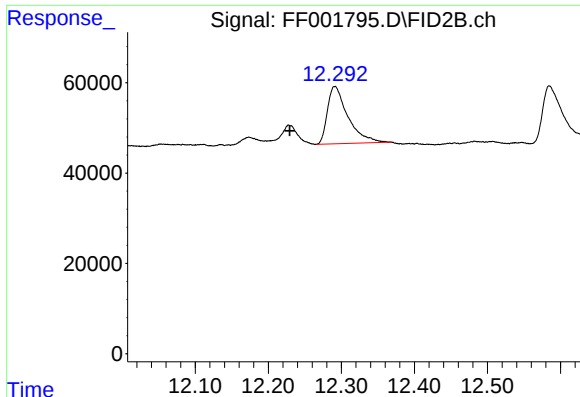

#7 N-EICOSANE


R.T.: 12.291 min
Delta R.T.: 0.062 min
Response: 246635
Conc: 1.65 ug/ml

Instrument :
FID_F
ClientSampleId :

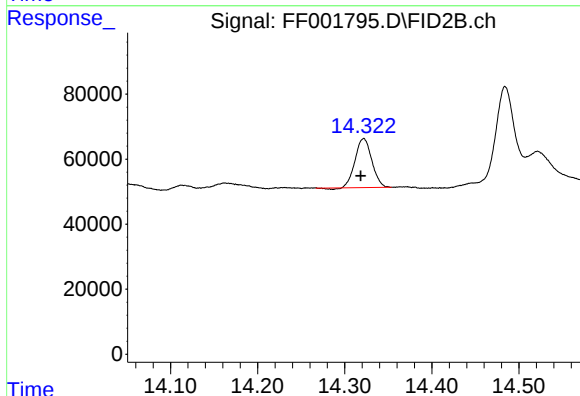


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.322 min
Delta R.T.: 0.003 min
Response: 199880
Conc: 1.58 ug/ml

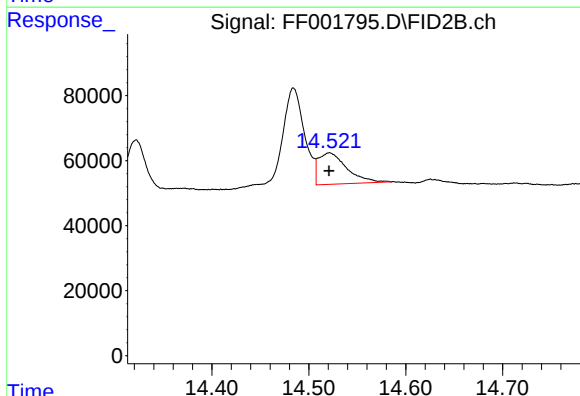


#10 N-TETRACOSANE

R.T.: 14.521 min
Delta R.T.: 0.000 min
Response: 197036
Conc: 1.38 ug/ml

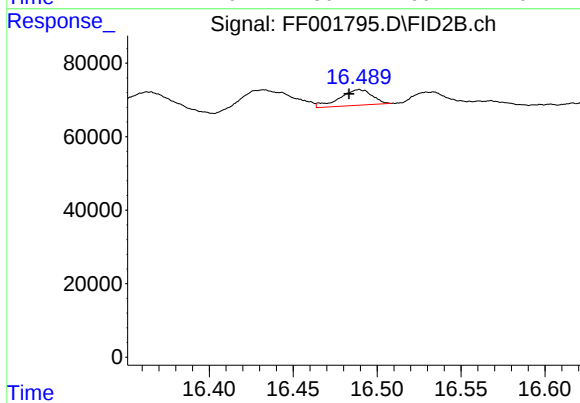

#12 N-OCTACOSANE


R.T.: 16.489 min
Delta R.T.: 0.006 min
Response: 57697
Conc: 0.41 ug/ml

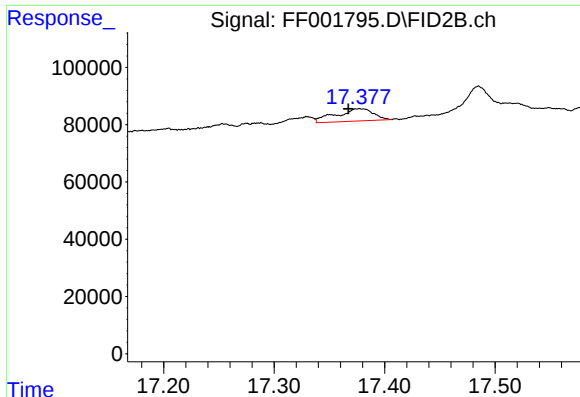

#13 N-TRIACONTANE


R.T.: 17.377 min
Delta R.T.: 0.010 min
Response: 100586
Conc: 0.73 ug/ml

Instrument :
FID_F
ClientSampleId :

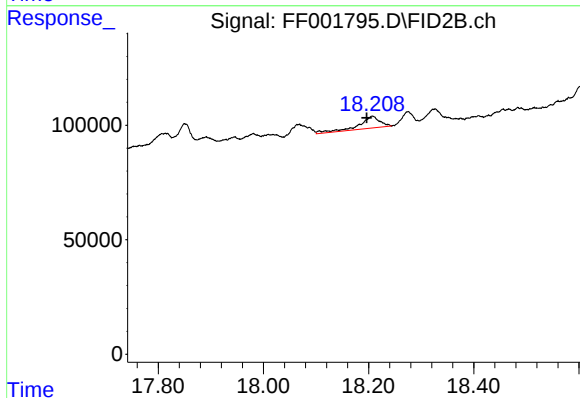


#14 N-DOTRIACONTANE

R.T.: 18.207 min
Delta R.T.: 0.011 min
Response: 142347
Conc: 1.09 ug/ml

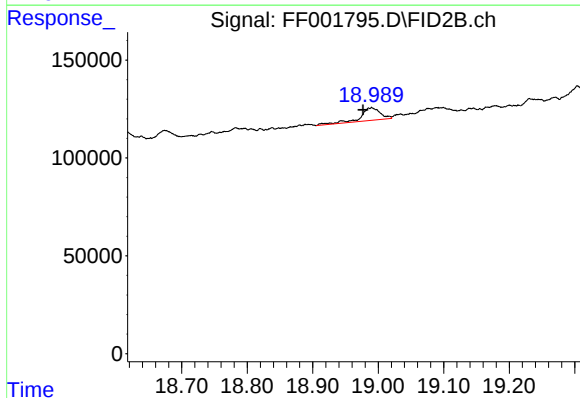

#15 N-TETRATRIACONTANE

R.T.: 18.990 min
Delta R.T.: 0.013 min
Response: 135094
Conc: 1.12 ug/ml

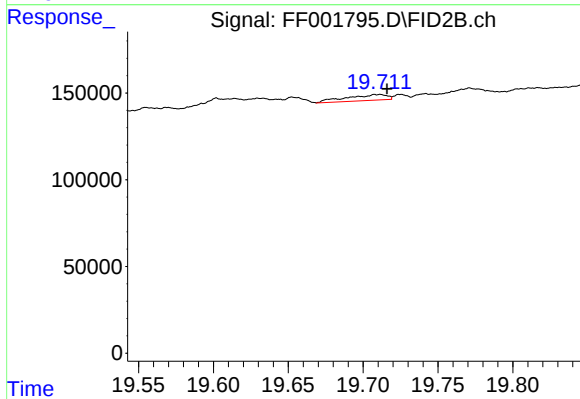

#16 N-HEXATRIACONTANE

R.T.: 19.710 min
Delta R.T.: -0.006 min
Response: 63834
Conc: 0.57 ug/ml