

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF081018\
 Data File : FF001797.D
 Signal(s) : FID2B.ch
 Acq On : 10 Aug 2018 19:51
 Operator : AJ\SJ
 Sample : J4272-19 10X
 Misc :
 ALS Vial : 69 Sample Multiplier: 1

Instrument :
 FID_F
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Aug 11 01:22:01 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF073018.M
 Quant Title :
 QLast Update : Fri Aug 03 12:00:27 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.322	196635	1.557 ug/ml
Target Compounds			
7) N-EICOSANE	12.292f	273431	1.835 ug/ml
10) N-TETRACOSANE	14.520	163788	1.148 ug/ml
12) N-OCTACOSANE	16.431f	93830	0.669 ug/ml
13) N-TRIACONTANE	17.379	125860	0.909 ug/ml
14) N-DOTRIACONTANE	18.209	92933	0.712 ug/ml
15) N-TETRATRIACONTANE	18.992	104677	0.866 ug/ml
16) N-HEXATRIACONTANE	19.730	98401	0.884 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF081018\
Data File : FF001797.D
Signal(s) : FID2B.ch
Acq On : 10 Aug 2018 19:51
Operator : AJ\SJ
Sample : J4272-19 10X
Misc :
ALS Vial : 69 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Aug 11 01:22:01 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF073018.M
Quant Title :
QLast Update : Fri Aug 03 12:00:27 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

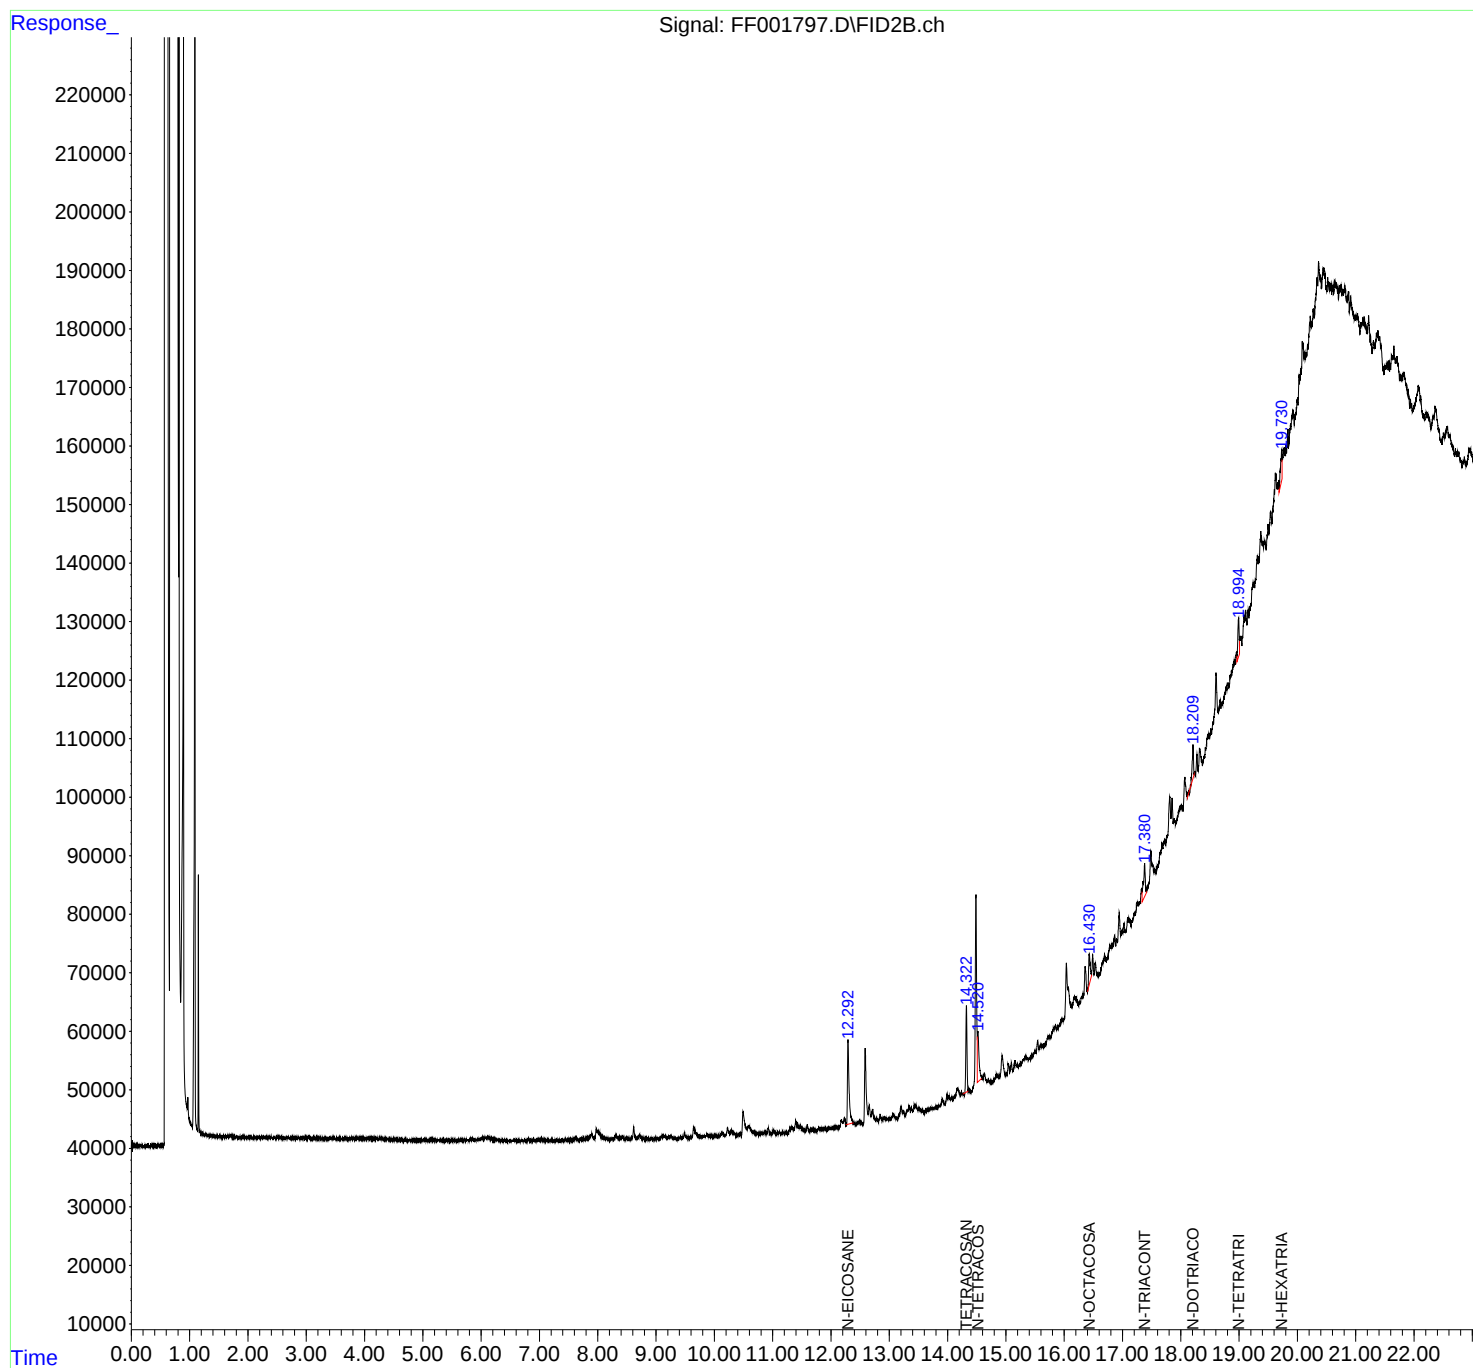


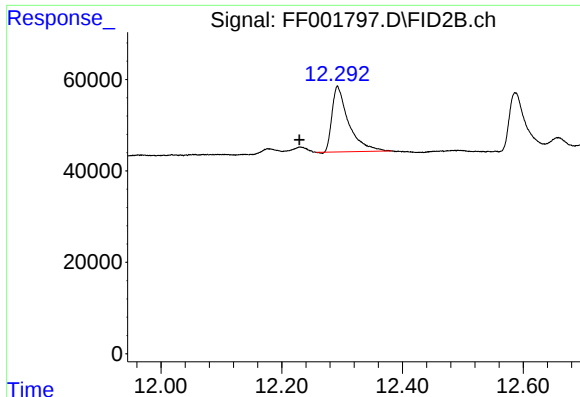

#7 N-EICOSANE


R.T.: 12.292 min
Delta R.T.: 0.063 min
Response: 273431
Conc: 1.83 ug/ml

Instrument :
FID_F
ClientSampleId :

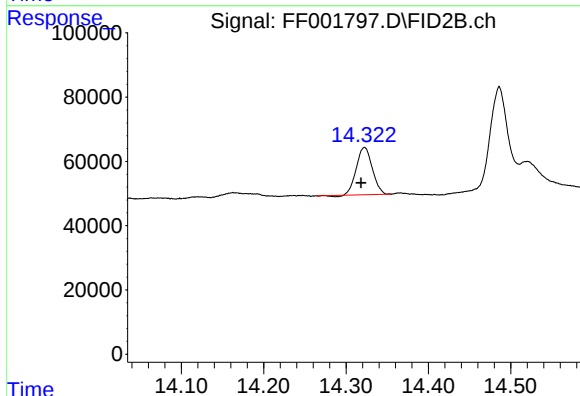


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.322 min
Delta R.T.: 0.004 min
Response: 196635
Conc: 1.56 ug/ml

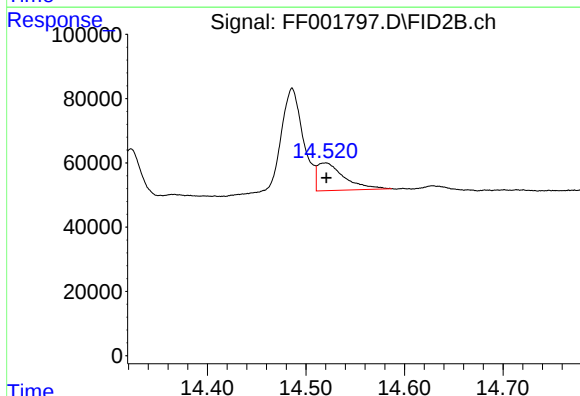


#10 N-TETRACOSANE

R.T.: 14.520 min
Delta R.T.: 0.000 min
Response: 163788
Conc: 1.15 ug/ml

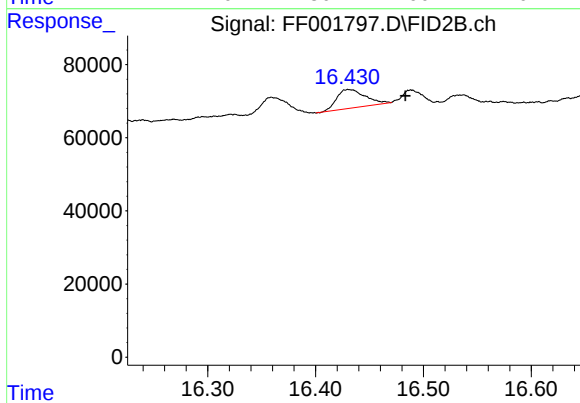

#12 N-OCTACOSANE


R.T.: 16.431 min
Delta R.T.: -0.053 min
Response: 93830
Conc: 0.67 ug/ml

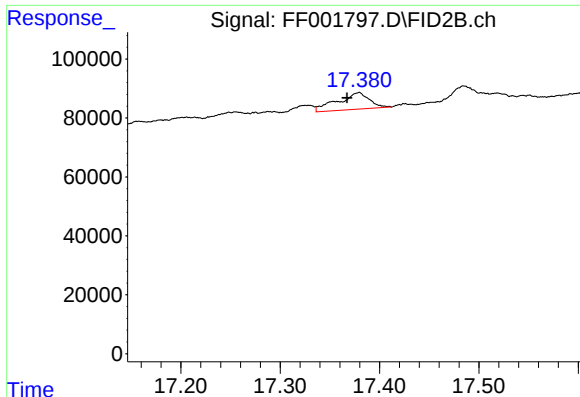

#13 N-TRIACONTANE


R.T.: 17.379 min
Delta R.T.: 0.012 min
Response: 125860
Conc: 0.91 ug/ml

Instrument :
FID_F
ClientSampleId :

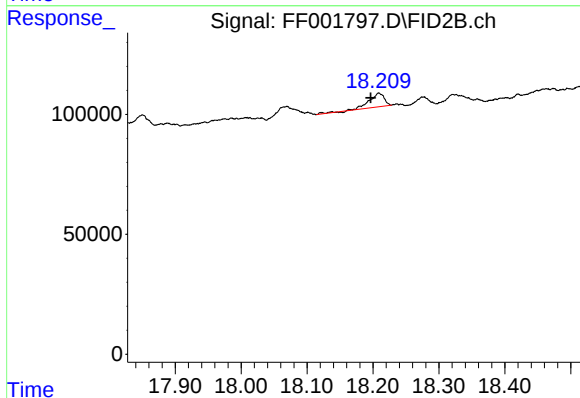


#14 N-DOTRIACONTANE

R.T.: 18.209 min
Delta R.T.: 0.012 min
Response: 92933
Conc: 0.71 ug/ml

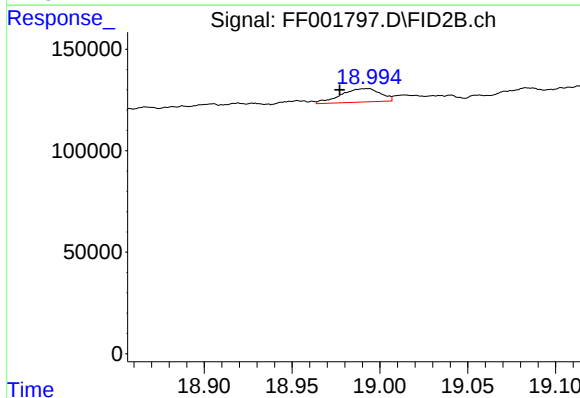

#15 N-TETRATRIACONTANE

R.T.: 18.992 min
Delta R.T.: 0.015 min
Response: 104677
Conc: 0.87 ug/ml

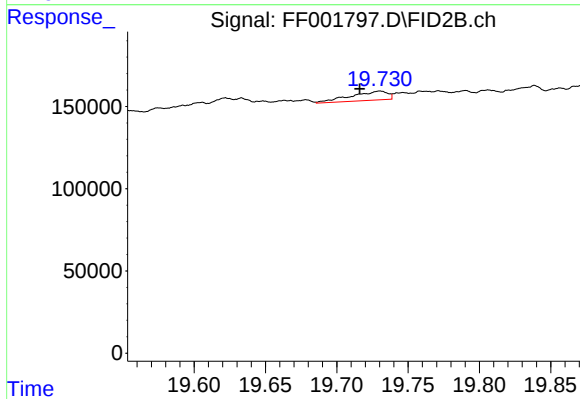

#16 N-HEXATRIACONTANE

R.T.: 19.730 min
Delta R.T.: 0.014 min
Response: 98401
Conc: 0.88 ug/ml