

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF081018\
 Data File : FF001799.D
 Signal(s) : FID2B.ch
 Acq On : 10 Aug 2018 20:53
 Operator : AJ\SJ
 Sample : J4274-01 10X
 Misc :
 ALS Vial : 71 Sample Multiplier: 1

Instrument :
 FID_F
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Aug 11 01:22:23 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF073018.M
 Quant Title :
 QLast Update : Fri Aug 03 12:00:27 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.323	161657	1.280 ug/ml
Target Compounds			
3) N-DODECANE	6.113	152393	1.022 ug/ml
4) N-TETRADECANE	7.896	322602	2.140 ug/ml
5) N-HEXADECANE	9.489	512007	3.420 ug/ml
6) N-OCTADECANE	10.925	461716	3.063 ug/ml
7) N-EICOSANE	12.230	341522	2.291 ug/ml
8) N-DOCOSANE	13.428	257116	1.760 ug/ml
10) N-TETRACOSANE	14.523	688516	4.827 ug/ml
11) N-HEXACOSANE	15.544	94182	0.669 ug/ml
13) N-TRIACONTANE	17.376	141395	1.021 ug/ml
14) N-DOTRIACONTANE	18.206	205786	1.577 ug/ml
15) N-TETRATRIACONTANE	18.991	229400	1.898 ug/ml
16) N-HEXATRIACONTANE	19.733	109520	0.984 ug/ml
17) N-OCTATRIACONTANE	20.440	298773	2.998 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF081018\
Data File : FF001799.D
Signal(s) : FID2B.ch
Acq On : 10 Aug 2018 20:53
Operator : AJ\SJ
Sample : J4274-01 10X
Misc :
ALS Vial : 71 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Aug 11 01:22:23 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF073018.M
Quant Title :
QLast Update : Fri Aug 03 12:00:27 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

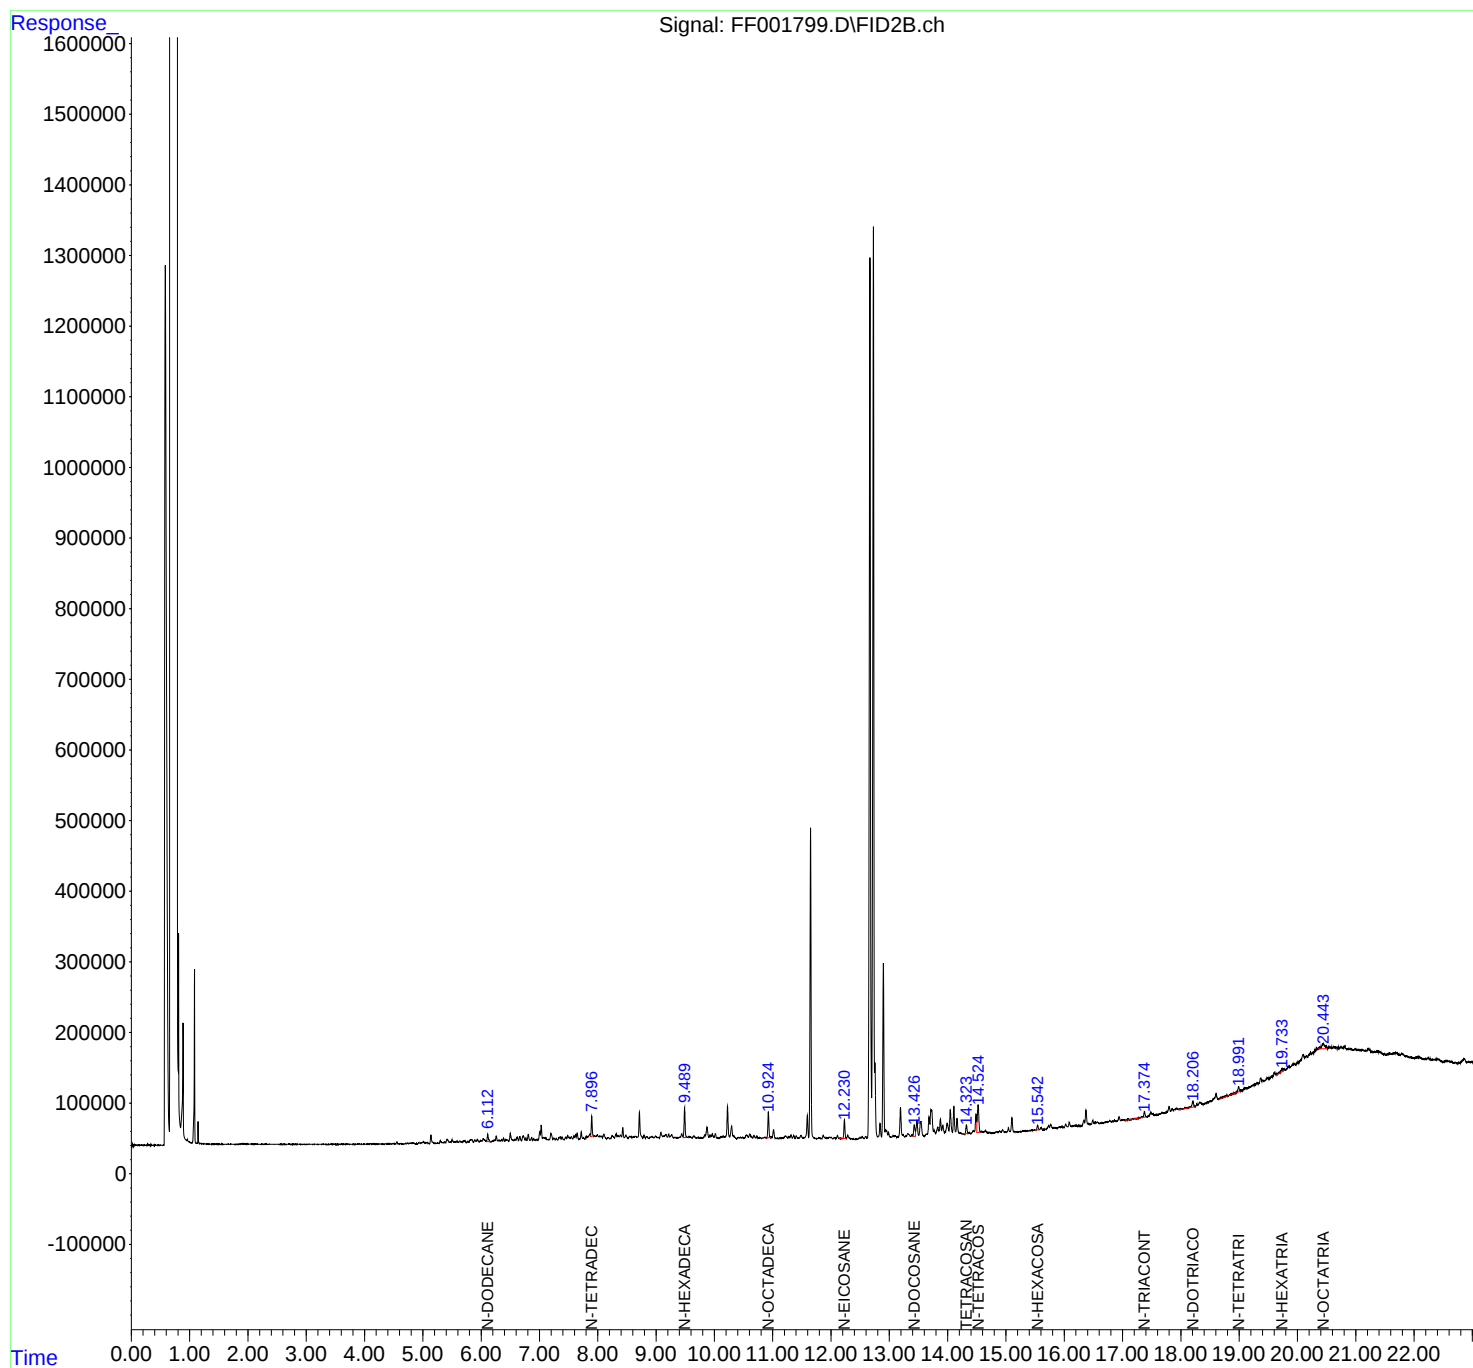


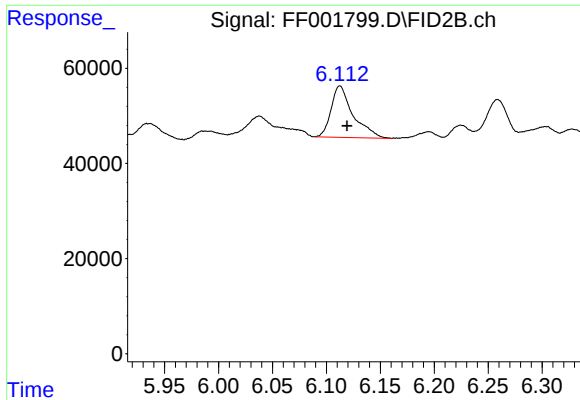

#3 N-DODECANE


R.T.: 6.113 min
Delta R.T.: -0.007 min
Response: 152393
Conc: 1.02 ug/ml

Instrument :
FID_F
ClientSampleId :

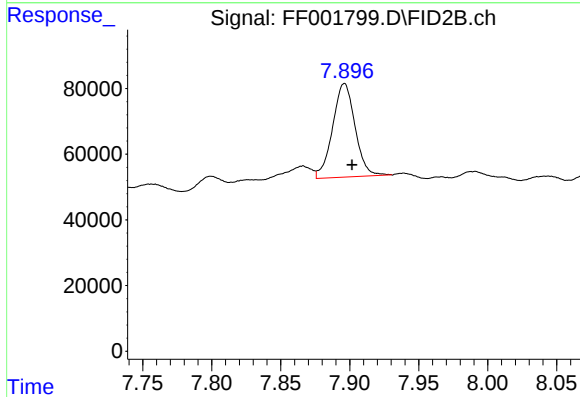


#4 N-TETRADECANE

R.T.: 7.896 min
Delta R.T.: -0.006 min
Response: 322602
Conc: 2.14 ug/ml

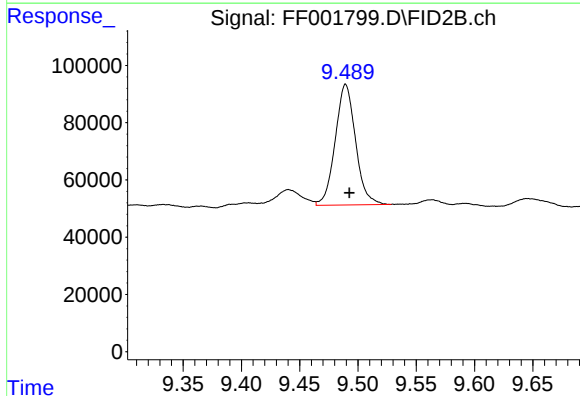


#5 N-HEXADECANE

R.T.: 9.489 min
Delta R.T.: -0.003 min
Response: 512007
Conc: 3.42 ug/ml

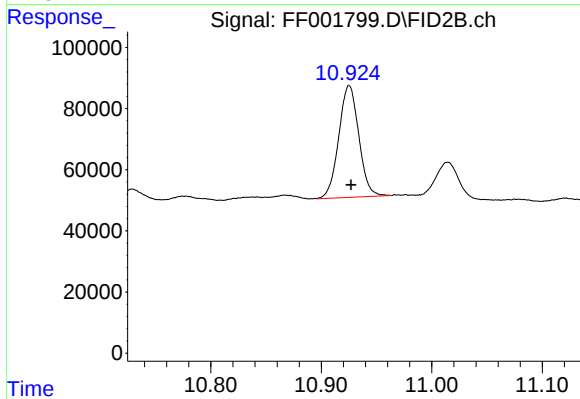

#6 N-OCTADECANE


R.T.: 10.925 min
Delta R.T.: -0.002 min
Response: 461716
Conc: 3.06 ug/ml

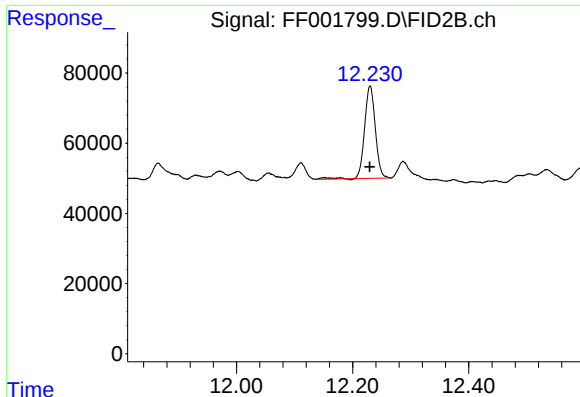

#7 N-EICOSANE


R.T.: 12.230 min
Delta R.T.: 0.000 min
Response: 341522
Conc: 2.29 ug/ml

Instrument :
FID_F
ClientSampleId :

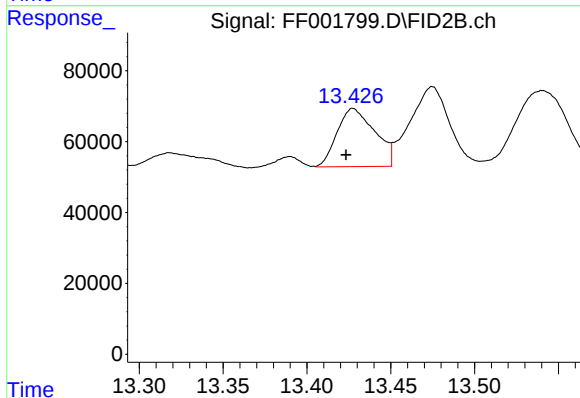


#8 N-DOCOSANE

R.T.: 13.428 min
Delta R.T.: 0.004 min
Response: 257116
Conc: 1.76 ug/ml

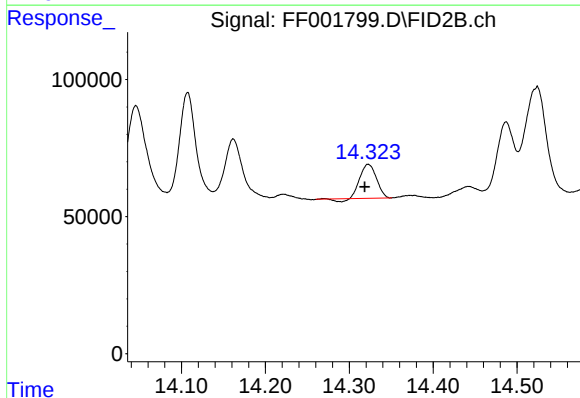


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.323 min
Delta R.T.: 0.004 min
Response: 161657
Conc: 1.28 ug/ml

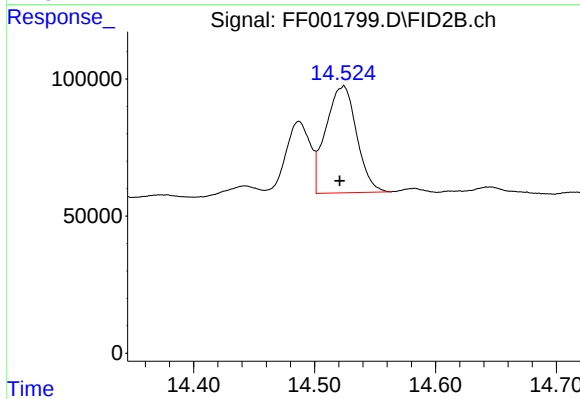

#10 N-TETRACOSANE


R.T.: 14.523 min
Delta R.T.: 0.002 min
Response: 688516
Conc: 4.83 ug/ml

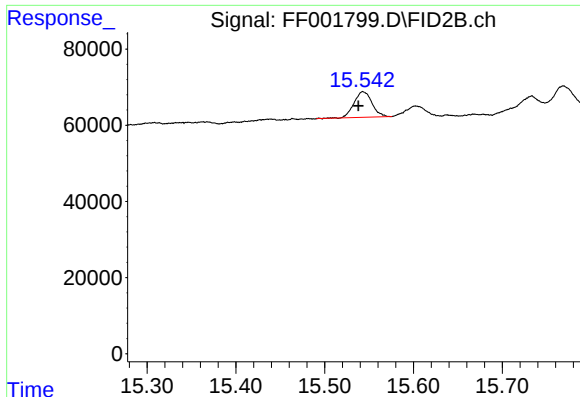

#11 N-HEXACOSANE


R.T.: 15.544 min
Delta R.T.: 0.006 min
Response: 94182
Conc: 0.67 ug/ml

Instrument :
FID_F
ClientSampleId :

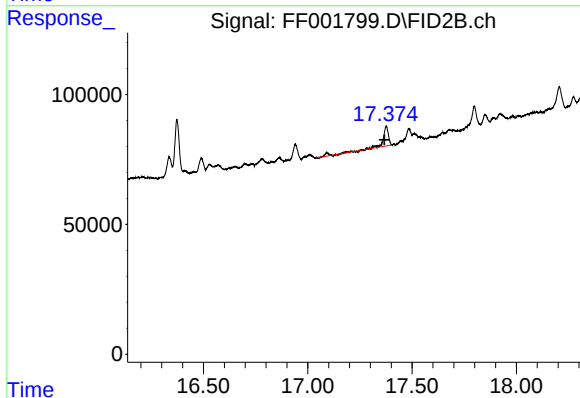


#13 N-TRIACONTANE

R.T.: 17.376 min
Delta R.T.: 0.009 min
Response: 141395
Conc: 1.02 ug/ml

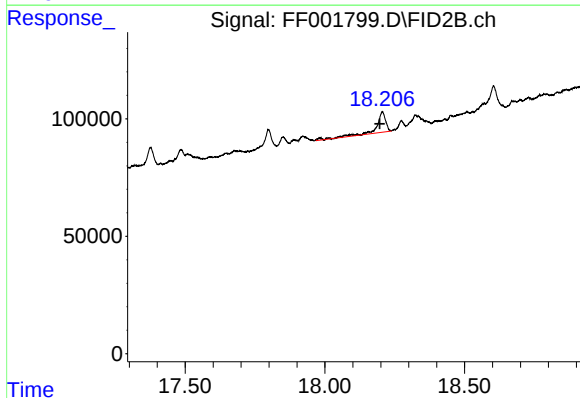


#14 N-DOTRIACONTANE

R.T.: 18.206 min
Delta R.T.: 0.009 min
Response: 205786
Conc: 1.58 ug/ml

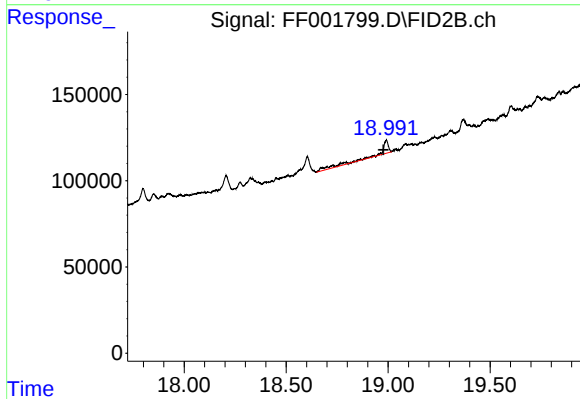

#15 N-TETRATRIACONTANE


R.T.: 18.991 min
Delta R.T.: 0.014 min
Response: 229400
Conc: 1.90 ug/ml

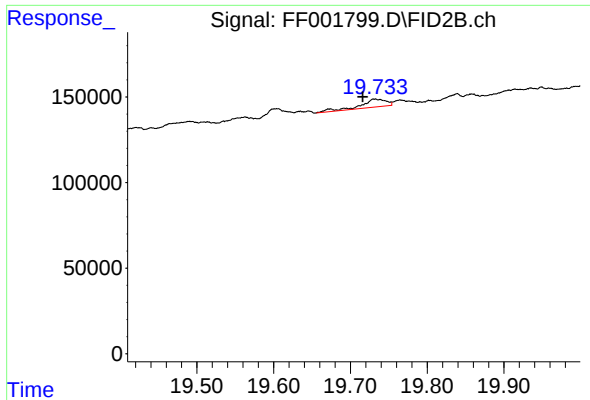

#16 N-HEXATRIACONTANE

R.T.: 19.733 min
Delta R.T.: 0.016 min
Response: 109520
Conc: 0.98 ug/ml

Instrument :
FID_F
ClientSampleId :

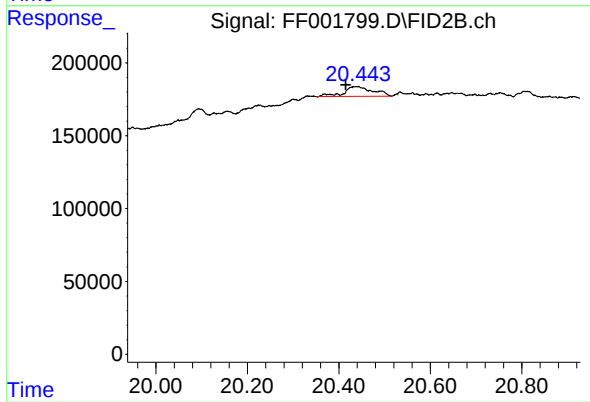

#17 N-OCTATRIACONTANE

R.T.: 20.440 min
Delta R.T.: 0.024 min
Response: 298773
Conc: 3.00 ug/ml