

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF081018\
 Data File : FF001800.D
 Signal(s) : FID2B.ch
 Acq On : 10 Aug 2018 21:24
 Operator : AJ\SJ
 Sample : J4282-01 10X
 Misc :
 ALS Vial : 72 Sample Multiplier: 1

Instrument :
 FID_F
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Aug 11 01:22:37 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF073018.M
 Quant Title :
 QLast Update : Fri Aug 03 12:00:27 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.322	232133	1.838 ug/ml
Target Compounds			
7) N-EICOSANE	12.281f	1503212	10.086 ug/ml
10) N-TETRACOSANE	14.504	820625	5.753 ug/ml
12) N-OCTACOSANE	16.524	171682	1.224 ug/ml
13) N-TRIACONTANE	17.376	173310	1.252 ug/ml
14) N-DOTRIACONTANE	18.207	195057	1.495 ug/ml
15) N-TETRATRIACONTANE	18.988	92928	0.769 ug/ml
16) N-HEXATRIACONTANE	19.700	127082	1.142 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF081018\
Data File : FF001800.D
Signal(s) : FID2B.ch
Acq On : 10 Aug 2018 21:24
Operator : AJ\SJ
Sample : J4282-01 10X
Misc :
ALS Vial : 72 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Aug 11 01:22:37 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF073018.M
Quant Title :
QLast Update : Fri Aug 03 12:00:27 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

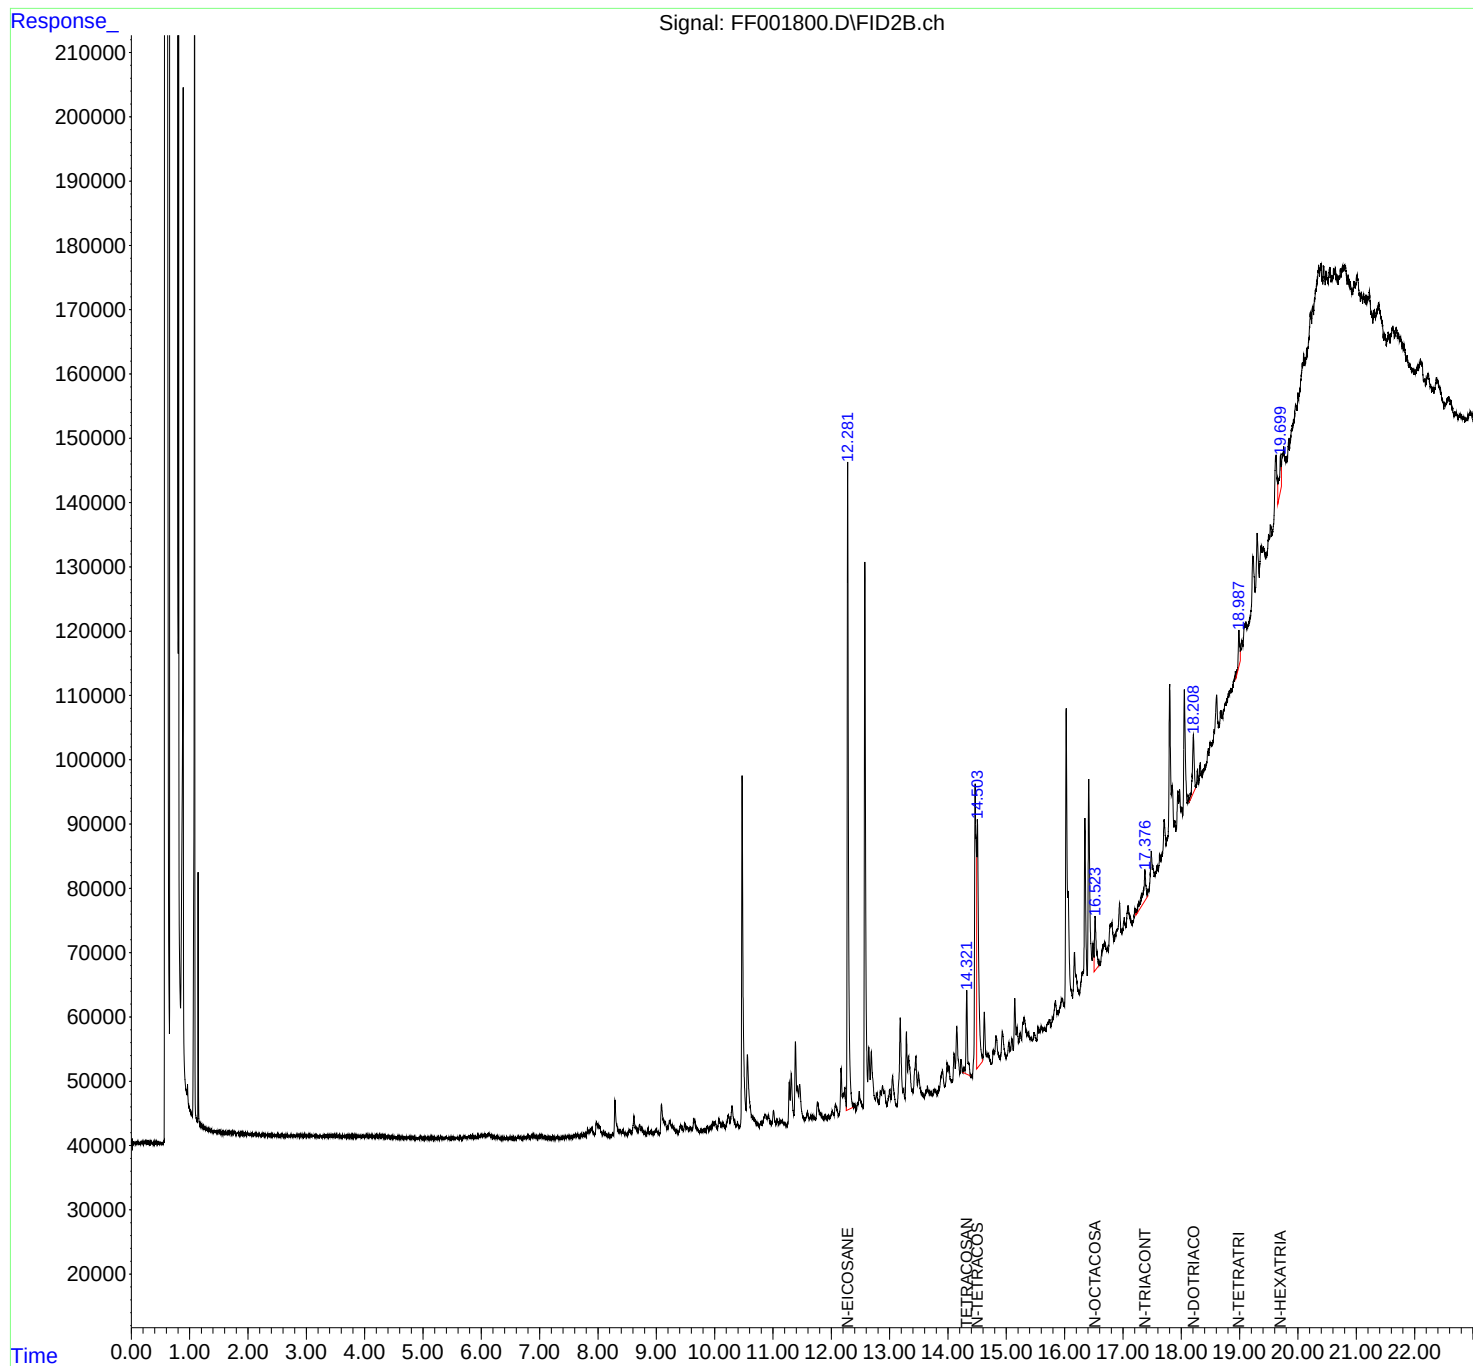


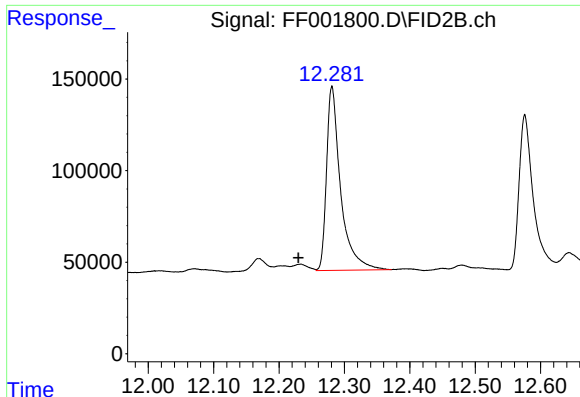

#7 N-EICOSANE


R.T.: 12.281 min
Delta R.T.: 0.051 min
Response: 1503212
Conc: 10.09 ug/ml

Instrument :
FID_F
ClientSampleId :

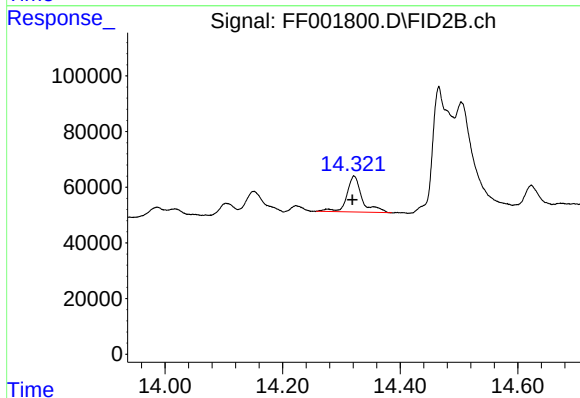


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.322 min
Delta R.T.: 0.003 min
Response: 232133
Conc: 1.84 ug/ml

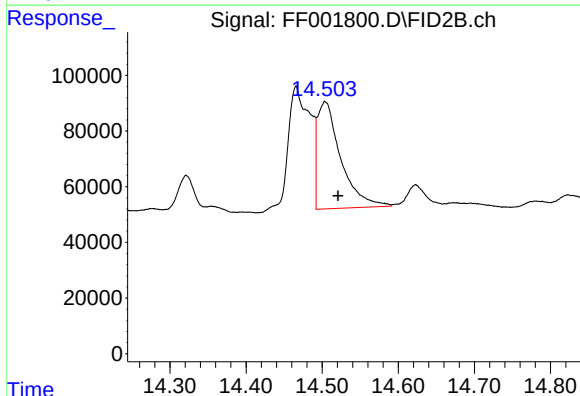


#10 N-TETRACOSANE

R.T.: 14.504 min
Delta R.T.: -0.017 min
Response: 820625
Conc: 5.75 ug/ml

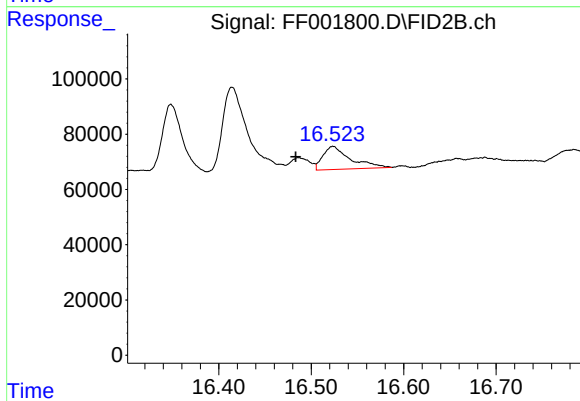

#12 N-OCTACOSANE


R.T.: 16.524 min
Delta R.T.: 0.040 min
Response: 171682
Conc: 1.22 ug/ml

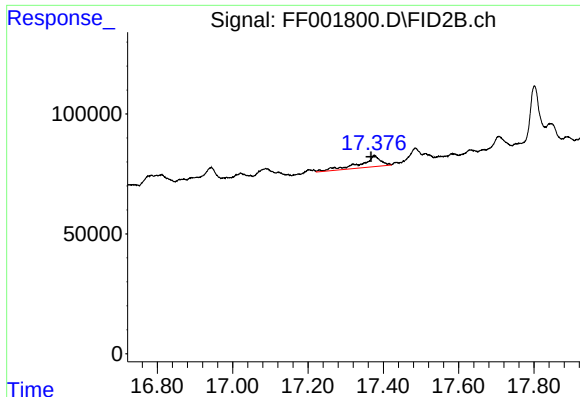

#13 N-TRIACONTANE


R.T.: 17.376 min
Delta R.T.: 0.009 min
Response: 173310
Conc: 1.25 ug/ml

Instrument :
FID_F
ClientSampleId :

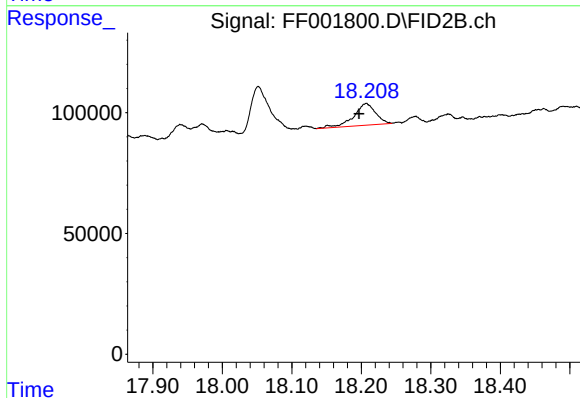


#14 N-DOTRIACONTANE

R.T.: 18.207 min
Delta R.T.: 0.010 min
Response: 195057
Conc: 1.50 ug/ml

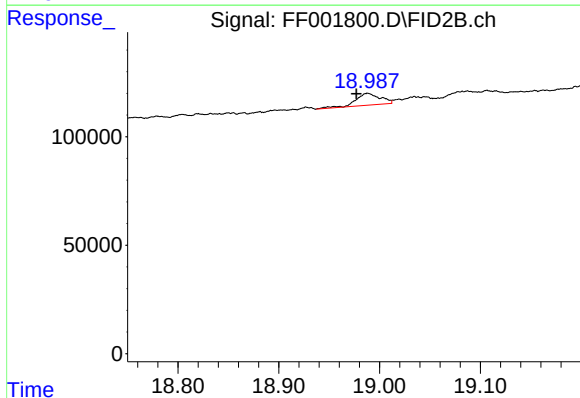

#15 N-TETRATRIACONTANE

R.T.: 18.988 min
Delta R.T.: 0.011 min
Response: 92928
Conc: 0.77 ug/ml

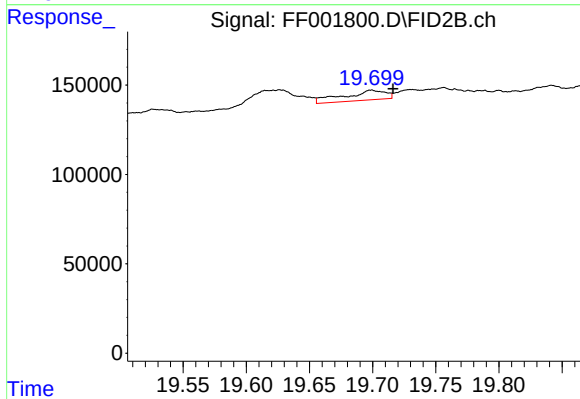

#16 N-HEXATRIACONTANE

R.T.: 19.700 min
Delta R.T.: -0.017 min
Response: 127082
Conc: 1.14 ug/ml