

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF081018\
 Data File : FF001801.D
 Signal(s) : FID2B.ch
 Acq On : 10 Aug 2018 21:56
 Operator : AJ\SJ
 Sample : J4282-03 10X
 Misc :
 ALS Vial : 73 Sample Multiplier: 1

Instrument :
 FID_F
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Aug 11 01:22:48 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF073018.M
 Quant Title :
 QLast Update : Fri Aug 03 12:00:27 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.321	142327	1.127 ug/ml
Target Compounds			
7) N-EICOSANE	12.289f	397450	2.667 ug/ml
10) N-TETRACOSANE	14.517	258081	1.809 ug/ml
12) N-OCTACOSANE	16.428f	141172	1.007 ug/ml
13) N-TRIACONTANE	17.377	143401	1.036 ug/ml
14) N-DOTRIACONTANE	18.209	128241	0.983 ug/ml
15) N-TETRATRIACONTANE	18.990	98649	0.816 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF081018\
Data File : FF001801.D
Signal(s) : FID2B.ch
Acq On : 10 Aug 2018 21:56
Operator : AJ\SJ
Sample : J4282-03 10X
Misc :
ALS Vial : 73 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Aug 11 01:22:48 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF073018.M
Quant Title :
QLast Update : Fri Aug 03 12:00:27 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

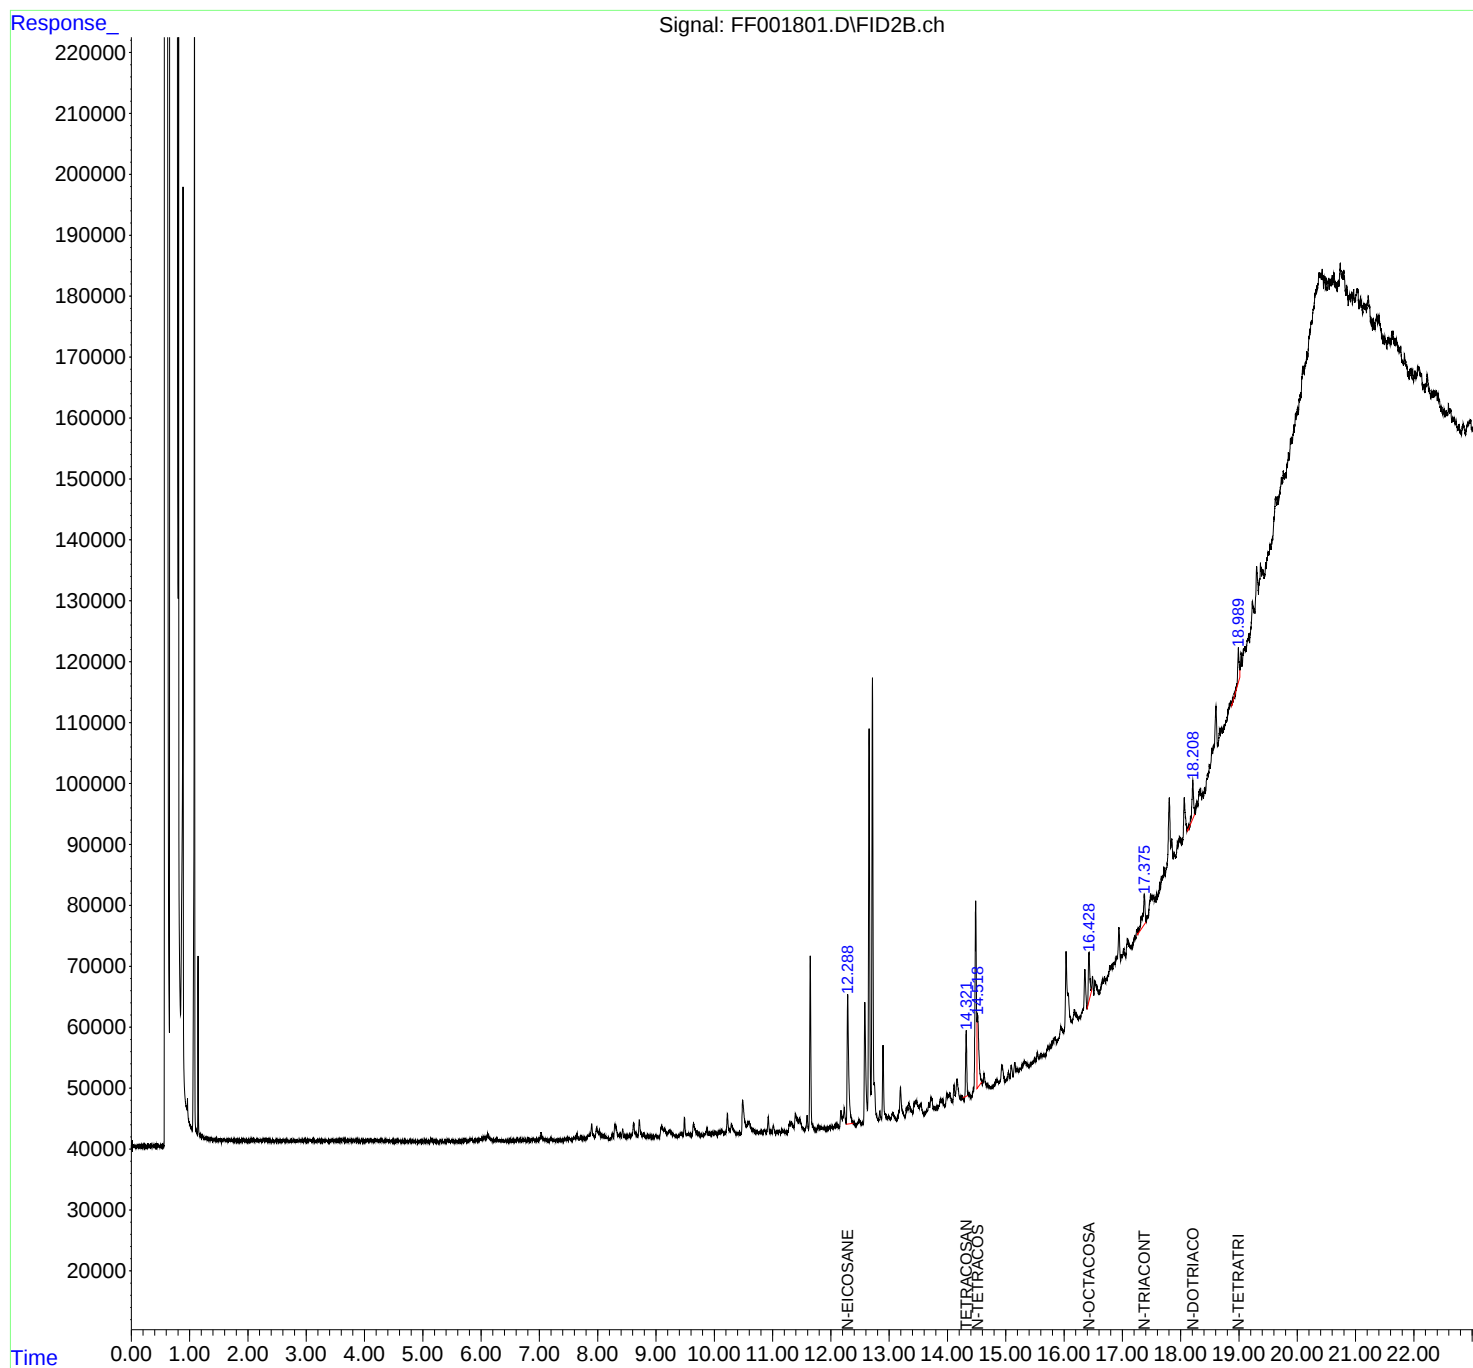


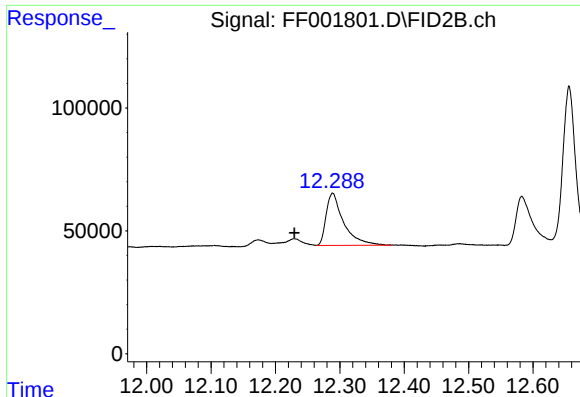

#7 N-EICOSANE


R.T.: 12.289 min
Delta R.T.: 0.059 min
Response: 397450
Conc: 2.67 ug/ml

Instrument :
FID_F
ClientSampleId :

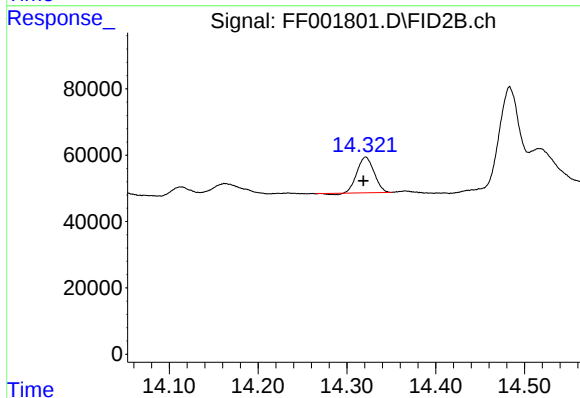


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.321 min
Delta R.T.: 0.003 min
Response: 142327
Conc: 1.13 ug/ml

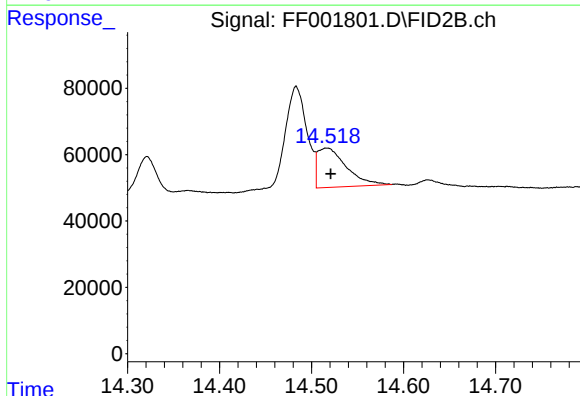


#10 N-TETRACOSANE

R.T.: 14.517 min
Delta R.T.: -0.004 min
Response: 258081
Conc: 1.81 ug/ml

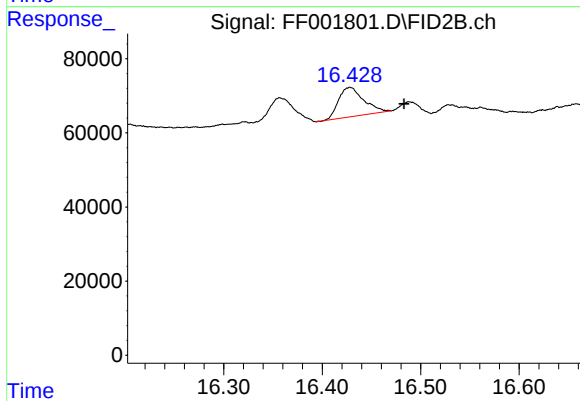

#12 N-OCTACOSANE


R.T.: 16.428 min
Delta R.T.: -0.055 min
Response: 141172
Conc: 1.01 ug/ml

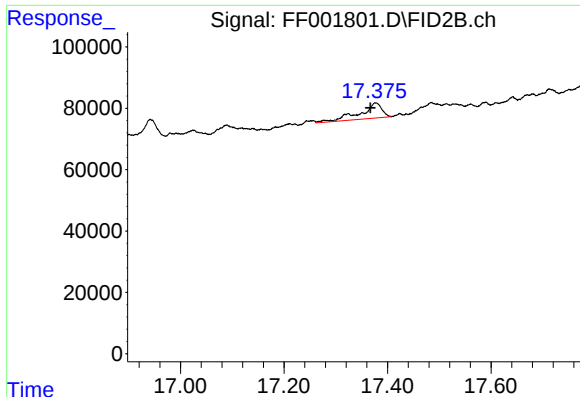

#13 N-TRIACONTANE


R.T.: 17.377 min
Delta R.T.: 0.010 min
Response: 143401
Conc: 1.04 ug/ml

Instrument :
FID_F
ClientSampleId :

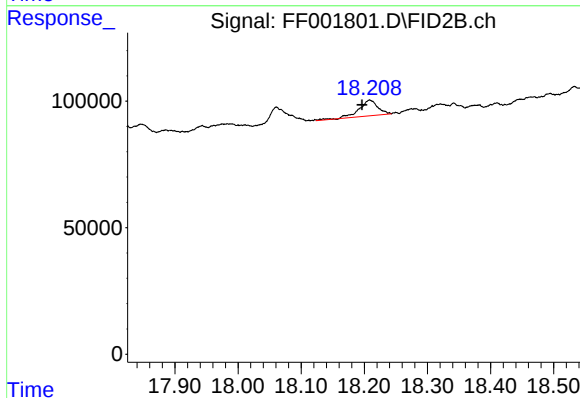

#14 N-DOTRIACONTANE

R.T.: 18.209 min
Delta R.T.: 0.012 min
Response: 128241
Conc: 0.98 ug/ml

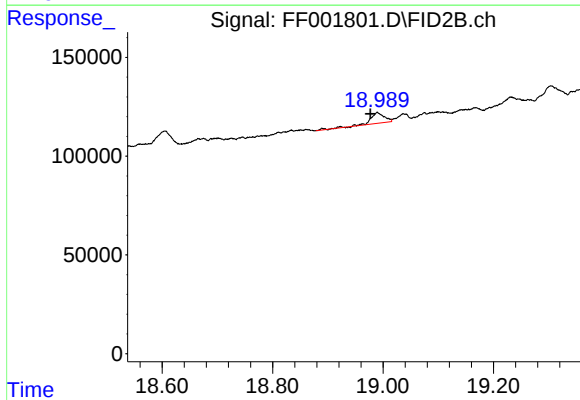

#15 N-TETRATRIACONTANE

R.T.: 18.990 min
Delta R.T.: 0.013 min
Response: 98649
Conc: 0.82 ug/ml