

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF081018\
 Data File : FF001802.D
 Signal(s) : FID2B.ch
 Acq On : 10 Aug 2018 22:27
 Operator : AJ\SJ
 Sample : J4272-01 5X
 Misc :
 ALS Vial : 74 Sample Multiplier: 1

Instrument :
 FID_F
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Aug 11 01:22:59 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF073018.M
 Quant Title :
 QLast Update : Fri Aug 03 12:00:27 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.322	363680	2.879 ug/ml
Target Compounds			
3) N-DODECANE	6.113	91421	0.613 ug/ml
4) N-TETRADECANE	7.897	216852	1.439 ug/ml
5) N-HEXADECANE	9.490	320875	2.143 ug/ml
6) N-OCTADECANE	10.925	284518	1.888 ug/ml
7) N-EICOSANE	12.231	224791	1.508 ug/ml
8) N-DOCOSANE	13.426	81567	0.558 ug/ml
10) N-TETRACOSANE	14.522	402701	2.823 ug/ml
11) N-HEXACOSANE	15.543	54846	0.389 ug/ml
12) N-OCTACOSANE	16.489	109125	0.778 ug/ml
13) N-TRIACONTANE	17.376	166147	1.200 ug/ml
14) N-DOTRIACONTANE	18.208	207686	1.592 ug/ml
15) N-TETRATRIACONTANE	18.989	217305	1.798 ug/ml
16) N-HEXATRIACONTANE	19.730	150995	1.357 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF081018\
Data File : FF001802.D
Signal(s) : FID2B.ch
Acq On : 10 Aug 2018 22:27
Operator : AJ\SJ
Sample : J4272-01 5X
Misc :
ALS Vial : 74 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Aug 11 01:22:59 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF073018.M
Quant Title :
QLast Update : Fri Aug 03 12:00:27 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

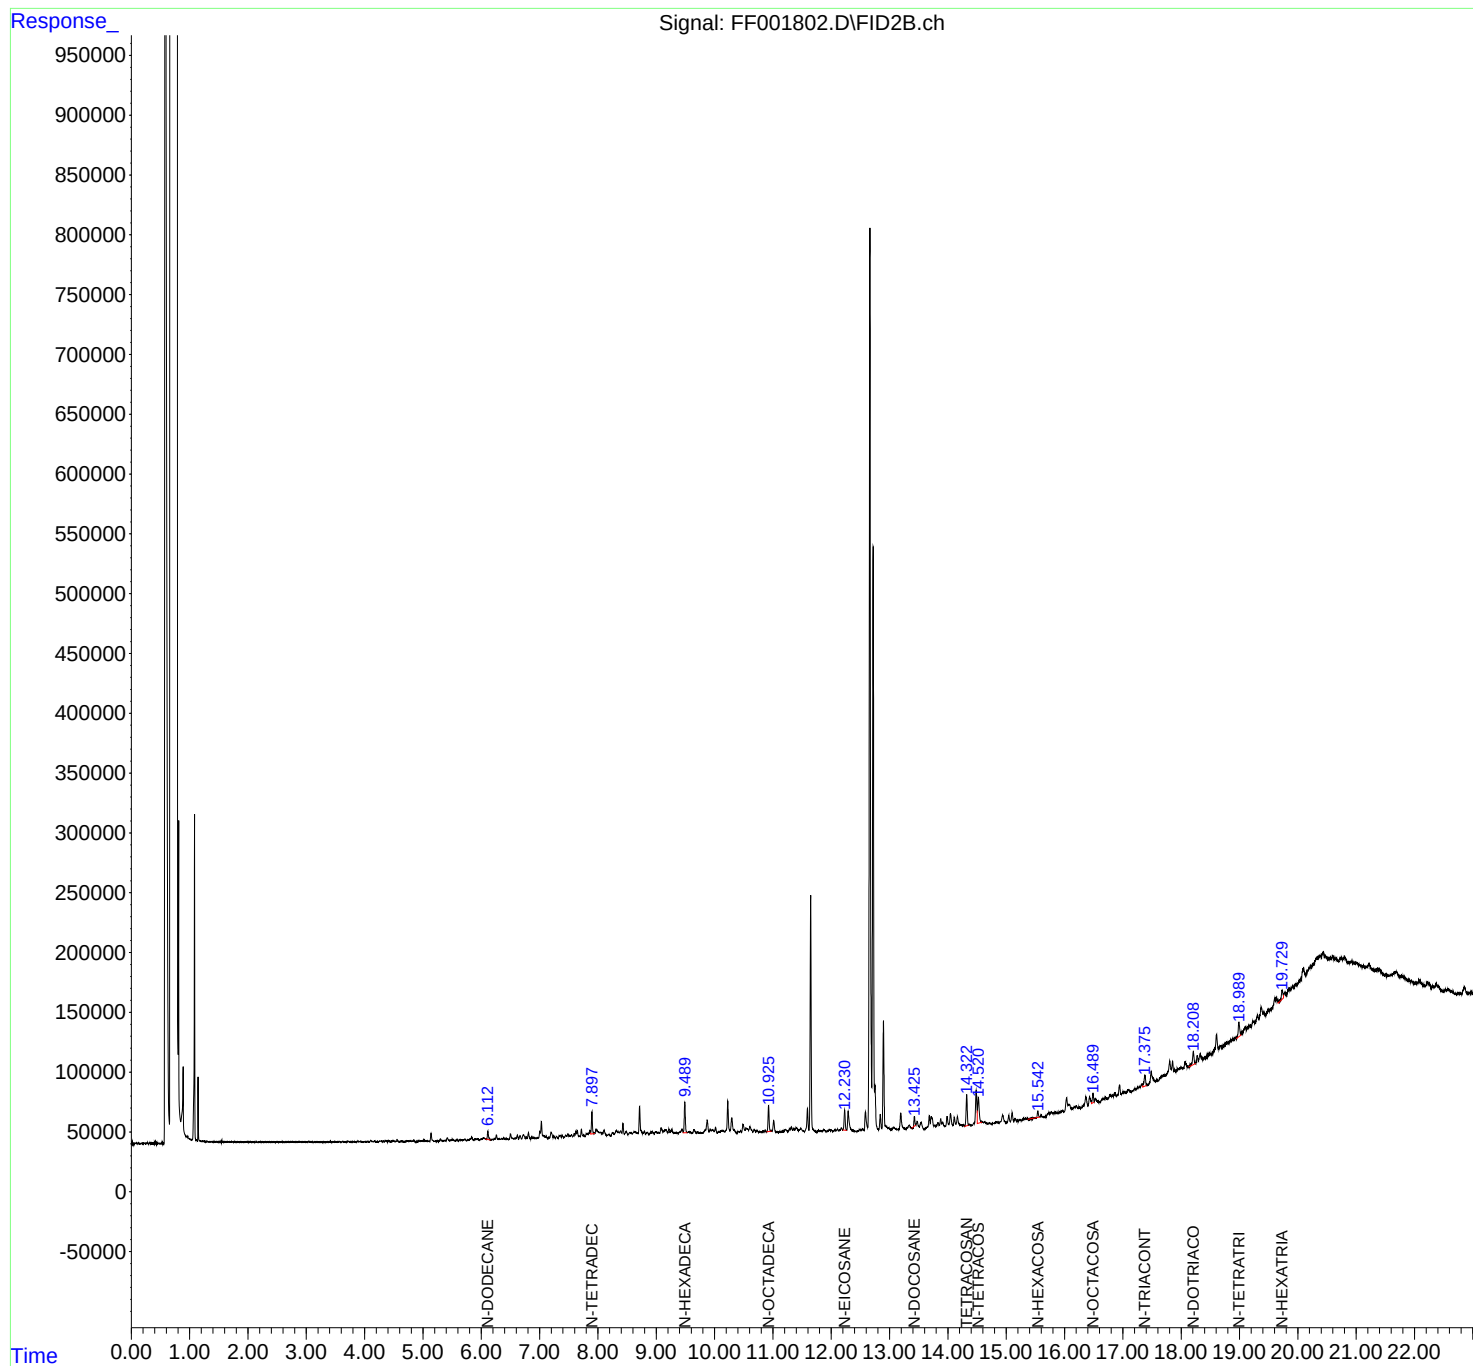


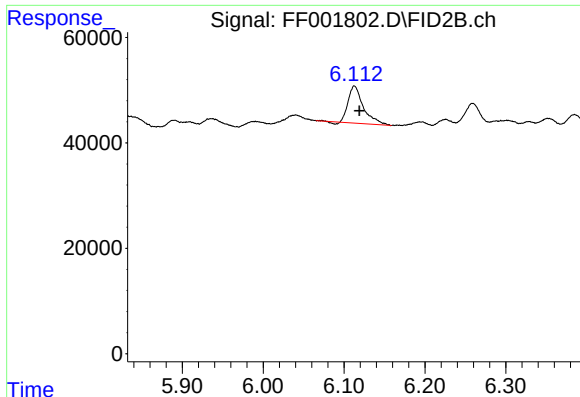

#3 N-DODECANE


R.T.: 6.113 min
Delta R.T.: -0.006 min
Response: 91421
Conc: 0.61 ug/ml

Instrument :
FID_F
ClientSampleId :

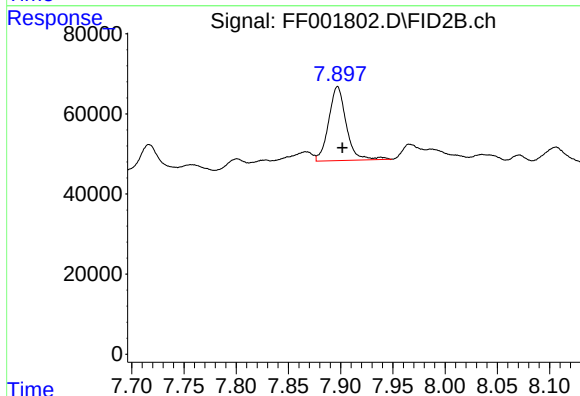


#4 N-TETRADECANE

R.T.: 7.897 min
Delta R.T.: -0.005 min
Response: 216852
Conc: 1.44 ug/ml

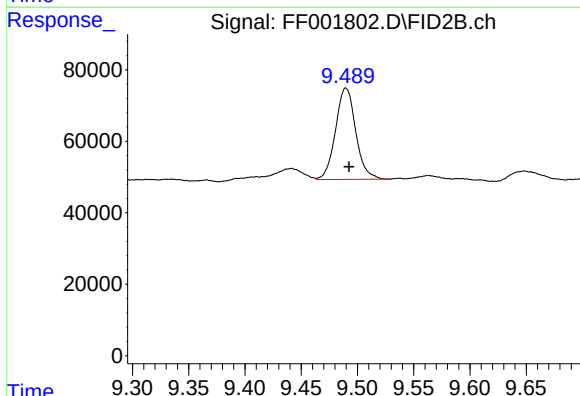


#5 N-HEXADECANE

R.T.: 9.490 min
Delta R.T.: -0.003 min
Response: 320875
Conc: 2.14 ug/ml

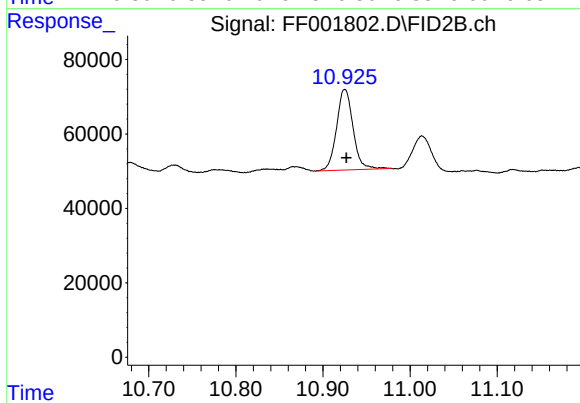

#6 N-OCTADECANE


R.T.: 10.925 min
Delta R.T.: -0.002 min
Response: 284518
Conc: 1.89 ug/ml

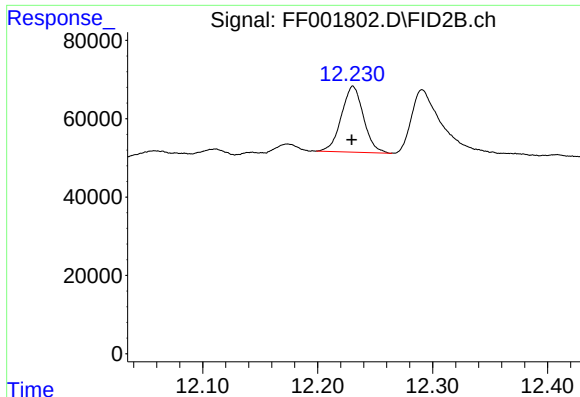

#7 N-EICOSANE


R.T.: 12.231 min
Delta R.T.: 0.001 min
Response: 224791
Conc: 1.51 ug/ml

Instrument :
FID_F
ClientSampleId :

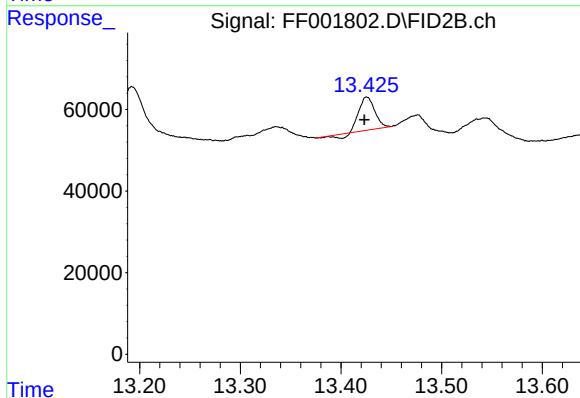


#8 N-DOCOSANE

R.T.: 13.426 min
Delta R.T.: 0.002 min
Response: 81567
Conc: 0.56 ug/ml

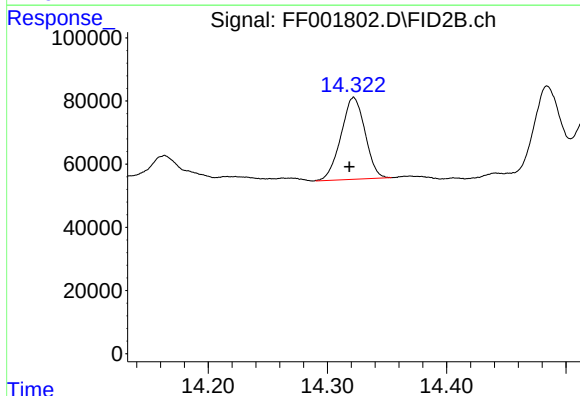


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.322 min
Delta R.T.: 0.004 min
Response: 363680
Conc: 2.88 ug/ml

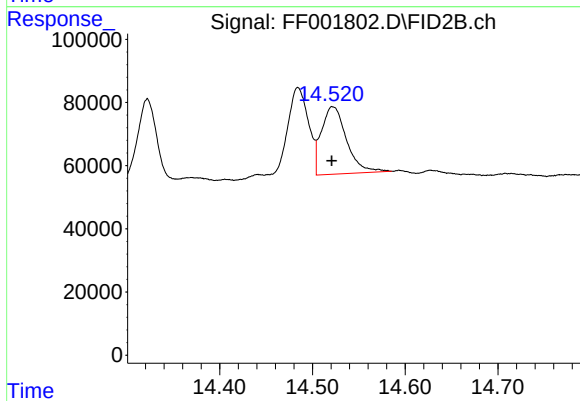

#10 N-TETRACOSANE


R.T.: 14.522 min
Delta R.T.: 0.000 min
Response: 402701
Conc: 2.82 ug/ml

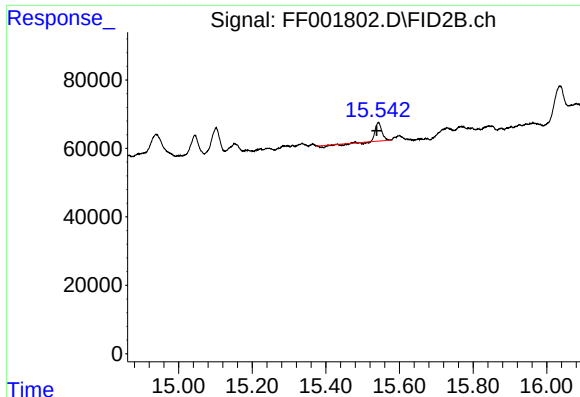

#11 N-HEXACOSANE


R.T.: 15.543 min
Delta R.T.: 0.005 min
Response: 54846
Conc: 0.39 ug/ml

Instrument :
FID_F
ClientSampleId :

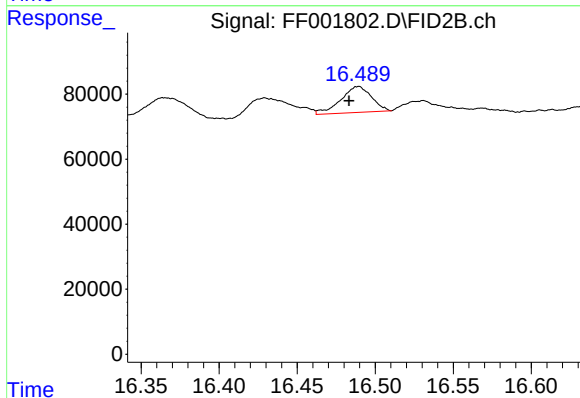


#12 N-OCTACOSANE

R.T.: 16.489 min
Delta R.T.: 0.006 min
Response: 109125
Conc: 0.78 ug/ml

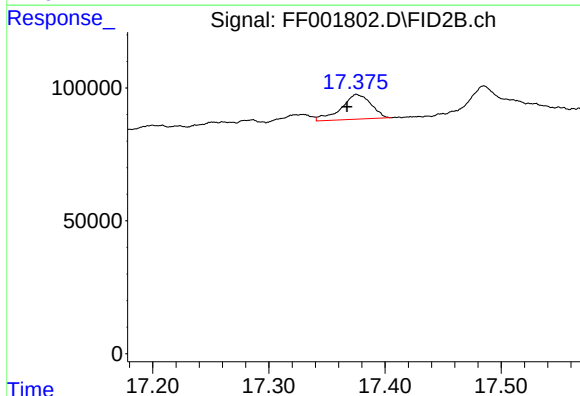


#13 N-TRIACONTANE

R.T.: 17.376 min
Delta R.T.: 0.008 min
Response: 166147
Conc: 1.20 ug/ml

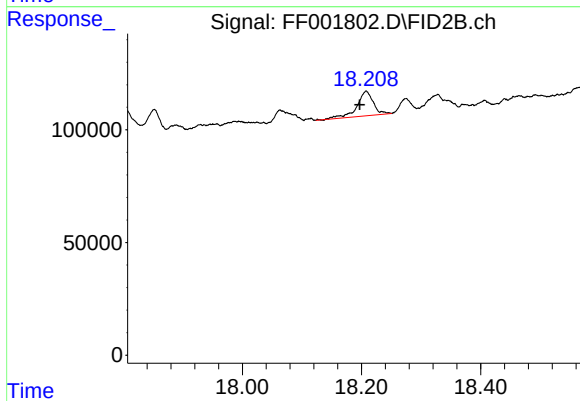

#14 N-DOTRIACONTANE


R.T.: 18.208 min
Delta R.T.: 0.011 min
Response: 207686
Conc: 1.59 ug/ml

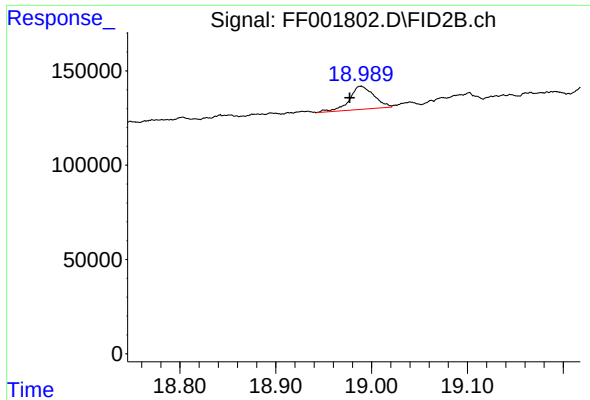

#15 N-TETRATRIACONTANE

R.T.: 18.989 min
Delta R.T.: 0.012 min
Response: 217305
Conc: 1.80 ug/ml

Instrument :
FID_F
ClientSampleId :

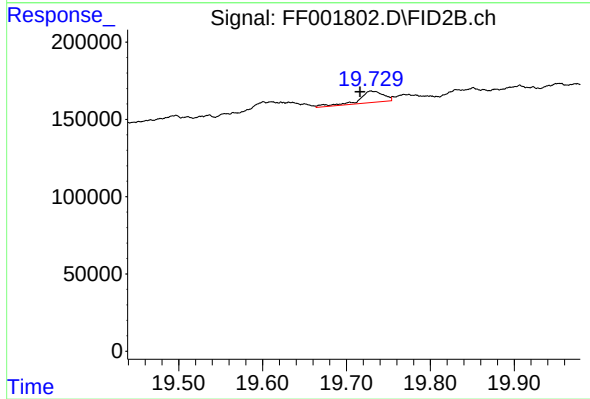

#16 N-HEXATRIACONTANE

R.T.: 19.730 min
Delta R.T.: 0.014 min
Response: 150995
Conc: 1.36 ug/ml