

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF081018\
 Data File : FF001803.D
 Signal(s) : FID2B.ch
 Acq On : 10 Aug 2018 22:58
 Operator : AJ\SJ
 Sample : I.BLK
 Misc :
 ALS Vial : 52 Sample Multiplier: 1

Instrument :
 FID_F
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Aug 11 01:23:12 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF073018.M
 Quant Title :
 QLast Update : Fri Aug 03 12:00:27 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.323	2420824	19.167 ug/ml
Target Compounds			
10) N-TETRACOSANE	14.487	360302	2.526 ug/ml
14) N-DOTRIACONTANE	18.208	96138	0.737 ug/ml
15) N-TETRATRIACONTANE	18.990	77149	0.638 ug/ml
16) N-HEXATRIACONTANE	19.730	92138	0.828 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF081018\
Data File : FF001803.D
Signal(s) : FID2B.ch
Acq On : 10 Aug 2018 22:58
Operator : AJ\SJ
Sample : I.BLK
Misc :
ALS Vial : 52 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Aug 11 01:23:12 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF073018.M
Quant Title :
QLast Update : Fri Aug 03 12:00:27 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

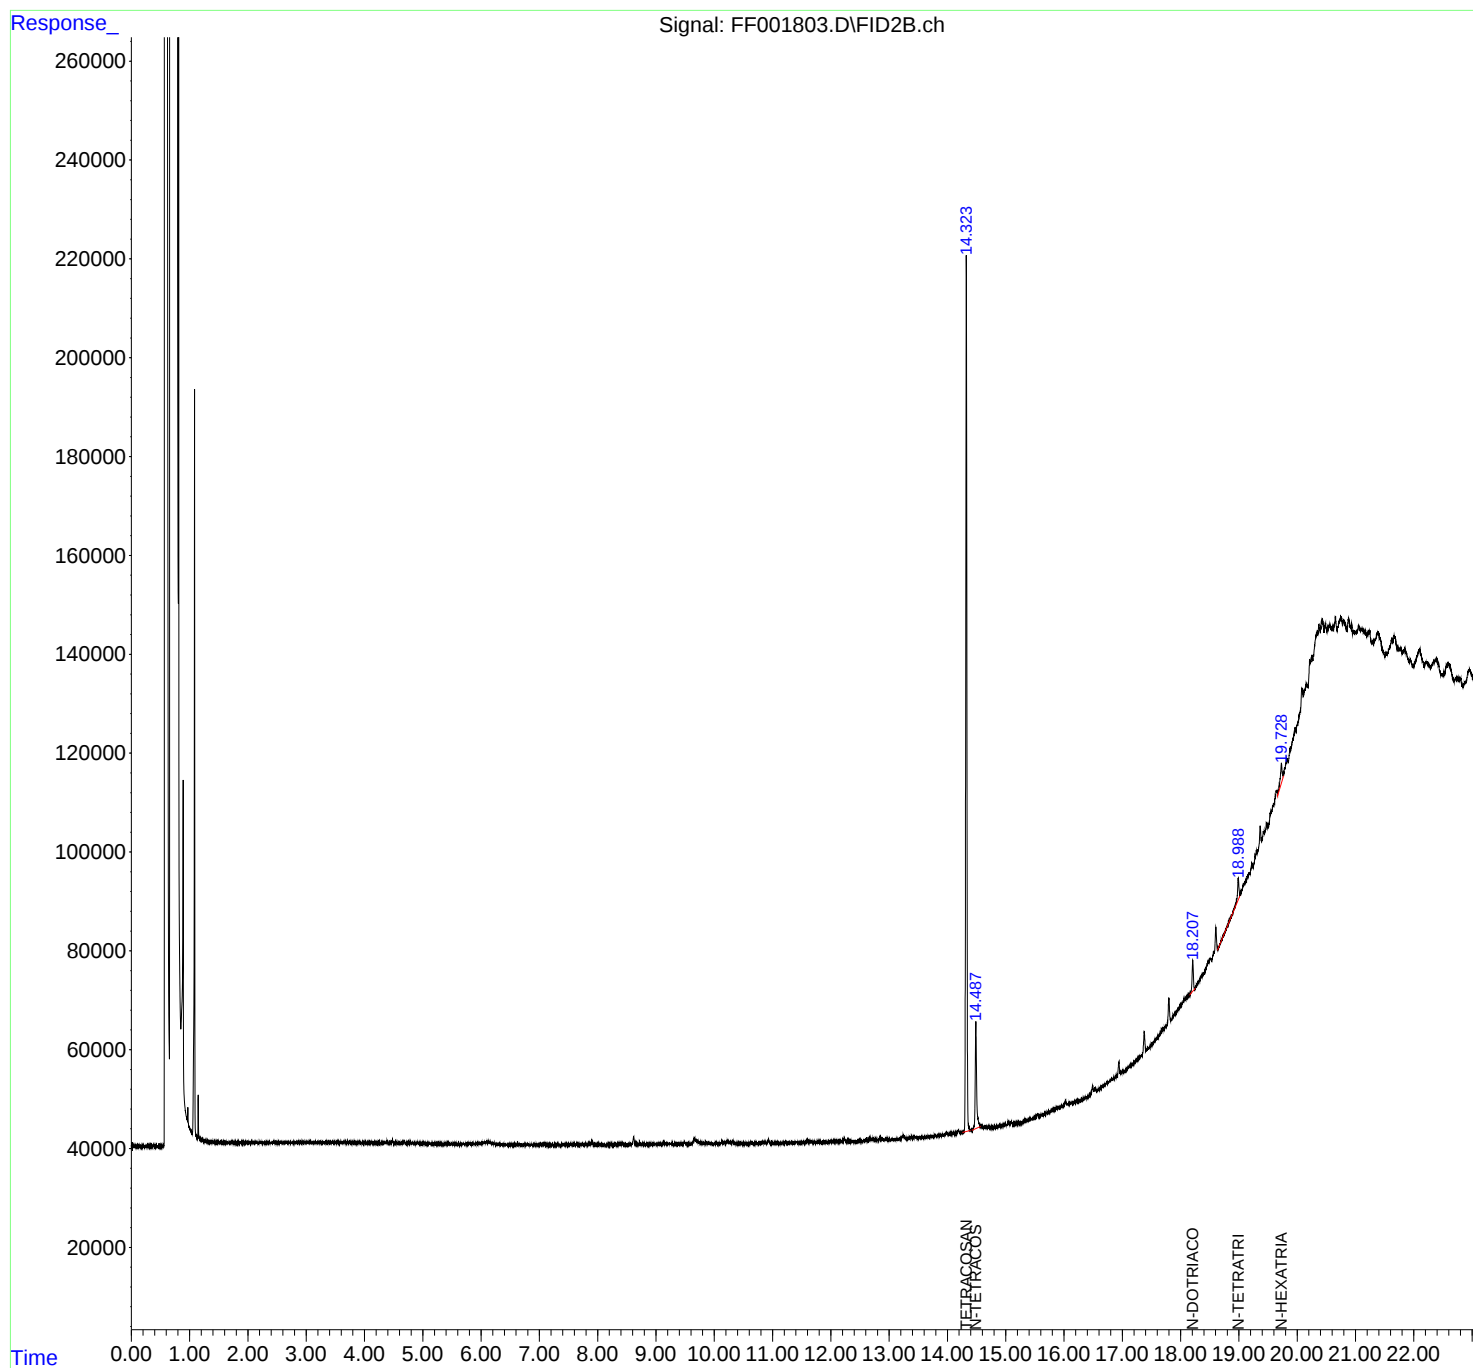


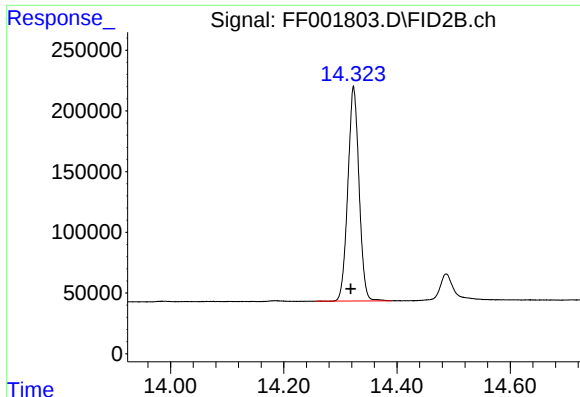

#9 TETRACOSANE-d50 (SURROGATE)


R.T.: 14.323 min
Delta R.T.: 0.005 min
Response: 2420824
Conc: 19.17 ug/ml

Instrument :
FID_F
ClientSampleId :

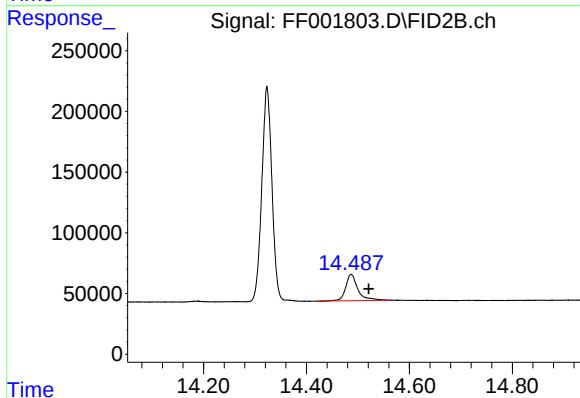


#10 N-TETRACOSANE

R.T.: 14.487 min
Delta R.T.: -0.034 min
Response: 360302
Conc: 2.53 ug/ml

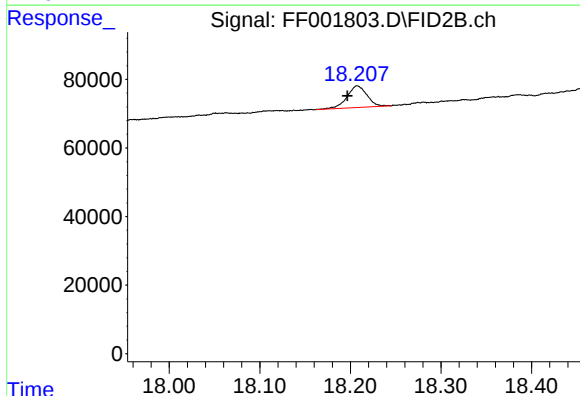


#14 N-DOTRIACONTANE

R.T.: 18.208 min
Delta R.T.: 0.011 min
Response: 96138
Conc: 0.74 ug/ml

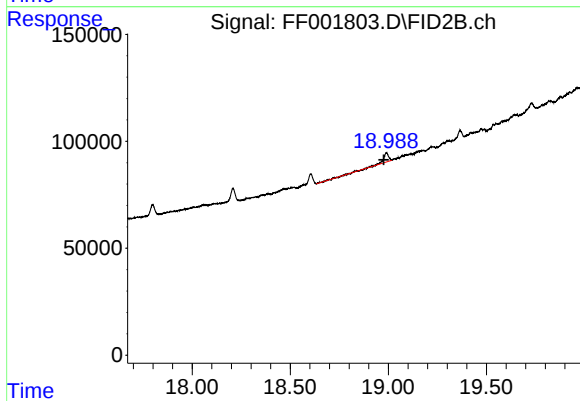

#15 N-TETRATRIACONTANE

R.T.: 18.990 min
Delta R.T.: 0.013 min
Response: 77149
Conc: 0.64 ug/ml

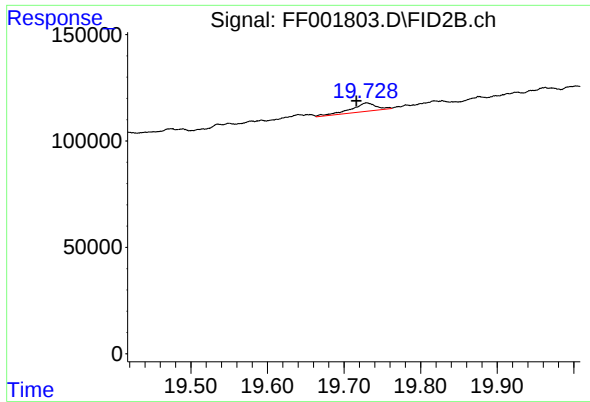

#16 N-HEXATRIACONTANE

R.T.: 19.730 min
Delta R.T.: 0.013 min
Response: 92138
Conc: 0.83 ug/ml

Instrument :
FID_F
ClientSampleId :