

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF081018\
 Data File : FF001808.D
 Signal(s) : FID2B.ch
 Acq On : 11 Aug 2018 02:03
 Operator : AJ\SJ
 Sample : J4409-03
 Misc :
 ALS Vial : 78 Sample Multiplier: 1

Instrument :
 FID_F
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Aug 13 01:16:25 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF073018.M
 Quant Title :
 QLast Update : Fri Aug 03 12:00:27 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.327	2257492	17.874 ug/ml
Target Compounds			
4) N-TETRADECANE	7.893	205902	1.366 ug/ml
5) N-HEXADECANE	9.493	166899	1.115 ug/ml
7) N-EICOSANE	12.231	361260	2.424 ug/ml
8) N-DOCOSANE	13.421	349682	2.394 ug/ml
10) N-TETRACOSANE	14.504	4953847	34.727 ug/ml
11) N-HEXACOSANE	15.552	636375	4.518 ug/ml
12) N-OCTACOSANE	16.510	1463766	10.439 ug/ml
13) N-TRIACONTANE	17.379	560675	4.050 ug/ml
14) N-DOTRIACONTANE	18.189	5122216	39.263 ug/ml
15) N-TETRATRIACONTANE	18.994	211130	1.747 ug/ml
16) N-HEXATRIACONTANE	19.753	5657802	50.849 ug/ml
17) N-OCTATRIACONTANE	20.455	213571	2.143 ug/ml
18) N-TETRACONTANE	21.205	2912143	29.232 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF081018\
Data File : FF001808.D
Signal(s) : FID2B.ch
Acq On : 11 Aug 2018 02:03
Operator : AJ\SJ
Sample : J4409-03
Misc :
ALS Vial : 78 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Aug 13 01:16:25 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF073018.M
Quant Title :
QLast Update : Fri Aug 03 12:00:27 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

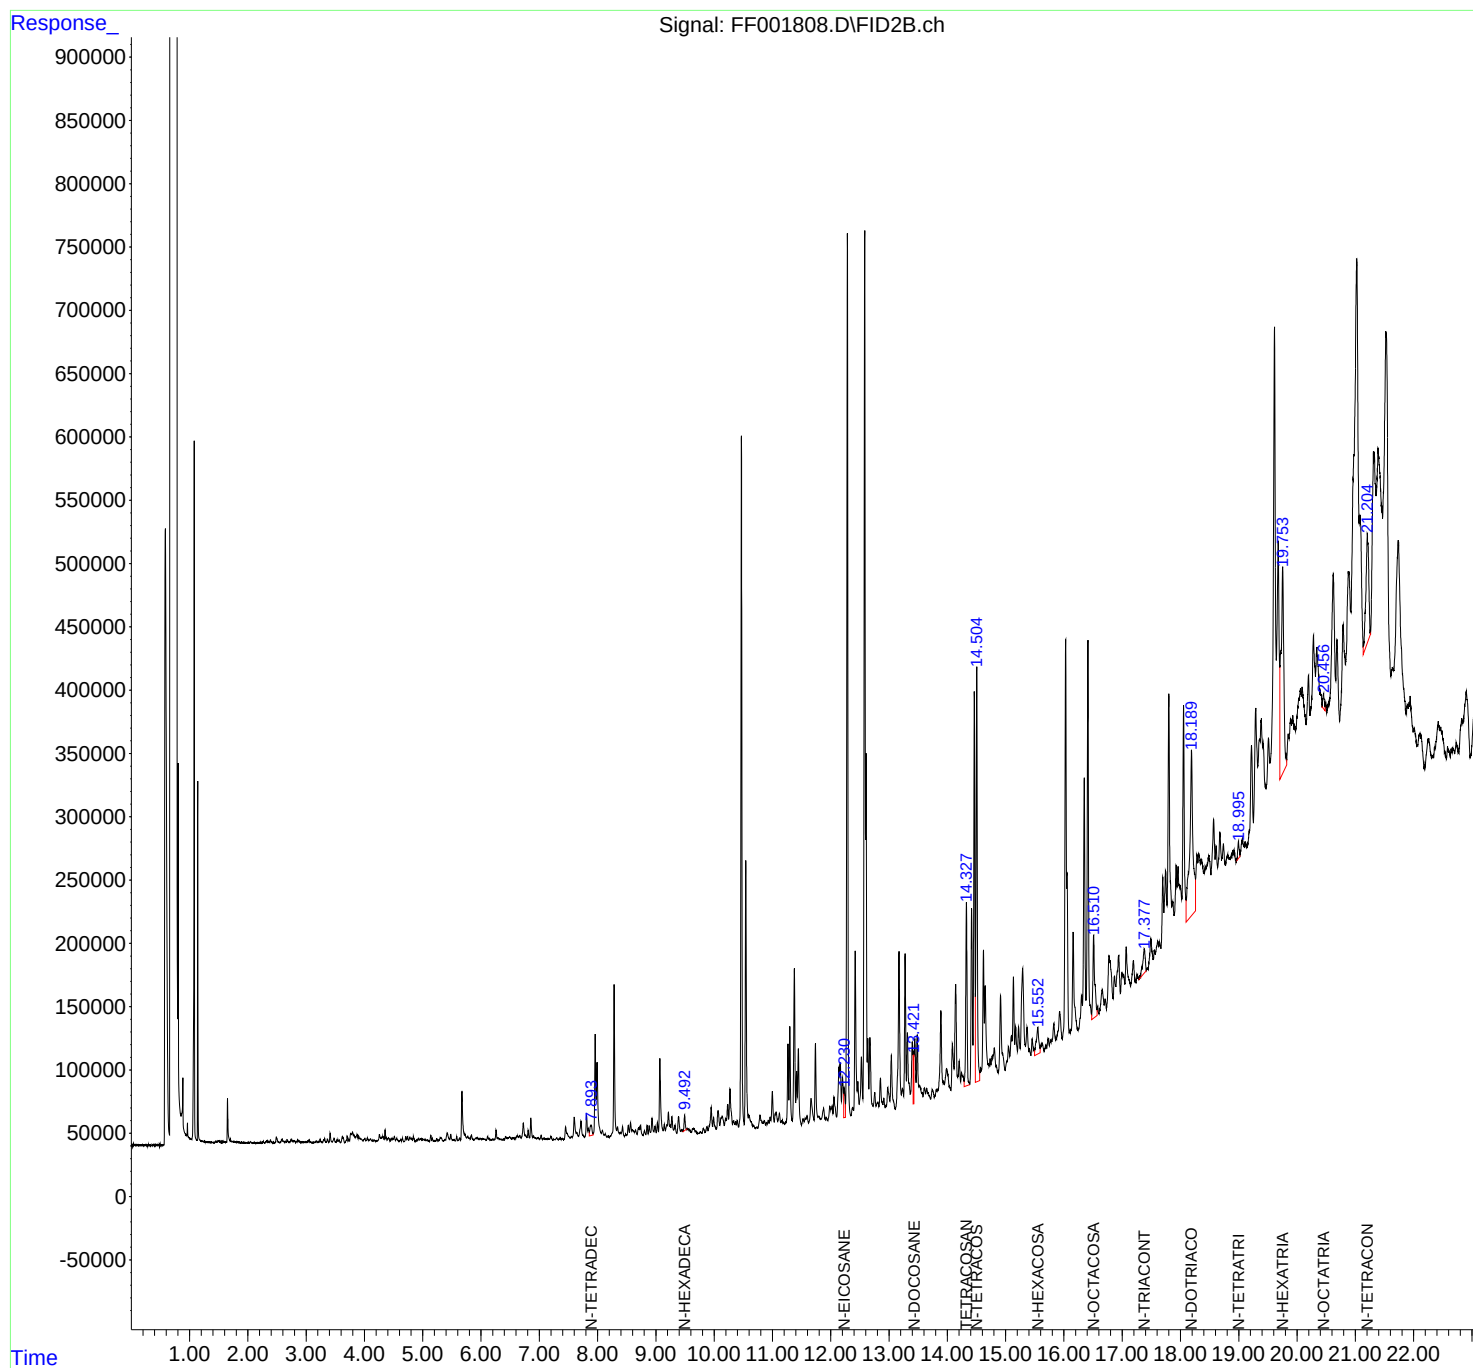


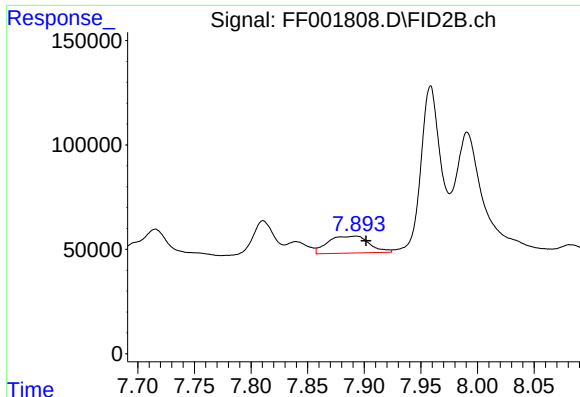

#4 N-TETRADECANE


R.T.: 7.893 min
Delta R.T.: -0.009 min
Response: 205902
Conc: 1.37 ug/ml

Instrument :
FID_F
ClientSampleId :

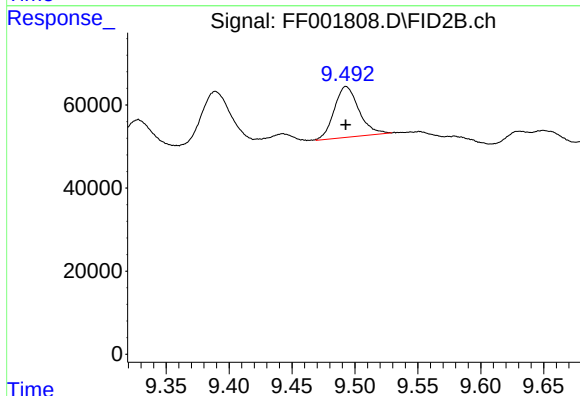


#5 N-HEXADECANE

R.T.: 9.493 min
Delta R.T.: 0.000 min
Response: 166899
Conc: 1.11 ug/ml

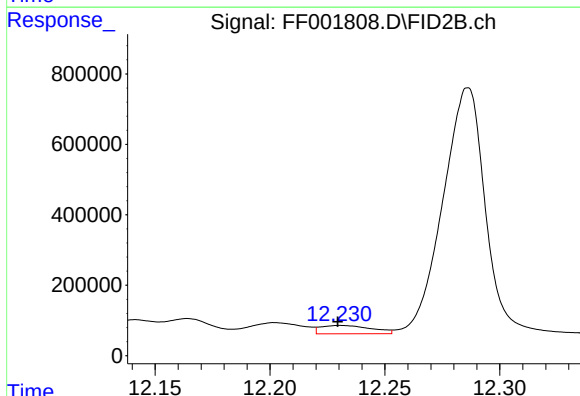


#7 N-EICOSANE

R.T.: 12.231 min
Delta R.T.: 0.001 min
Response: 361260
Conc: 2.42 ug/ml

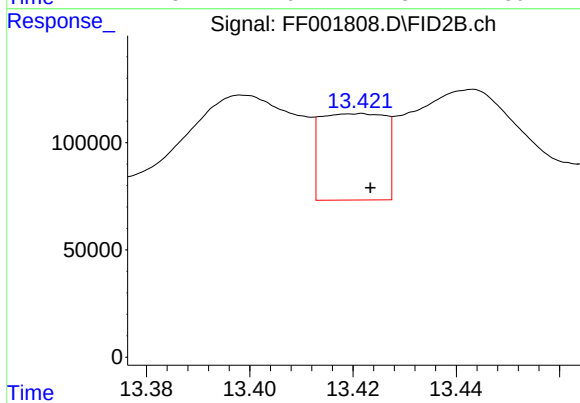

#8 N-DOCOSANE


R.T.: 13.421 min
Delta R.T.: -0.002 min
Response: 349682
Conc: 2.39 ug/ml

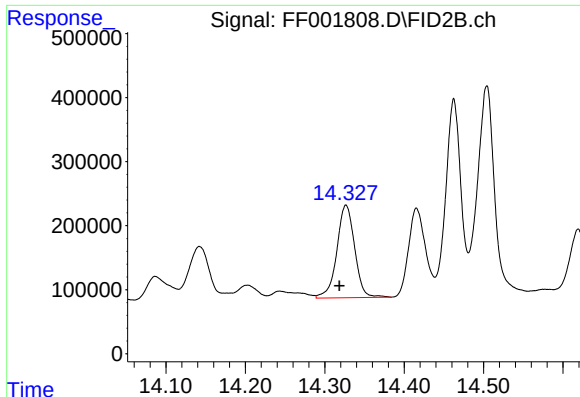

#9 TETRACOSANE-d50 (SURROGATE)


R.T.: 14.327 min
Delta R.T.: 0.008 min
Response: 2257492
Conc: 17.87 ug/ml

Instrument :
FID_F
ClientSampleId :

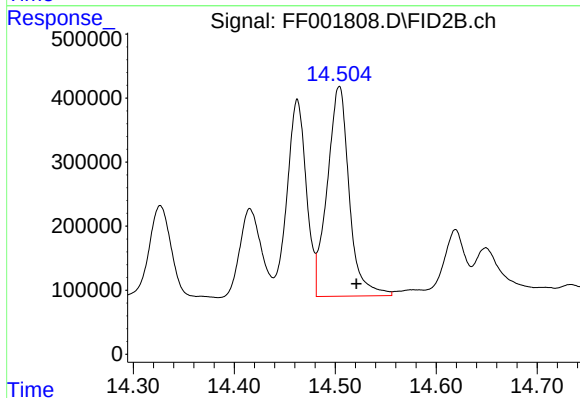


#10 N-TETRACOSANE

R.T.: 14.504 min
Delta R.T.: -0.017 min
Response: 4953847
Conc: 34.73 ug/ml

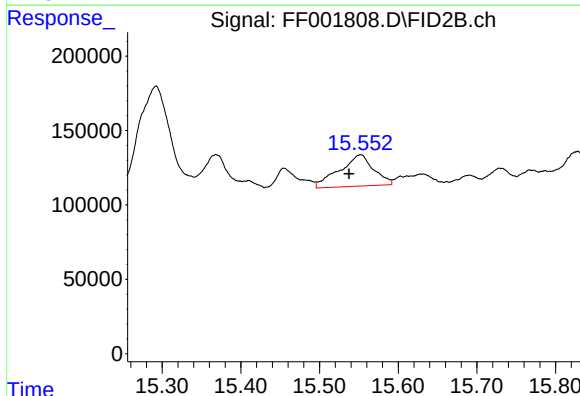


#11 N-HEXACOSANE

R.T.: 15.552 min
Delta R.T.: 0.014 min
Response: 636375
Conc: 4.52 ug/ml

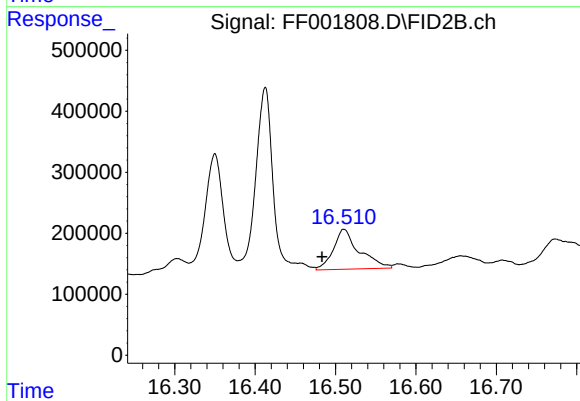

#12 N-OCTACOSANE


R.T.: 16.510 min
Delta R.T.: 0.027 min
Response: 1463766
Conc: 10.44 ug/ml

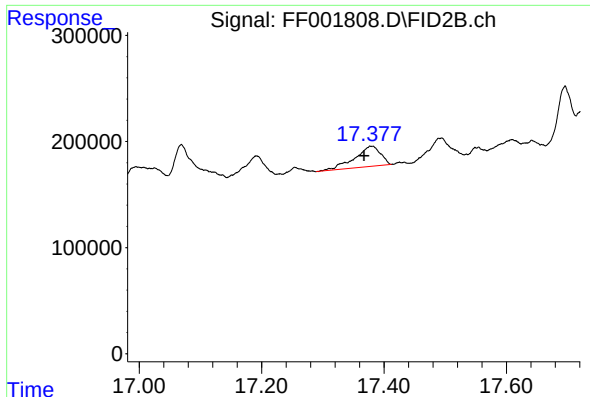

#13 N-TRIACONTANE


R.T.: 17.379 min
Delta R.T.: 0.012 min
Response: 560675
Conc: 4.05 ug/ml

Instrument :
FID_F
ClientSampleId :

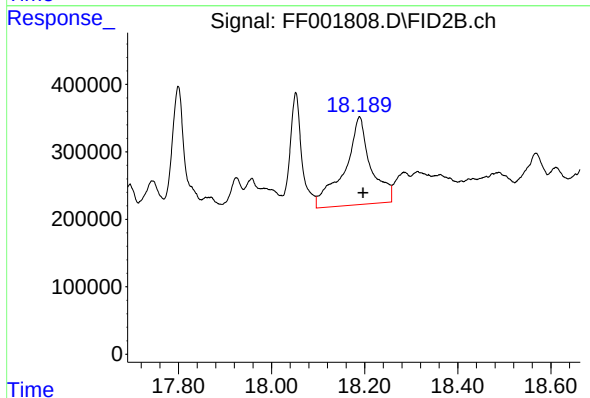


#14 N-DOTRIACONTANE

R.T.: 18.189 min
Delta R.T.: -0.008 min
Response: 5122216
Conc: 39.26 ug/ml

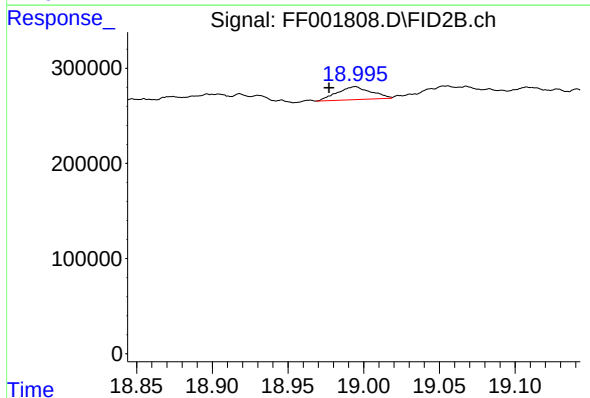


#15 N-TETRATRIACONTANE

R.T.: 18.994 min
Delta R.T.: 0.017 min
Response: 211130
Conc: 1.75 ug/ml

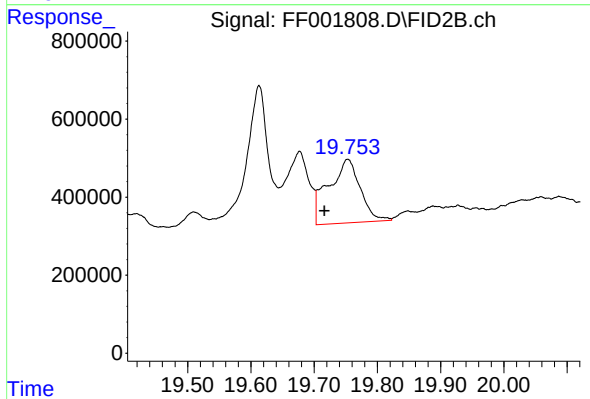

#16 N-HEXATRIACONTANE


R.T.: 19.753 min
Delta R.T.: 0.037 min
Response: 5657802
Conc: 50.85 ug/ml

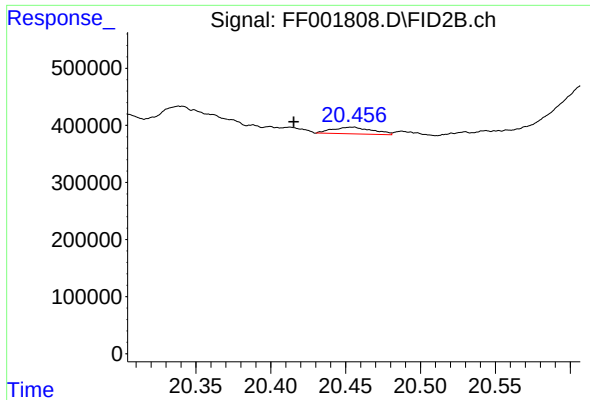

#17 N-OCTATRIACONTANE

R.T.: 20.455 min
Delta R.T.: 0.039 min
Response: 213571
Conc: 2.14 ug/ml

Instrument :
FID_F
ClientSampleId :

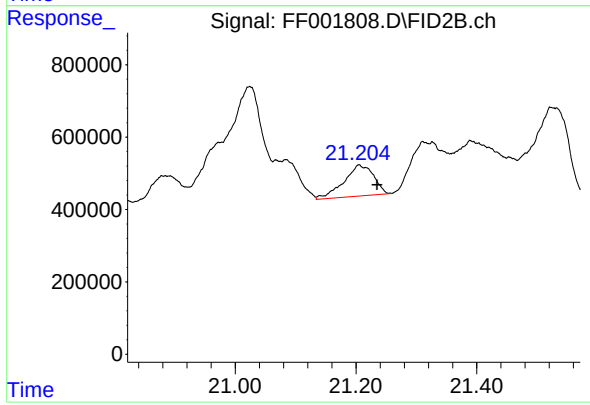

#18 N-TETRACONTANE

R.T.: 21.205 min
Delta R.T.: -0.030 min
Response: 2912143
Conc: 29.23 ug/ml