

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF081018\
 Data File : FF001811.D
 Signal(s) : FID2B.ch
 Acq On : 11 Aug 2018 10:41
 Operator : AJ\SJ
 Sample : J4409-05
 Misc :
 ALS Vial : 79 Sample Multiplier: 1

Instrument :
 FID_F
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Aug 13 01:17:05 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF073018.M
 Quant Title :
 QLast Update : Fri Aug 03 12:00:27 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.334	4031667	31.921 ug/ml
Target Compounds			
3) N-DODECANE	6.112	133459	0.895 ug/ml
4) N-TETRADECANE	7.894	314205	2.085 ug/ml
5) N-HEXADECANE	9.492	833149	5.565 ug/ml
6) N-OCTADECANE	10.933	193824	1.286 ug/ml
7) N-EICOSANE	12.241	1319998	8.856 ug/ml
8) N-DOCOSANE	13.453	7337490	50.234 ug/ml
10) N-TETRACOSANE	14.531	18086993	126.791 ug/ml
11) N-HEXACOSANE	15.529	697425	4.951 ug/ml
12) N-OCTACOSANE	16.446	21401977	152.634 ug/ml
13) N-TRIACONTANE	17.383	2169129	15.669 ug/ml
14) N-DOTRIACONTANE	18.207	6723248	51.535 ug/ml
15) N-TETRATRIACONTANE	19.005	409830	3.391 ug/ml
16) N-HEXATRIACONTANE	19.723	1313316	11.803 ug/ml
18) N-TETRACONTANE	21.249	712610	7.153 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF081018\
Data File : FF001811.D
Signal(s) : FID2B.ch
Acq On : 11 Aug 2018 10:41
Operator : AJ\SJ
Sample : J4409-05
Misc :
ALS Vial : 79 Sample Multiplier: 1

Instrument :
FID_F
ClientSampled :

Integration File: autoint1.e
Quant Time: Aug 13 01:17:05 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF073018.M
Quant Title :
QLast Update : Fri Aug 03 12:00:27 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

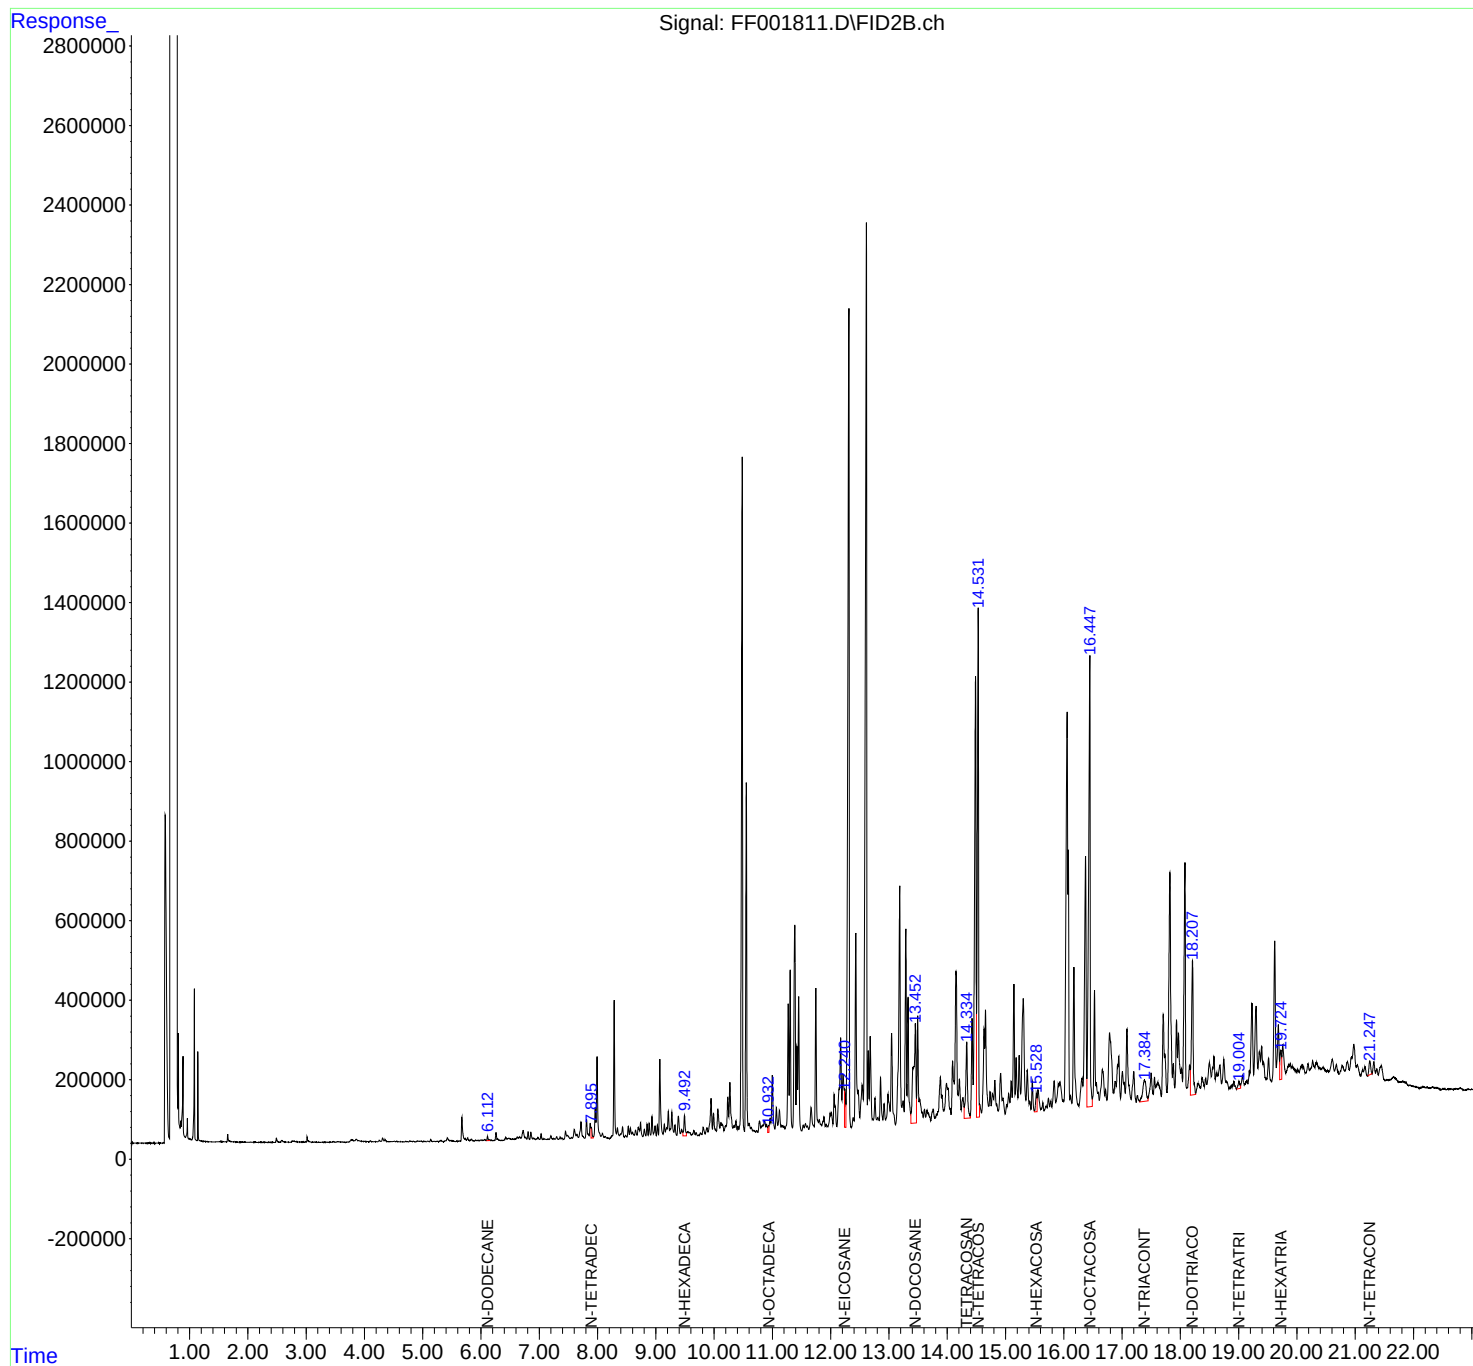


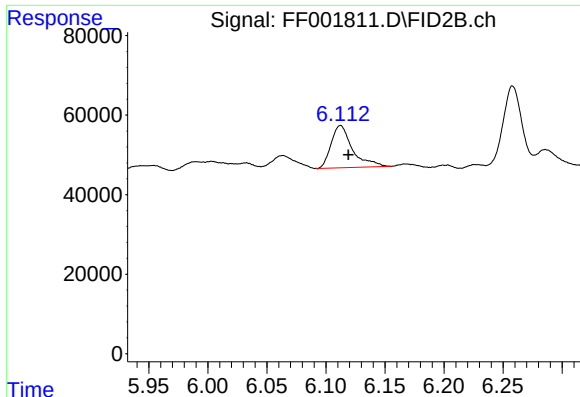

#3 N-DODECANE


R.T.: 6.112 min
Delta R.T.: -0.007 min
Response: 133459
Conc: 0.90 ug/ml

Instrument :
FID_F
ClientSampleId :

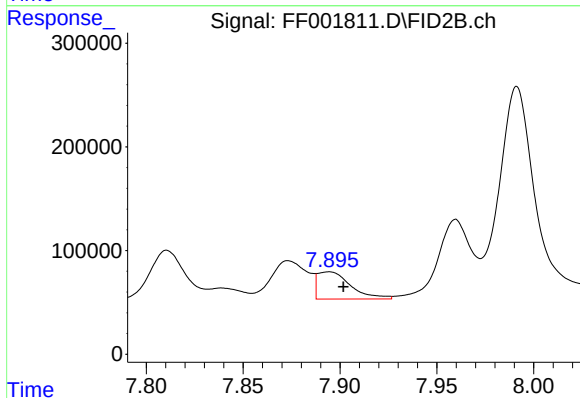


#4 N-TETRADECANE

R.T.: 7.894 min
Delta R.T.: -0.007 min
Response: 314205
Conc: 2.08 ug/ml

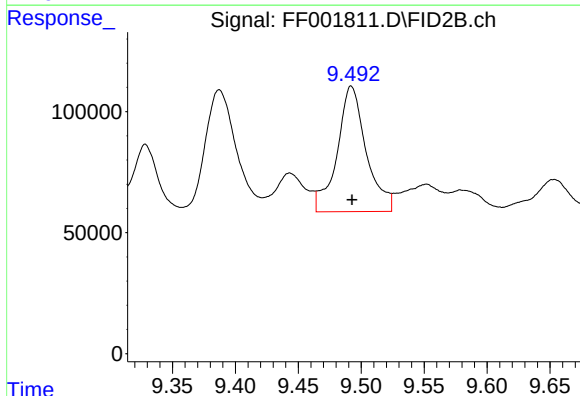


#5 N-HEXADECANE

R.T.: 9.492 min
Delta R.T.: 0.000 min
Response: 833149
Conc: 5.57 ug/ml

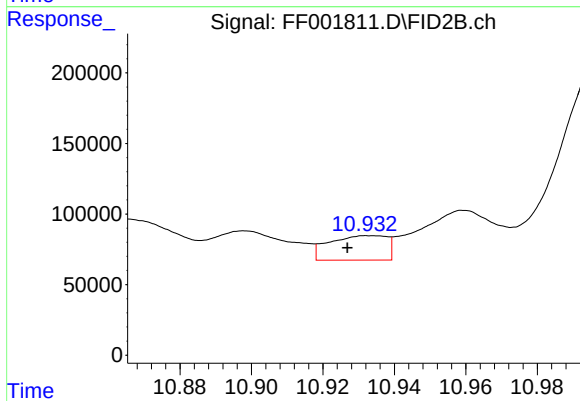

#6 N-OCTADECANE


R.T.: 10.933 min
Delta R.T.: 0.006 min
Response: 193824
Conc: 1.29 ug/ml

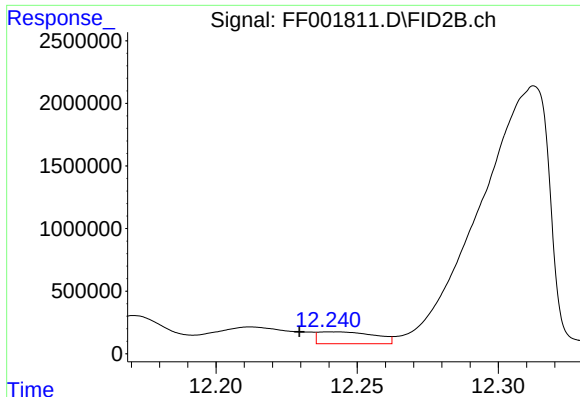

#7 N-EICOSANE


R.T.: 12.241 min
Delta R.T.: 0.012 min
Response: 1319998
Conc: 8.86 ug/ml

Instrument :
FID_F
ClientSampleId :

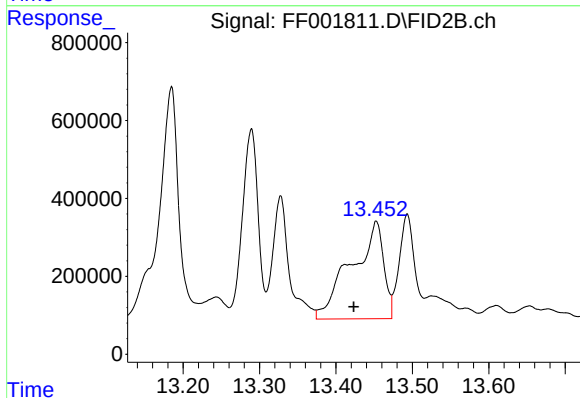


#8 N-DOCOSANE

R.T.: 13.453 min
Delta R.T.: 0.030 min
Response: 7337490
Conc: 50.23 ug/ml

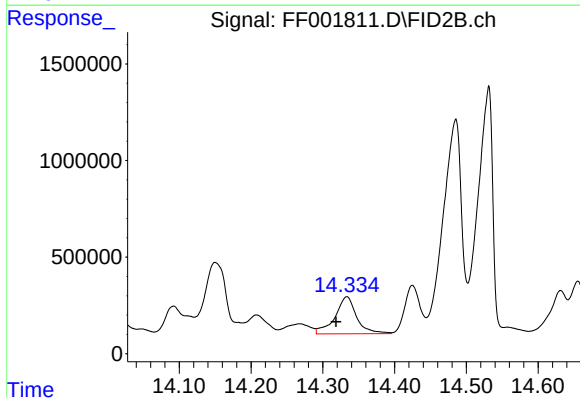


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.334 min
Delta R.T.: 0.015 min
Response: 4031667
Conc: 31.92 ug/ml

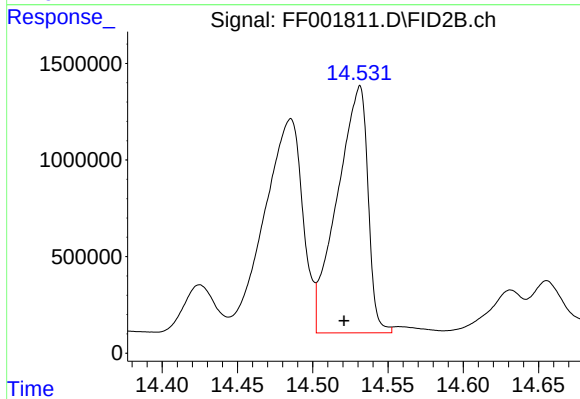

#10 N-TETRACOSANE


R.T.: 14.531 min
Delta R.T.: 0.010 min
Response: 18086993
Conc: 126.79 ug/ml

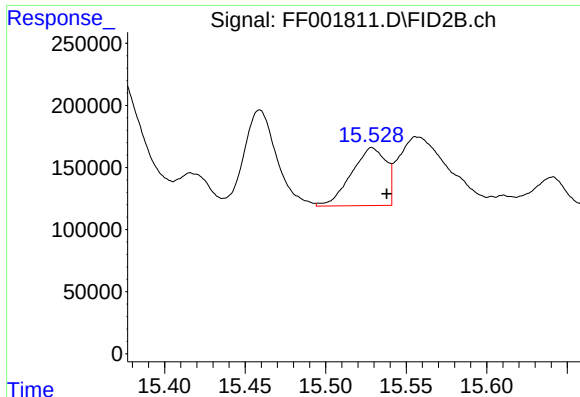

#11 N-HEXACOSANE


R.T.: 15.529 min
Delta R.T.: -0.009 min
Response: 697425
Conc: 4.95 ug/ml

Instrument :
FID_F
ClientSampleId :

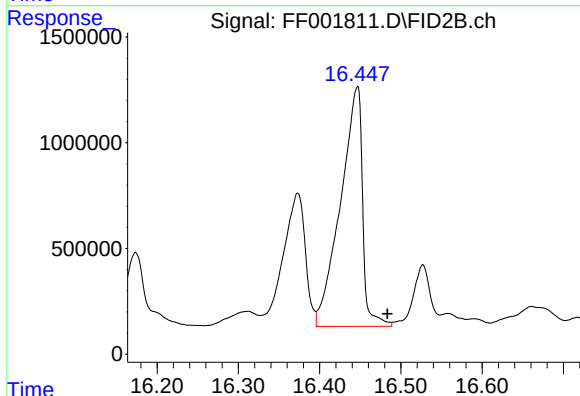


#12 N-OCTACOSANE

R.T.: 16.446 min
Delta R.T.: -0.037 min
Response: 21401977
Conc: 152.63 ug/ml

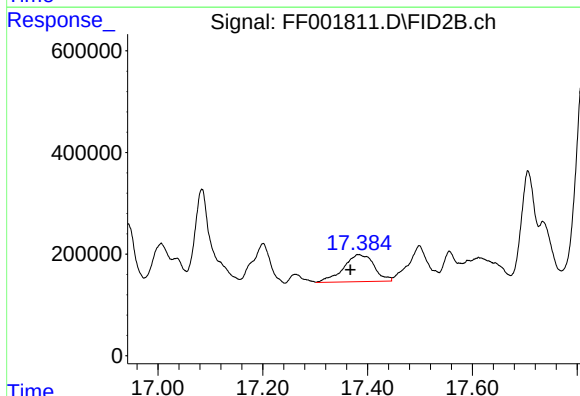


#13 N-TRIACONTANE

R.T.: 17.383 min
Delta R.T.: 0.016 min
Response: 2169129
Conc: 15.67 ug/ml

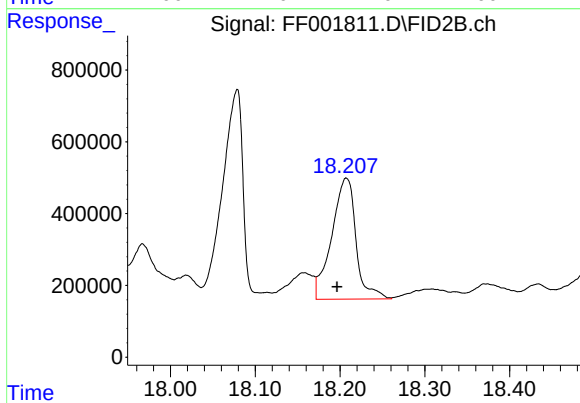

#14 N-DOTRIACONTANE


R.T.: 18.207 min
Delta R.T.: 0.011 min
Response: 6723248
Conc: 51.54 ug/ml

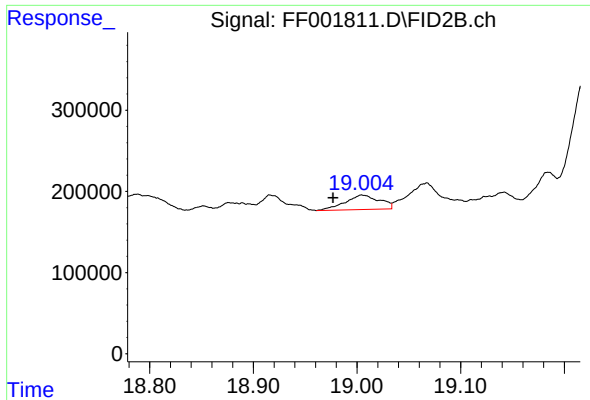

#15 N-TETRATRIACONTANE


R.T.: 19.005 min
Delta R.T.: 0.028 min
Response: 409830
Conc: 3.39 ug/ml

Instrument :
FID_F
ClientSampleId :

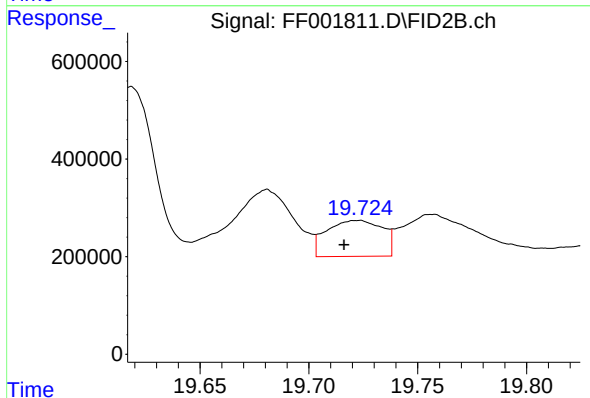

#16 N-HEXATRIACONTANE

R.T.: 19.723 min
Delta R.T.: 0.007 min
Response: 1313316
Conc: 11.80 ug/ml

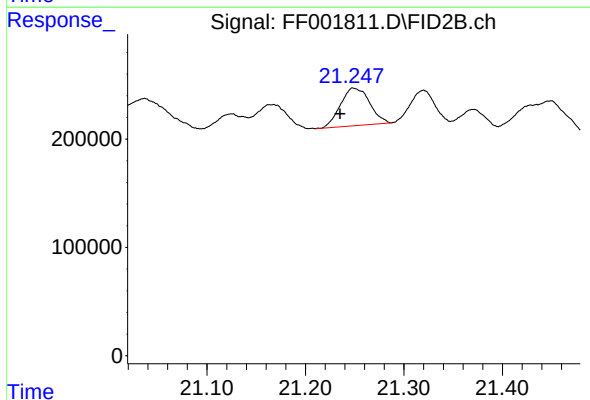

#18 N-TETRACONTANE

R.T.: 21.249 min
Delta R.T.: 0.014 min
Response: 712610
Conc: 7.15 ug/ml