

Data Path : Z:\pestpcbsrv\HPCHEM1\FID\_F\Data\FF081018\  
 Data File : FF001813.D  
 Signal(s) : FID2B.ch  
 Acq On : 11 Aug 2018 11:43  
 Operator : AJ\SJ  
 Sample : J4409-09  
 Misc :  
 ALS Vial : 81 Sample Multiplier: 1

Instrument :  
 FID\_F  
 ClientSampleId :

Integration File: autoint1.e  
 Quant Time: Aug 13 01:17:32 2018  
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID\_F\Method\FF073018.M  
 Quant Title :  
 QLast Update : Fri Aug 03 12:00:27 2018  
 Response via : Initial Calibration  
 Integrator: ChemStation

Volume Inj. : 1uL  
 Signal Phase : Rxi-1ms  
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units
-----			
System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.327	2061837	16.325 ug/ml
Target Compounds			
4) N-TETRADECANE	7.959f	739137	4.904 ug/ml
5) N-HEXADECANE	9.496	138023	0.922 ug/ml
7) N-EICOSANE	12.231	251744	1.689 ug/ml
8) N-DOCOSANE	13.439	811484	5.556 ug/ml
10) N-TETRACOSANE	14.500	3638116	25.503 ug/ml
11) N-HEXACOSANE	15.548	405250	2.877 ug/ml
12) N-OCTACOSANE	16.506	1107737	7.900 ug/ml
13) N-TRIACONTANE	17.380	811455	5.862 ug/ml
14) N-DOTRIACONTANE	18.185	1351877	10.362 ug/ml
15) N-TETRATRIACONTANE	18.994	200625	1.660 ug/ml
16) N-HEXATRIACONTANE	19.740	1173435	10.546 ug/ml
18) N-TETRACONTANE	21.242	701131	7.038 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID\_F\Data\FF081018\  
 Data File : FF001813.D  
 Signal(s) : FID2B.ch  
 Acq On : 11 Aug 2018 11:43  
 Operator : AJ\SJ  
 Sample : J4409-09  
 Misc :  
 ALS Vial : 81 Sample Multiplier: 1

Instrument :  
 FID\_F  
 ClientSampled :

Integration File: autoint1.e  
 Quant Time: Aug 13 01:17:32 2018  
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID\_F\Method\FF073018.M  
 Quant Title :  
 QLast Update : Fri Aug 03 12:00:27 2018  
 Response via : Initial Calibration  
 Integrator: ChemStation

Volume Inj. : 1uL  
 Signal Phase : Rxi-1ms  
 Signal Info : 20mx0.18mmx0.18um

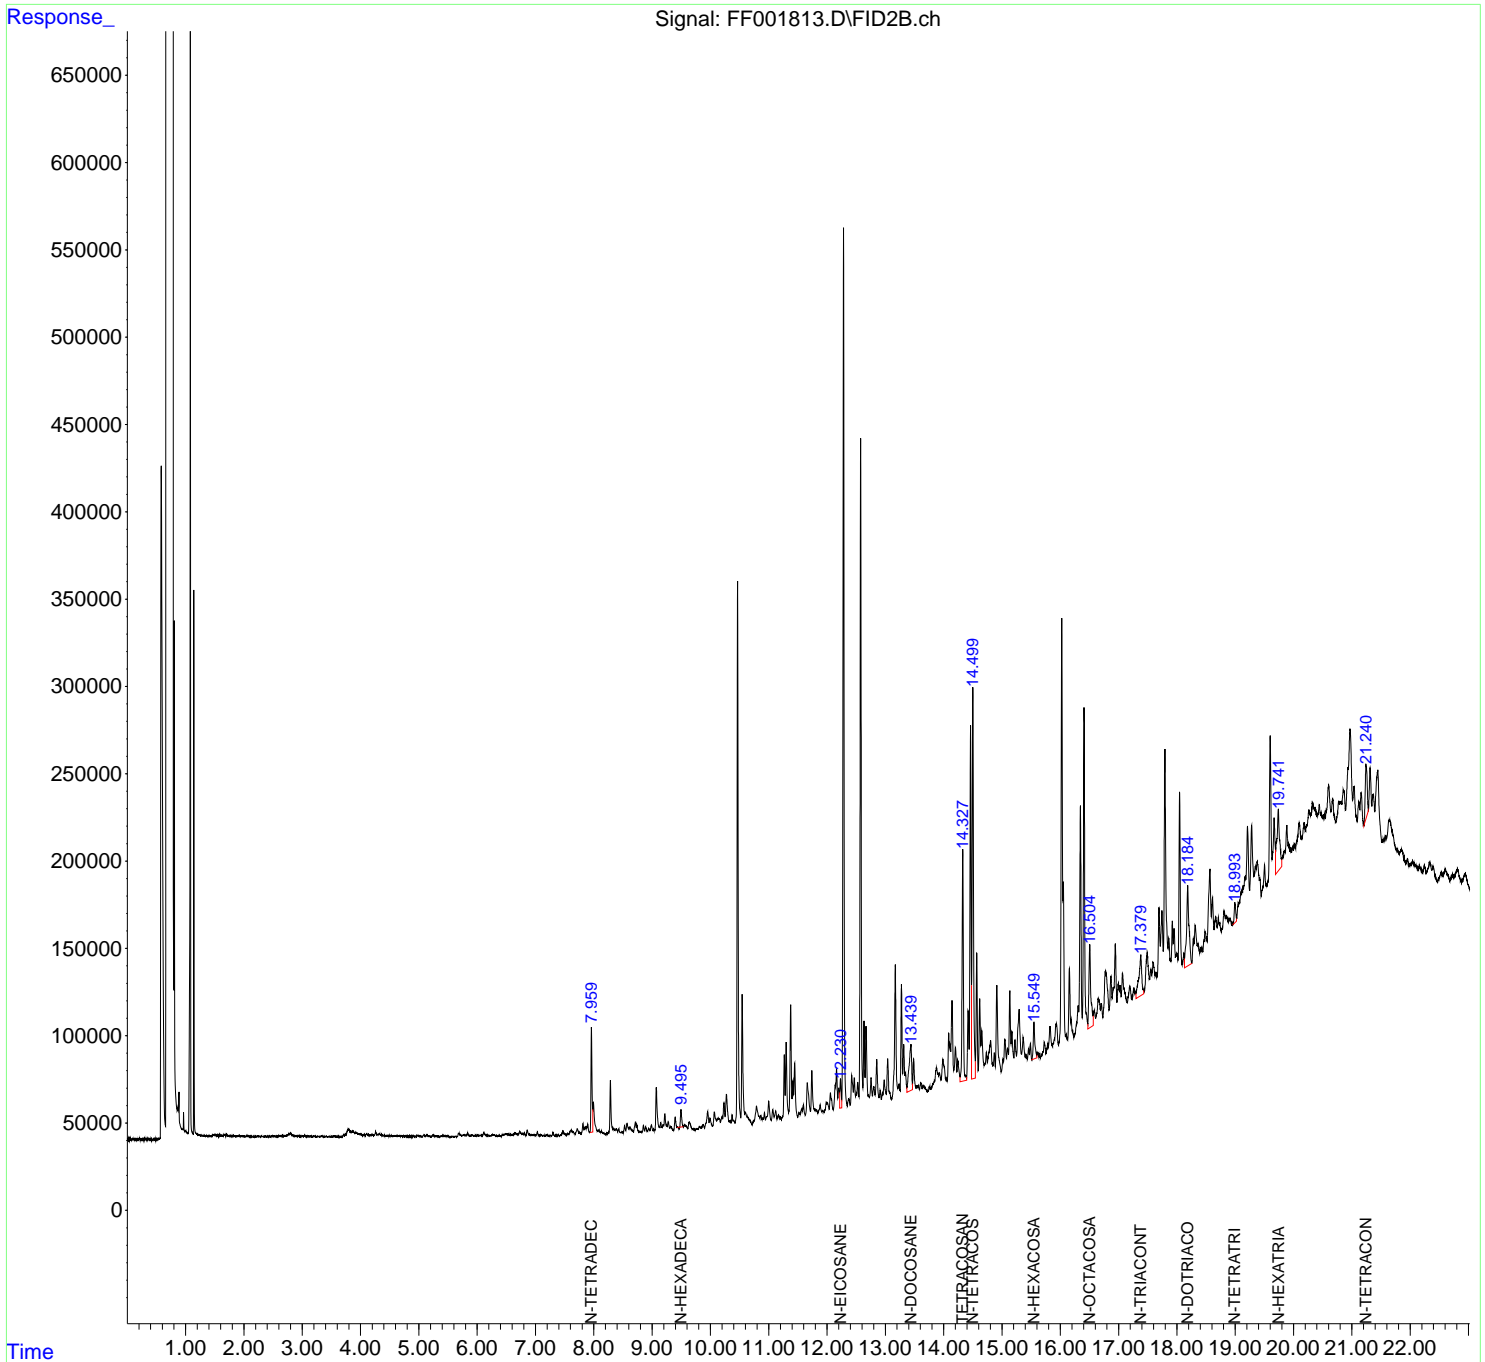


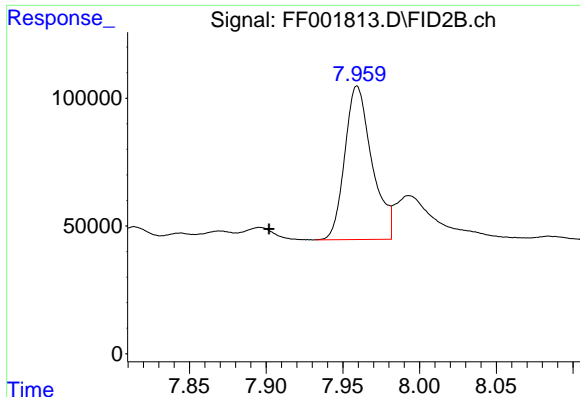

#4 N-TETRADECANE


R.T.: 7.959 min  
 Delta R.T.: 0.058 min  
 Response: 739137  
 Conc: 4.90 ug/ml

Instrument :  
 FID\_F  
 ClientSampleId :

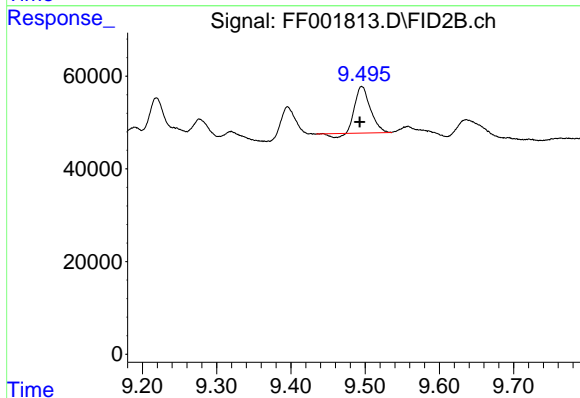


#5 N-HEXADECANE

R.T.: 9.496 min  
 Delta R.T.: 0.003 min  
 Response: 138023  
 Conc: 0.92 ug/ml

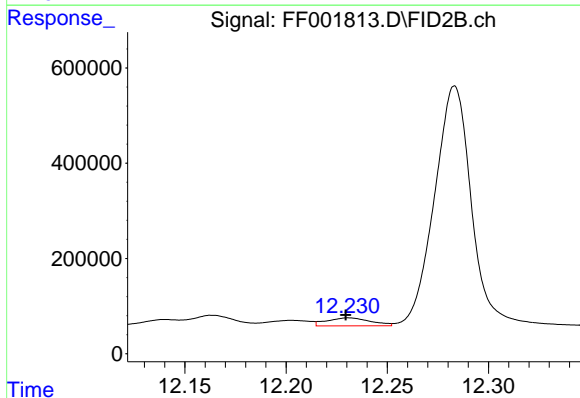


#7 N-EICOSANE

R.T.: 12.231 min  
 Delta R.T.: 0.002 min  
 Response: 251744  
 Conc: 1.69 ug/ml

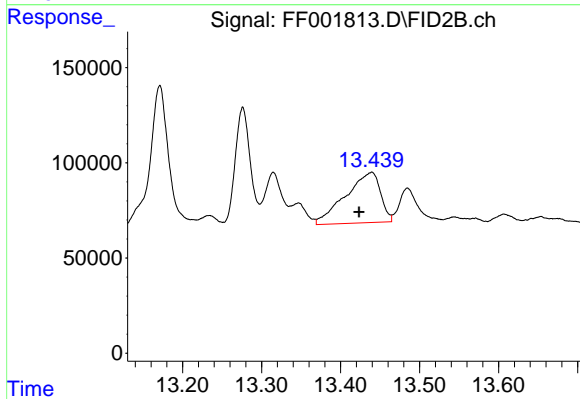

#8 N-DOCOSANE


R.T.: 13.439 min  
 Delta R.T.: 0.016 min  
 Response: 811484  
 Conc: 5.56 ug/ml

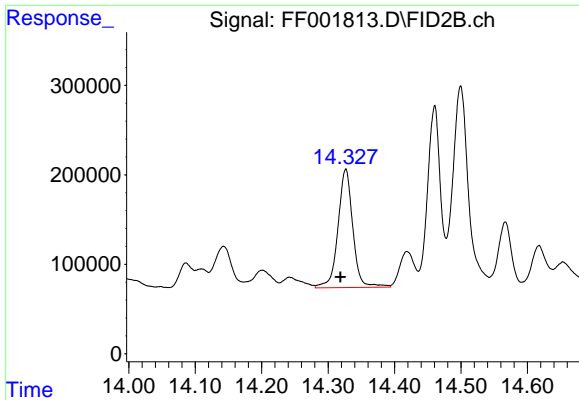

#9 TETRACOSANE-d50 (SURROGATE)


R.T.: 14.327 min  
Delta R.T.: 0.008 min  
Response: 2061837  
Conc: 16.32 ug/ml

Instrument :  
FID\_F  
ClientSampled :

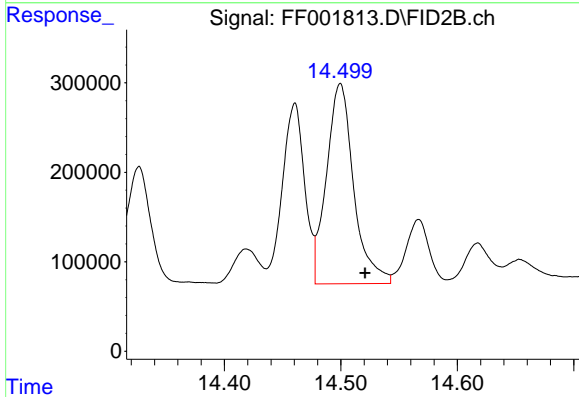


#10 N-TETRACOSANE

R.T.: 14.500 min  
Delta R.T.: -0.021 min  
Response: 3638116  
Conc: 25.50 ug/ml

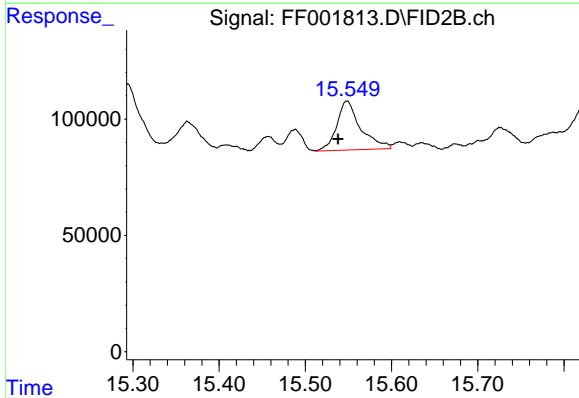


#11 N-HEXACOSANE

R.T.: 15.548 min  
Delta R.T.: 0.010 min  
Response: 405250  
Conc: 2.88 ug/ml

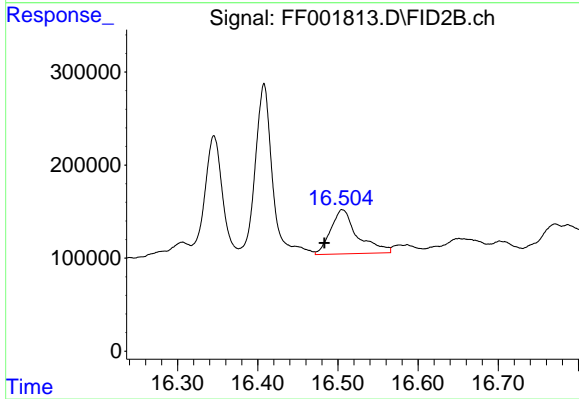

#12 N-OCTACOSANE


R.T.: 16.506 min  
Delta R.T.: 0.022 min  
Response: 1107737  
Conc: 7.90 ug/ml

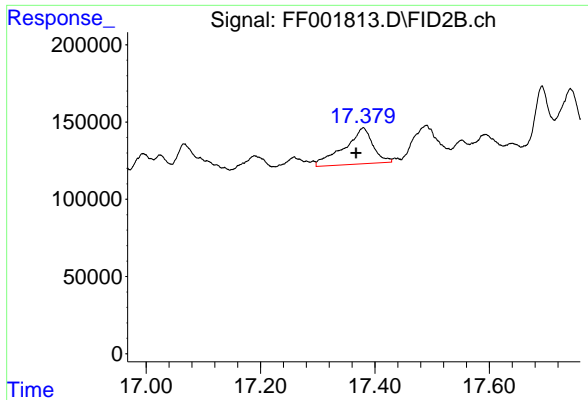

#13 N-TRIACONTANE


R.T.: 17.380 min  
 Delta R.T.: 0.013 min  
 Response: 811455  
 Conc: 5.86 ug/ml

Instrument :  
 FID\_F  
 ClientSampleId :

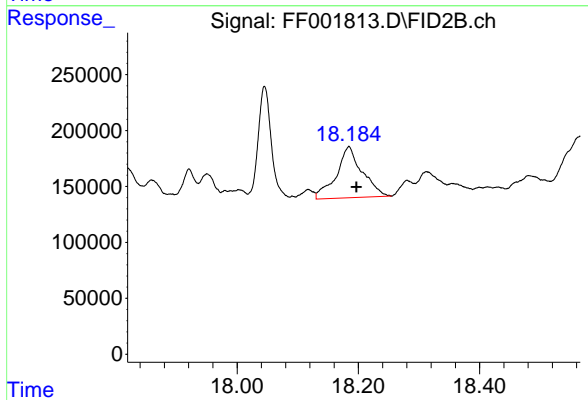


#14 N-DOTRIACONTANE

R.T.: 18.185 min  
 Delta R.T.: -0.012 min  
 Response: 1351877  
 Conc: 10.36 ug/ml

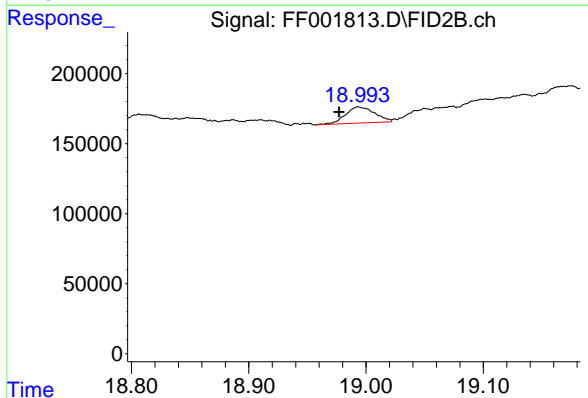


#15 N-TETRATRIACONTANE

R.T.: 18.994 min  
 Delta R.T.: 0.016 min  
 Response: 200625  
 Conc: 1.66 ug/ml

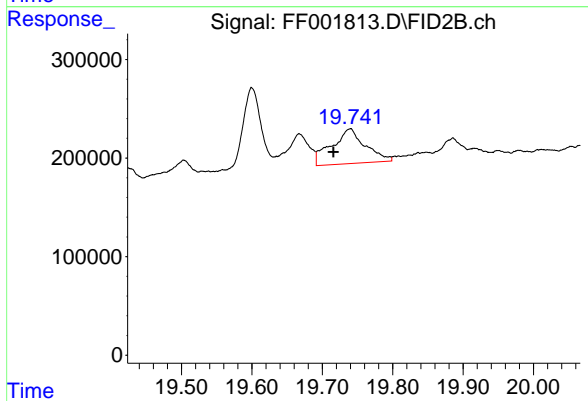

#16 N-HEXATRIACONTANE

R.T.: 19.740 min  
 Delta R.T.: 0.024 min  
 Response: 1173435  
 Conc: 10.55 ug/ml

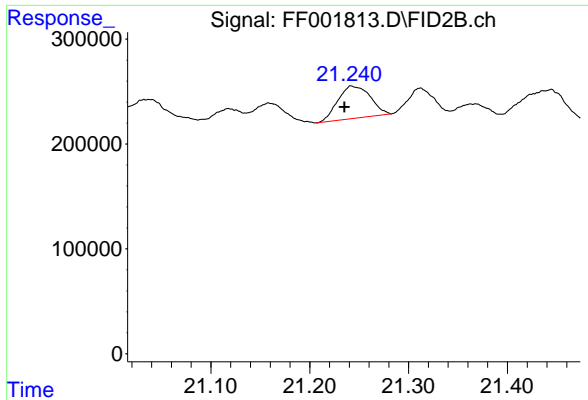

#18 N-TETRACONTANE

R.T.: 21.242 min  
Delta R.T.: 0.007 min  
Response: 701131  
Conc: 7.04 ug/ml

Instrument :  
FID\_F  
ClientSampleId :