

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF081018\
 Data File : FF001814.D
 Signal(s) : FID2B.ch
 Acq On : 11 Aug 2018 12:14
 Operator : AJ\SJ
 Sample : J4409-11
 Misc :
 ALS Vial : 82 Sample Multiplier: 1

Instrument :
 FID_F
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Aug 13 01:17:45 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF073018.M
 Quant Title :
 QLast Update : Fri Aug 03 12:00:27 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.325	2006908	15.890 ug/ml
Target Compounds			
4) N-TETRADECANE	7.959f	698480	4.634 ug/ml
6) N-OCTADECANE	10.926	79427	0.527 ug/ml
7) N-EICOSANE	12.230	180622	1.212 ug/ml
8) N-DOCOSANE	13.438	399724	2.737 ug/ml
10) N-TETRACOSANE	14.497	1900818	13.325 ug/ml
11) N-HEXACOSANE	15.546	169080	1.200 ug/ml
12) N-OCTACOSANE	16.502	909898	6.489 ug/ml
13) N-TRIACONTANE	17.380	538529	3.890 ug/ml
14) N-DOTRIACONTANE	18.185	951535	7.294 ug/ml
15) N-TETRATRIACONTANE	18.994	178817	1.479 ug/ml
16) N-HEXATRIACONTANE	19.736	503376	4.524 ug/ml
18) N-TETRACONTANE	21.233	326617	3.279 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF081018\
Data File : FF001814.D
Signal(s) : FID2B.ch
Acq On : 11 Aug 2018 12:14
Operator : AJ\SJ
Sample : J4409-11
Misc :
ALS Vial : 82 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Aug 13 01:17:45 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF073018.M
Quant Title :
QLast Update : Fri Aug 03 12:00:27 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

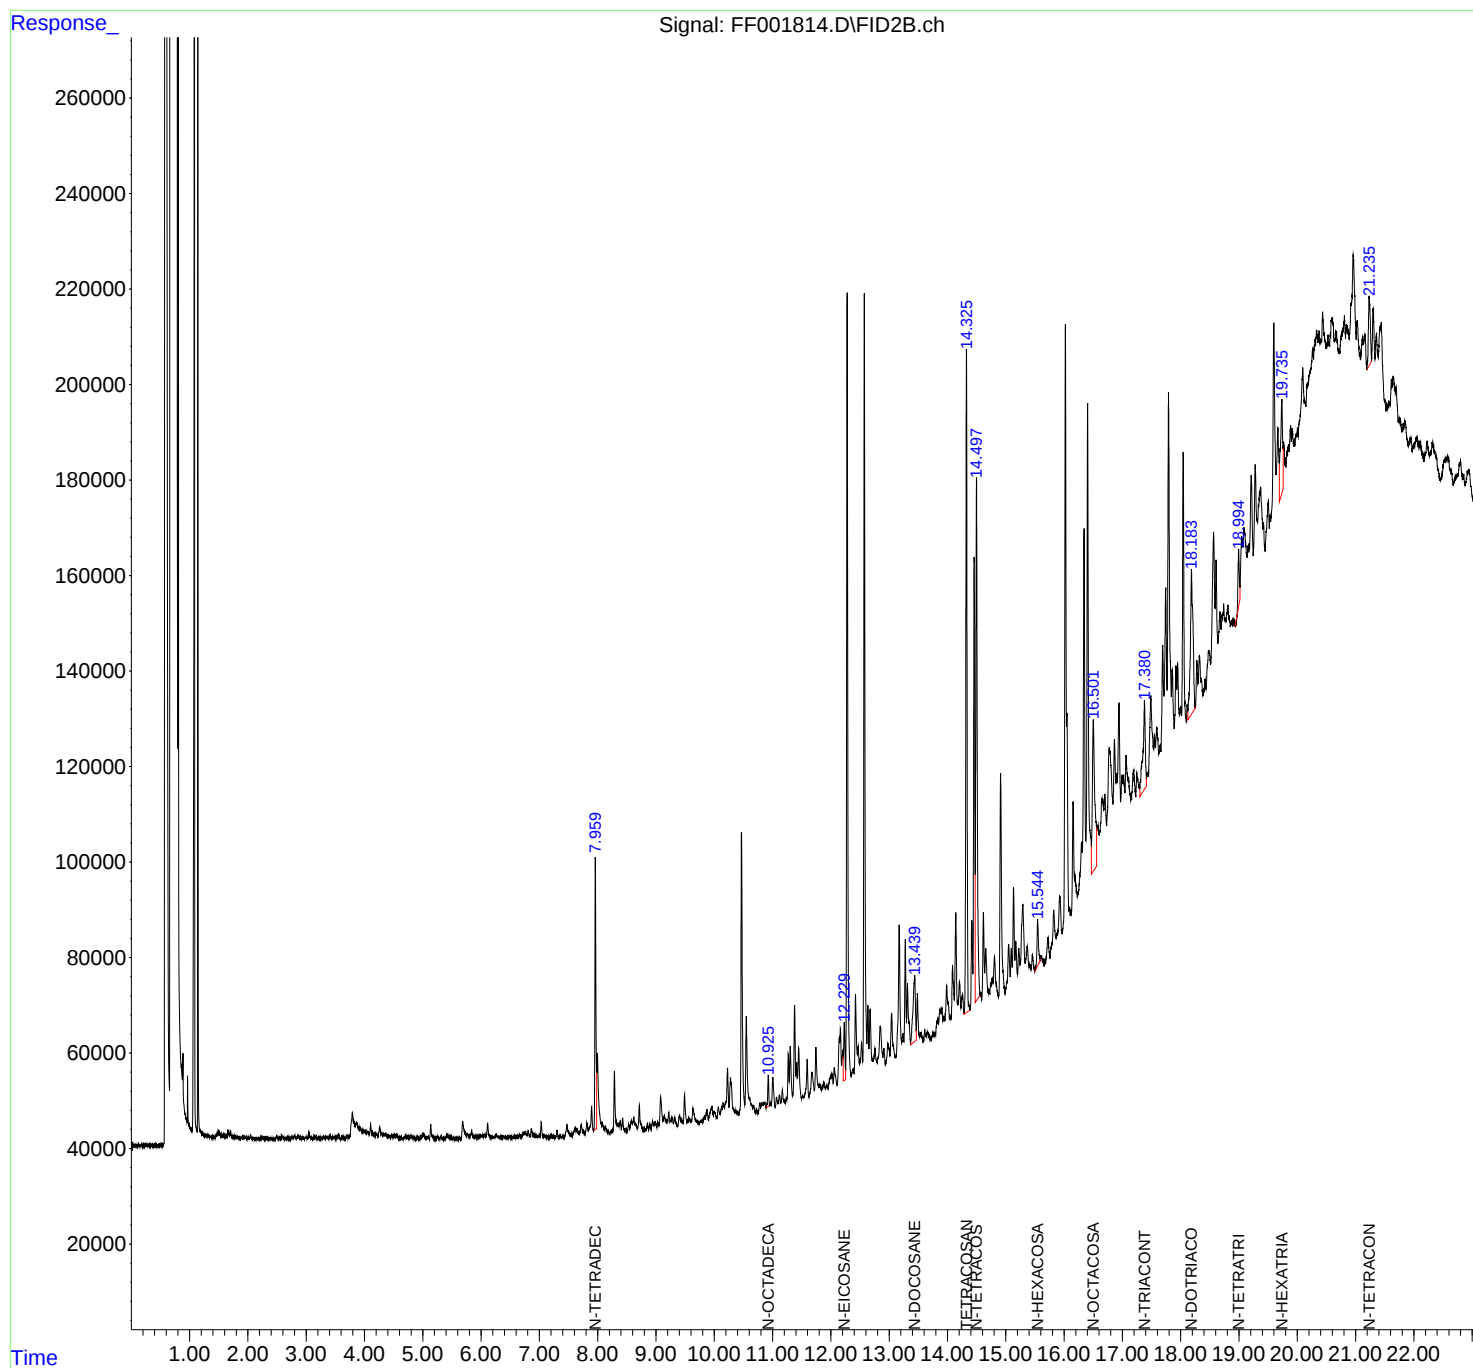


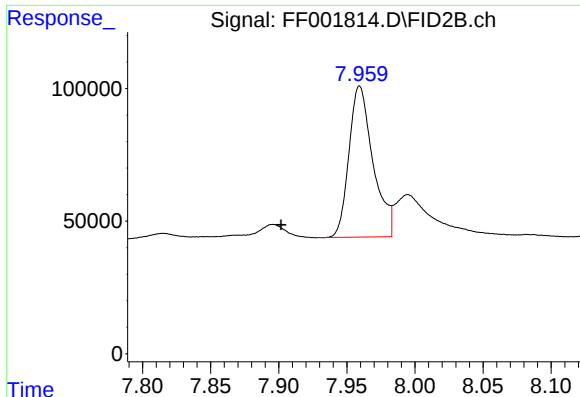

#4 N-TETRADECANE


R.T.: 7.959 min
Delta R.T.: 0.058 min
Response: 698480
Conc: 4.63 ug/ml

Instrument :
FID_F
ClientSampleId :

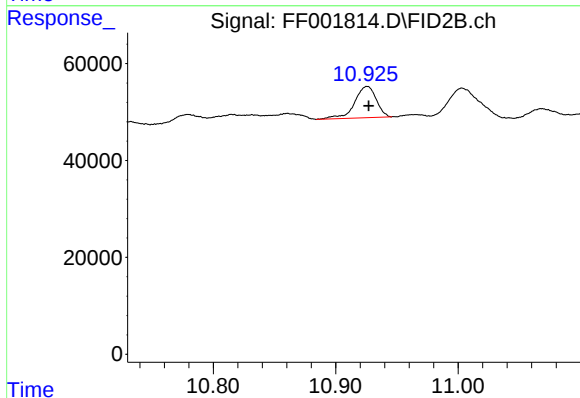


#6 N-OCTADECANE

R.T.: 10.926 min
Delta R.T.: -0.001 min
Response: 79427
Conc: 0.53 ug/ml

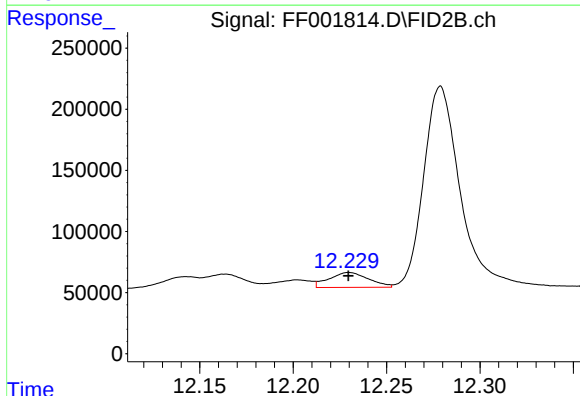


#7 N-EICOSANE

R.T.: 12.230 min
Delta R.T.: 0.000 min
Response: 180622
Conc: 1.21 ug/ml

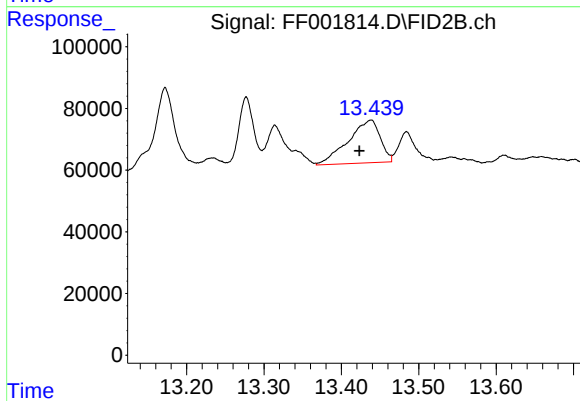

#8 N-DOCOSANE


R.T.: 13.438 min
Delta R.T.: 0.015 min
Response: 399724
Conc: 2.74 ug/ml

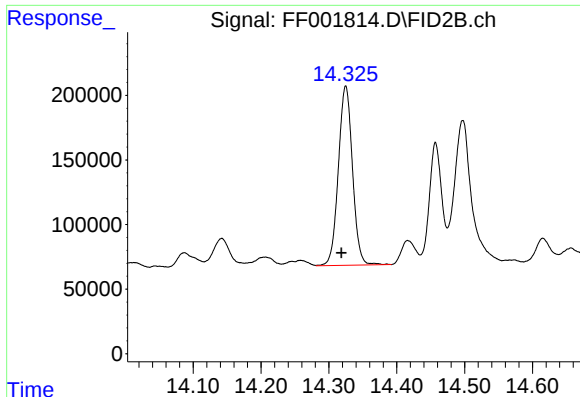

#9 TETRACOSANE-d50 (SURROGATE)


R.T.: 14.325 min
Delta R.T.: 0.006 min
Response: 2006908
Conc: 15.89 ug/ml

Instrument :
FID_F
ClientSampleId :

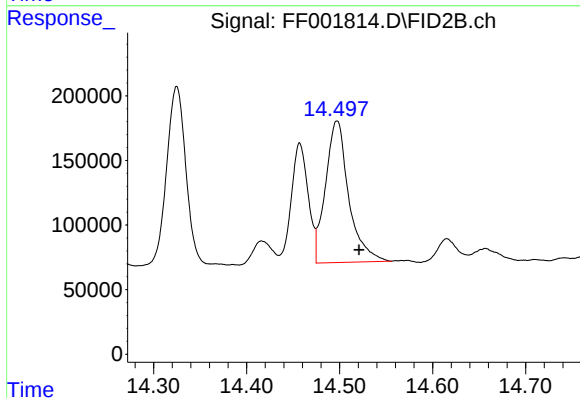


#10 N-TETRACOSANE

R.T.: 14.497 min
Delta R.T.: -0.024 min
Response: 1900818
Conc: 13.32 ug/ml

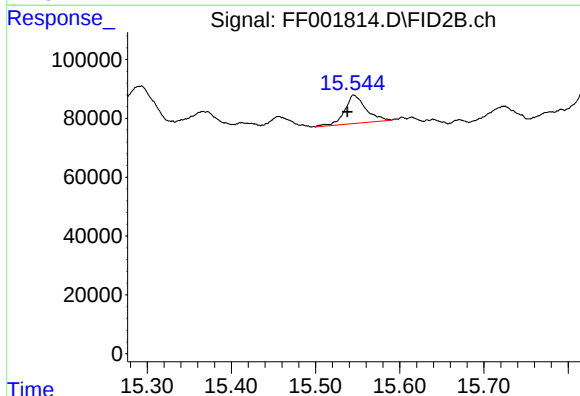


#11 N-HEXACOSANE

R.T.: 15.546 min
Delta R.T.: 0.008 min
Response: 169080
Conc: 1.20 ug/ml

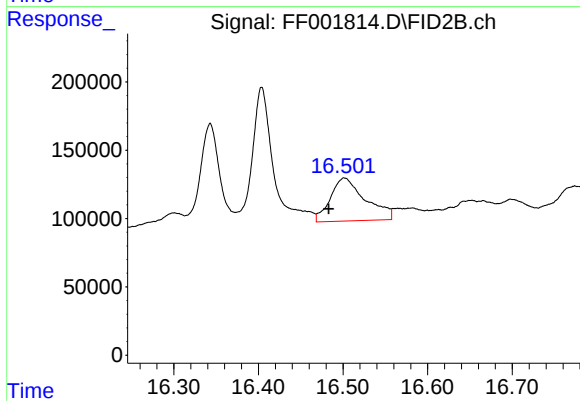

#12 N-OCTACOSANE


R.T.: 16.502 min
Delta R.T.: 0.018 min
Response: 909898
Conc: 6.49 ug/ml

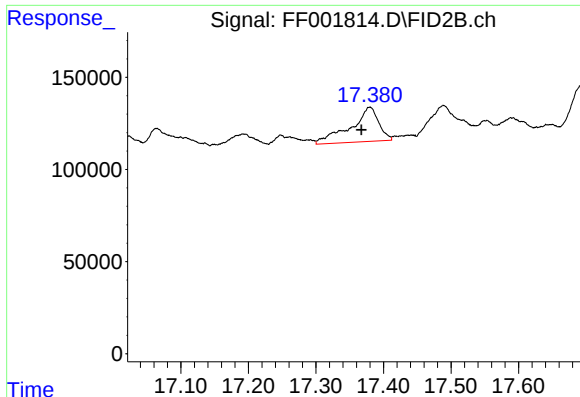

#13 N-TRIACONTANE


R.T.: 17.380 min
Delta R.T.: 0.013 min
Response: 538529
Conc: 3.89 ug/ml

Instrument :
FID_F
ClientSampleId :

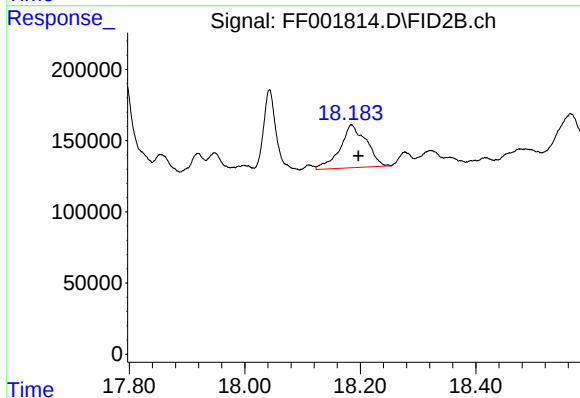


#14 N-DOTRIACONTANE

R.T.: 18.185 min
Delta R.T.: -0.012 min
Response: 951535
Conc: 7.29 ug/ml

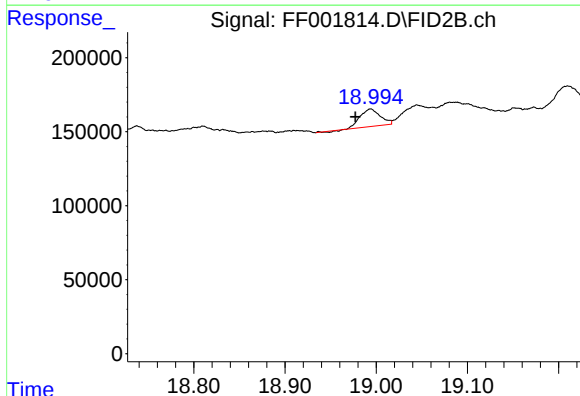


#15 N-TETRATRIACONTANE

R.T.: 18.994 min
Delta R.T.: 0.017 min
Response: 178817
Conc: 1.48 ug/ml

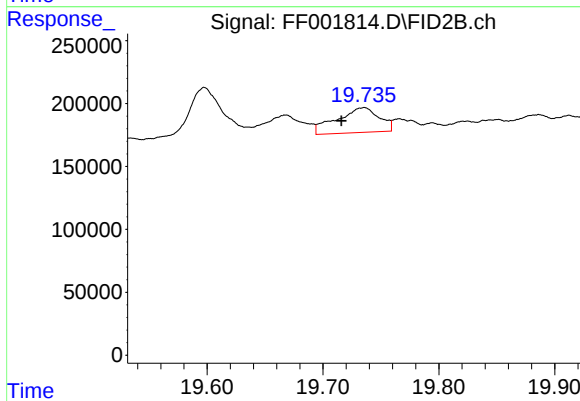

#16 N-HEXATRIACONTANE

R.T.: 19.736 min
Delta R.T.: 0.019 min
Response: 503376
Conc: 4.52 ug/ml

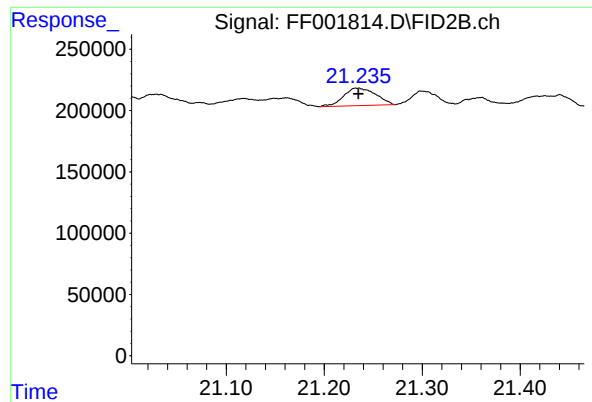

#18 N-TETRACONTANE

R.T.: 21.233 min
Delta R.T.: -0.002 min
Response: 326617
Conc: 3.28 ug/ml

Instrument :
FID_F
ClientSampleId :