

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF081018\
 Data File : FF001816.D
 Signal(s) : FID2B.ch
 Acq On : 11 Aug 2018 13:15
 Operator : AJ\SJ
 Sample : J4409-01 50X
 Misc :
 ALS Vial : 84 Sample Multiplier: 1

Instrument :
 FID_F
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Aug 13 01:18:11 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF073018.M
 Quant Title :
 QLast Update : Fri Aug 03 12:00:27 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.336	323172	2.559 ug/ml
Target Compounds			
4) N-TETRADECANE	7.840f	356830	2.368 ug/ml
5) N-HEXADECANE	9.499	199279	1.331 ug/ml
7) N-EICOSANE	12.230	269513	1.808 ug/ml
8) N-DOCOSANE	13.442	552742	3.784 ug/ml
10) N-TETRACOSANE	14.500	3742677	26.236 ug/ml
12) N-OCTACOSANE	16.508	332566	2.372 ug/ml
13) N-TRIACONTANE	17.391	190527	1.376 ug/ml
14) N-DOTRIACONTANE	18.182	1185857	9.090 ug/ml
15) N-TETRATRIACONTANE	18.997	23872	0.197 ug/ml
16) N-HEXATRIACONTANE	19.734	446109	4.009 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF081018\
Data File : FF001816.D
Signal(s) : FID2B.ch
Acq On : 11 Aug 2018 13:15
Operator : AJ\SJ
Sample : J4409-01 50X
Misc :
ALS Vial : 84 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Aug 13 01:18:11 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF073018.M
Quant Title :
QLast Update : Fri Aug 03 12:00:27 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

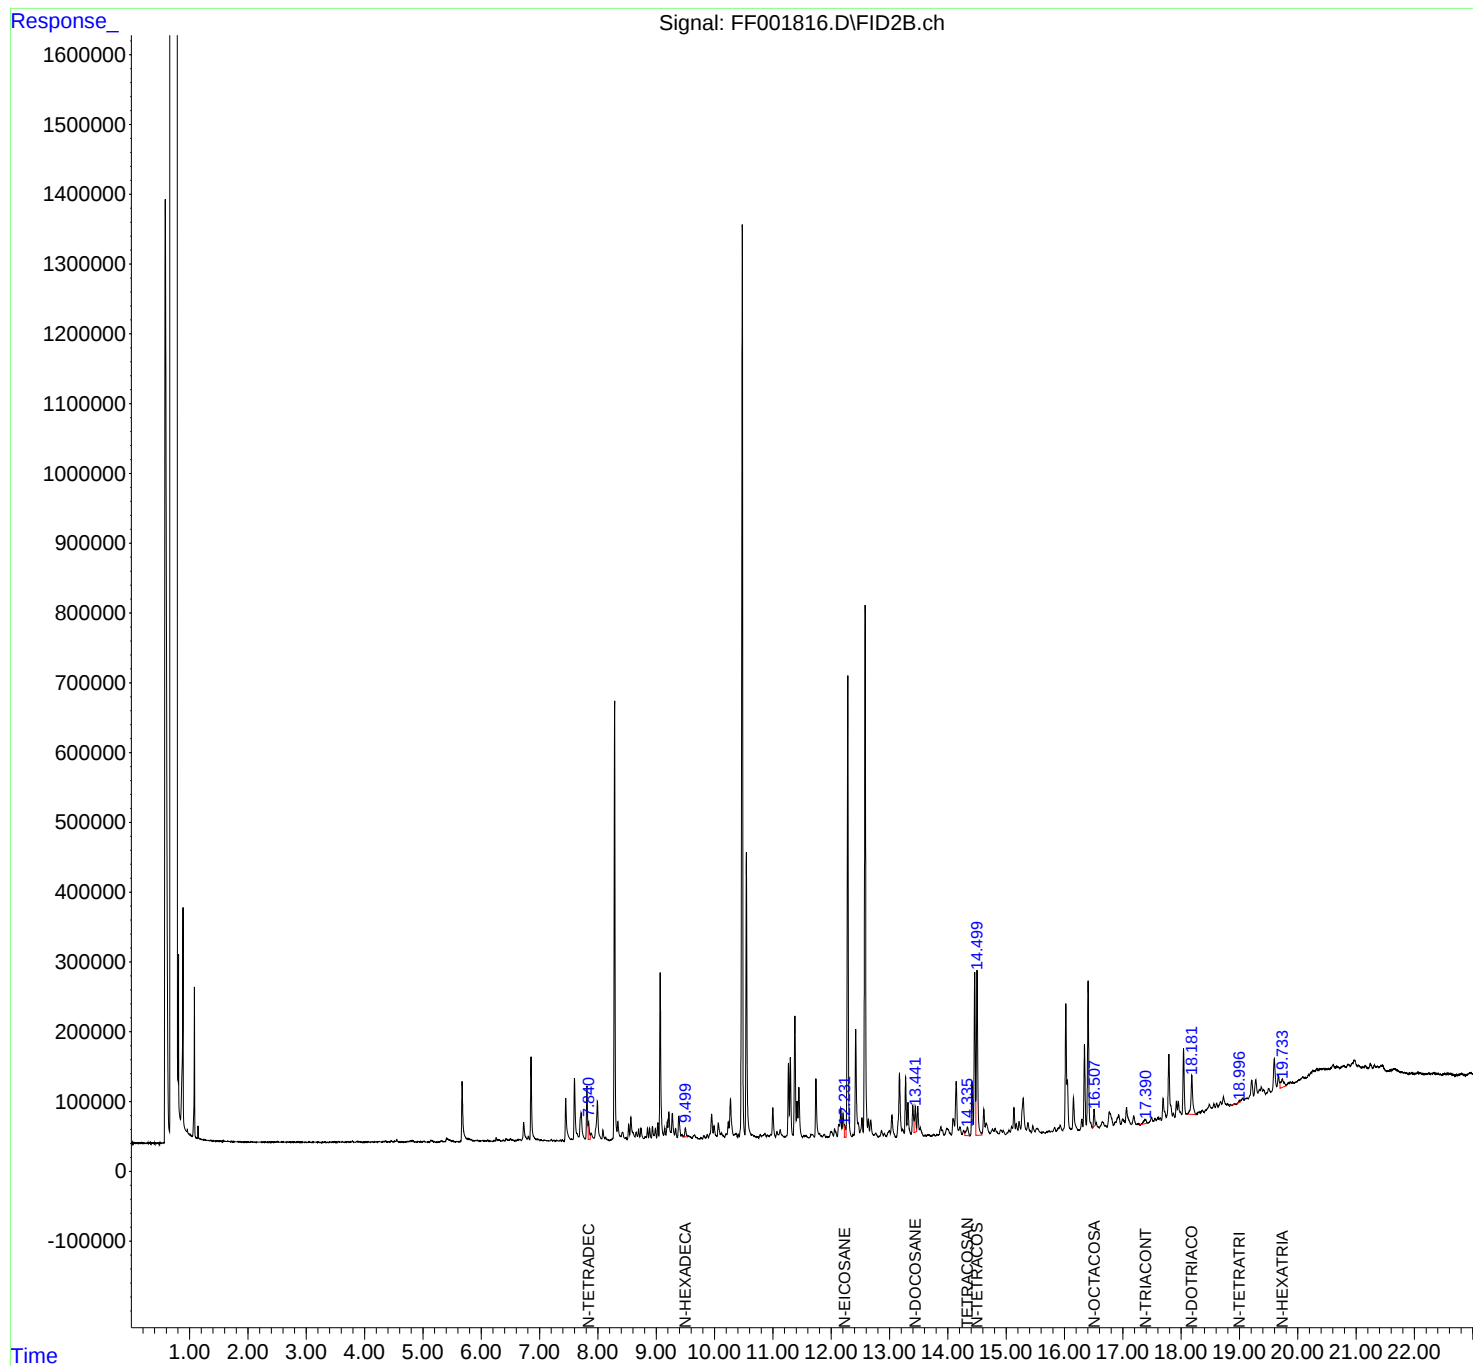


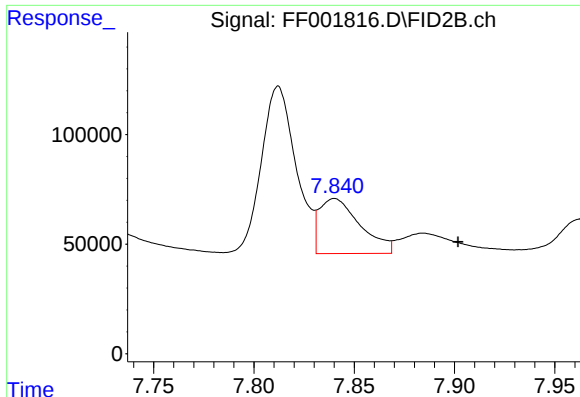

#4 N-TETRADECANE


R.T.: 7.840 min
Delta R.T.: -0.061 min
Response: 356830
Conc: 2.37 ug/ml

Instrument :
FID_F
ClientSampleId :

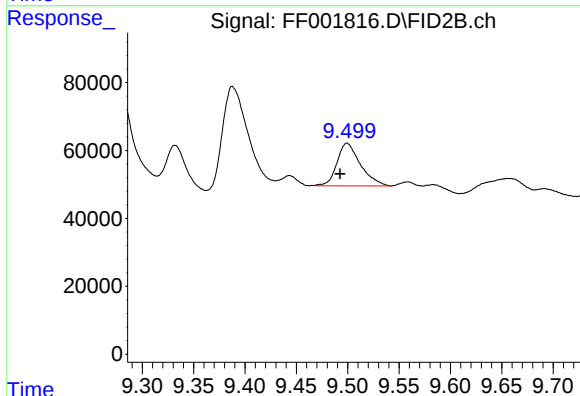


#5 N-HEXADECANE

R.T.: 9.499 min
Delta R.T.: 0.007 min
Response: 199279
Conc: 1.33 ug/ml

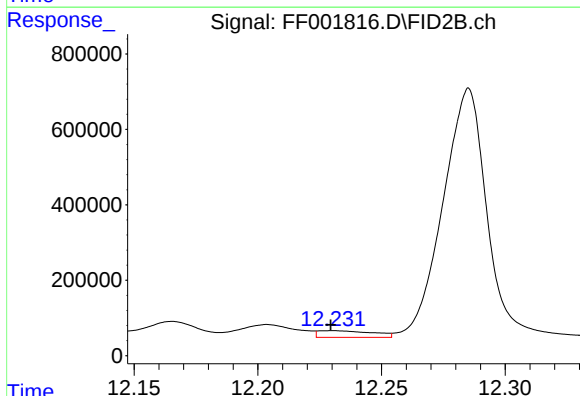


#7 N-EICOSANE

R.T.: 12.230 min
Delta R.T.: 0.000 min
Response: 269513
Conc: 1.81 ug/ml

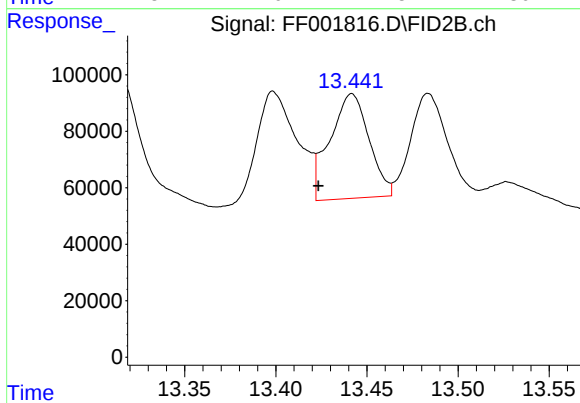

#8 N-DOCOSANE


R.T.: 13.442 min
Delta R.T.: 0.018 min
Response: 552742
Conc: 3.78 ug/ml

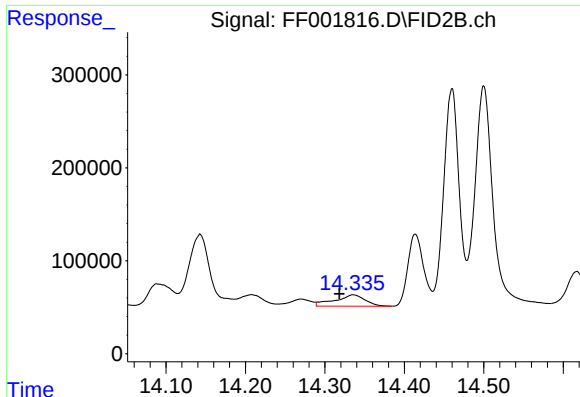

#9 TETRACOSANE-d50 (SURROGATE)


R.T.: 14.336 min
Delta R.T.: 0.017 min
Response: 323172
Conc: 2.56 ug/ml

Instrument :
FID_F
ClientSampleId :

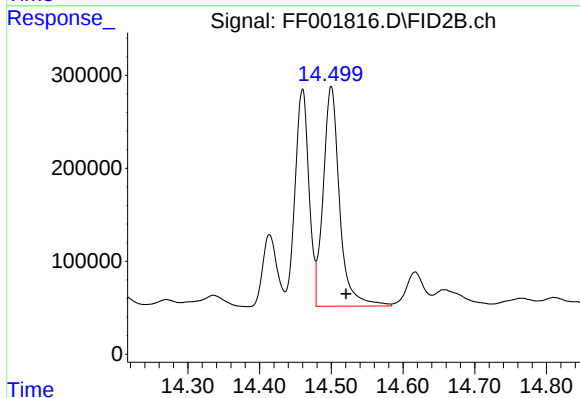


#10 N-TETRACOSANE

R.T.: 14.500 min
Delta R.T.: -0.021 min
Response: 3742677
Conc: 26.24 ug/ml

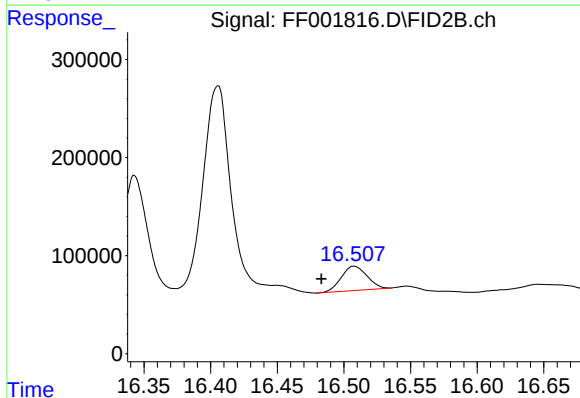


#12 N-OCTACOSANE

R.T.: 16.508 min
Delta R.T.: 0.024 min
Response: 332566
Conc: 2.37 ug/ml

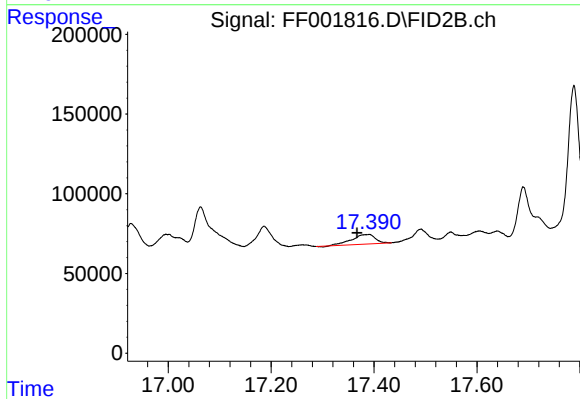

#13 N-TRIACONTANE


R.T.: 17.391 min
Delta R.T.: 0.023 min
Response: 190527
Conc: 1.38 ug/ml

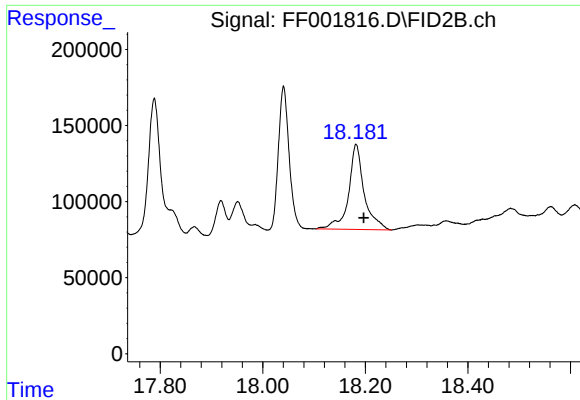

#14 N-DOTRIACONTANE


R.T.: 18.182 min
Delta R.T.: -0.015 min
Response: 1185857
Conc: 9.09 ug/ml

Instrument :
FID_F
ClientSampleId :

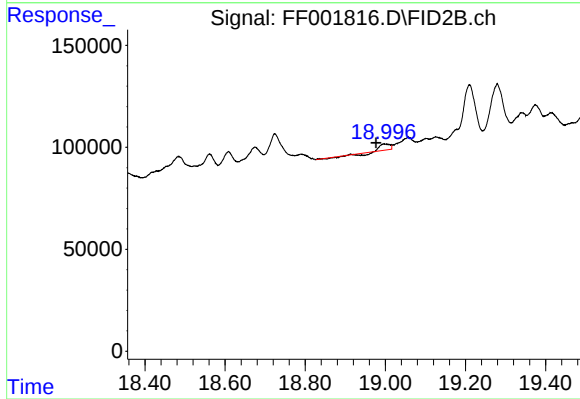

#15 N-TETRATRIACONTANE

R.T.: 18.997 min
Delta R.T.: 0.020 min
Response: 23872
Conc: 0.20 ug/ml

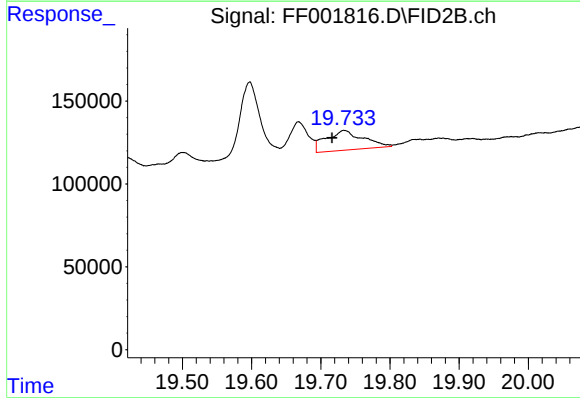

#16 N-HEXATRIACONTANE

R.T.: 19.734 min
Delta R.T.: 0.018 min
Response: 446109
Conc: 4.01 ug/ml