

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF081018\
 Data File : FF001817.D
 Signal(s) : FID2B.ch
 Acq On : 11 Aug 2018 13:46
 Operator : AJ\SJ
 Sample : J4409-03 2X
 Misc :
 ALS Vial : 85 Sample Multiplier: 1

Instrument :
 FID_F
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Aug 13 01:18:23 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF073018.M
 Quant Title :
 QLast Update : Fri Aug 03 12:00:27 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.323	1284846	10.173 ug/ml
Target Compounds			
4) N-TETRADECANE	7.960f	390990	2.594 ug/ml
7) N-EICOSANE	12.228	203803	1.367 ug/ml
8) N-DOCOSANE	13.441	543588	3.721 ug/ml
10) N-TETRACOSANE	14.498	2860374	20.051 ug/ml
11) N-HEXACOSANE	15.547	220066	1.562 ug/ml
12) N-OCTACOSANE	16.505	713661	5.090 ug/ml
13) N-TRIACONTANE	17.378	497684	3.595 ug/ml
14) N-DOTRIACONTANE	18.185	1410572	10.812 ug/ml
15) N-TETRATRIACONTANE	18.993	288834	2.390 ug/ml
16) N-HEXATRIACONTANE	19.733	424378	3.814 ug/ml
17) N-OCTATRIACONTANE	20.440	125510	1.259 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF081018\
Data File : FF001817.D
Signal(s) : FID2B.ch
Acq On : 11 Aug 2018 13:46
Operator : AJ\SJ
Sample : J4409-03 2X
Misc :
ALS Vial : 85 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Aug 13 01:18:23 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF073018.M
Quant Title :
QLast Update : Fri Aug 03 12:00:27 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

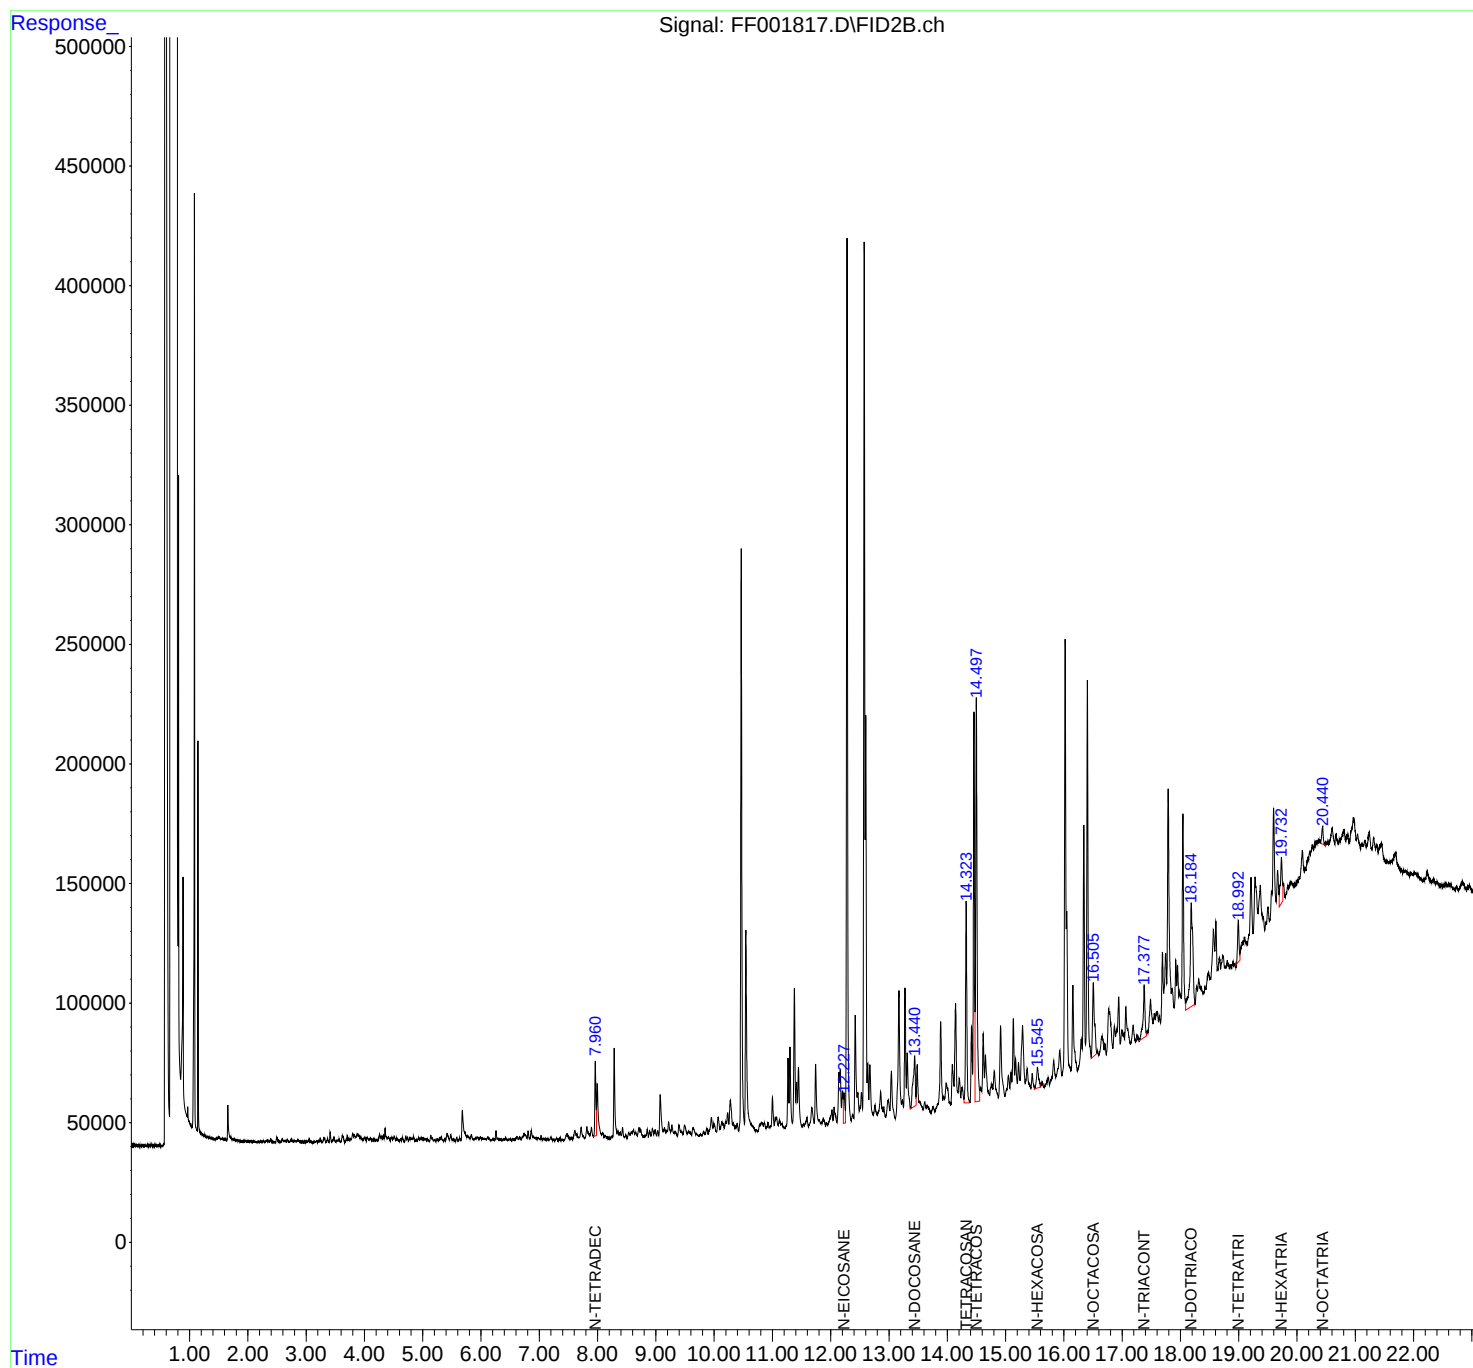


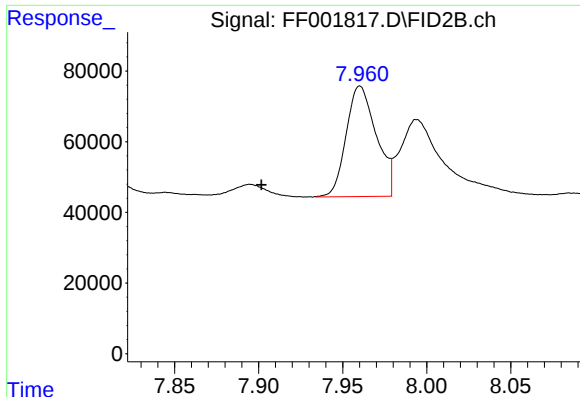

#4 N-TETRADECANE


R.T.: 7.960 min
Delta R.T.: 0.059 min
Response: 390990
Conc: 2.59 ug/ml

Instrument :
FID_F
ClientSampleId :

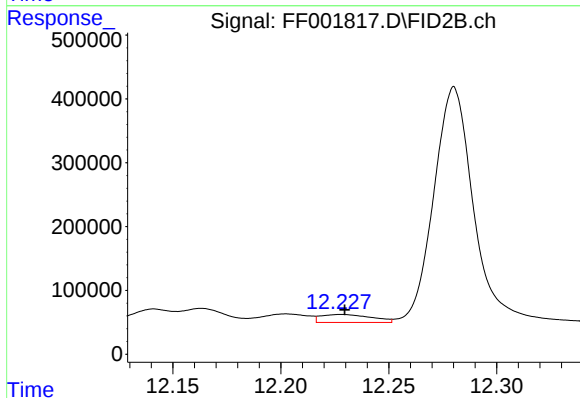


#7 N-EICOSANE

R.T.: 12.228 min
Delta R.T.: -0.002 min
Response: 203803
Conc: 1.37 ug/ml

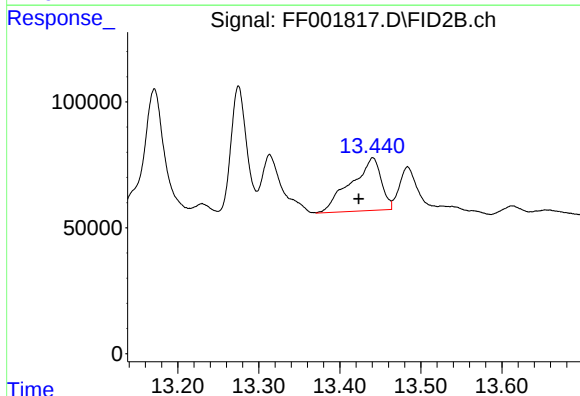


#8 N-DOCOSANE

R.T.: 13.441 min
Delta R.T.: 0.017 min
Response: 543588
Conc: 3.72 ug/ml

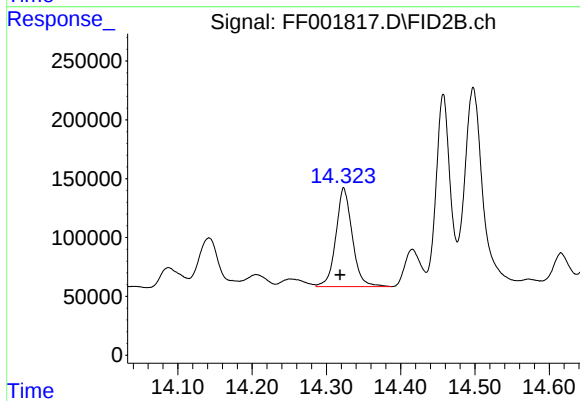

#9 TETRACOSANE-d50 (SURROGATE)


R.T.: 14.323 min
Delta R.T.: 0.005 min
Response: 1284846
Conc: 10.17 ug/ml

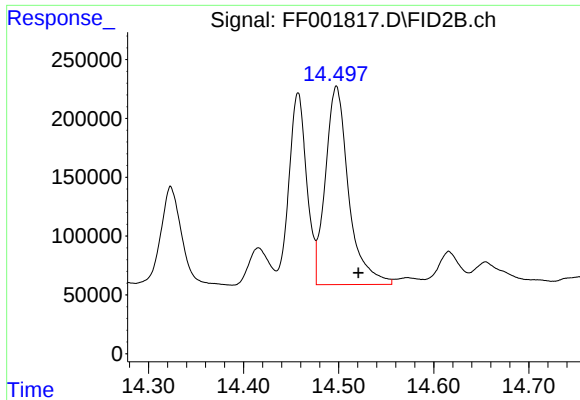

#10 N-TETRACOSANE


R.T.: 14.498 min
Delta R.T.: -0.023 min
Response: 2860374
Conc: 20.05 ug/ml

Instrument :
FID_F
ClientSampleId :

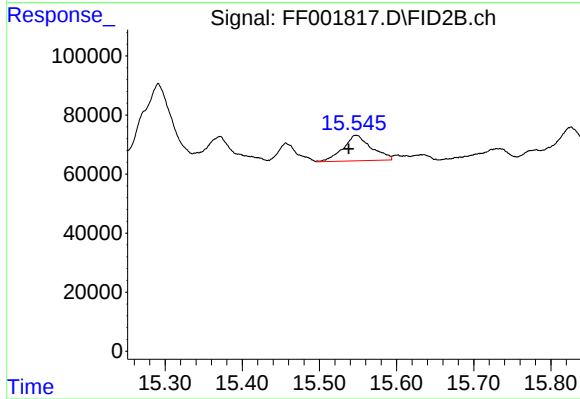


#11 N-HEXACOSANE

R.T.: 15.547 min
Delta R.T.: 0.010 min
Response: 220066
Conc: 1.56 ug/ml

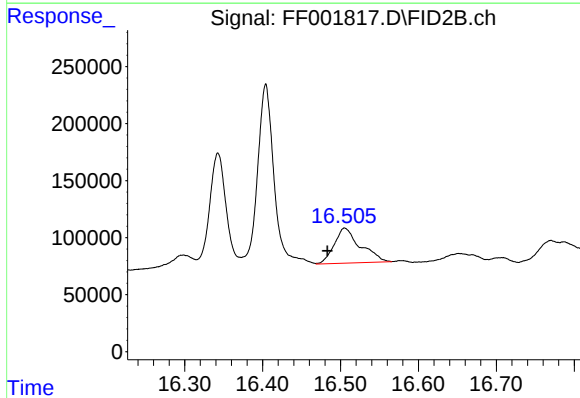


#12 N-OCTACOSANE

R.T.: 16.505 min
Delta R.T.: 0.022 min
Response: 713661
Conc: 5.09 ug/ml

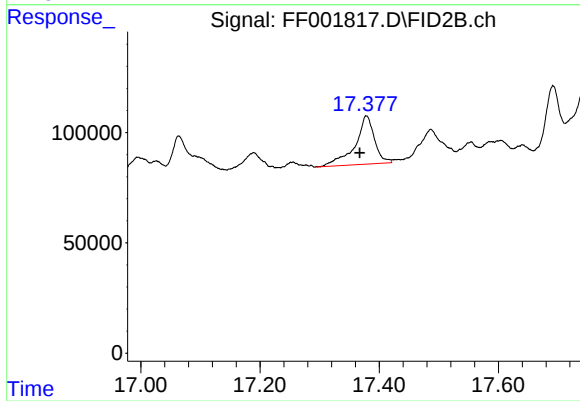

#13 N-TRIACONTANE


R.T.: 17.378 min
Delta R.T.: 0.011 min
Response: 497684
Conc: 3.60 ug/ml

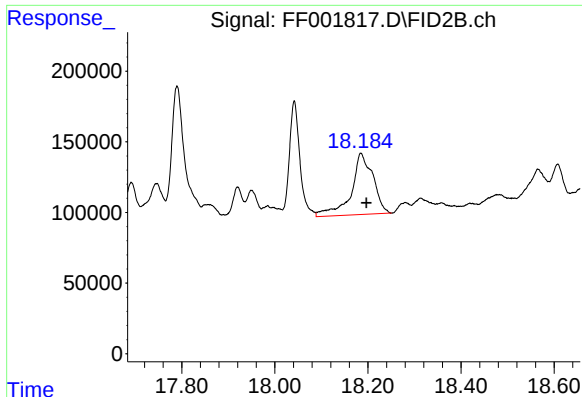

#14 N-DOTRIACONTANE


R.T.: 18.185 min
Delta R.T.: -0.012 min
Response: 1410572
Conc: 10.81 ug/ml

Instrument :
FID_F
ClientSampleId :

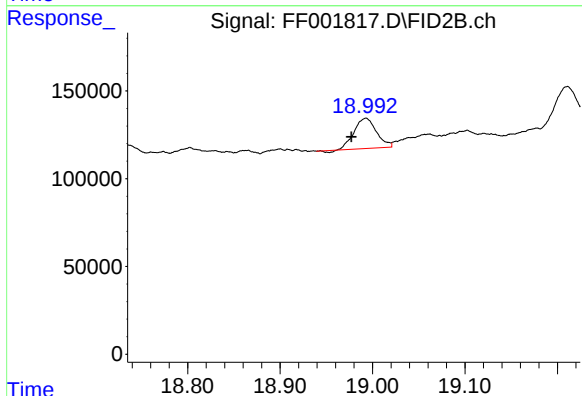


#15 N-TETRATRIACONTANE

R.T.: 18.993 min
Delta R.T.: 0.016 min
Response: 288834
Conc: 2.39 ug/ml

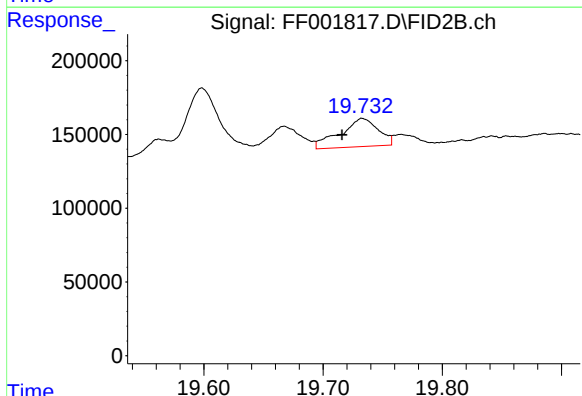

#16 N-HEXATRIACONTANE

R.T.: 19.733 min
Delta R.T.: 0.017 min
Response: 424378
Conc: 3.81 ug/ml

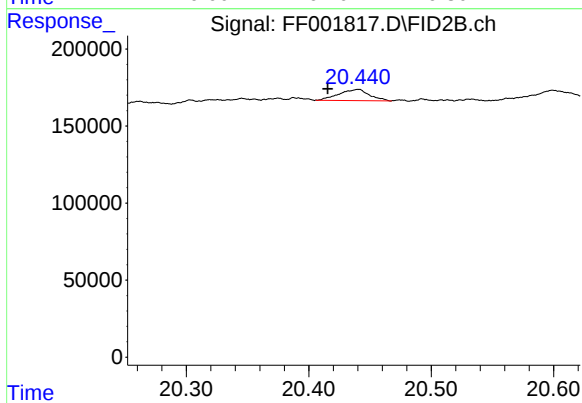

#17 N-OCTATRIACONTANE

R.T.: 20.440 min
Delta R.T.: 0.025 min
Response: 125510
Conc: 1.26 ug/ml