

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF081018\
 Data File : FF001818.D
 Signal(s) : FID2B.ch
 Acq On : 11 Aug 2018 14:17
 Operator : AJ\SJ
 Sample : J4409-05 10X
 Misc :
 ALS Vial : 86 Sample Multiplier: 1

Instrument :
 FID_F
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Aug 13 01:18:36 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF073018.M
 Quant Title :
 QLast Update : Fri Aug 03 12:00:27 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.323	394243	3.121 ug/ml
Target Compounds			
7) N-EICOSANE	12.228	190678	1.279 ug/ml
8) N-DOCOSANE	13.439	388172	2.657 ug/ml
10) N-TETRACOSANE	14.497	2448388	17.163 ug/ml
12) N-OCTACOSANE	16.506	412565	2.942 ug/ml
13) N-TRIACONTANE	17.372	183319	1.324 ug/ml
14) N-DOTRIACONTANE	18.181	877149	6.724 ug/ml
16) N-HEXATRIACONTANE	19.731	386715	3.476 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF081018\
Data File : FF001818.D
Signal(s) : FID2B.ch
Acq On : 11 Aug 2018 14:17
Operator : AJ\SJ
Sample : J4409-05 10X
Misc :
ALS Vial : 86 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Aug 13 01:18:36 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF073018.M
Quant Title :
QLast Update : Fri Aug 03 12:00:27 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

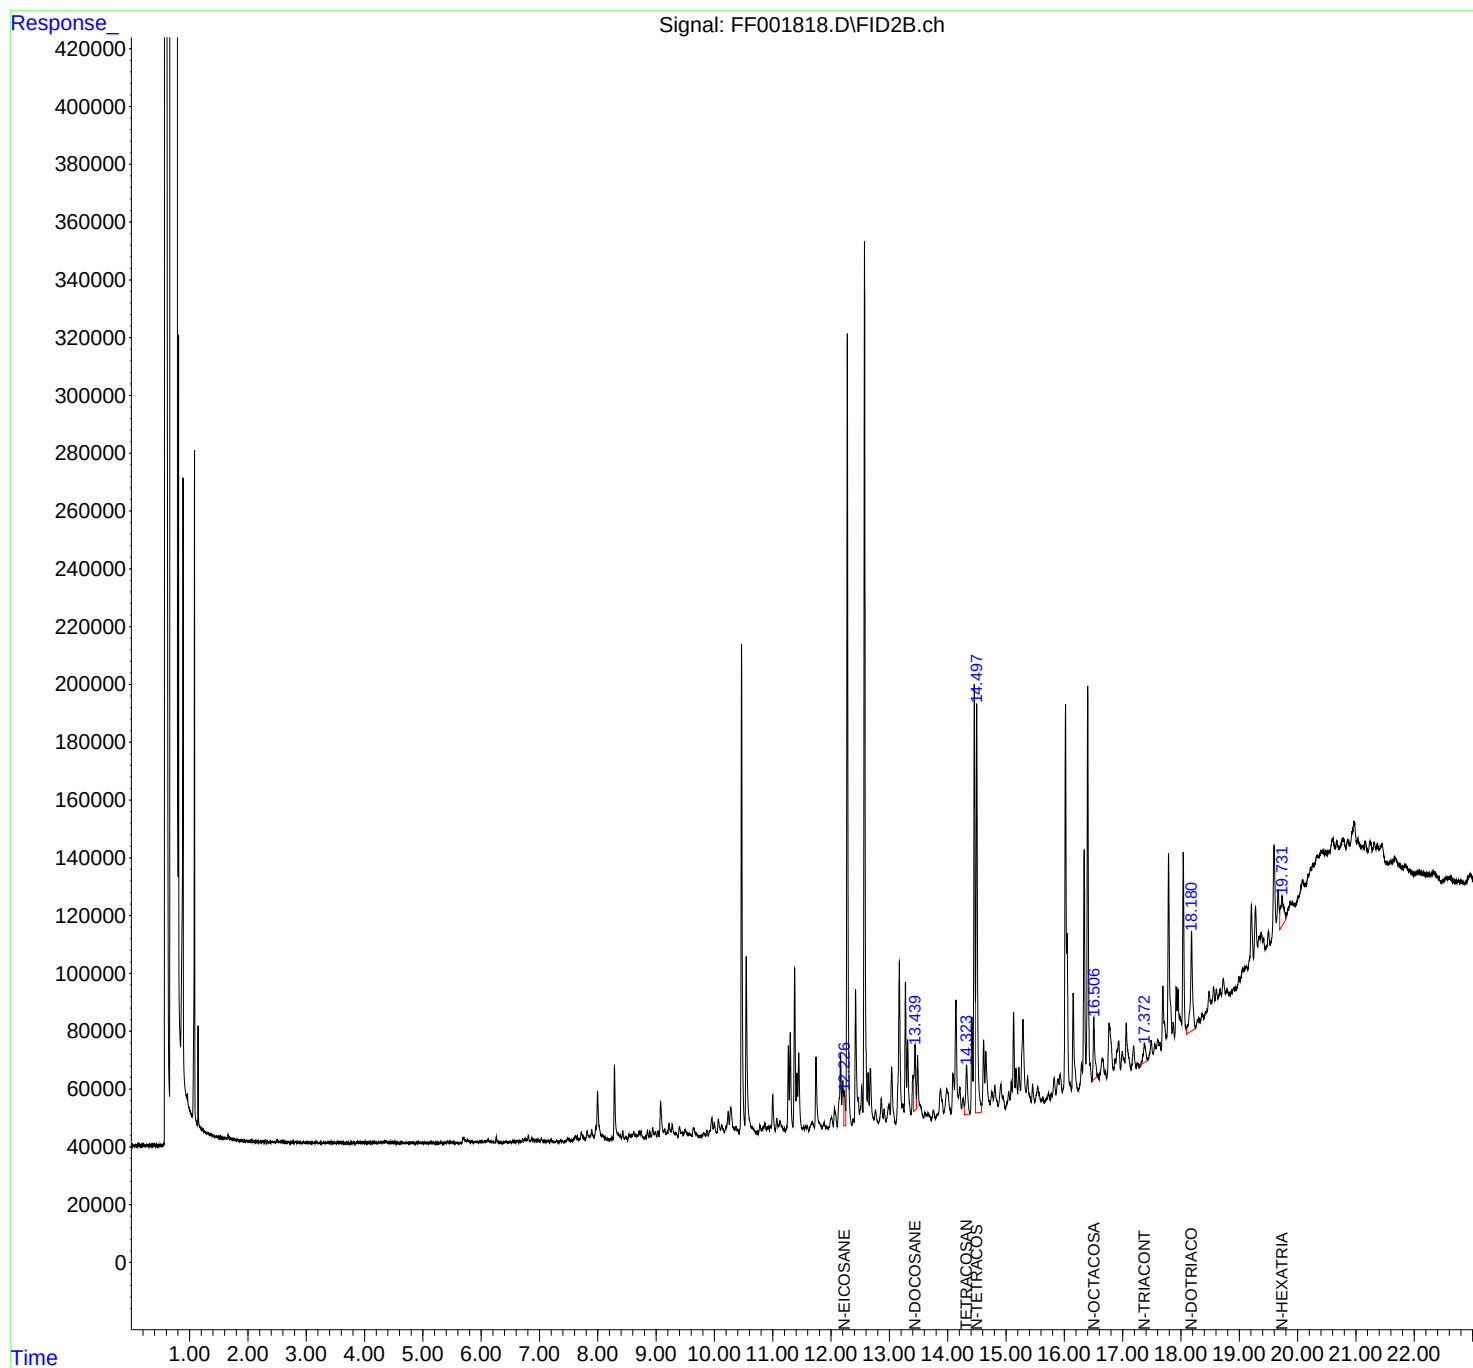


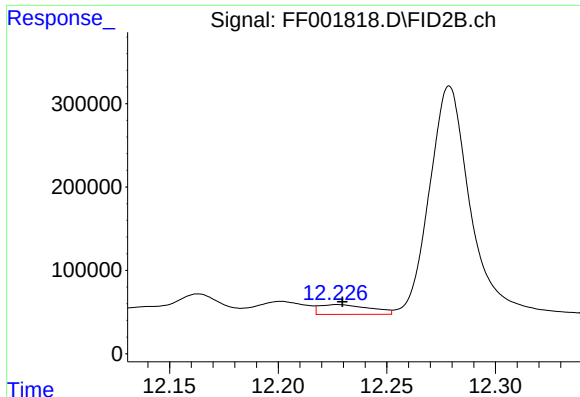

#7 N-EICOSANE


R.T.: 12.228 min
Delta R.T.: -0.002 min
Response: 190678
Conc: 1.28 ug/ml

Instrument :
FID_F
ClientSampleId :

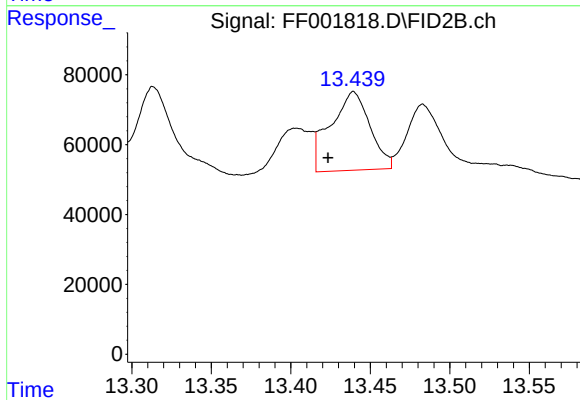


#8 N-DOCOSANE

R.T.: 13.439 min
Delta R.T.: 0.016 min
Response: 388172
Conc: 2.66 ug/ml

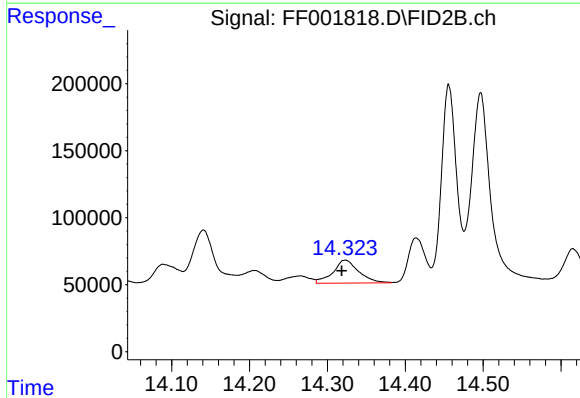


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.323 min
Delta R.T.: 0.004 min
Response: 394243
Conc: 3.12 ug/ml

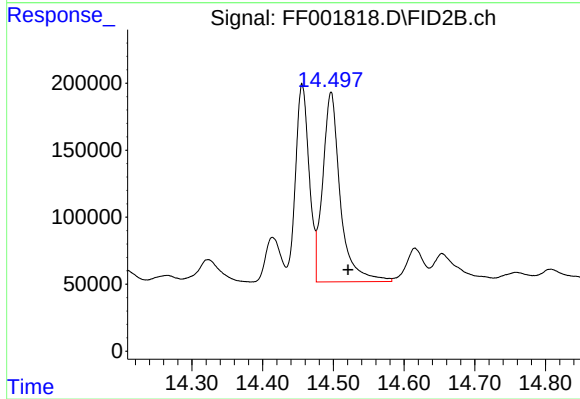

#10 N-TETRACOSANE


R.T.: 14.497 min
Delta R.T.: -0.024 min
Response: 2448388
Conc: 17.16 ug/ml

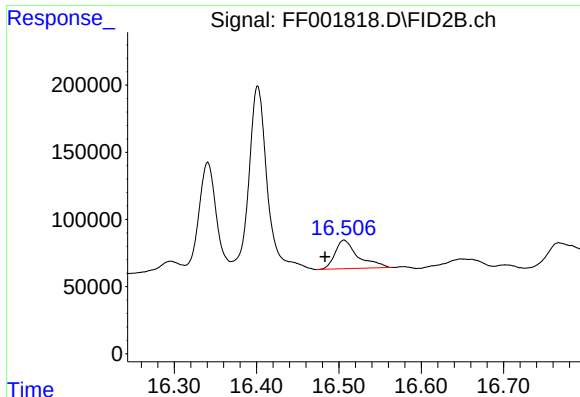

#12 N-OCTACOSANE


R.T.: 16.506 min
Delta R.T.: 0.023 min
Response: 412565
Conc: 2.94 ug/ml

Instrument :
FID_F
ClientSampleId :

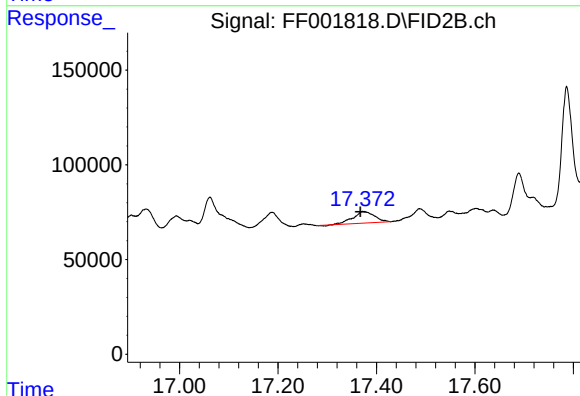


#13 N-TRIACONTANE

R.T.: 17.372 min
Delta R.T.: 0.005 min
Response: 183319
Conc: 1.32 ug/ml

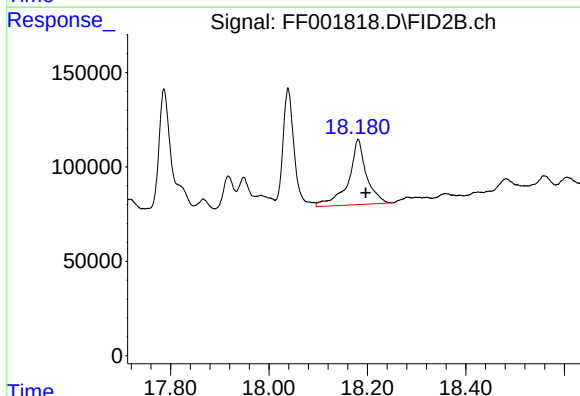

#14 N-DOTRIACONTANE

R.T.: 18.181 min
Delta R.T.: -0.015 min
Response: 877149
Conc: 6.72 ug/ml

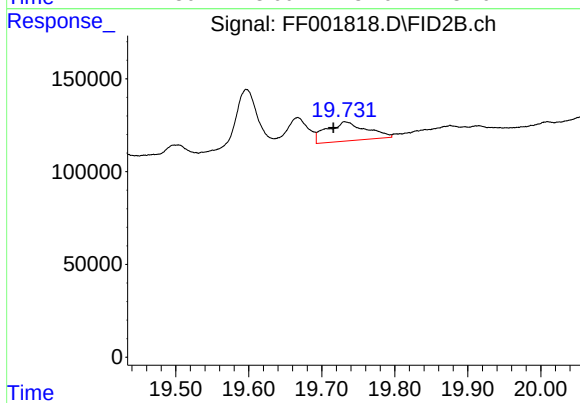

#16 N-HEXATRIACONTANE

R.T.: 19.731 min
Delta R.T.: 0.015 min
Response: 386715
Conc: 3.48 ug/ml