

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF081018\
 Data File : FF001819.D
 Signal(s) : FID2B.ch
 Acq On : 11 Aug 2018 14:47
 Operator : AJ\SJ
 Sample : J4409-07 20X
 Misc :
 ALS Vial : 87 Sample Multiplier: 1

Instrument :
 FID_F
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Aug 13 01:18:47 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF073018.M
 Quant Title :
 QLast Update : Fri Aug 03 12:00:27 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.330	350005	2.771 ug/ml
Target Compounds			
7) N-EICOSANE	12.227	264767	1.776 ug/ml
8) N-DOCOSANE	13.440	458393	3.138 ug/ml
10) N-TETRACOSANE	14.497	2784363	19.519 ug/ml
12) N-OCTACOSANE	16.506	566687	4.041 ug/ml
13) N-TRIACONTANE	17.378	205375	1.484 ug/ml
14) N-DOTRIACONTANE	18.181	1075402	8.243 ug/ml
16) N-HEXATRIACONTANE	19.732	337896	3.037 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF081018\
Data File : FF001819.D
Signal(s) : FID2B.ch
Acq On : 11 Aug 2018 14:47
Operator : AJ\SJ
Sample : J4409-07 20X
Misc :
ALS Vial : 87 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Aug 13 01:18:47 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF073018.M
Quant Title :
QLast Update : Fri Aug 03 12:00:27 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

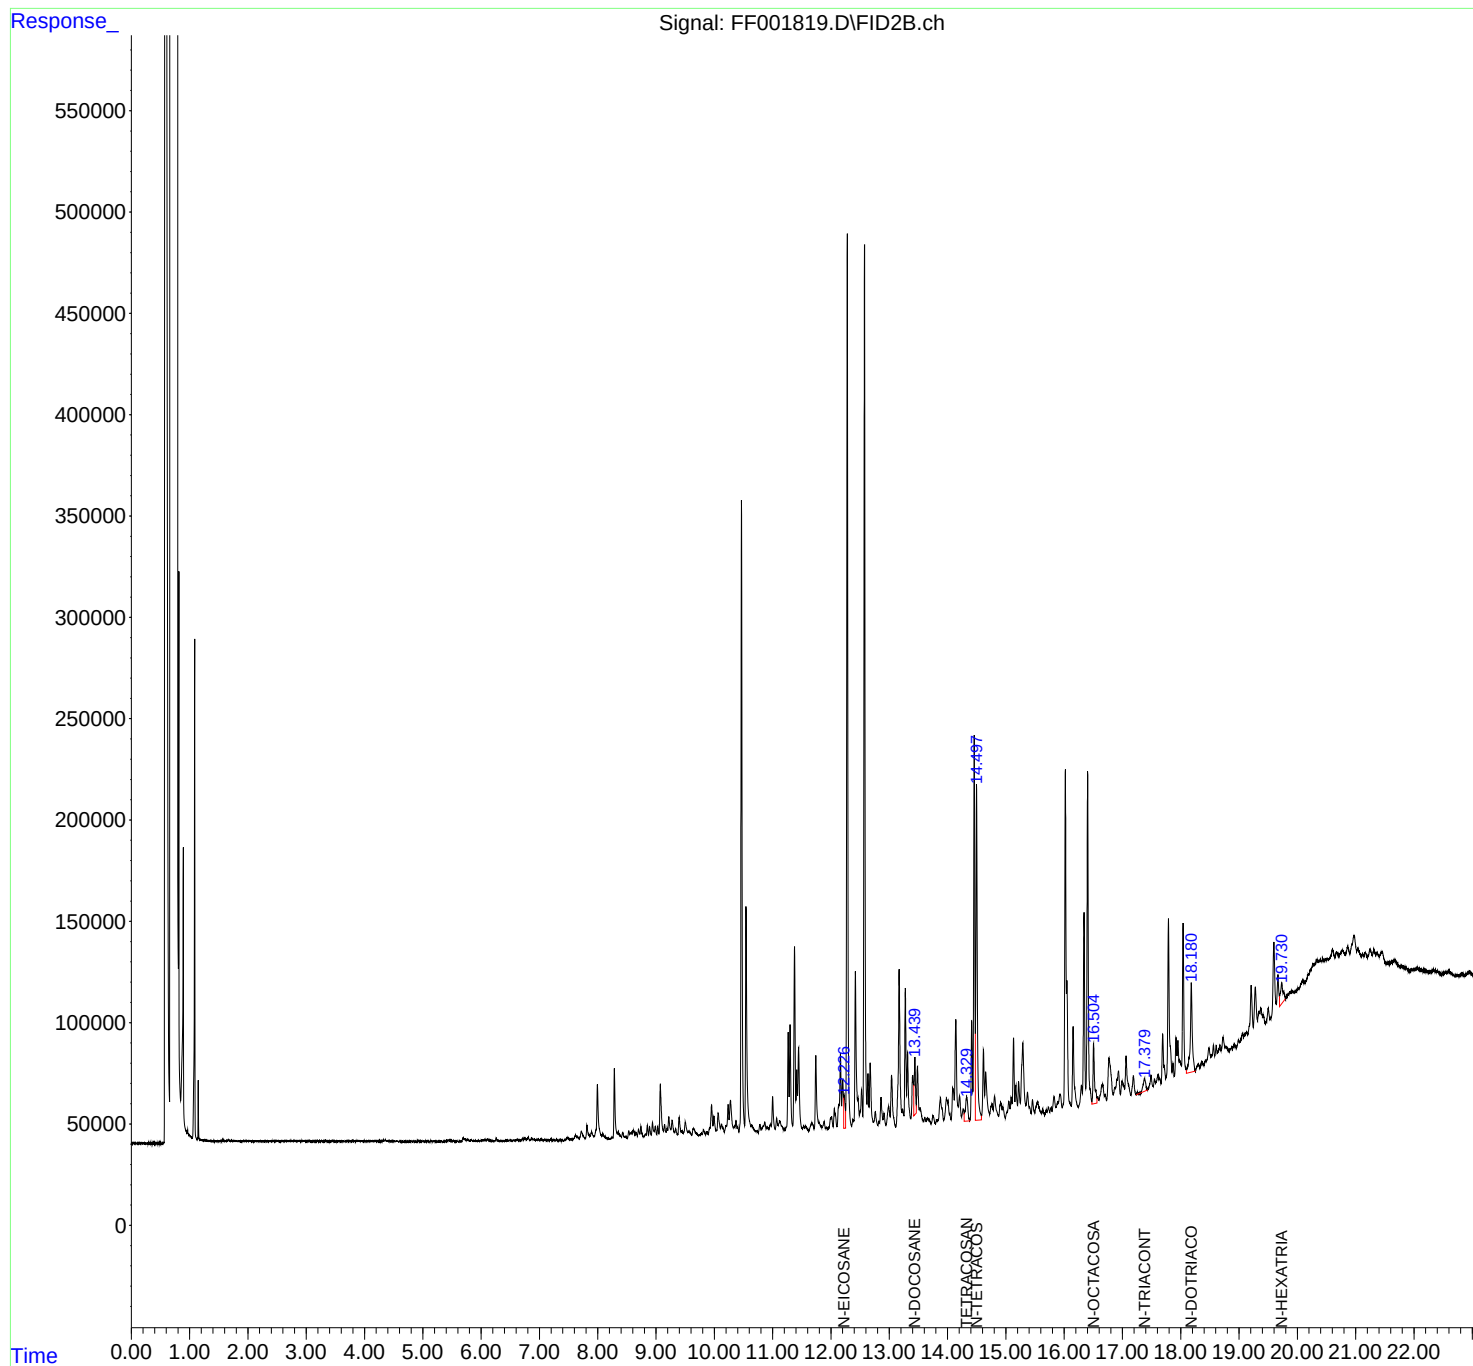


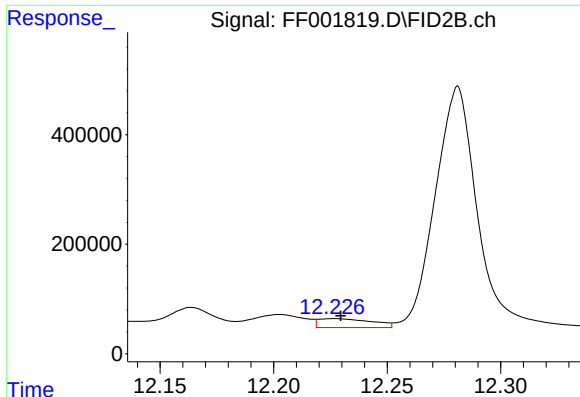

#7 N-EICOSANE


R.T.: 12.227 min
Delta R.T.: -0.003 min
Response: 264767
Conc: 1.78 ug/ml

Instrument :
FID_F
ClientSampleId :

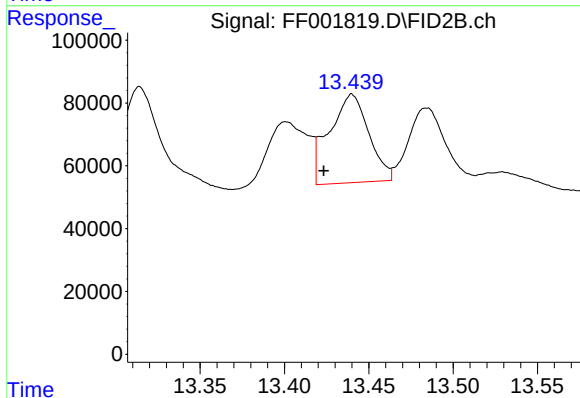


#8 N-DOCOSANE

R.T.: 13.440 min
Delta R.T.: 0.017 min
Response: 458393
Conc: 3.14 ug/ml

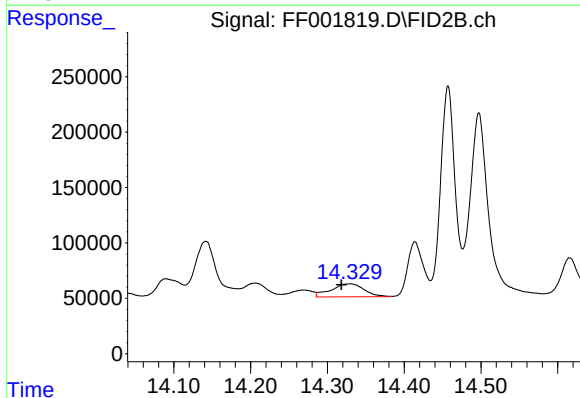


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.330 min
Delta R.T.: 0.011 min
Response: 350005
Conc: 2.77 ug/ml

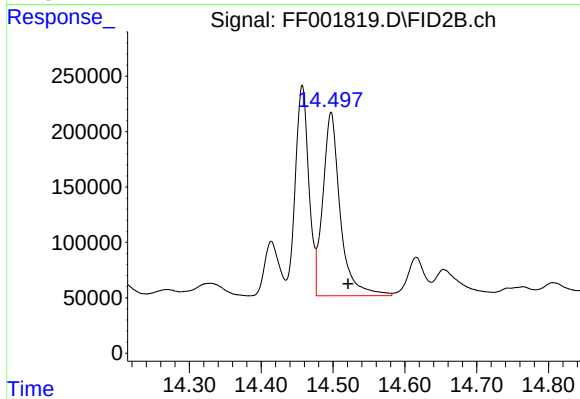

#10 N-TETRACOSANE


R.T.: 14.497 min
Delta R.T.: -0.024 min
Response: 2784363
Conc: 19.52 ug/ml

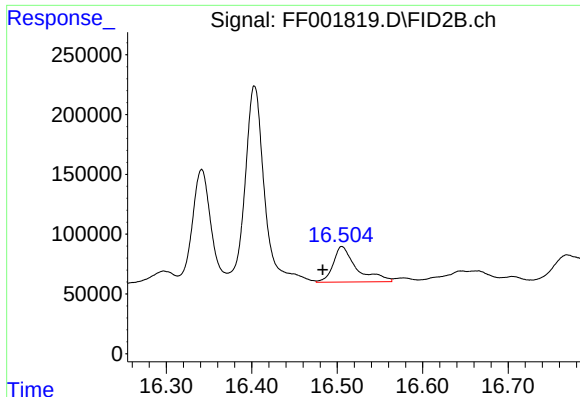

#12 N-OCTACOSANE


R.T.: 16.506 min
Delta R.T.: 0.023 min
Response: 566687
Conc: 4.04 ug/ml

Instrument :
FID_F
ClientSampleId :

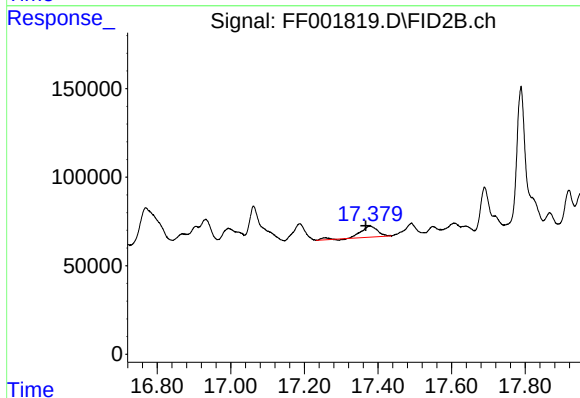


#13 N-TRIACONTANE

R.T.: 17.378 min
Delta R.T.: 0.011 min
Response: 205375
Conc: 1.48 ug/ml

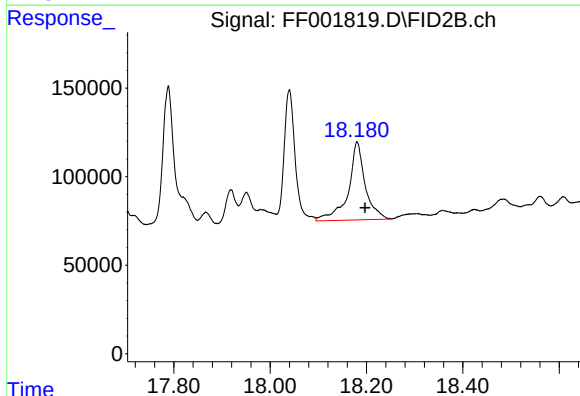

#14 N-DOTRIACONTANE

R.T.: 18.181 min
Delta R.T.: -0.016 min
Response: 1075402
Conc: 8.24 ug/ml

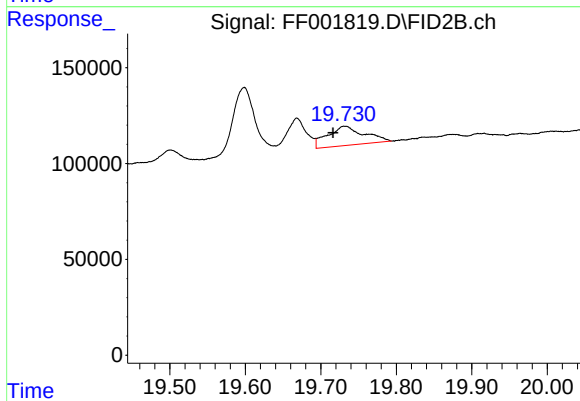

#16 N-HEXATRIACONTANE

R.T.: 19.732 min
Delta R.T.: 0.016 min
Response: 337896
Conc: 3.04 ug/ml