

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF081018\
 Data File : FF001820.D
 Signal(s) : FID2B.ch
 Acq On : 11 Aug 2018 15:18
 Operator : AJ\SJ
 Sample : J4409-09 2X
 Misc :
 ALS Vial : 88 Sample Multiplier: 1

Instrument :
 FID_F
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Aug 13 01:18:58 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF073018.M
 Quant Title :
 QLast Update : Fri Aug 03 12:00:27 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.323	1137033	9.003 ug/ml
Target Compounds			
4) N-TETRADECANE	7.961f	362357	2.404 ug/ml
7) N-EICOSANE	12.230	141276	0.948 ug/ml
8) N-DOCOSANE	13.439	434000	2.971 ug/ml
10) N-TETRACOSANE	14.497	2057627	14.424 ug/ml
11) N-HEXACOSANE	15.545	219959	1.561 ug/ml
12) N-OCTACOSANE	16.505	584476	4.168 ug/ml
13) N-TRIACONTANE	17.377	353537	2.554 ug/ml
14) N-DOTRIACONTANE	18.196	837039	6.416 ug/ml
15) N-TETRATRIACONTANE	18.991	106178	0.878 ug/ml
16) N-HEXATRIACONTANE	19.732	427053	3.838 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF081018\
Data File : FF001820.D
Signal(s) : FID2B.ch
Acq On : 11 Aug 2018 15:18
Operator : AJ\SJ
Sample : J4409-09 2X
Misc :
ALS Vial : 88 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Aug 13 01:18:58 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF073018.M
Quant Title :
QLast Update : Fri Aug 03 12:00:27 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

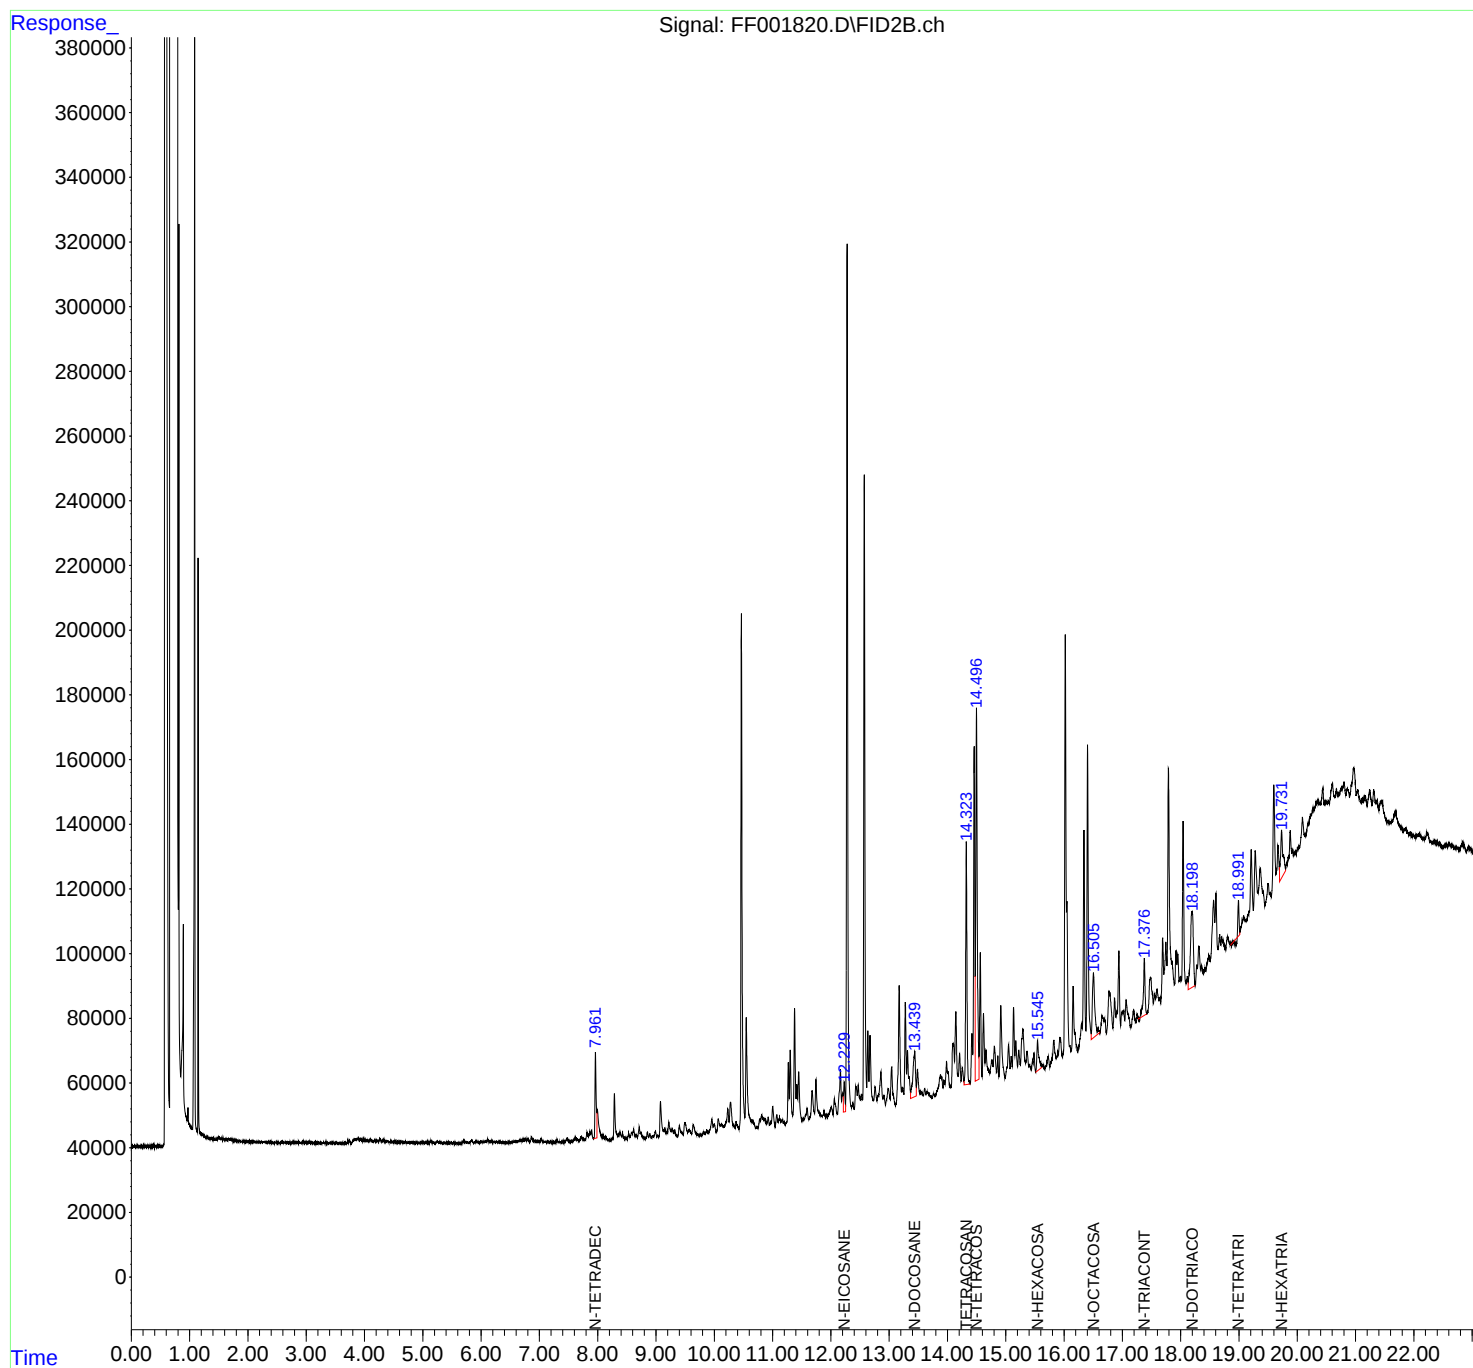


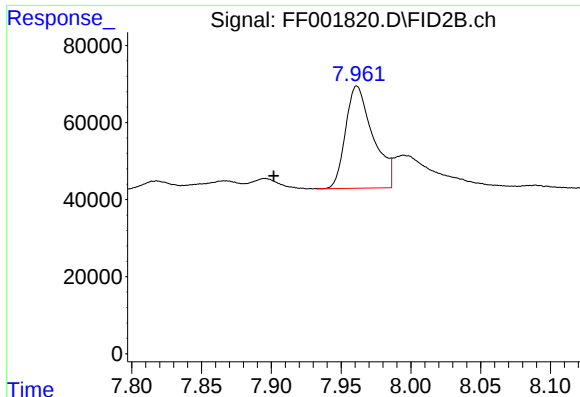

#4 N-TETRADECANE


R.T.: 7.961 min
Delta R.T.: 0.060 min
Response: 362357
Conc: 2.40 ug/ml

Instrument :
FID_F
ClientSampleId :

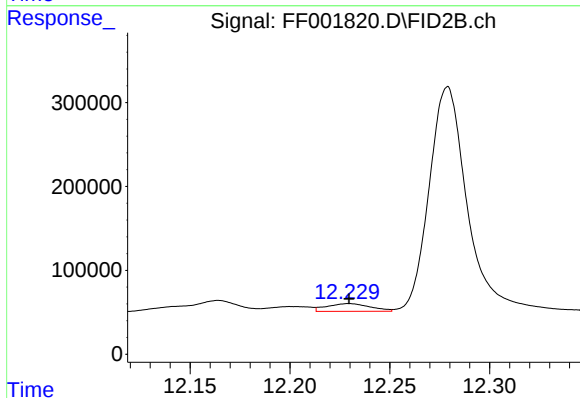


#7 N-EICOSANE

R.T.: 12.230 min
Delta R.T.: 0.000 min
Response: 141276
Conc: 0.95 ug/ml

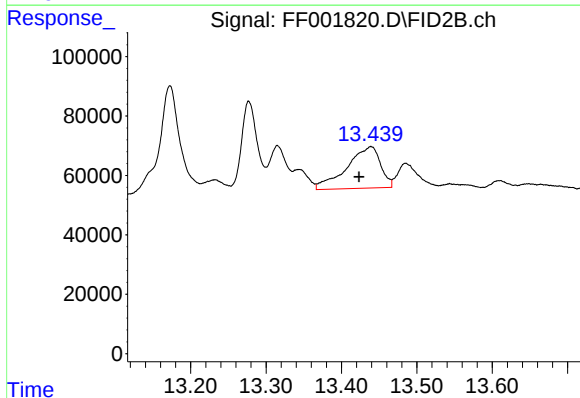


#8 N-DOCOSANE

R.T.: 13.439 min
Delta R.T.: 0.016 min
Response: 434000
Conc: 2.97 ug/ml

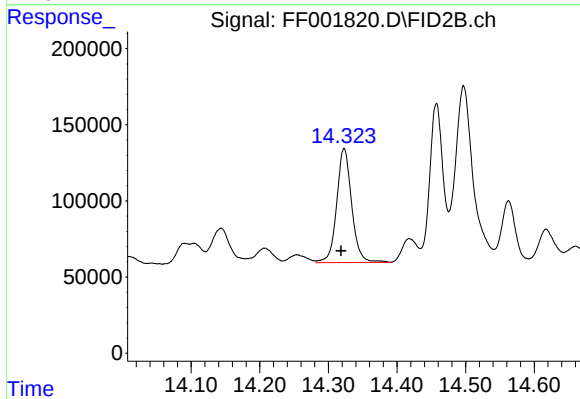

#9 TETRACOSANE-d50 (SURROGATE)


R.T.: 14.323 min
Delta R.T.: 0.005 min
Response: 1137033
Conc: 9.00 ug/ml

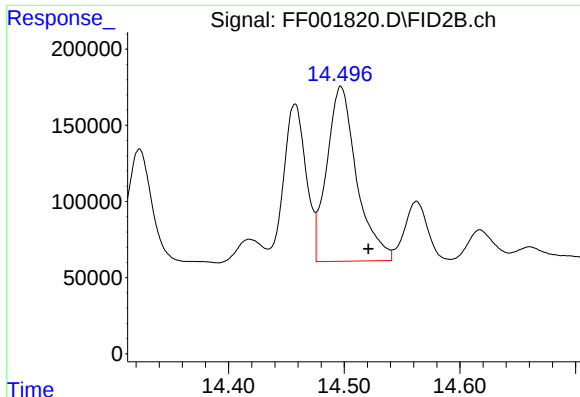

#10 N-TETRACOSANE


R.T.: 14.497 min
Delta R.T.: -0.024 min
Response: 2057627
Conc: 14.42 ug/ml

Instrument :
FID_F
ClientSampleId :

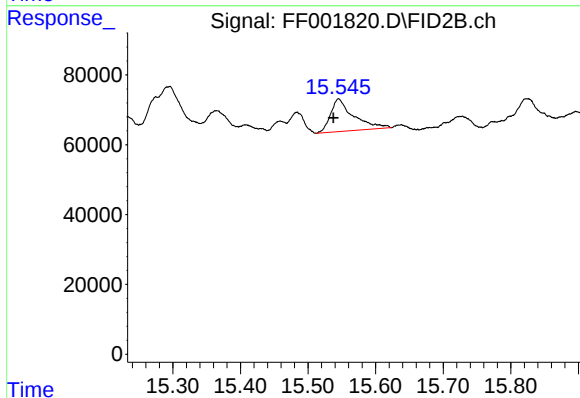


#11 N-HEXACOSANE

R.T.: 15.545 min
Delta R.T.: 0.008 min
Response: 219959
Conc: 1.56 ug/ml

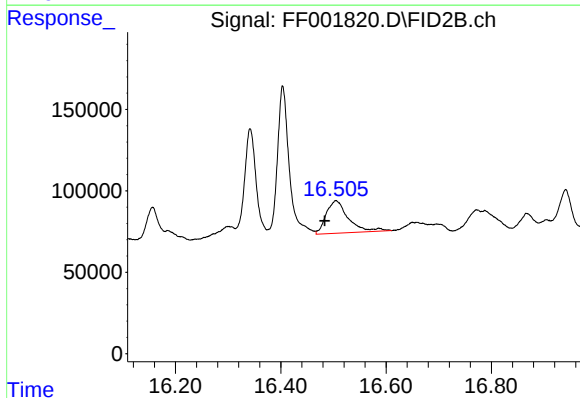


#12 N-OCTACOSANE

R.T.: 16.505 min
Delta R.T.: 0.022 min
Response: 584476
Conc: 4.17 ug/ml

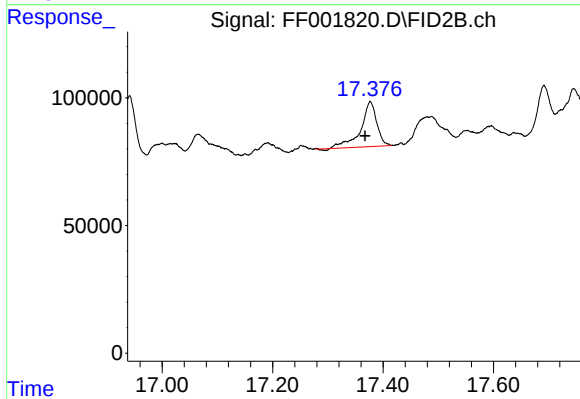

#13 N-TRIACONTANE


R.T.: 17.377 min
Delta R.T.: 0.010 min
Response: 353537
Conc: 2.55 ug/ml

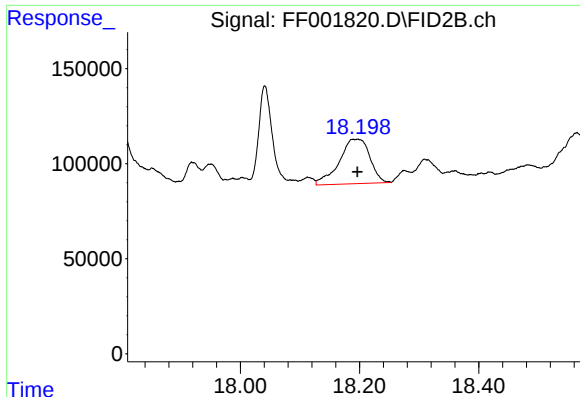

#14 N-DOTRIACONTANE


R.T.: 18.196 min
Delta R.T.: -0.001 min
Response: 837039
Conc: 6.42 ug/ml

Instrument :
FID_F
ClientSampleId :

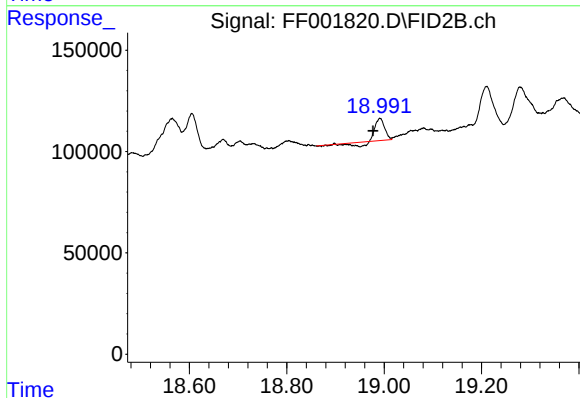

#15 N-TETRATRIACONTANE

R.T.: 18.991 min
Delta R.T.: 0.014 min
Response: 106178
Conc: 0.88 ug/ml

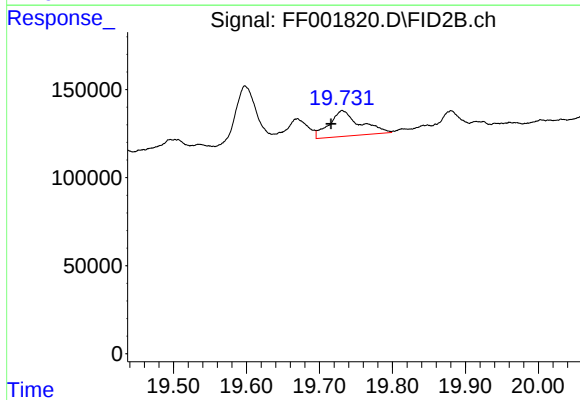

#16 N-HEXATRIACONTANE

R.T.: 19.732 min
Delta R.T.: 0.016 min
Response: 427053
Conc: 3.84 ug/ml