

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF081018\
 Data File : FF001822.D
 Signal(s) : FID2B.ch
 Acq On : 11 Aug 2018 16:19
 Operator : AJ\SJ
 Sample : I.BLK
 Misc :
 ALS Vial : 52 Sample Multiplier: 1

Instrument :
 FID_F
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Aug 13 01:19:22 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF073018.M
 Quant Title :
 QLast Update : Fri Aug 03 12:00:27 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.323	2327416	18.427 ug/ml
Target Compounds			
10) N-TETRACOSANE	14.485	421188	2.953 ug/ml
13) N-TRIACONTANE	17.376	111086	0.802 ug/ml
14) N-DOTRIACONTANE	18.206	203874	1.563 ug/ml
15) N-TETRATRIACONTANE	18.989	141808	1.173 ug/ml
16) N-HEXATRIACONTANE	19.731	267430	2.404 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF081018\
Data File : FF001822.D
Signal(s) : FID2B.ch
Acq On : 11 Aug 2018 16:19
Operator : AJ\SJ
Sample : I.BLK
Misc :
ALS Vial : 52 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Aug 13 01:19:22 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF073018.M
Quant Title :
QLast Update : Fri Aug 03 12:00:27 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

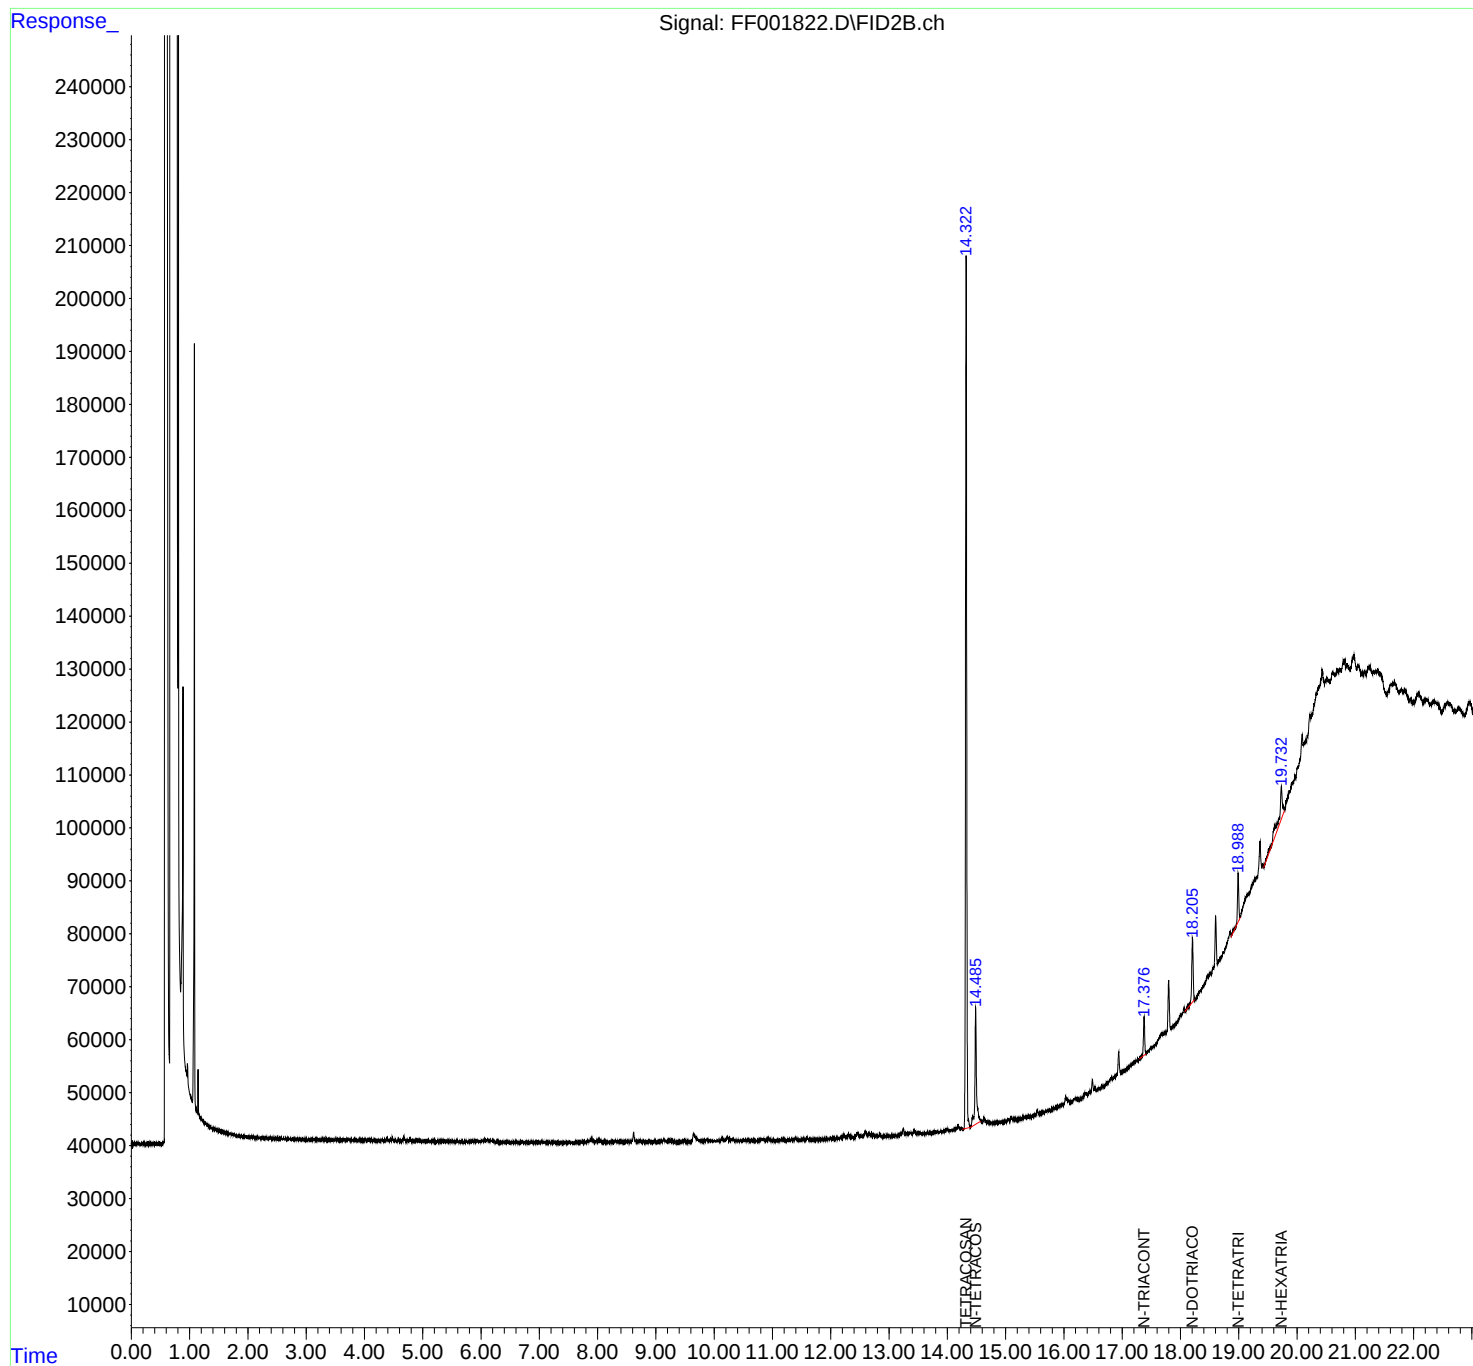


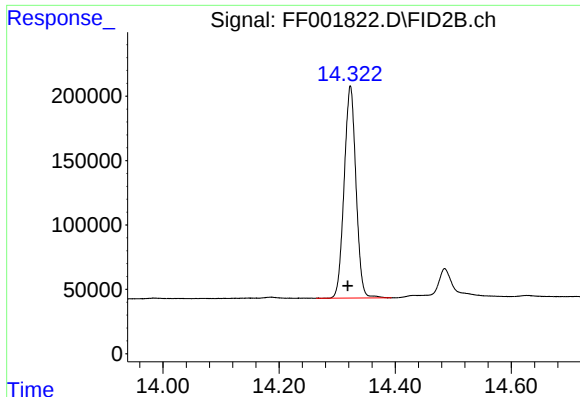

#9 TETRACOSANE-d50 (SURROGATE)


R.T.: 14.323 min
Delta R.T.: 0.005 min
Response: 2327416
Conc: 18.43 ug/ml

Instrument :
FID_F
ClientSampleId :

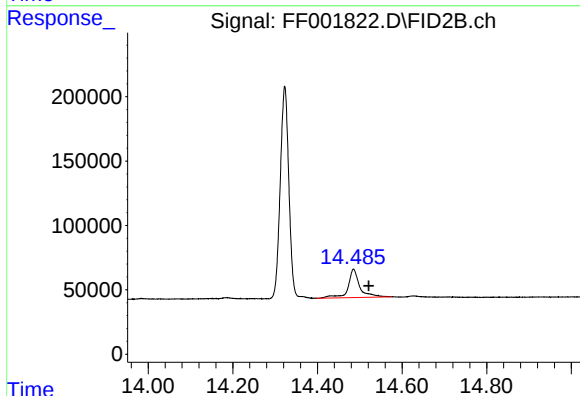


#10 N-TETRACOSANE

R.T.: 14.485 min
Delta R.T.: -0.036 min
Response: 421188
Conc: 2.95 ug/ml

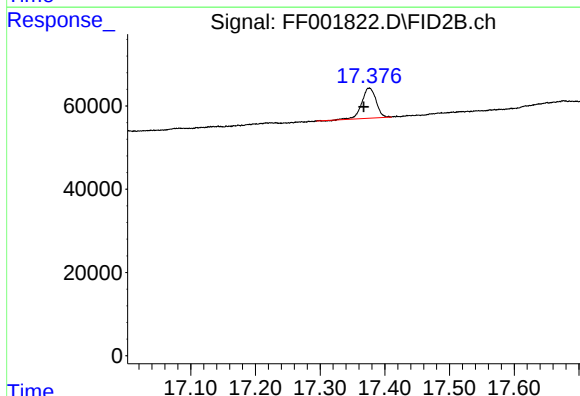


#13 N-TRIACONTANE

R.T.: 17.376 min
Delta R.T.: 0.009 min
Response: 111086
Conc: 0.80 ug/ml

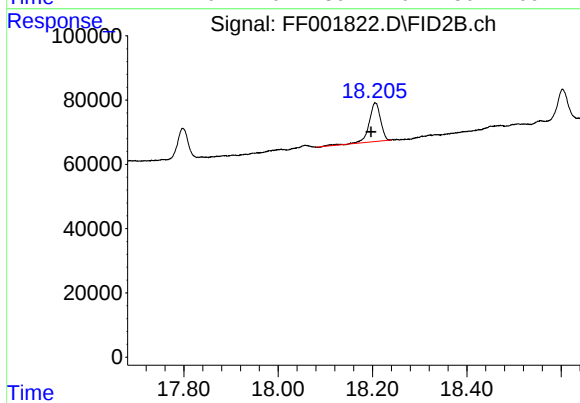

#14 N-DOTRIACONTANE


R.T.: 18.206 min
Delta R.T.: 0.009 min
Response: 203874
Conc: 1.56 ug/ml

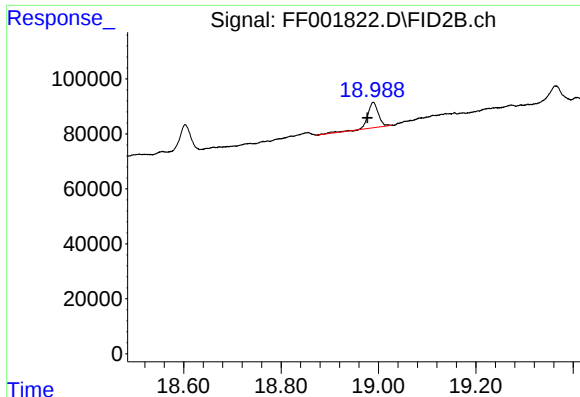

#15 N-TETRATRIACONTANE

R.T.: 18.989 min
Delta R.T.: 0.012 min
Response: 141808
Conc: 1.17 ug/ml

Instrument :
FID_F
ClientSampleId :

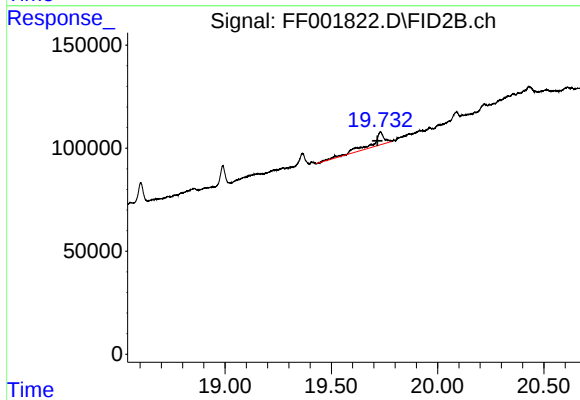

#16 N-HEXATRIACONTANE

R.T.: 19.731 min
Delta R.T.: 0.015 min
Response: 267430
Conc: 2.40 ug/ml