

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF081018\
 Data File : FF001785.D
 Signal(s) : FID2B.ch
 Acq On : 10 Aug 2018 13:39
 Operator : AJ\SJ
 Sample : PB111928BS
 Misc :
 ALS Vial : 59 Sample Multiplier: 1

Instrument :
 FID_F
 ClientSampleId :
 PB111928BS

Integration File: autoint1.e
 Quant Time: Aug 11 01:19:32 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF073018.M
 Quant Title :
 QLast Update : Fri Aug 03 12:00:27 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.323	2740627	21.699 ug/ml
Target Compounds			
2) N-DECANE	4.104	3268618	22.413 ug/ml
3) N-DODECANE	6.112	3368292	22.596 ug/ml
4) N-TETRADECANE	7.897	3475812	23.062 ug/ml
5) N-HEXADECANE	9.490	3437487	22.962 ug/ml
6) N-OCTADECANE	10.926	3401656	22.569 ug/ml
7) N-EICOSANE	12.232	3332952	22.362 ug/ml
8) N-DOCOSANE	13.425	3245897	22.222 ug/ml
10) N-TETRACOSANE	14.526	3326791	23.321 ug/ml
11) N-HEXACOSANE	15.543	2986109	21.199 ug/ml
12) N-OCTACOSANE	16.492	2902635	20.701 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF081018\
Data File : FF001785.D
Signal(s) : FID2B.ch
Acq On : 10 Aug 2018 13:39
Operator : AJ\SJ
Sample : PB111928BS
Misc :
ALS Vial : 59 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :
PB111928BS

Integration File: autoint1.e
Quant Time: Aug 11 01:19:32 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF073018.M
Quant Title :
QLast Update : Fri Aug 03 12:00:27 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

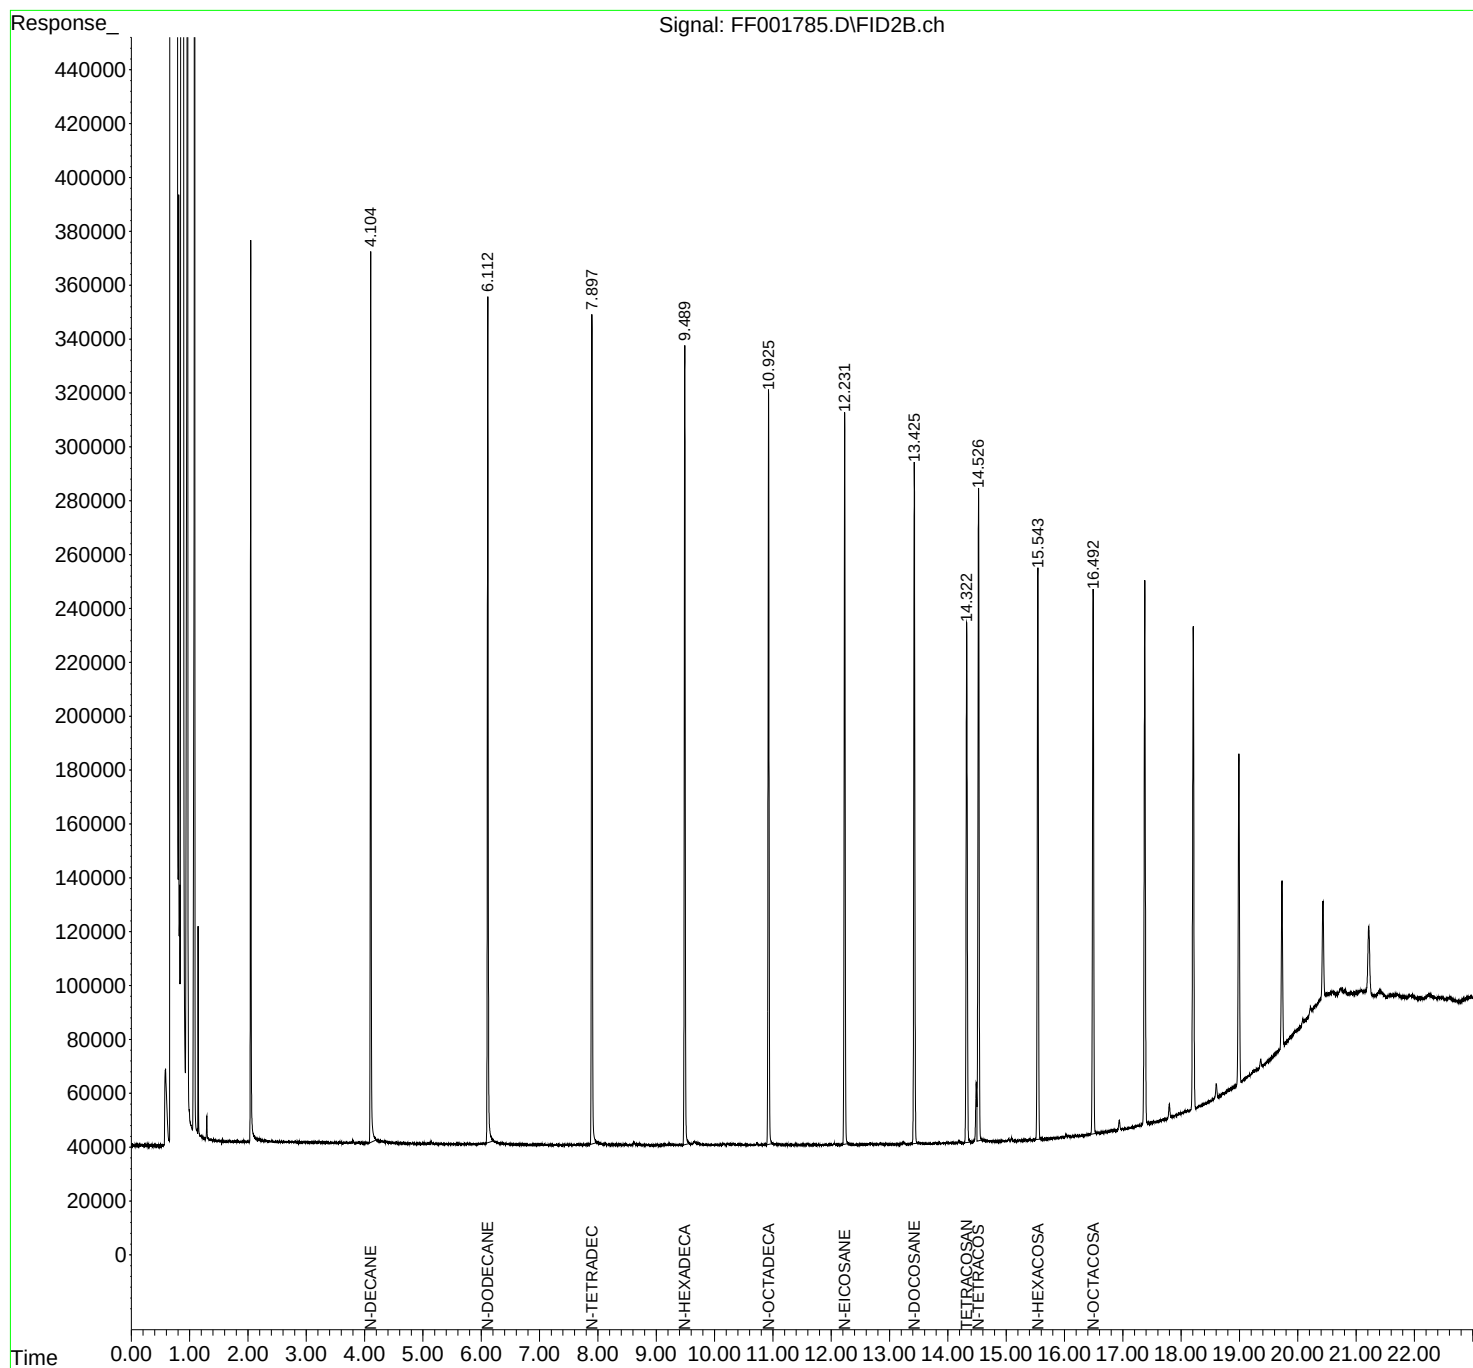


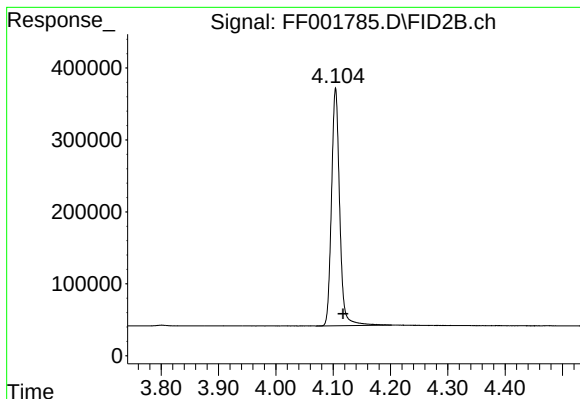

#2 N-DECANE


R.T.: 4.104 min
Delta R.T.: -0.013 min
Response: 3268618
Conc: 22.41 ug/ml

Instrument :
FID_F
ClientSampleId :
PB111928BS

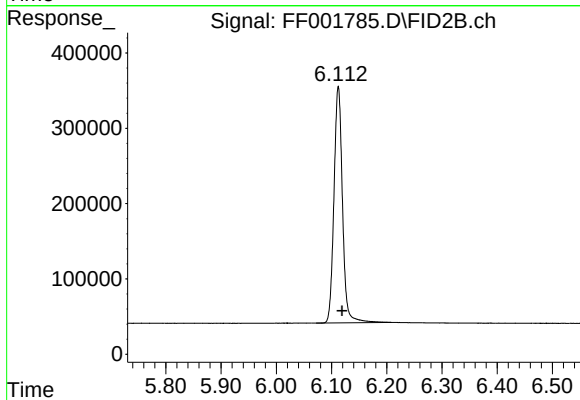


#3 N-DODECANE

R.T.: 6.112 min
Delta R.T.: -0.007 min
Response: 3368292
Conc: 22.60 ug/ml

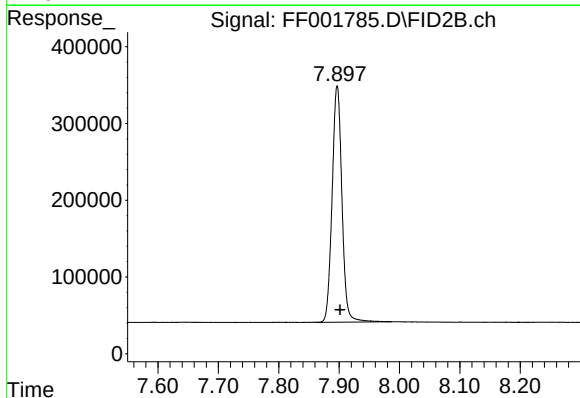


#4 N-TETRADECANE

R.T.: 7.897 min
Delta R.T.: -0.005 min
Response: 3475812
Conc: 23.06 ug/ml

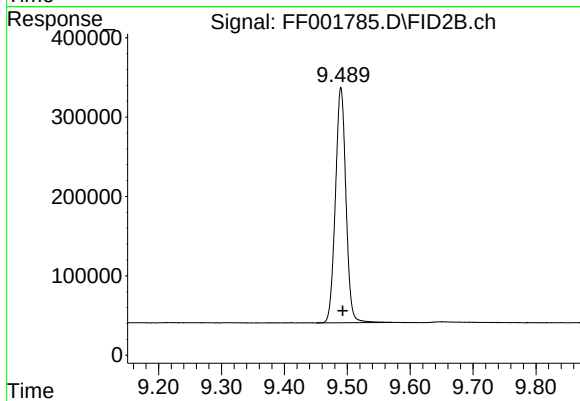

#5 N-HEXADECANE


R.T.: 9.490 min
Delta R.T.: -0.003 min
Response: 3437487
Conc: 22.96 ug/ml

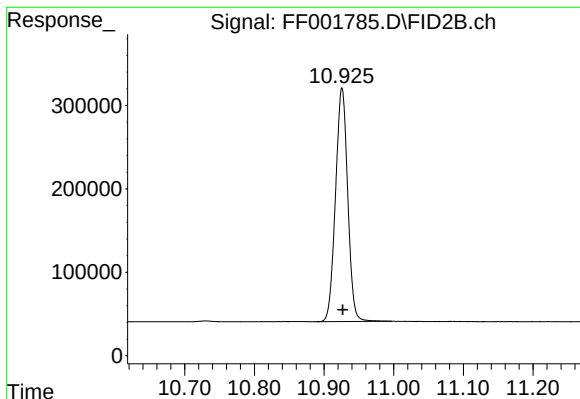

#6 N-OCTADECANE


R.T.: 10.926 min
Delta R.T.: 0.000 min
Response: 3401656
Conc: 22.57 ug/ml

Instrument :
FID_F
ClientSampleId :
PB111928BS

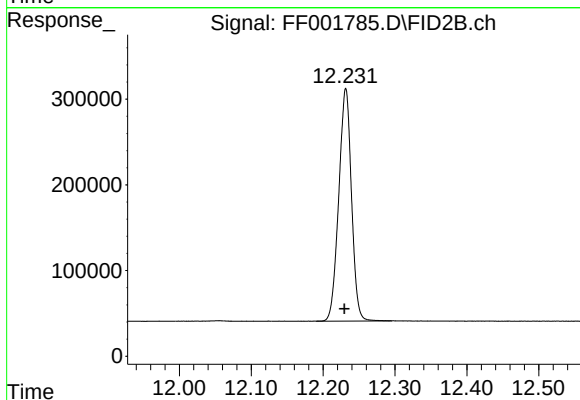


#7 N-EICOSANE

R.T.: 12.232 min
Delta R.T.: 0.002 min
Response: 3332952
Conc: 22.36 ug/ml

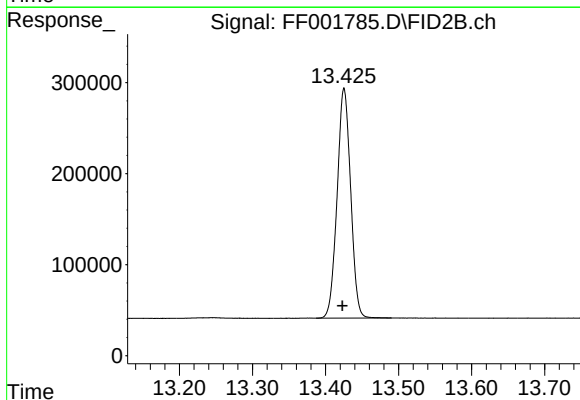


#8 N-DOCOSANE

R.T.: 13.425 min
Delta R.T.: 0.002 min
Response: 3245897
Conc: 22.22 ug/ml

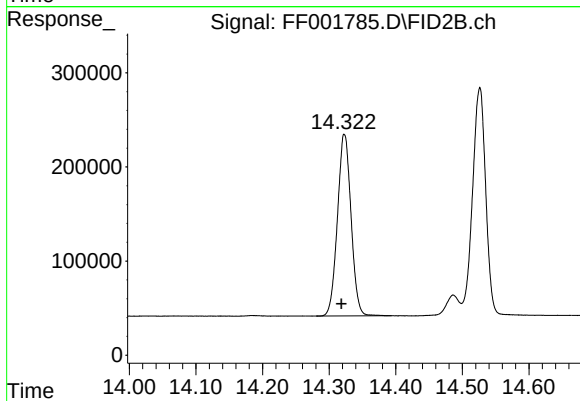

#9 TETRACOSANE-d50 (SURROGATE)


R.T.: 14.323 min
Delta R.T.: 0.004 min
Response: 2740627
Conc: 21.70 ug/ml

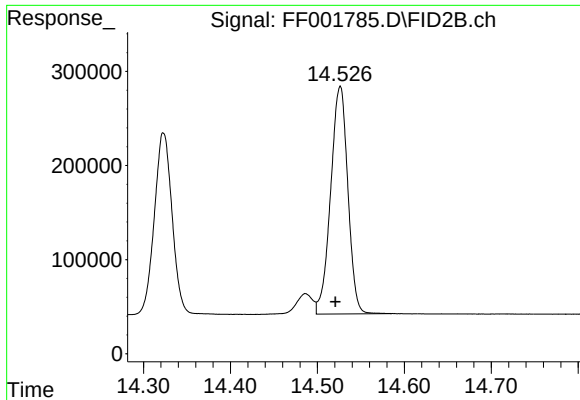

#10 N-TETRACOSANE


R.T.: 14.526 min
Delta R.T.: 0.005 min
Response: 3326791
Conc: 23.32 ug/ml

Instrument :
FID_F
ClientSampleId :
PB111928BS

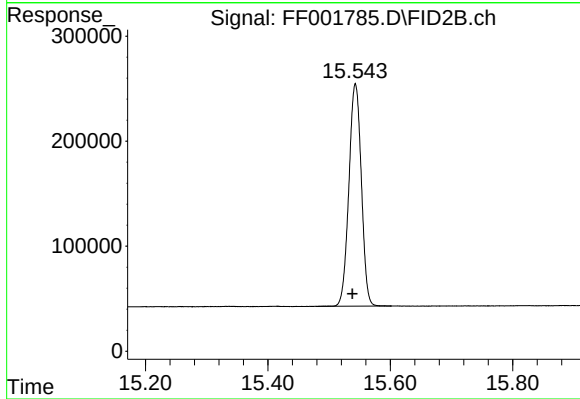

#11 N-HEXACOSANE

R.T.: 15.543 min
Delta R.T.: 0.005 min
Response: 2986109
Conc: 21.20 ug/ml

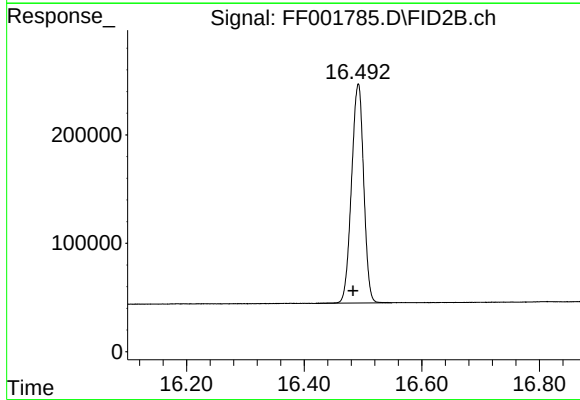

#12 N-OCTACOSANE

R.T.: 16.492 min
Delta R.T.: 0.009 min
Response: 2902635
Conc: 20.70 ug/ml