

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF081020\
 Data File : FF007312.D
 Signal(s) : FID2B.ch
 Acq On : 10 Aug 2020 13:04
 Operator : DD\AJ
 Sample : L3502-01RE
 Misc :
 ALS Vial : 55 Sample Multiplier: 1

Instrument :
 FID_F
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Aug 10 14:35:35 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF072820.M
 Quant Title :
 QLast Update : Wed Jul 29 09:33:32 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.755	546201	4.001 ug/ml
Target Compounds			
4) N-TETRADECANE	8.348f	212987	1.464 ug/ml
7) N-EICOSANE	12.648	230075	1.486 ug/ml
8) N-DOCOSANE	13.852	193111	1.237 ug/ml
10) N-TETRACOSANE	14.946	567109	3.591 ug/ml
11) N-HEXACOSANE	15.984	203117	1.296 ug/ml
12) N-OCTACOSANE	16.941	587390	3.743 ug/ml
13) N-TRIACONTANE	17.833	566408	3.612 ug/ml
14) N-DOTRIACONTANE	18.667	482238	3.255 ug/ml
15) N-TETRATRIACONTANE	19.459	1046258	8.651 ug/ml
16) N-HEXATRIACONTANE	20.204	2485441	26.870 ug/ml
17) N-OCTATRIACONTANE	20.966	1484673	20.902 ug/ml
18) N-TETRACONTANE	21.888	96481	1.443 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF081020\
Data File : FF007312.D
Signal(s) : FID2B.ch
Acq On : 10 Aug 2020 13:04
Operator : DD\AJ
Sample : L3502-01RE
Misc :
ALS Vial : 55 Sample Multiplier: 1

Instrument :
FID_F
ClientSampled :

Integration File: autoint1.e
Quant Time: Aug 10 14:35:35 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF072820.M
Quant Title :
QLast Update : Wed Jul 29 09:33:32 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

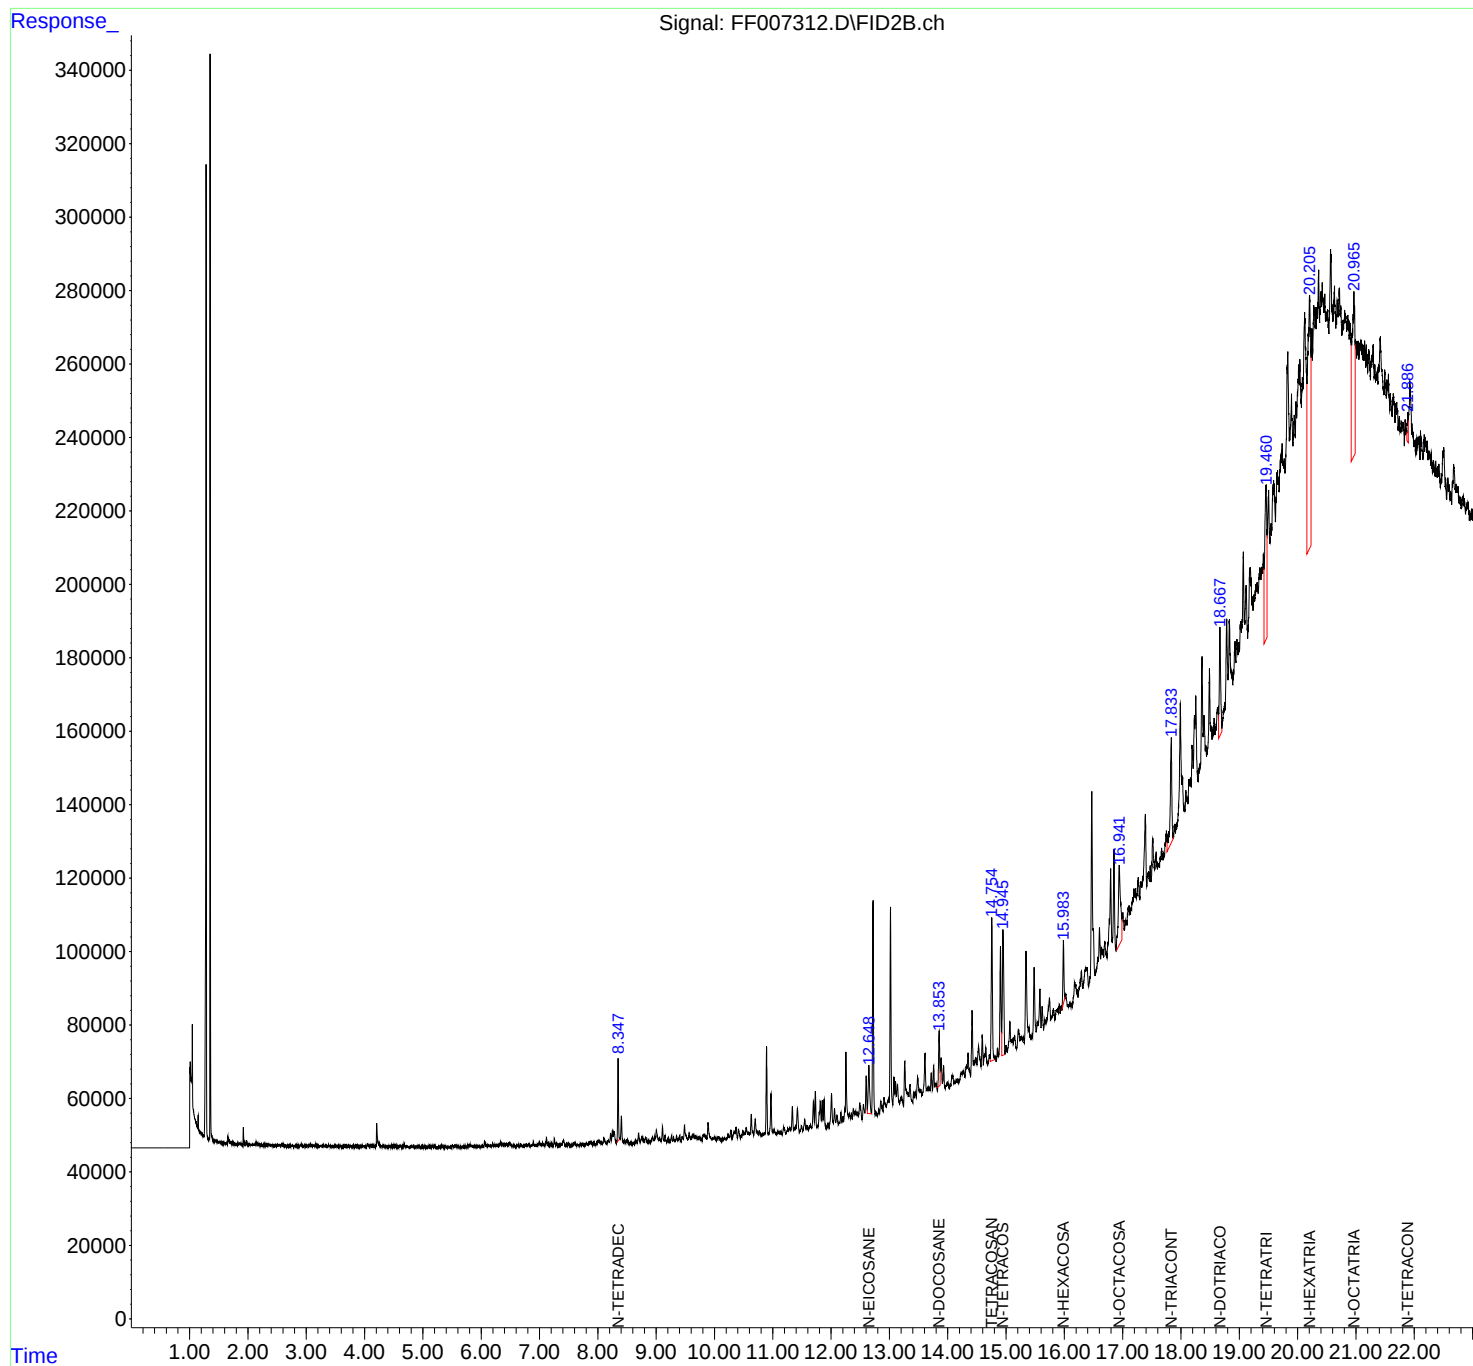


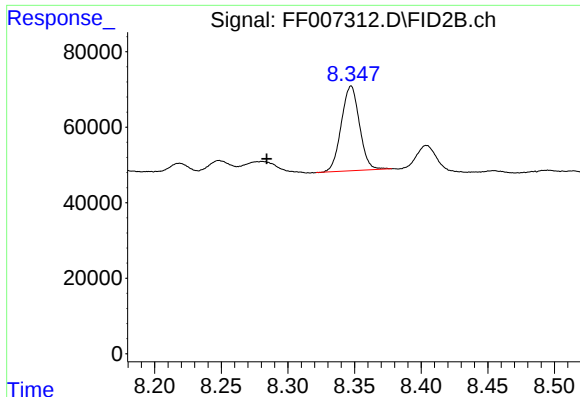

#4 N-TETRADECANE


R.T.: 8.348 min
Delta R.T.: 0.063 min
Response: 212987
Conc: 1.46 ug/ml

Instrument :
FID_F
ClientSampleId :

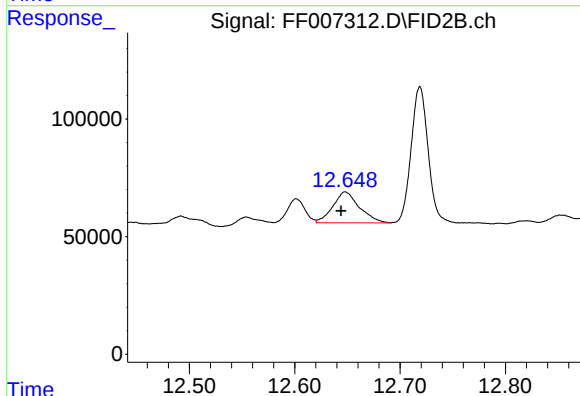


#7 N-EICOSANE

R.T.: 12.648 min
Delta R.T.: 0.004 min
Response: 230075
Conc: 1.49 ug/ml

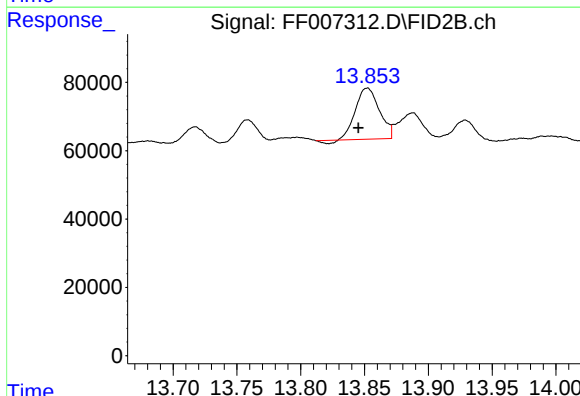


#8 N-DOCOSANE

R.T.: 13.852 min
Delta R.T.: 0.007 min
Response: 193111
Conc: 1.24 ug/ml

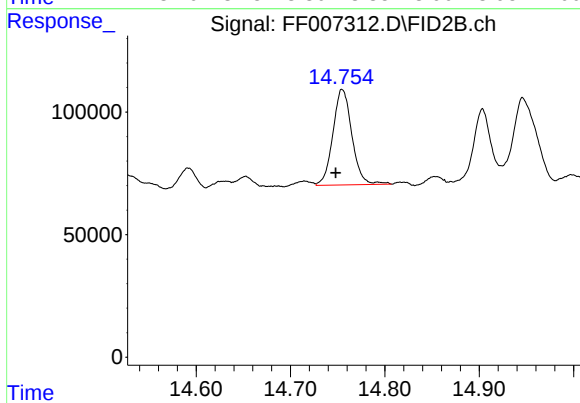

#9 TETRACOSANE-d50 (SURROGATE)


R.T.: 14.755 min
Delta R.T.: 0.007 min
Response: 546201
Conc: 4.00 ug/ml

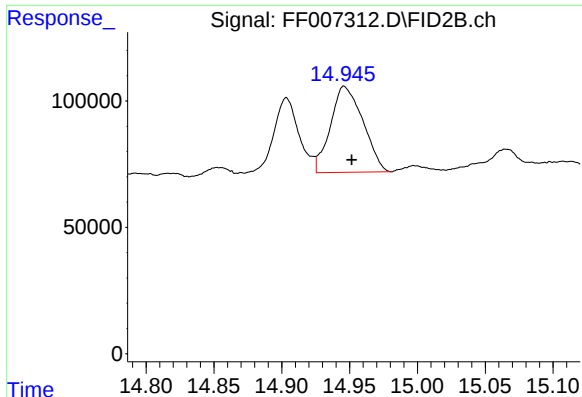

#10 N-TETRACOSANE


R.T.: 14.946 min
Delta R.T.: -0.005 min
Response: 567109
Conc: 3.59 ug/ml

Instrument :
FID_F
ClientSampleId :

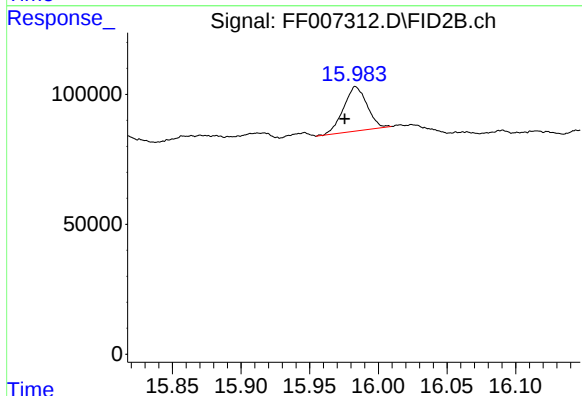


#11 N-HEXACOSANE

R.T.: 15.984 min
Delta R.T.: 0.008 min
Response: 203117
Conc: 1.30 ug/ml

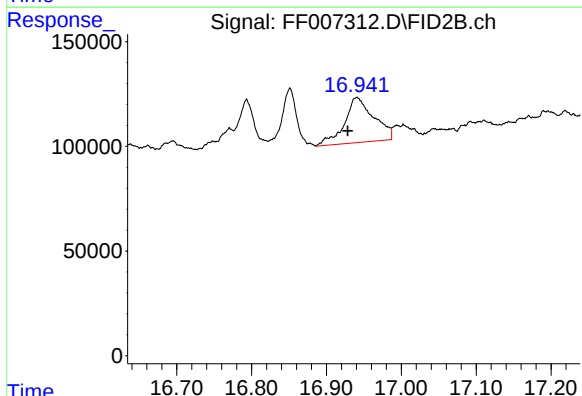


#12 N-OCTACOSANE

R.T.: 16.941 min
Delta R.T.: 0.013 min
Response: 587390
Conc: 3.74 ug/ml

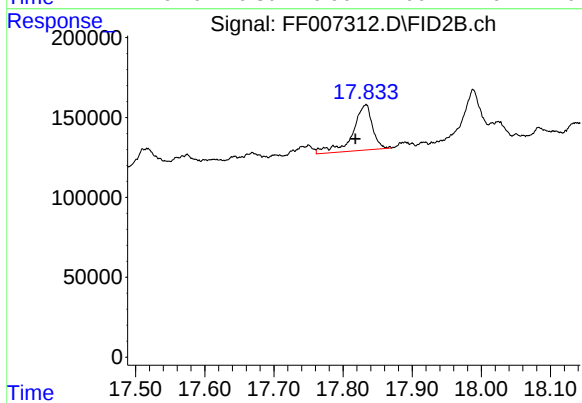

#13 N-TRIACONTANE


R.T.: 17.833 min
Delta R.T.: 0.015 min
Response: 566408
Conc: 3.61 ug/ml

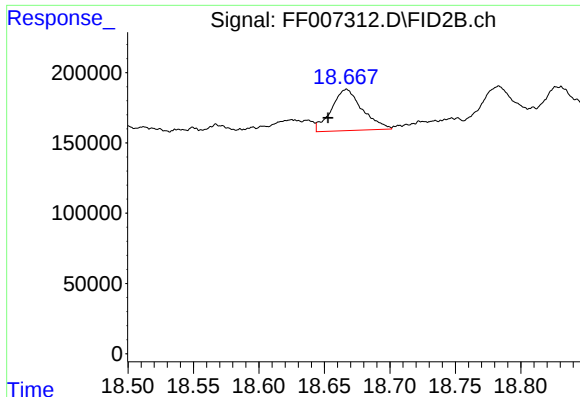

#14 N-DOTRIACONTANE


R.T.: 18.667 min
Delta R.T.: 0.014 min
Response: 482238
Conc: 3.25 ug/ml

Instrument :
FID_F
ClientSampleId :

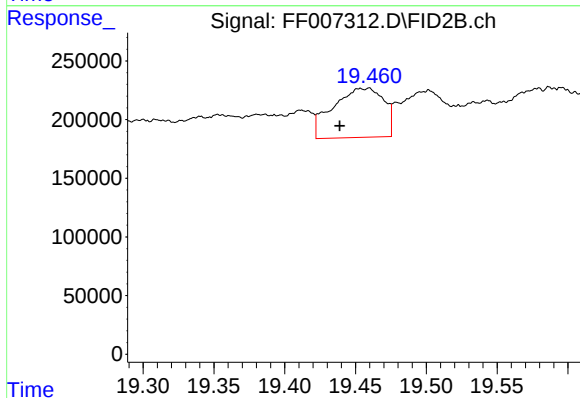


#15 N-TETRATRIACONTANE

R.T.: 19.459 min
Delta R.T.: 0.021 min
Response: 1046258
Conc: 8.65 ug/ml

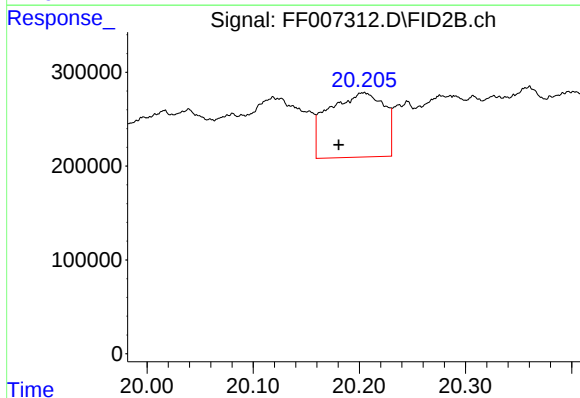


#16 N-HEXATRIACONTANE

R.T.: 20.204 min
Delta R.T.: 0.023 min
Response: 2485441
Conc: 26.87 ug/ml

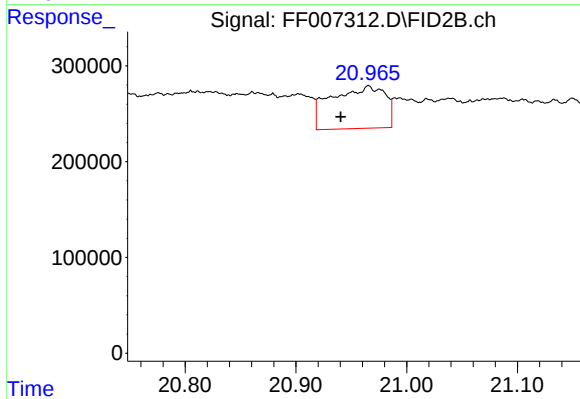

#17 N-OCTATRIACONTANE

R.T.: 20.966 min
Delta R.T.: 0.025 min
Response: 1484673
Conc: 20.90 ug/ml

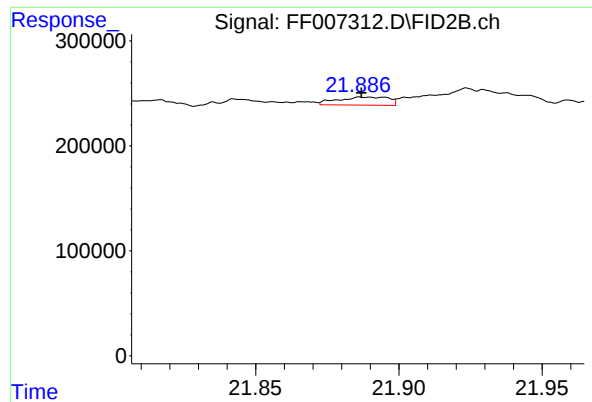

#18 N-TETRACONTANE

R.T.: 21.888 min
Delta R.T.: 0.000 min
Response: 96481
Conc: 1.44 ug/ml

Instrument :
FID_F
ClientSampleId :