

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB081018\
 Data File : FB017245.D
 Signal(s) : FID2B.CH
 Acq On : 10 Aug 2018 12:19
 Operator : MJ/SJ
 Sample : BSF0810S1
 Misc : 5.00g/5.00mL DI Water
 ALS Vial : 3 Sample Multiplier: 1

Integration File: Calibration.e
 Quant Time: Aug 13 08:11:23 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB072718.M
 Quant Title :
 QLast Update : Fri Jul 27 13:23:50 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	9.113	161034	20.348 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.965	410122	28.412 ng/ml
2) t 2,2,4-Trimethylpentane	7.729	414734	29.647 ng/ml
3) t n-Heptane	8.069	132622	9.431 ng/ml
4) t Benzene	8.208	168937	9.616 ng/ml
6) t Toluene	10.963	410867	29.919 ng/ml
7) t Ethylbenzene	13.413	136826	10.034 ng/ml
8) t m-Xylene	13.546	294428	20.464 ng/ml
9) t O-Xylene	14.277	306193	20.077 ng/ml
10) t 1,2,4-Trimethylbenzene	16.560	364569	19.752 ng/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB081018\
Data File : FB017245.D
Signal(s) : FID2B.CH
Acq On : 10 Aug 2018 12:19
Operator : MJ/SJ
Sample : BSF0810S1
Misc : 5.00g/5.00mL DI Water
ALS Vial : 3 Sample Multiplier: 1

Integration File: Calibration.e
Quant Time: Aug 13 08:11:23 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB072718.M
Quant Title :
QLast Update : Fri Jul 27 13:23:50 2018
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

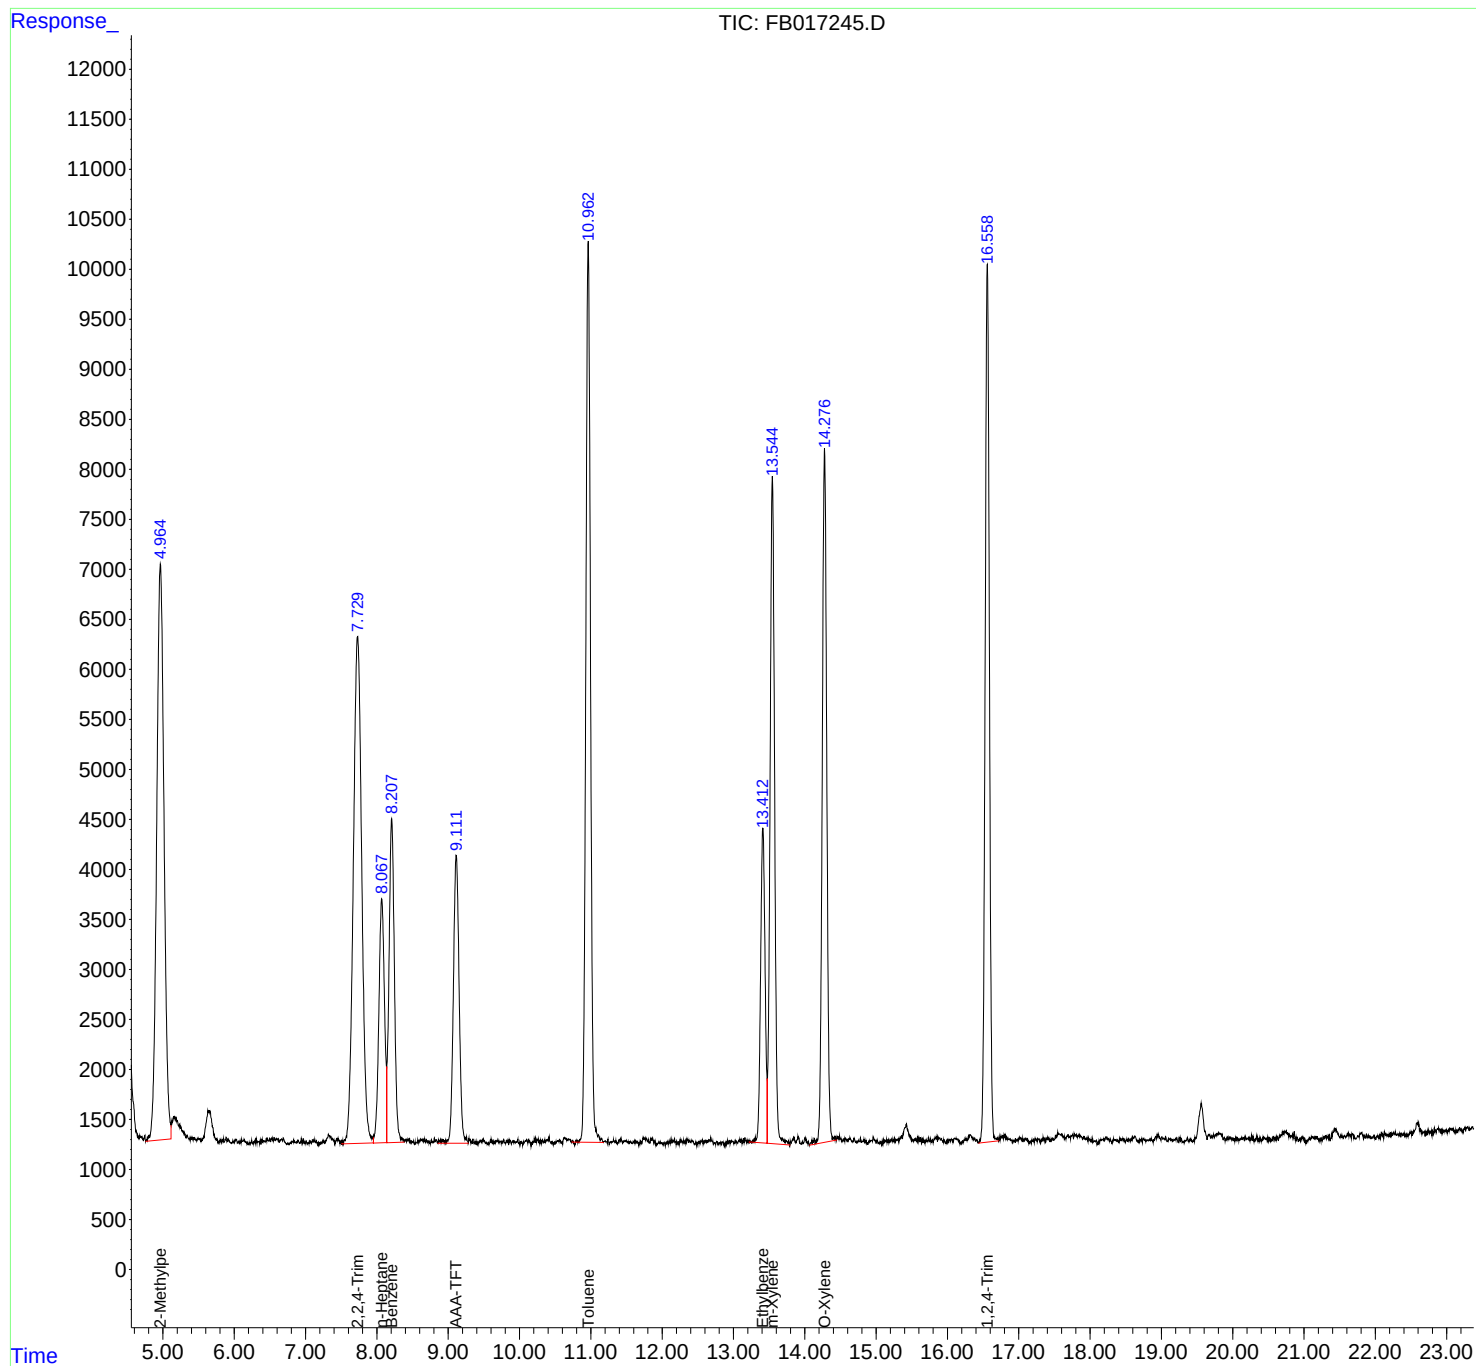

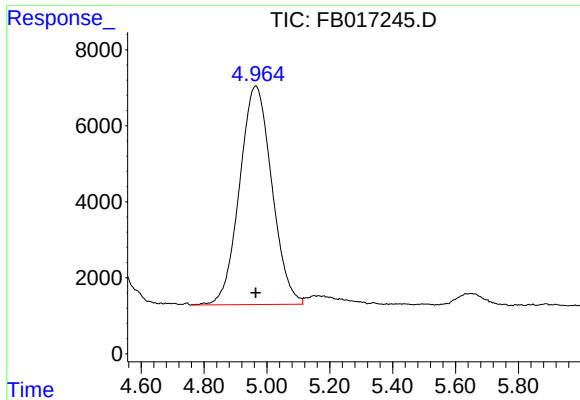


#1 2-Methylpentane

R.T.: 4.965 min
Delta R.T.: 0.001 min
Response: 410122
Conc: 28.41 ng/ml

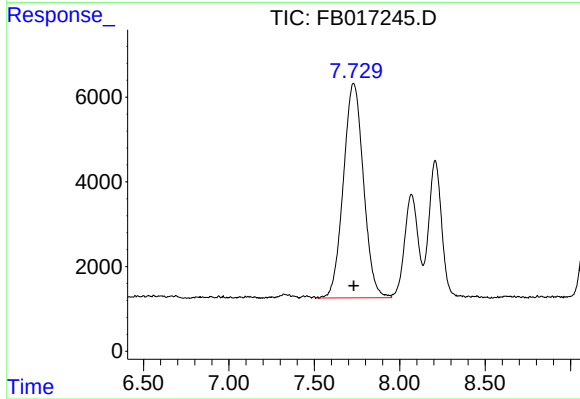


#2 2,2,4-Trimethylpentane

R.T.: 7.729 min
Delta R.T.: -0.001 min
Response: 414734
Conc: 29.65 ng/ml

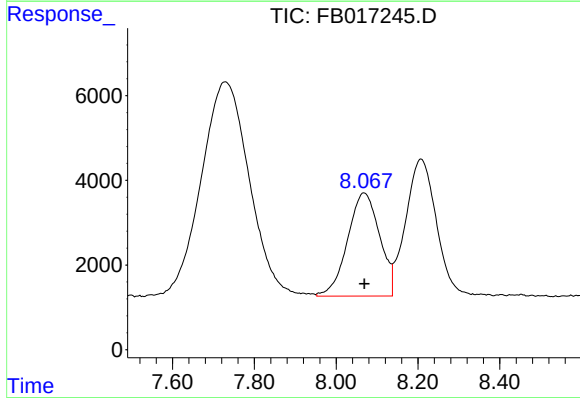


#3 n-Heptane

R.T.: 8.069 min
Delta R.T.: 0.000 min
Response: 132622
Conc: 9.43 ng/ml

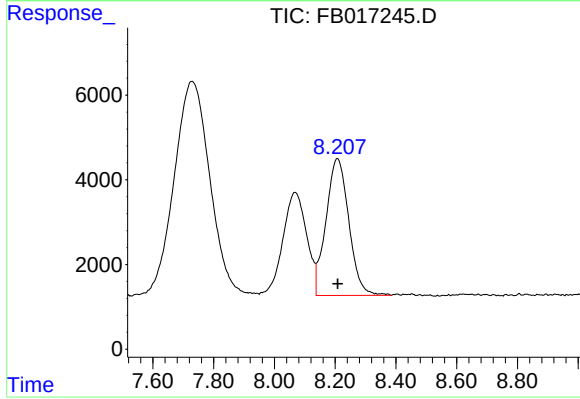


#4 Benzene

R.T.: 8.208 min
Delta R.T.: 0.000 min
Response: 168937
Conc: 9.62 ng/ml

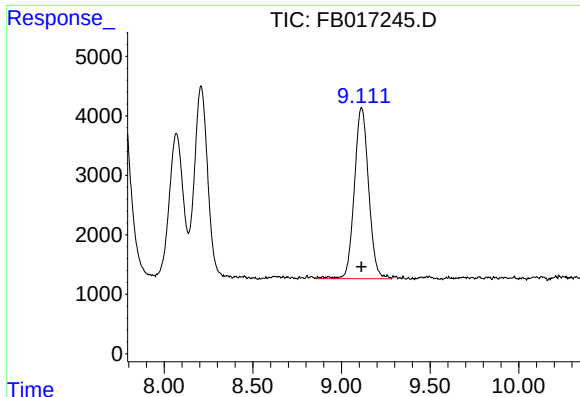


#5 AAA-TFT

R.T.: 9.113 min
Delta R.T.: 0.000 min
Response: 161034
Conc: 20.35 ng/ml

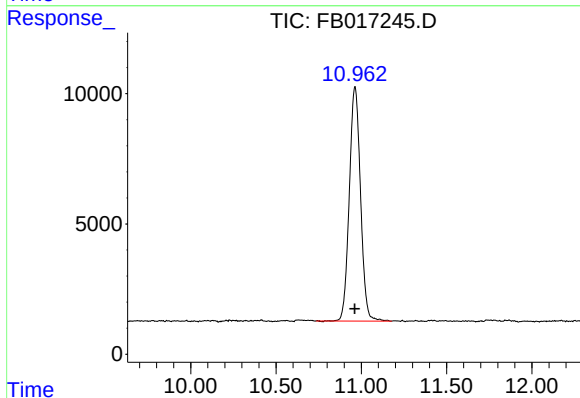


#6 Toluene

R.T.: 10.963 min
Delta R.T.: 0.000 min
Response: 410867
Conc: 29.92 ng/ml

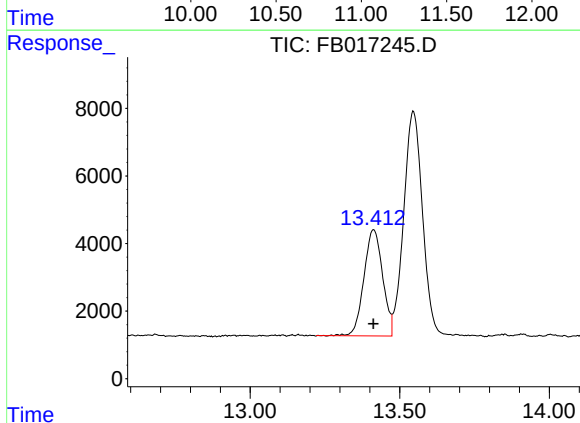


#7 Ethylbenzene

R.T.: 13.413 min
Delta R.T.: 0.001 min
Response: 136826
Conc: 10.03 ng/ml

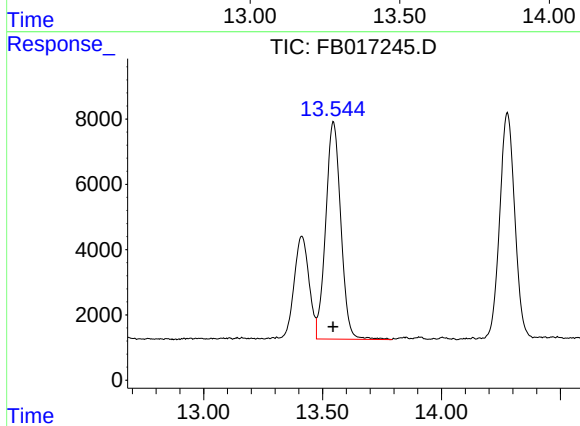


#8 m-Xylene

R.T.: 13.546 min
Delta R.T.: 0.001 min
Response: 294428
Conc: 20.46 ng/ml

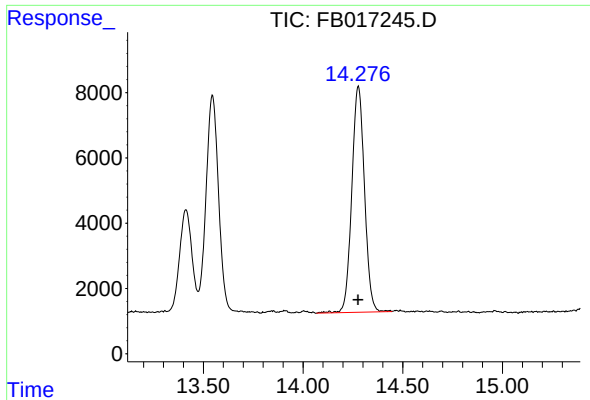

#9 O-Xylene

R.T.: 14.277 min
Delta R.T.: 0.002 min
Response: 306193
Conc: 20.08 ng/ml

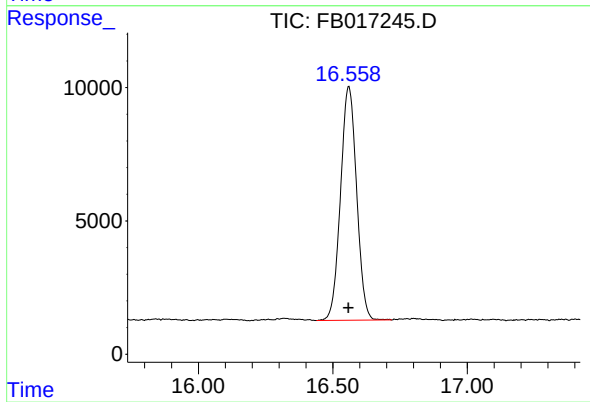

#10 1,2,4-Trimethylbenzene

R.T.: 16.560 min
Delta R.T.: 0.001 min
Response: 364569
Conc: 19.75 ng/ml