

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF081118\
 Data File : FF001832.D
 Signal(s) : FID2B.ch
 Acq On : 11 Aug 2018 22:41
 Operator : AJ\SJ
 Sample : J4442-55
 Misc :
 ALS Vial : 62 Sample Multiplier: 1

Integration File: autoint1.e
 Quant Time: Aug 13 02:04:17 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\C44-FF080418.M
 Quant Title :
 QLast Update : Mon Aug 06 12:04:39 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 ul
 Signal Phase : Rxi-1ms
 Signal Info : 20m x 0.18mm x 0.18um

	Compound	R.T.	Response	Conc Units

System Monitoring Compounds				
13) S	TETRACOSANE-d50 (SURR...	14.324	5737375	14.233 ug/ml
Target Compounds				
6)	N-TETRADECANE	7.962	927151	2.971 ug/ml
10)	N-TETRACOSANE	14.522	440585	1.387 ug/ml
11)	N-OCTACOSANE	16.531	307660	0.956 ug/ml
12)	N-DOTRIACONTANE	18.204	724179	2.220 ug/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF081118\
Data File : FF001832.D
Signal(s) : FID2B.ch
Acq On : 11 Aug 2018 22:41
Operator : AJ\SJ
Sample : J4442-55
Misc :
ALS Vial : 62 Sample Multiplier: 1

Integration File: autoint1.e
Quant Time: Aug 13 02:04:17 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\C44-FF080418.M
Quant Title :
QLast Update : Mon Aug 06 12:04:39 2018
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 1 ul
Signal Phase : Rxi-1ms
Signal Info : 20m x 0.18mm x 0.18um

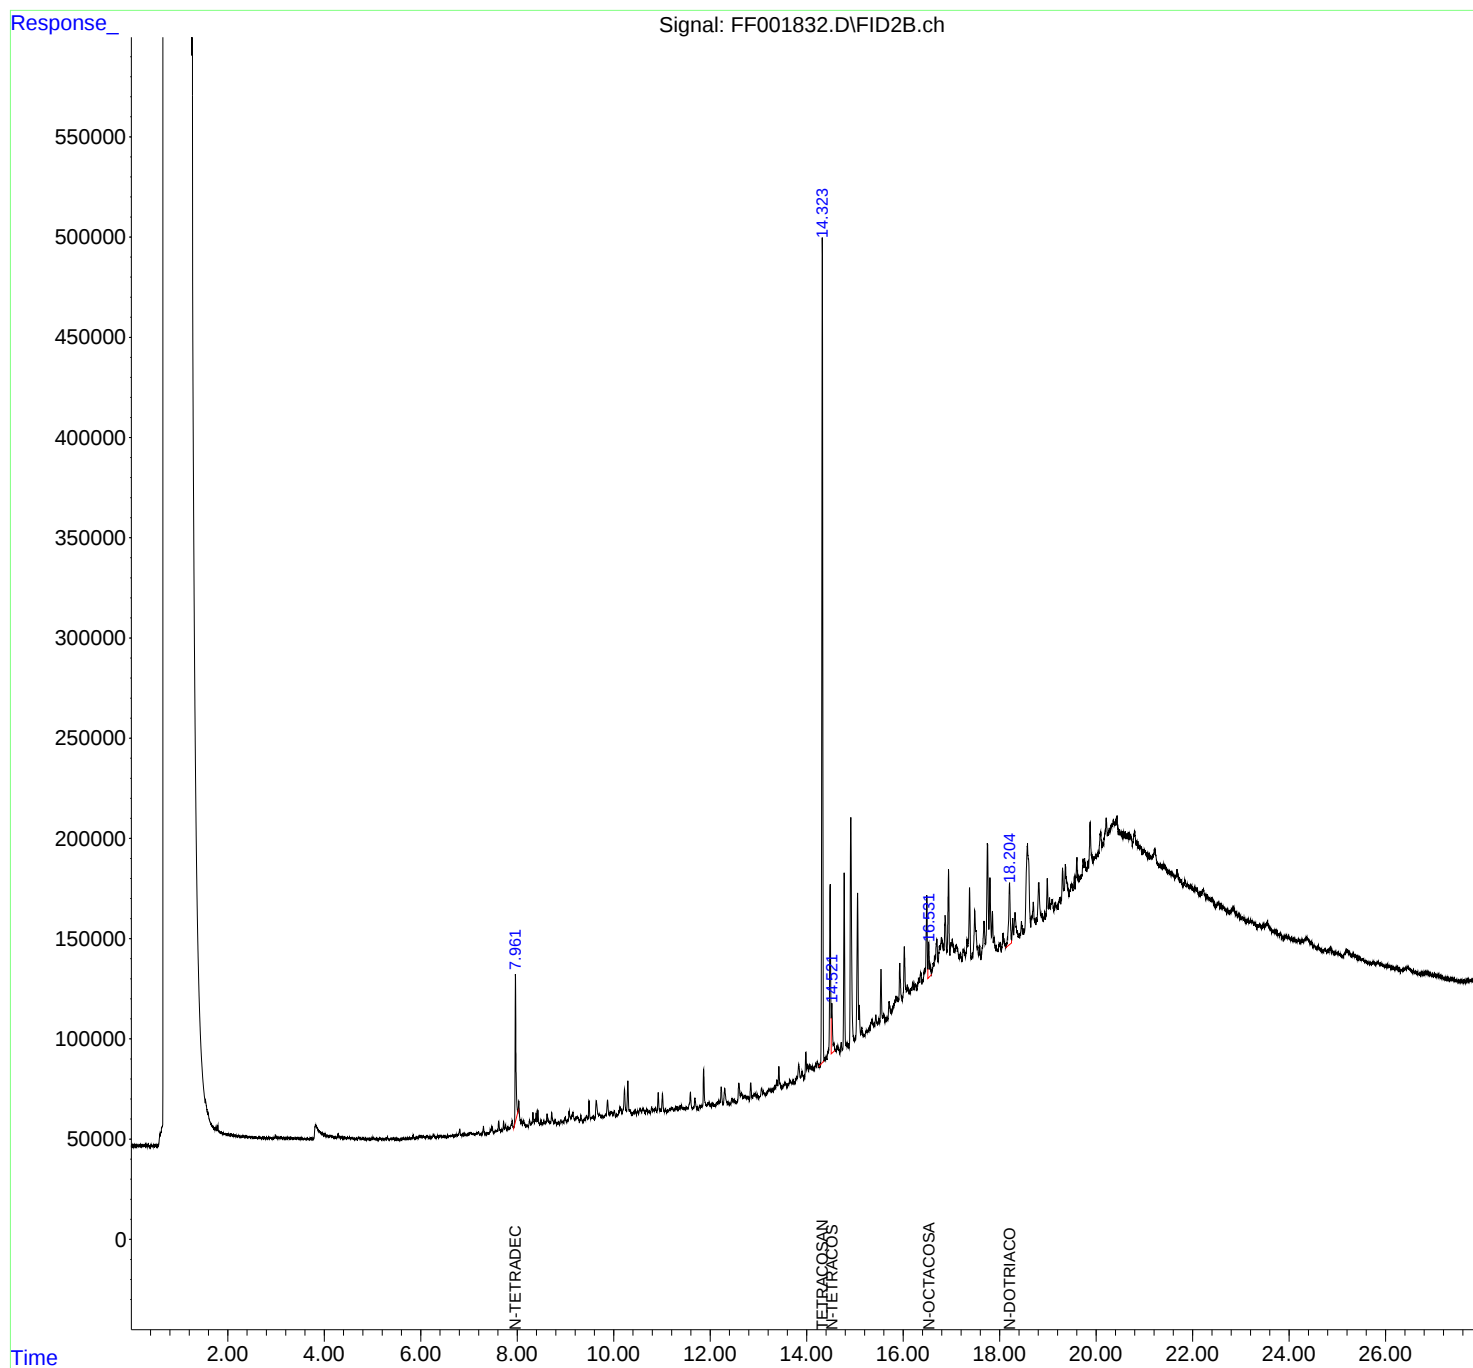

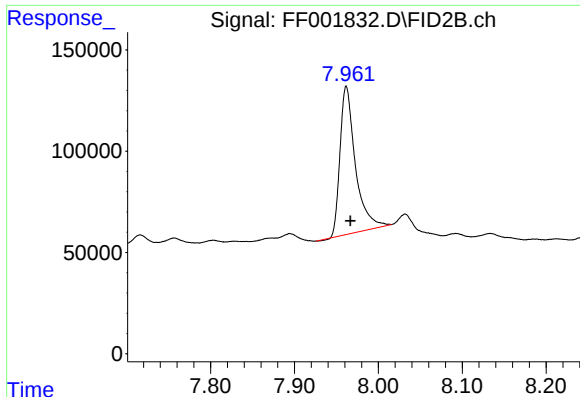


#6 N-TETRADECANE

R.T.: 7.962 min
Delta R.T.: -0.005 min
Response: 927151
Conc: 2.97 ug/ml

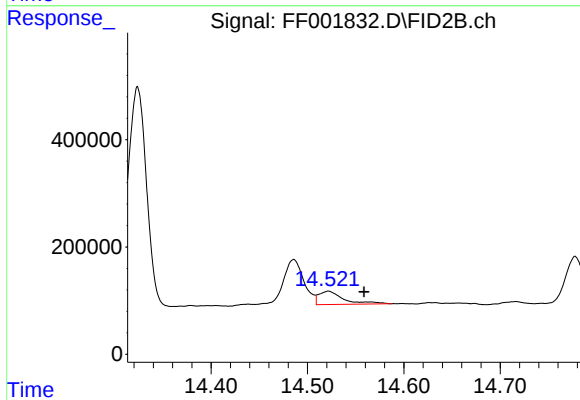


#10 N-TETRACOSANE

R.T.: 14.522 min
Delta R.T.: -0.037 min
Response: 440585
Conc: 1.39 ug/ml

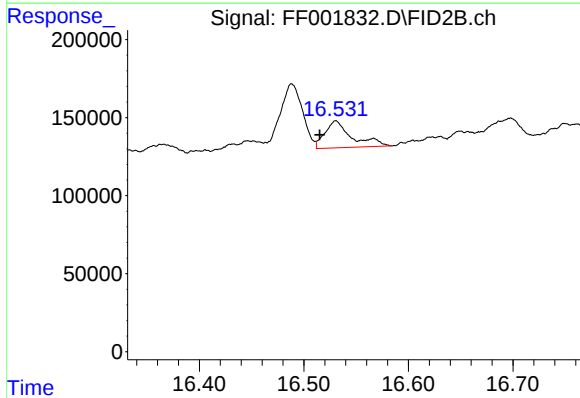


#11 N-OCTACOSANE

R.T.: 16.531 min
Delta R.T.: 0.016 min
Response: 307660
Conc: 0.96 ug/ml

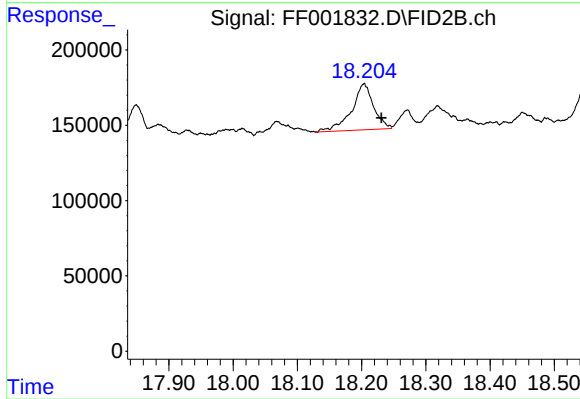

#12 N-DOTRIACONTANE

R.T.: 18.204 min
Delta R.T.: -0.027 min
Response: 724179
Conc: 2.22 ug/ml

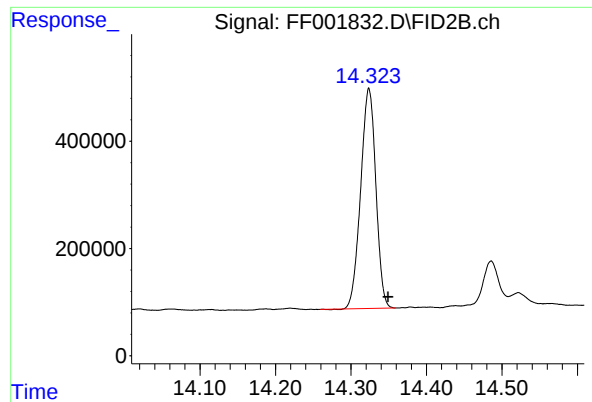

#13 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.324 min
Delta R.T.: -0.025 min
Response: 5737375
Conc: 14.23 ug/ml