

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF081118\
Data File : FF001833.D
Signal(s) : FID2B.ch
Acq On : 11 Aug 2018 23:18
Operator : AJ\SJ
Sample : J4443-02
Misc :
ALS Vial : 63 Sample Multiplier: 1

Integration File: autoint1.e
Quant Time: Aug 13 02:04:27 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\C44-FF080418.M
Quant Title :
QLast Update : Mon Aug 06 12:04:39 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 ul
Signal Phase : Rxi-1ms
Signal Info : 20m x 0.18mm x 0.18um

Compound		R.T.	Response	Conc Units

System Monitoring Compounds				
13) S	TETRACOSANE-d50 (SURR...	14.322	5474834	13.582 ug/ml
Target Compounds				
6)	N-TETRADECANE	7.962	1218886	3.906 ug/ml
10)	N-TETRACOSANE	14.520	307119	0.967 ug/ml
11)	N-OCTACOSANE	16.528	408433	1.269 ug/ml
12)	N-DOTRIACONTANE	18.202	644786	1.976 ug/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF081118\
Data File : FF001833.D
Signal(s) : FID2B.ch
Acq On : 11 Aug 2018 23:18
Operator : AJ\SJ
Sample : J4443-02
Misc :
ALS Vial : 63 Sample Multiplier: 1

Integration File: autoint1.e
Quant Time: Aug 13 02:04:27 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\C44-FF080418.M
Quant Title :
QLast Update : Mon Aug 06 12:04:39 2018
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 1 ul
Signal Phase : Rxi-1ms
Signal Info : 20m x 0.18mm x 0.18um

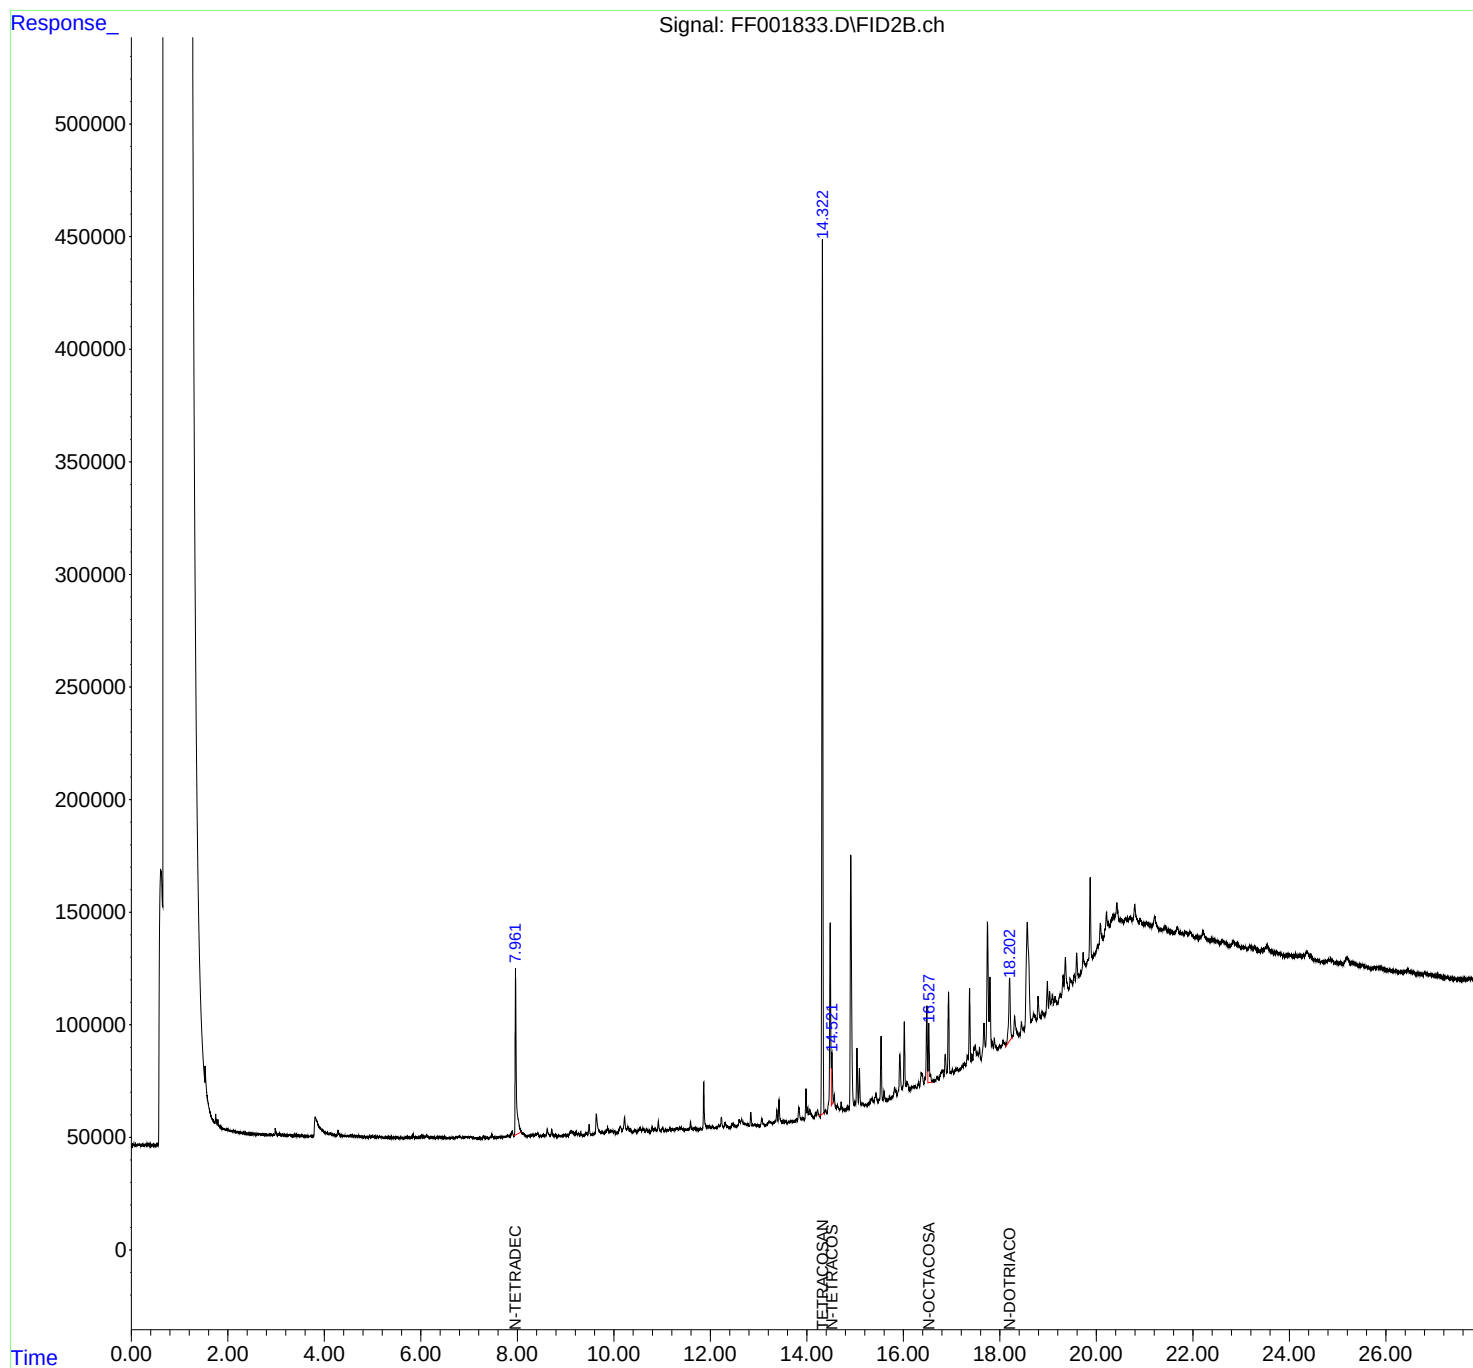

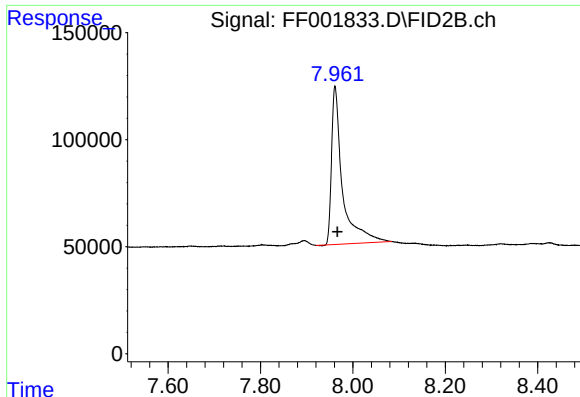


#6 N-TETRADECANE

R.T.: 7.962 min
Delta R.T.: -0.005 min
Response: 1218886
Conc: 3.91 ug/ml

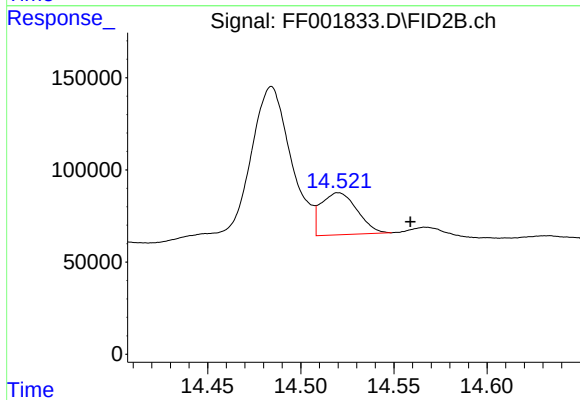


#10 N-TETRACOSANE

R.T.: 14.520 min
Delta R.T.: -0.039 min
Response: 307119
Conc: 0.97 ug/ml

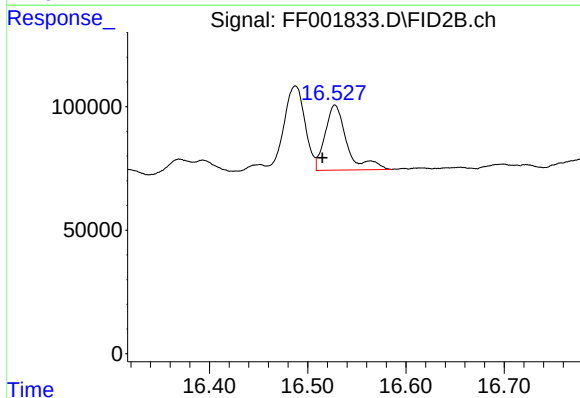


#11 N-OCTACOSANE

R.T.: 16.528 min
Delta R.T.: 0.013 min
Response: 408433
Conc: 1.27 ug/ml

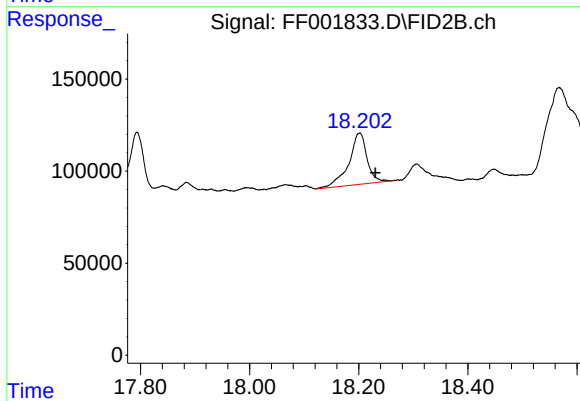

#12 N-DOTRIACONTANE

R.T.: 18.202 min
Delta R.T.: -0.029 min
Response: 644786
Conc: 1.98 ug/ml

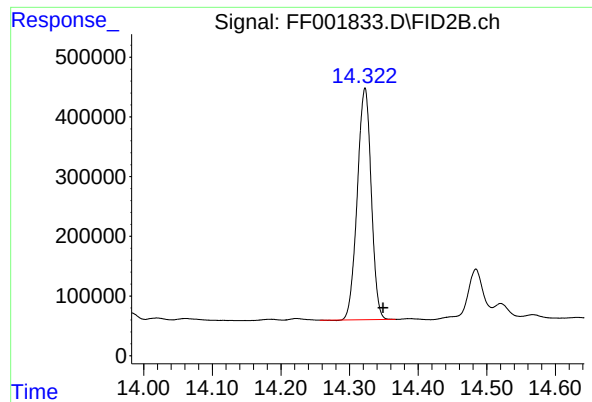

#13 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.322 min
Delta R.T.: -0.027 min
Response: 5474834
Conc: 13.58 ug/ml