

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF081118\
 Data File : FF001834.D
 Signal(s) : FID2B.ch
 Acq On : 11 Aug 2018 23:54
 Operator : AJ\SJ
 Sample : J4443-03
 Misc :
 ALS Vial : 64 Sample Multiplier: 1

Integration File: autoint1.e
 Quant Time: Aug 13 02:04:37 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\C44-FF080418.M
 Quant Title :
 QLast Update : Mon Aug 06 12:04:39 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 ul
 Signal Phase : Rxi-1ms
 Signal Info : 20m x 0.18mm x 0.18um

	Compound	R.T.	Response	Conc Units

System Monitoring Compounds				
13) S	TETRACOSANE-d50 (SURR...	14.323	6869257	17.041 ug/ml
Target Compounds				
6)	N-TETRADECANE	7.961	2108080	6.755 ug/ml
10)	N-TETRACOSANE	14.520	359978	1.133 ug/ml
11)	N-OCTACOSANE	16.487	451405	1.403 ug/ml
12)	N-DOTRIACONTANE	18.202	919676	2.819 ug/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF081118\
Data File : FF001834.D
Signal(s) : FID2B.ch
Acq On : 11 Aug 2018 23:54
Operator : AJ\SJ
Sample : J4443-03
Misc :
ALS Vial : 64 Sample Multiplier: 1

Integration File: autoint1.e
Quant Time: Aug 13 02:04:37 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\C44-FF080418.M
Quant Title :
QLast Update : Mon Aug 06 12:04:39 2018
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 1 u1
Signal Phase : Rxi-1ms
Signal Info : 20m x 0.18mm x 0.18um

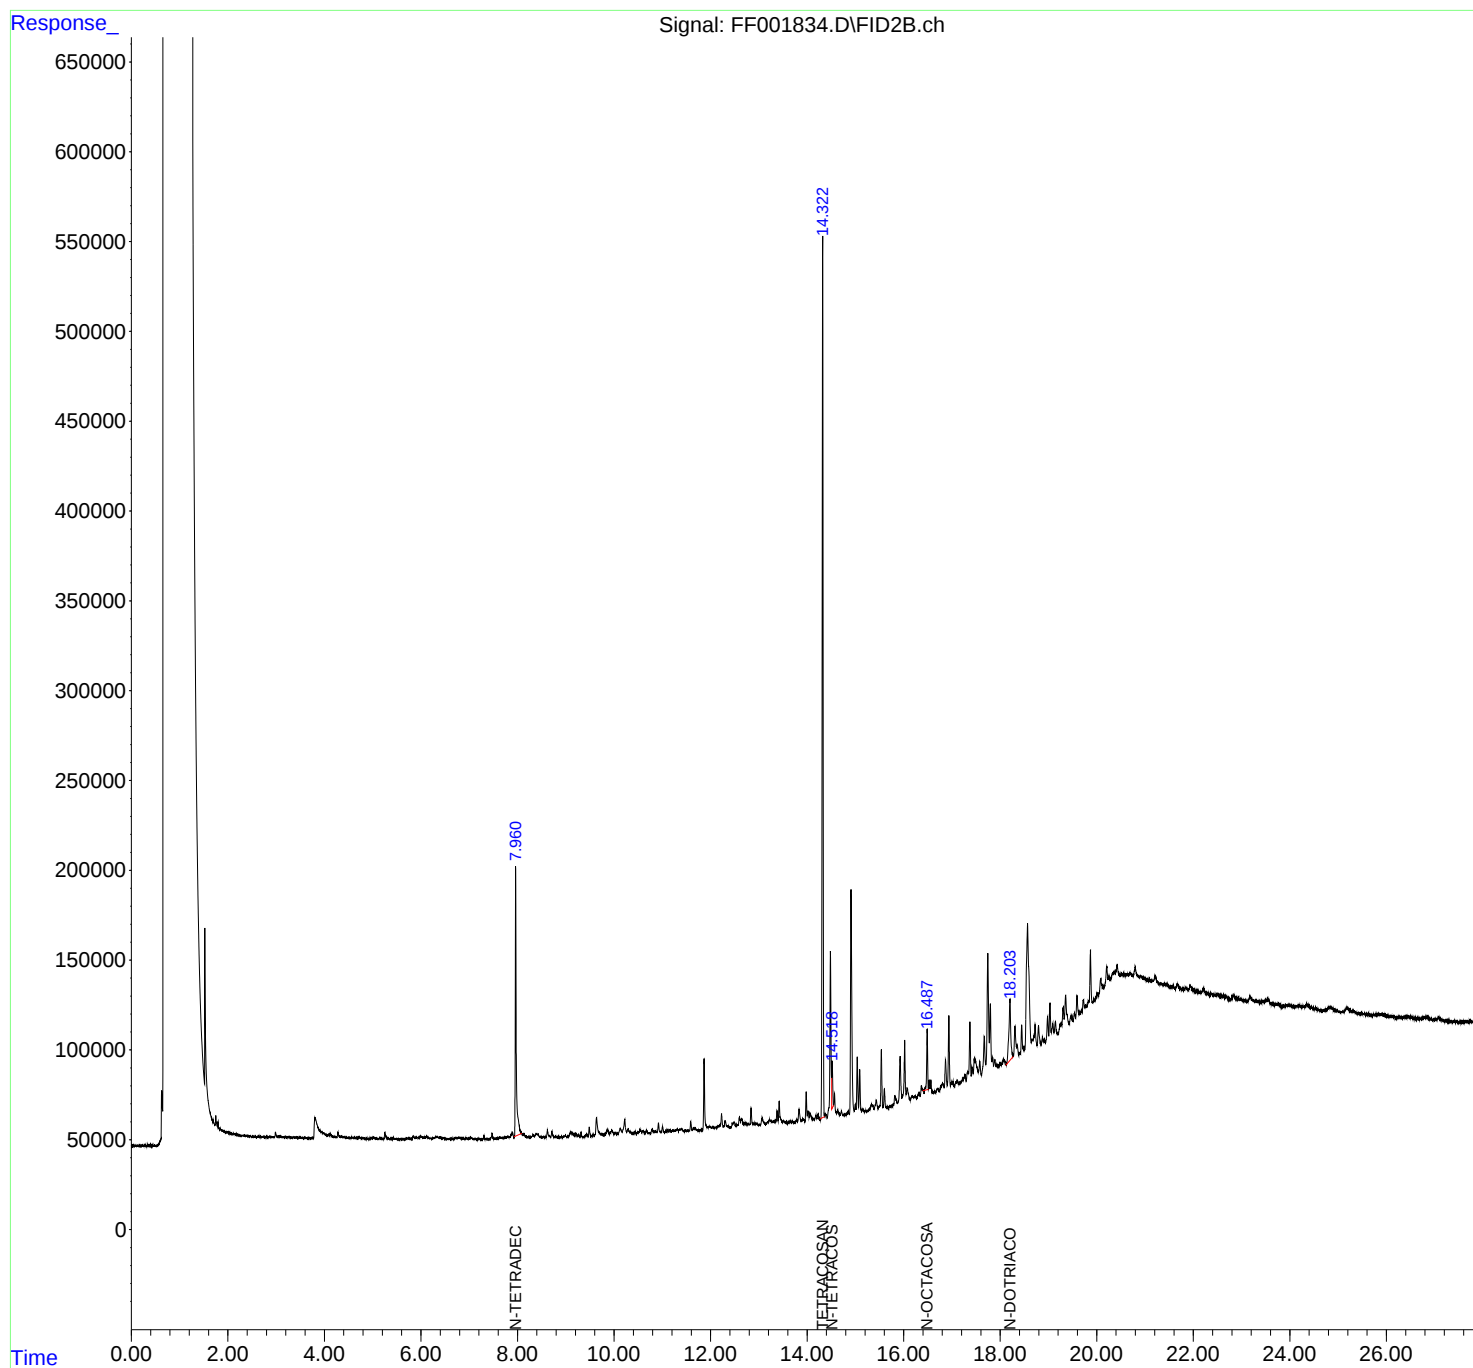

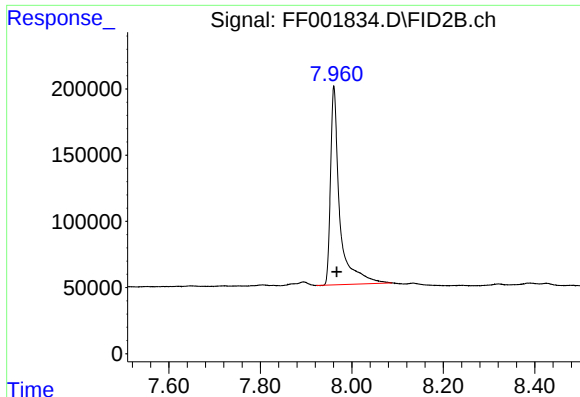


#6 N-TETRADECANE

R.T.: 7.961 min
Delta R.T.: -0.006 min
Response: 2108080
Conc: 6.76 ug/ml

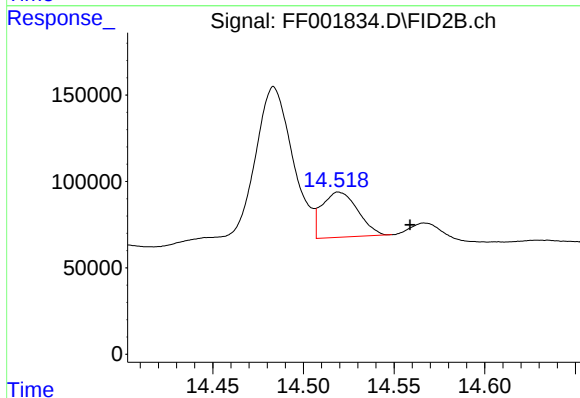


#10 N-TETRACOSANE

R.T.: 14.520 min
Delta R.T.: -0.039 min
Response: 359978
Conc: 1.13 ug/ml

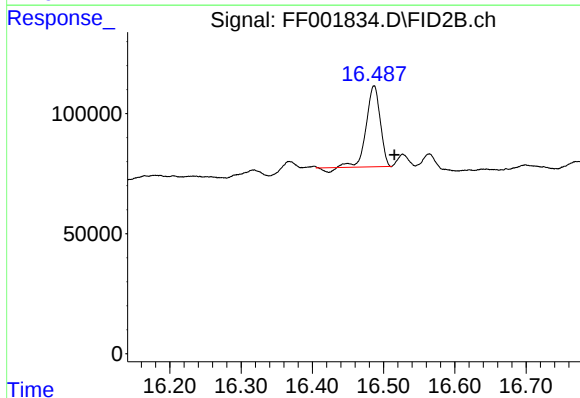


#11 N-OCTACOSANE

R.T.: 16.487 min
Delta R.T.: -0.028 min
Response: 451405
Conc: 1.40 ug/ml

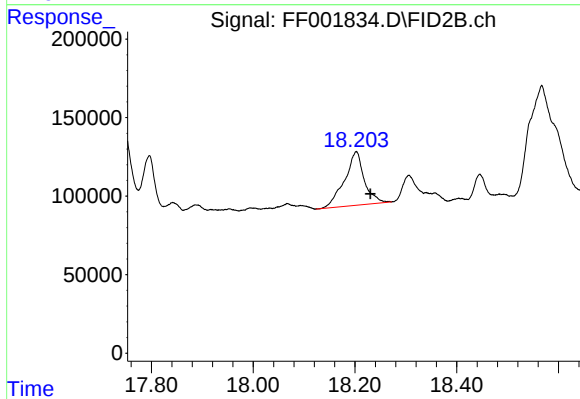

#12 N-DOTRIACONTANE

R.T.: 18.202 min
Delta R.T.: -0.028 min
Response: 919676
Conc: 2.82 ug/ml

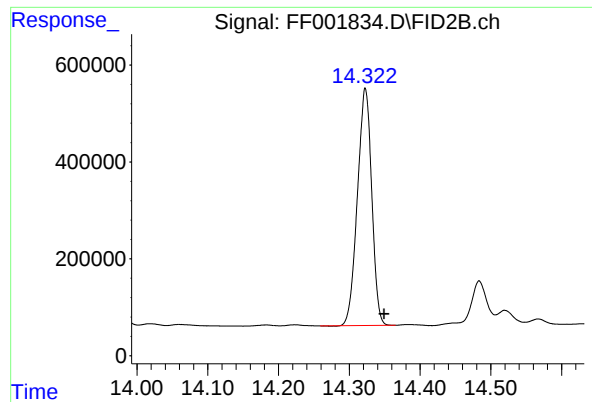

#13 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.323 min
Delta R.T.: -0.026 min
Response: 6869257
Conc: 17.04 ug/ml