

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF081118\
Data File : FF001843.D
Signal(s) : FID2B.ch
Acq On : 12 Aug 2018 06:01
Operator : AJ\SJ
Sample : J4447-01
Misc :
ALS Vial : 71 Sample Multiplier: 1

Integration File: autoint1.e
Quant Time: Aug 13 02:06:12 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\C44-FF080418.M
Quant Title :
QLast Update : Mon Aug 06 12:04:39 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 ul
Signal Phase : Rxi-1ms
Signal Info : 20m x 0.18mm x 0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
13) S TETRACOSANE-d50 (SURR...	14.322	6839278	16.967 ug/ml
Target Compounds			
6) N-TETRADECANE	7.962	1252195	4.013 ug/ml
8) N-OCTADECANE	11.009	374913	1.189 ug/ml
9) N-EICOSANE	12.296	368555	1.168 ug/ml
10) N-TETRACOSANE	14.520	468333	1.474 ug/ml
11) N-OCTACOSANE	16.530	542348	1.685 ug/ml
12) N-DOTRIACONTANE	18.204	1275342	3.909 ug/ml
14) N-HEXATRIACONTANE	19.764	199912	0.678 ug/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF081118\
Data File : FF001843.D
Signal(s) : FID2B.ch
Acq On : 12 Aug 2018 06:01
Operator : AJ\SJ
Sample : J4447-01
Misc :
ALS Vial : 71 Sample Multiplier: 1

Integration File: autoint1.e
Quant Time: Aug 13 02:06:12 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\C44-FF080418.M
Quant Title :
QLast Update : Mon Aug 06 12:04:39 2018
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 1 ul
Signal Phase : Rxi-1ms
Signal Info : 20m x 0.18mm x 0.18um

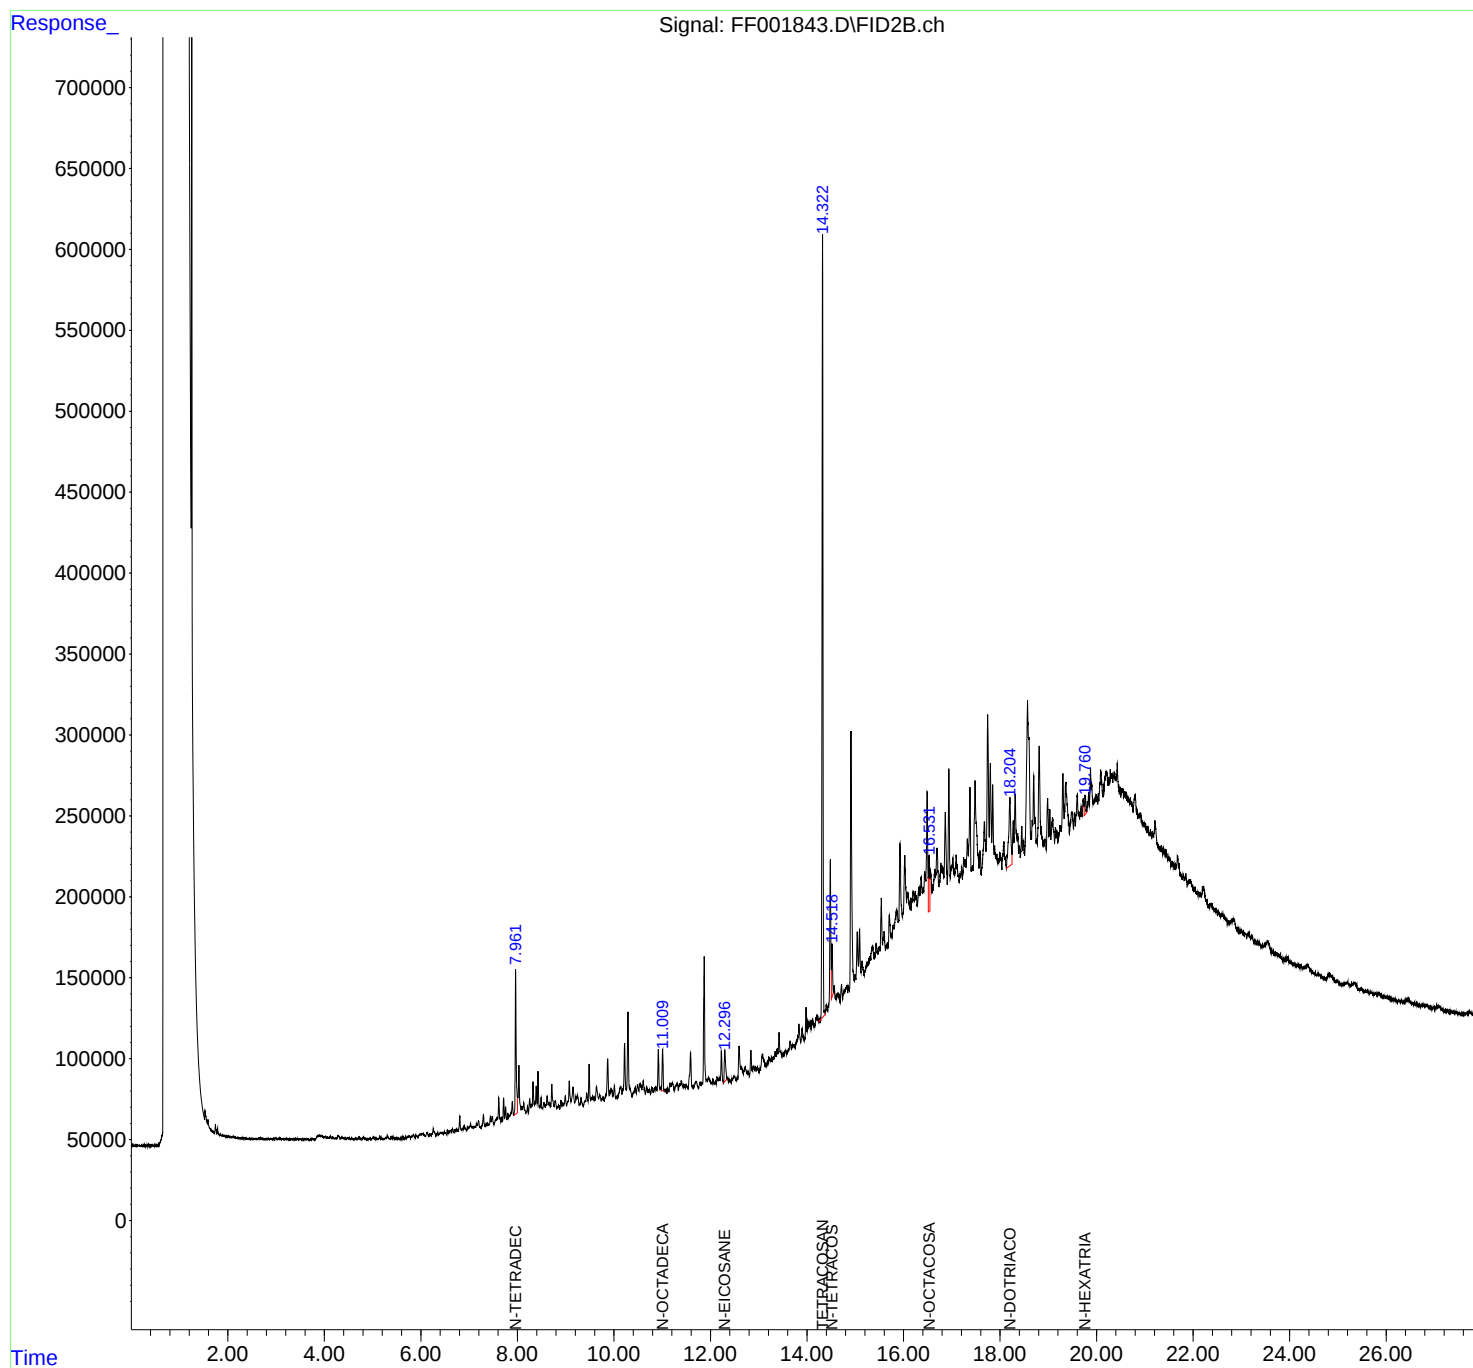

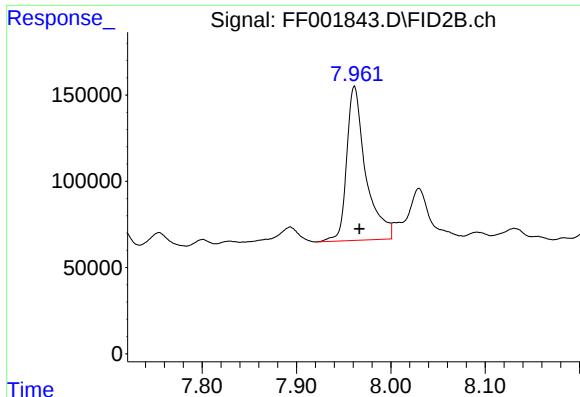


#6 N-TETRADECANE

R.T.: 7.962 min
Delta R.T.: -0.005 min
Response: 1252195
Conc: 4.01 ug/ml

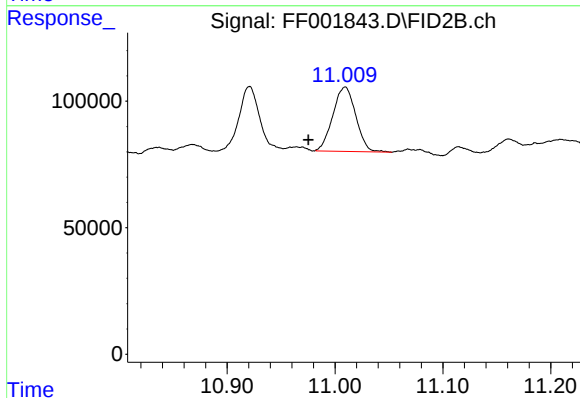


#8 N-OCTADECANE

R.T.: 11.009 min
Delta R.T.: 0.034 min
Response: 374913
Conc: 1.19 ug/ml

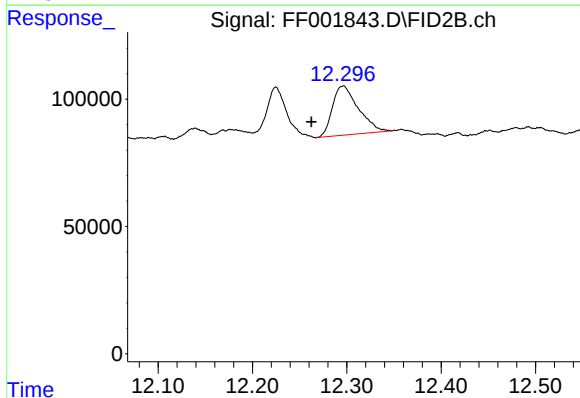


#9 N-EICOSANE

R.T.: 12.296 min
Delta R.T.: 0.034 min
Response: 368555
Conc: 1.17 ug/ml

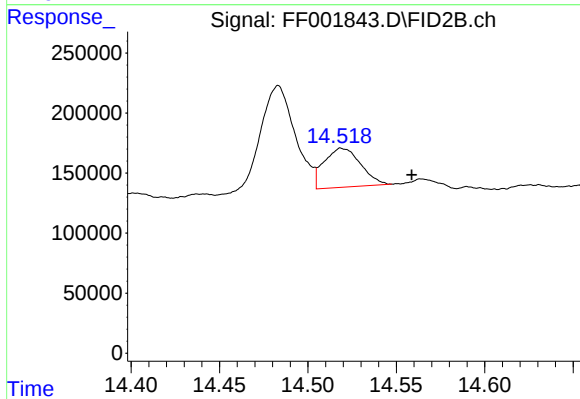


#10 N-TETRACOSANE

R.T.: 14.520 min
Delta R.T.: -0.039 min
Response: 468333
Conc: 1.47 ug/ml

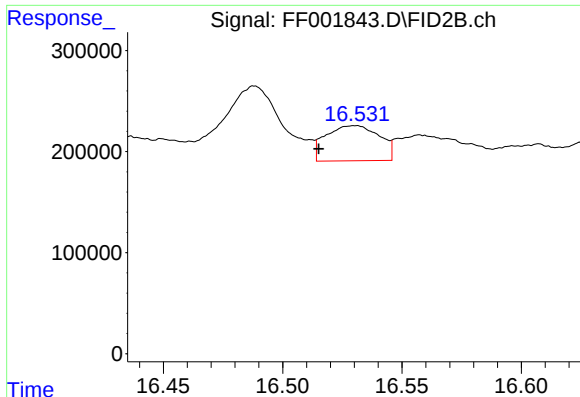


#11 N-OCTACOSANE

R.T.: 16.530 min
Delta R.T.: 0.015 min
Response: 542348
Conc: 1.69 ug/ml

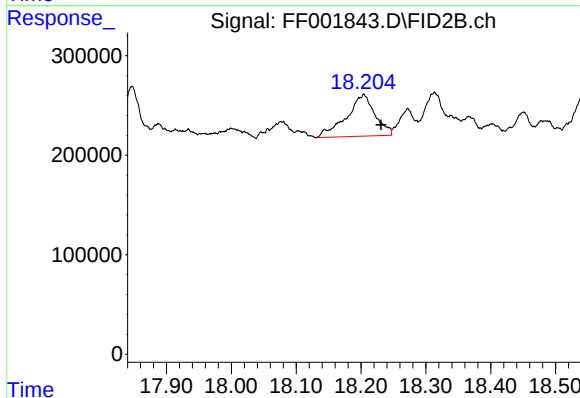


#12 N-DOTRIACONTANE

R.T.: 18.204 min
Delta R.T.: -0.026 min
Response: 1275342
Conc: 3.91 ug/ml

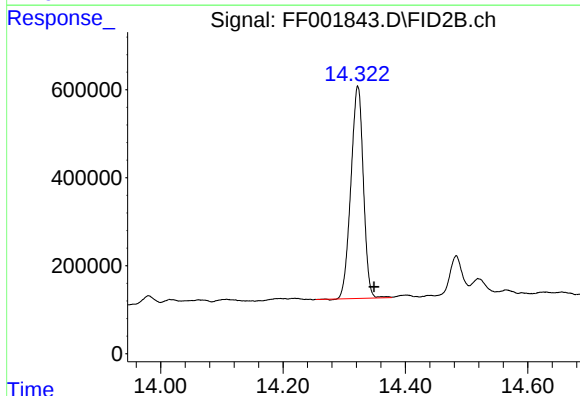

#13 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.322 min
Delta R.T.: -0.027 min
Response: 6839278
Conc: 16.97 ug/ml

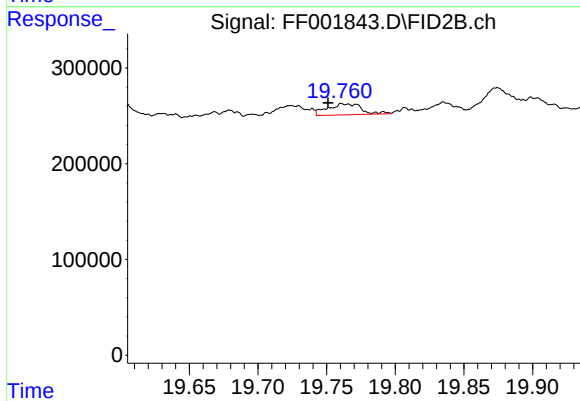

#14 N-HEXATRIACONTANE

R.T.: 19.764 min
Delta R.T.: 0.013 min
Response: 199912
Conc: 0.68 ug/ml