

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF081118\
 Data File : FF001845.D
 Signal(s) : FID2B.ch
 Acq On : 12 Aug 2018 07:13
 Operator : AJ\SJ
 Sample : J4447-03
 Misc :
 ALS Vial : 73 Sample Multiplier: 1

Integration File: autoint1.e
 Quant Time: Aug 13 02:06:35 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\C44-FF080418.M
 Quant Title :
 QLast Update : Mon Aug 06 12:04:39 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 ul
 Signal Phase : Rxi-1ms
 Signal Info : 20m x 0.18mm x 0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
13) S TETRACOSANE-d50 (SURR...	14.324	6996958	17.358 ug/ml
Target Compounds			
6) N-TETRADECANE	7.961	1304241	4.180 ug/ml
8) N-OCTADECANE	11.009	362245	1.148 ug/ml
9) N-EICOSANE	12.226	290317	0.920 ug/ml
10) N-TETRACOSANE	14.524	351050	1.105 ug/ml
11) N-OCTACOSANE	16.530	248916	0.773 ug/ml
12) N-DOTRIACONTANE	18.205	1284503	3.937 ug/ml
14) N-HEXATRIACONTANE	19.769	363295	1.232 ug/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF081118\
Data File : FF001845.D
Signal(s) : FID2B.ch
Acq On : 12 Aug 2018 07:13
Operator : AJ\SJ
Sample : J4447-03
Misc :
ALS Vial : 73 Sample Multiplier: 1

Integration File: autoint1.e
Quant Time: Aug 13 02:06:35 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\C44-FF080418.M
Quant Title :
QLast Update : Mon Aug 06 12:04:39 2018
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 1 uL
Signal Phase : Rxi-1ms
Signal Info : 20m x 0.18mm x 0.18um

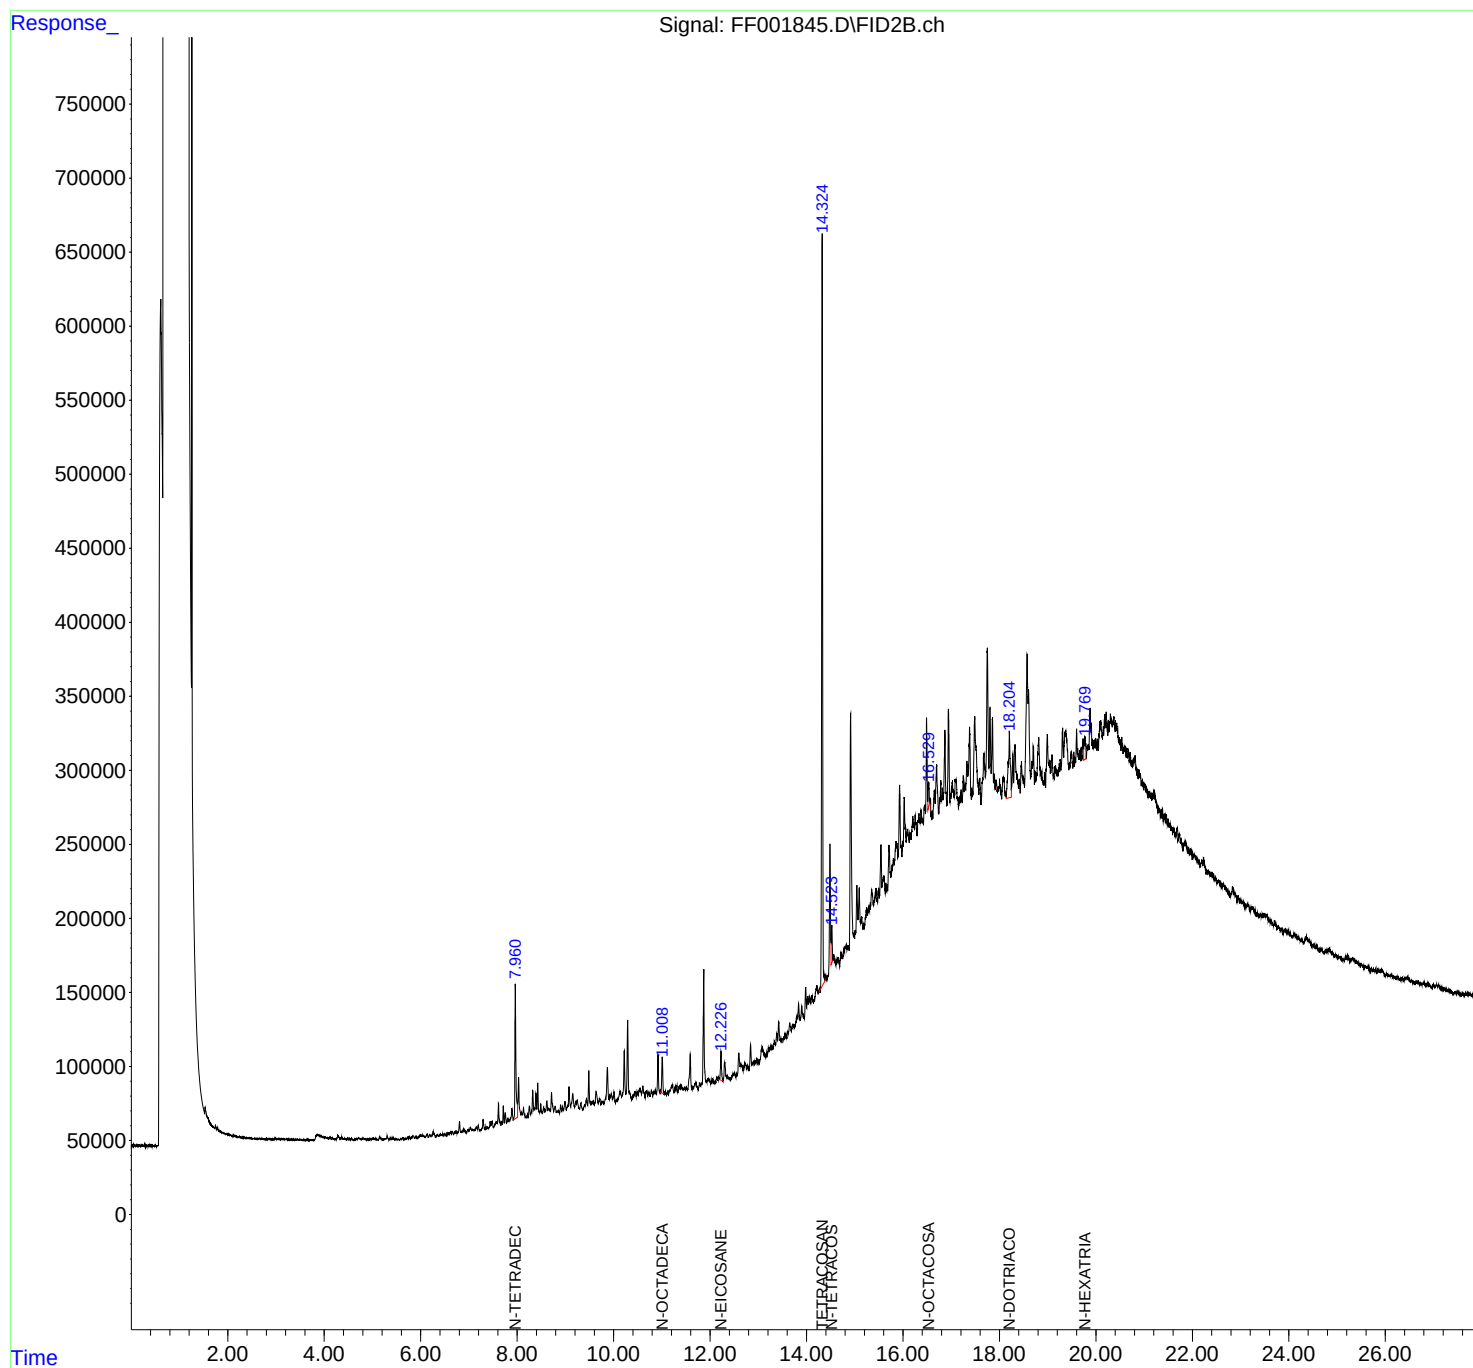

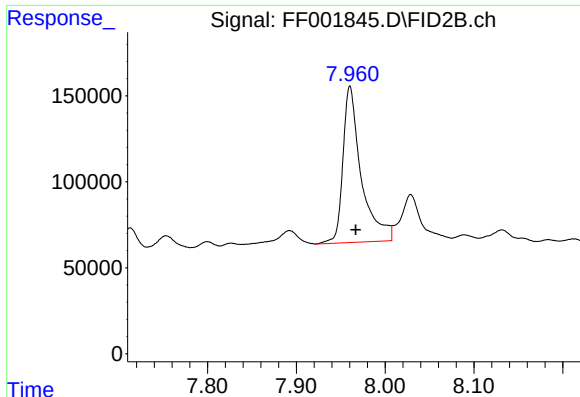


#6 N-TETRADECANE

R.T.: 7.961 min
Delta R.T.: -0.006 min
Response: 1304241
Conc: 4.18 ug/ml

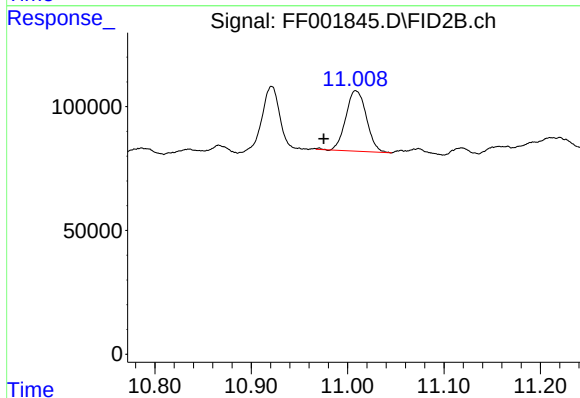


#8 N-OCTADECANE

R.T.: 11.009 min
Delta R.T.: 0.033 min
Response: 362245
Conc: 1.15 ug/ml

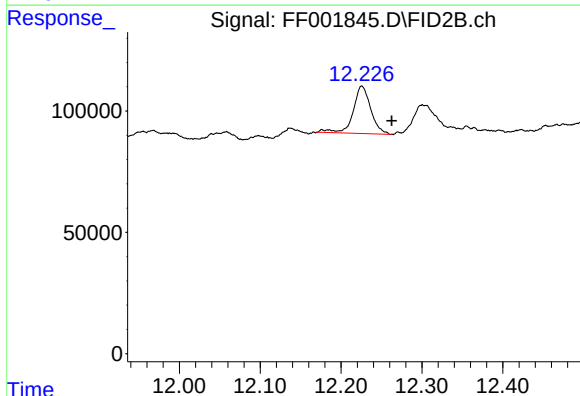


#9 N-EICOSANE

R.T.: 12.226 min
Delta R.T.: -0.037 min
Response: 290317
Conc: 0.92 ug/ml

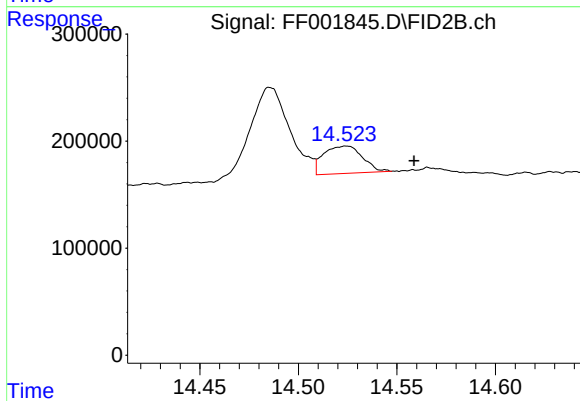


#10 N-TETRACOSANE

R.T.: 14.524 min
Delta R.T.: -0.035 min
Response: 351050
Conc: 1.11 ug/ml

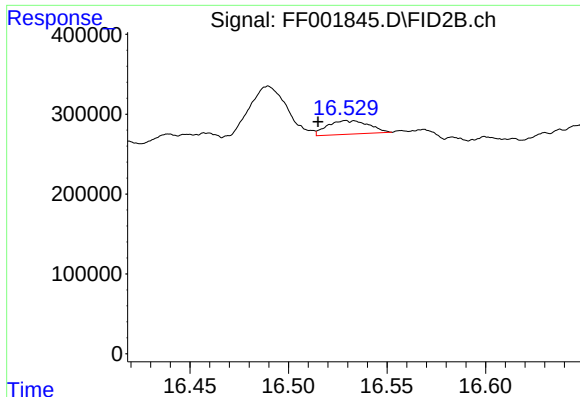


#11 N-OCTACOSANE

R.T.: 16.530 min
Delta R.T.: 0.015 min
Response: 248916
Conc: 0.77 ug/ml

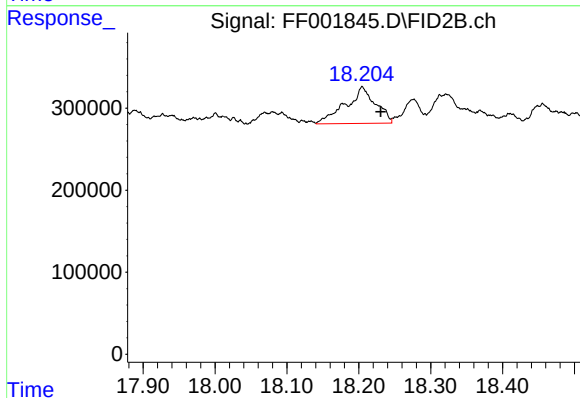


#12 N-DOTRIACONTANE

R.T.: 18.205 min
Delta R.T.: -0.025 min
Response: 1284503
Conc: 3.94 ug/ml

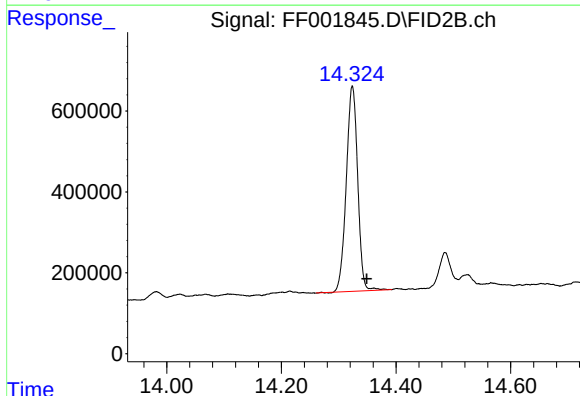

#13 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.324 min
Delta R.T.: -0.025 min
Response: 6996958
Conc: 17.36 ug/ml

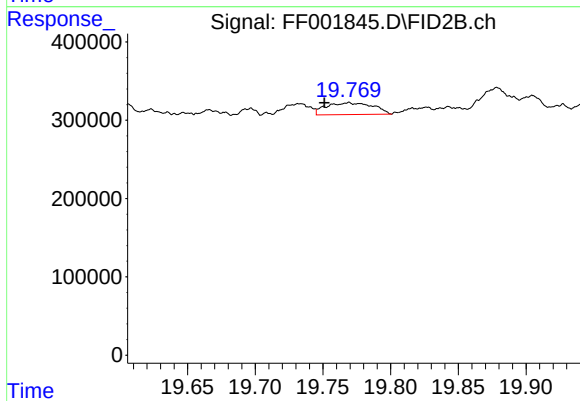

#14 N-HEXATRIACONTANE

R.T.: 19.769 min
Delta R.T.: 0.018 min
Response: 363295
Conc: 1.23 ug/ml