

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF081120\
Data File : FF007327.D
Signal(s) : FID2B.ch
Acq On : 11 Aug 2020 18:17
Operator : DD\AJ
Sample : I.BLK
Misc :
ALS Vial : 52 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :
I.BLK

Integration File: autoint1.e
Quant Time: Aug 13 01:36:34 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF072820.M
Quant Title :
QLast Update : Wed Jul 29 09:33:32 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.760	1997511	14.634 ug/ml
Target Compounds			
14) N-DOTRIACONTANE	18.667	55251	0.373 ug/ml
15) N-TETRATRIACONTANE	19.451	30370	0.251 ug/ml
16) N-HEXATRIACONTANE	20.197	24614	0.266 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF081120\
Data File : FF07327.D
Signal(s) : FID2B.ch
Acq On : 11 Aug 2020 18:17
Operator : DD\AJ
Sample : I.BLK
Misc :
ALS Vial : 52 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :
I.BLK

Integration File: autoint1.e
Quant Time: Aug 13 01:36:34 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF072820.M
Quant Title :
QLast Update : Wed Jul 29 09:33:32 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

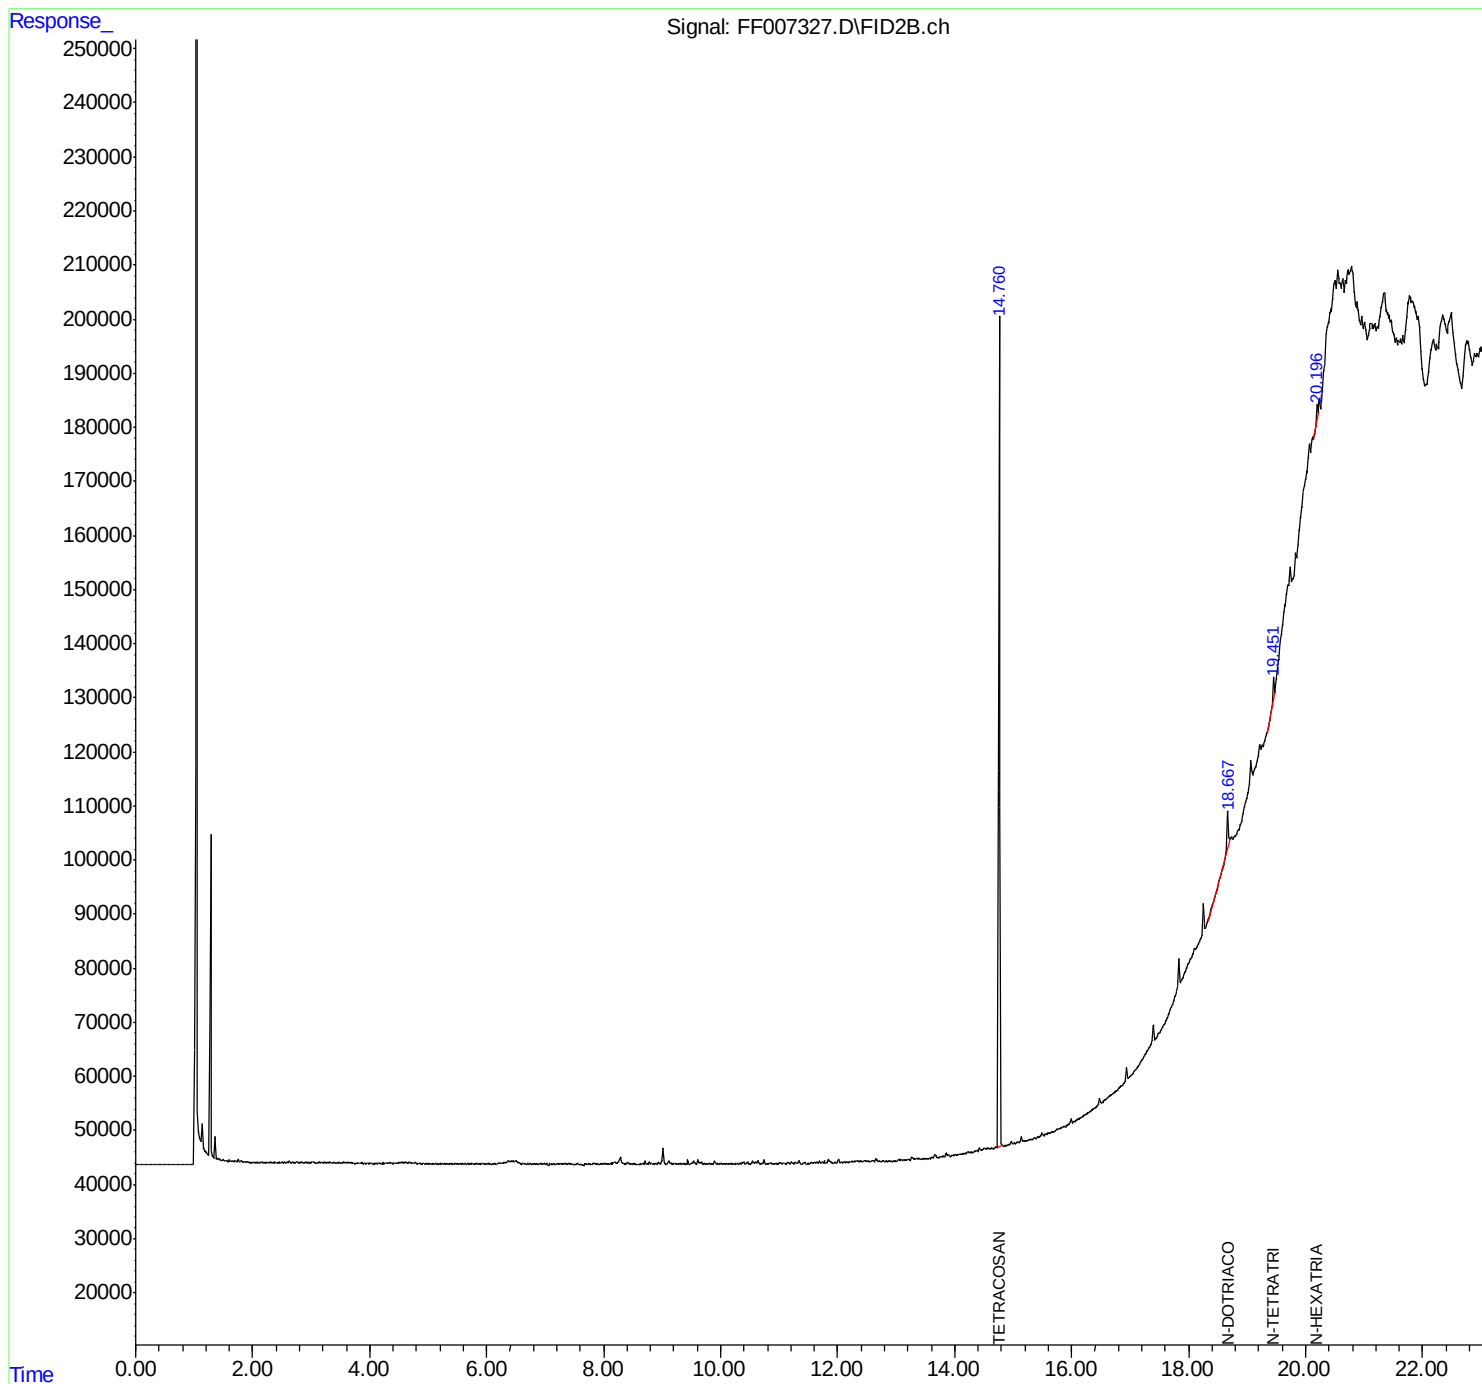


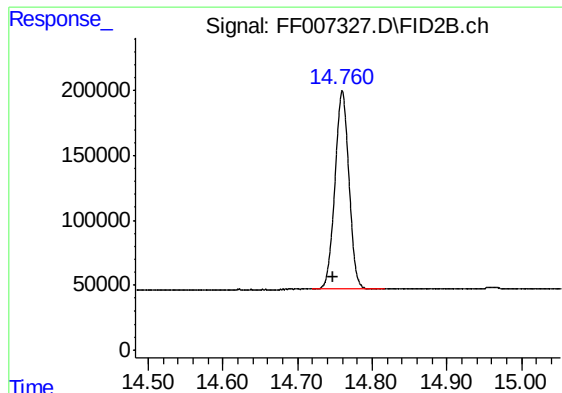

#9 TETRACOSANE-d50 (SURROGATE)


R.T.: 14.760 min
Delta R.T.: 0.012 min
Response: 1997511
Conc: 14.63 ug/ml

Instrument :
FID_F
ClientSampleId :
I.BLK

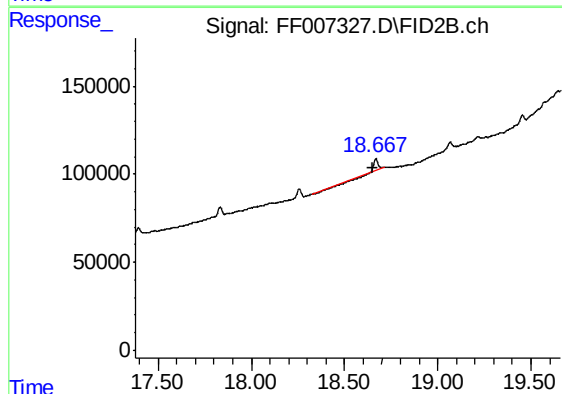


#14 N-DOTRIACONTANE

R.T.: 18.667 min
Delta R.T.: 0.015 min
Response: 55251
Conc: 0.37 ug/ml

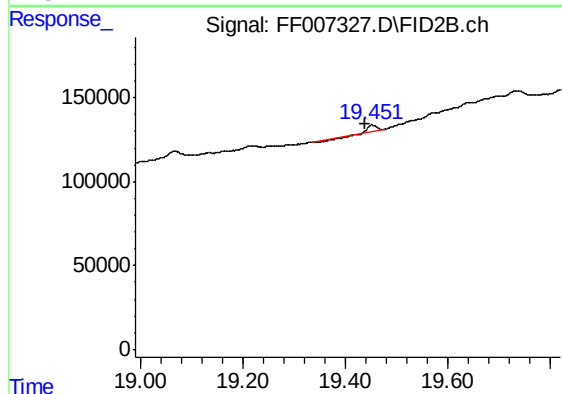

#15 N-TETRATRIACONTANE

R.T.: 19.451 min
Delta R.T.: 0.012 min
Response: 30370
Conc: 0.25 ug/ml

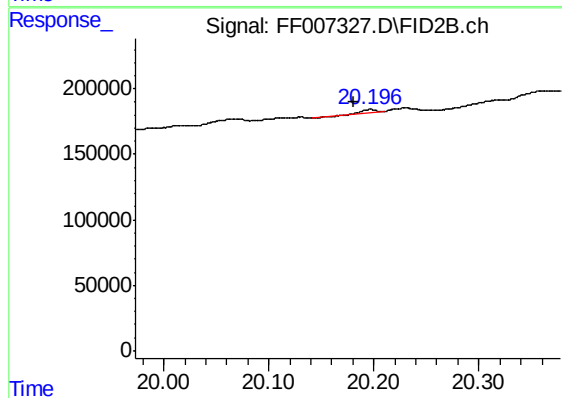

#16 N-HEXATRIACONTANE

R.T.: 20.197 min
Delta R.T.: 0.016 min
Response: 24614
Conc: 0.27 ug/ml