

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF081120\
 Data File : FF007329.D
 Signal(s) : FID2B.ch
 Acq On : 11 Aug 2020 19:20
 Operator : DD\AJ
 Sample : RT MARKER
 Misc :
 ALS Vial : 54 Sample Multiplier: 1

Instrument :
 FID_F
 ClientSampleId :
 RT MARKER

Integration File: autoint1.e
 Quant Time: Aug 13 01:38:45 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF072820.M
 Quant Title :
 QLast Update : Wed Jul 29 09:33:32 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
Target Compounds			
3) N-DODECANE	6.492	2999675	21.089 ug/ml
12) N-OCTACOSANE	16.941	2682165	17.090 ug/ml
14) N-DOTRIACONTANE	18.664	89355	0.603 ug/ml
15) N-TETRATRIACONTANE	19.451	26535	0.219 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF081120\
Data File : FF007329.D
Signal(s) : FID2B.ch
Acq On : 11 Aug 2020 19:20
Operator : DD\AJ
Sample : RT MARKER
Misc :
ALS Vial : 54 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :
RT MARKER

Integration File: autoint1.e
Quant Time: Aug 13 01:38:45 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF072820.M
Quant Title :
QLast Update : Wed Jul 29 09:33:32 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

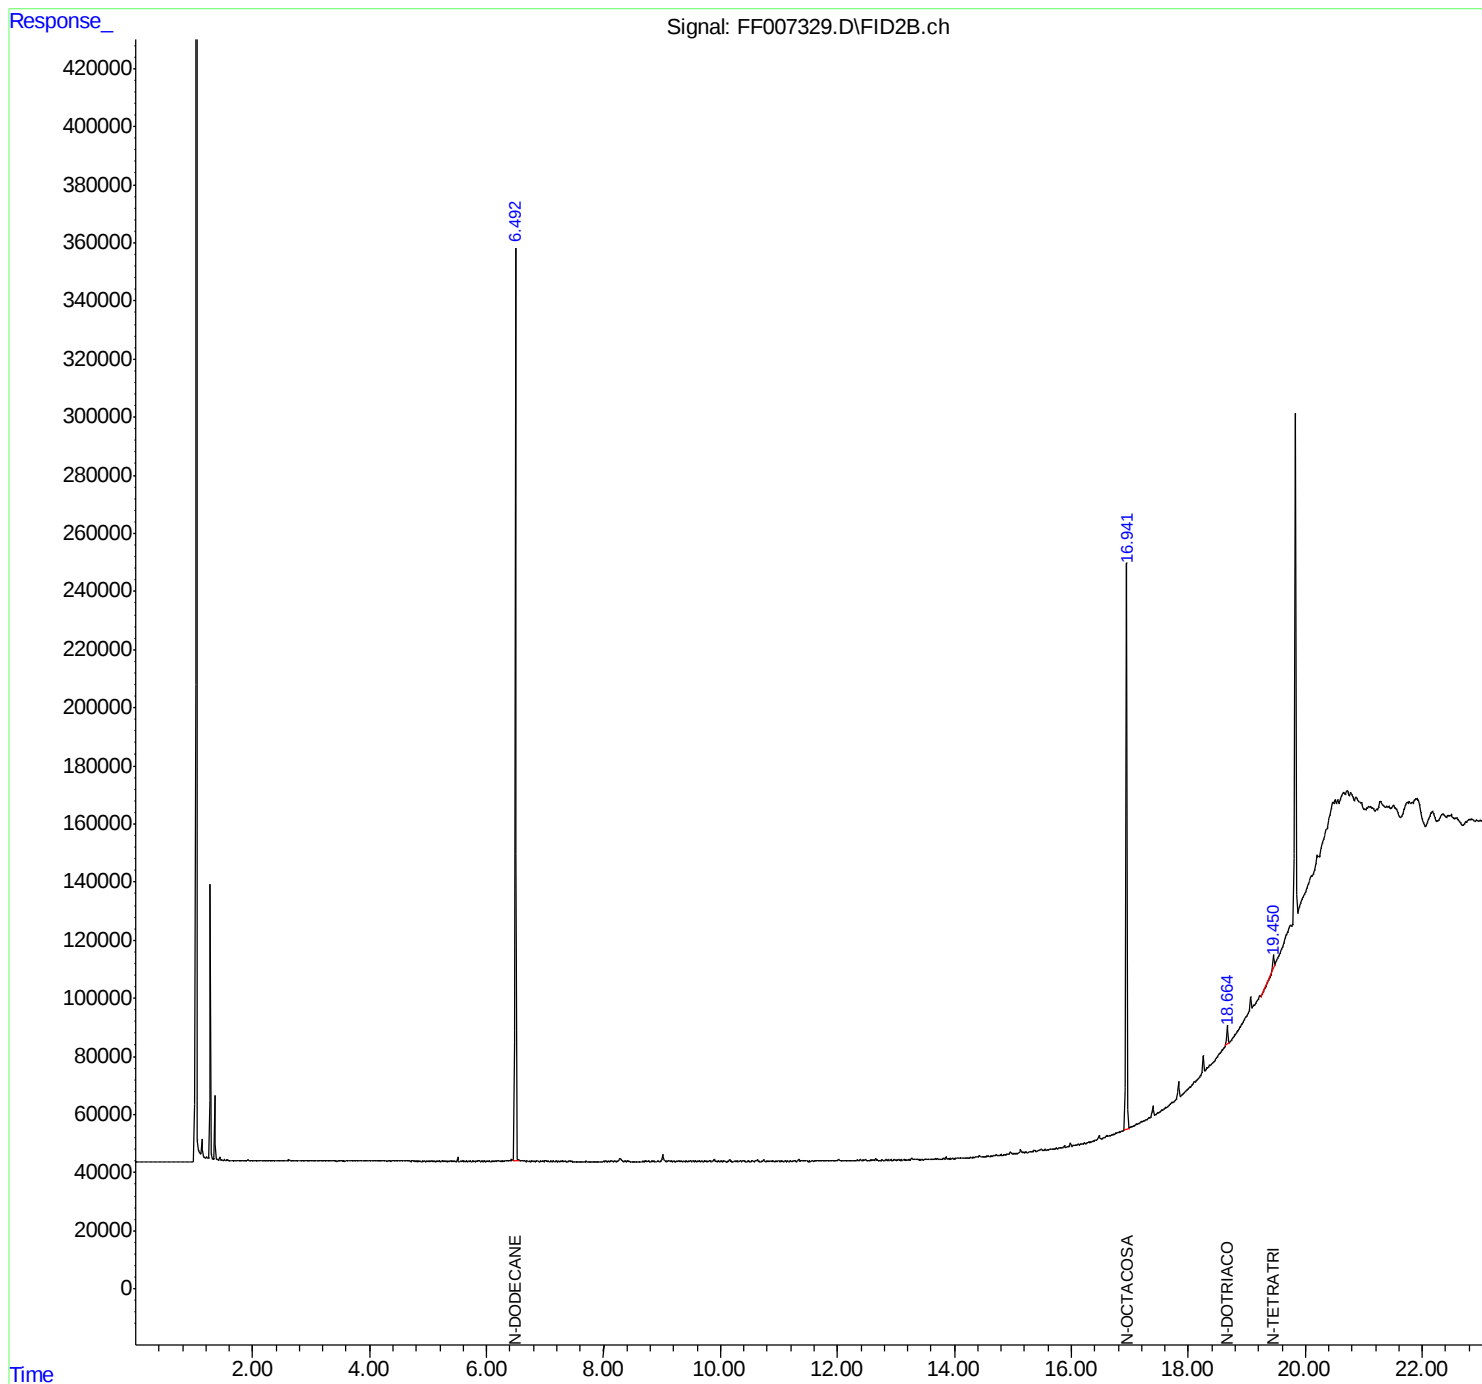


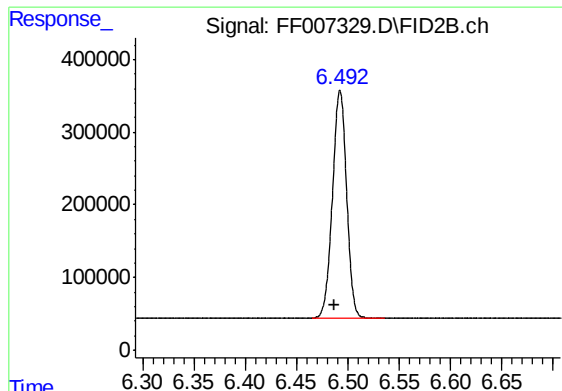

#3 N-DODECANE


R.T.: 6.492 min
Delta R.T.: 0.006 min
Response: 2999675
Conc: 21.09 ug/ml

Instrument :
FID_F
ClientSampleId :
RT MARKER

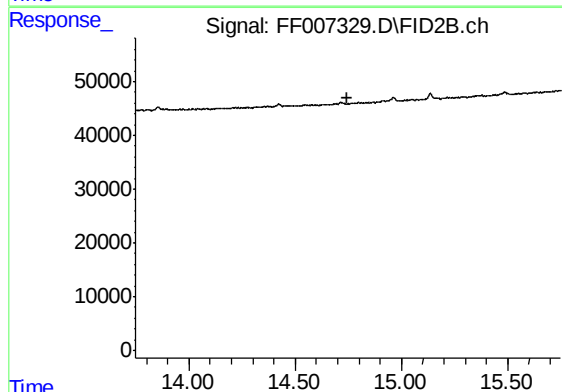


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 0.000 min
Exp R.T. : 14.748 min
Response: 0
Conc: N.D.

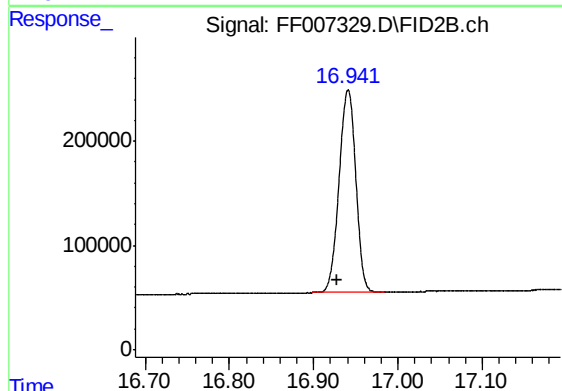


#12 N-OCTACOSANE

R.T.: 16.941 min
Delta R.T.: 0.013 min
Response: 2682165
Conc: 17.09 ug/ml

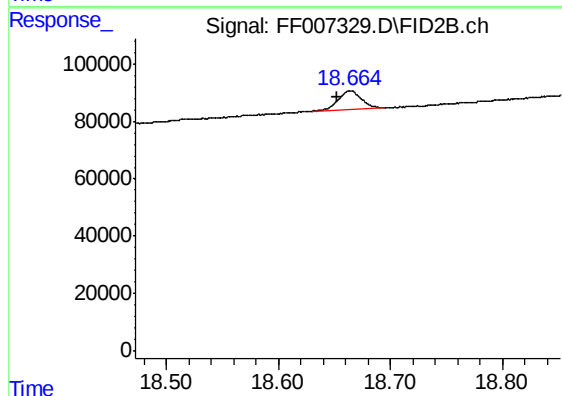

#14 N-DOTRIACONTANE

R.T.: 18.664 min
Delta R.T.: 0.011 min
Response: 89355
Conc: 0.60 ug/ml

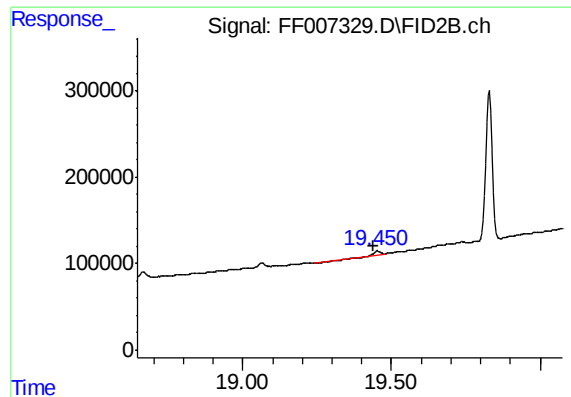

#15 N-TETRATRIACONTANE

R.T.: 19.451 min
Delta R.T.: 0.013 min
Response: 26535
Conc: 0.22 ug/ml

Instrument :
FID_F
ClientSampleId :
RT MARKER