

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF081120\
 Data File : FF007330.D
 Signal(s) : FID2B.ch
 Acq On : 11 Aug 2020 19:51
 Operator : DD\AJ
 Sample : L3637-09 5X
 Misc :
 ALS Vial : 61 Sample Multiplier: 1

Instrument :
 FID_F
 ClientSampleId :
 CAR-WASH-AREA-TPH-1

Integration File: autoint1.e
 Quant Time: Aug 13 01:38:56 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF072820.M
 Quant Title :
 QLast Update : Wed Jul 29 09:33:32 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.757	412346	3.021 ug/ml
Target Compounds			
4) N-TETRADECANE	8.351f	75249	0.517 ug/ml
8) N-DOCOSANE	13.882	157477	1.009 ug/ml
10) N-TETRACOSANE	14.949	355106	2.248 ug/ml
12) N-OCTACOSANE	16.956	208503	1.328 ug/ml
13) N-TRIACONTANE	17.831	246068	1.569 ug/ml
14) N-DOTRIACONTANE	18.667	116541	0.787 ug/ml
15) N-TETRATRIACONTANE	19.452	49307	0.408 ug/ml
16) N-HEXATRIACONTANE	20.168	73418	0.794 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF081120\
Data File : FF077330.D
Signal(s) : FID2B.ch
Acq On : 11 Aug 2020 19:51
Operator : DD\AJ
Sample : L3637-09 5X
Misc :
ALS Vial : 61 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :
CAR-WASH-AREA-TPH-1

Integration File: autoint1.e
Quant Time: Aug 13 01:38:56 2020
Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF072820.M
Quant Title :
QLast Update : Wed Jul 29 09:33:32 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

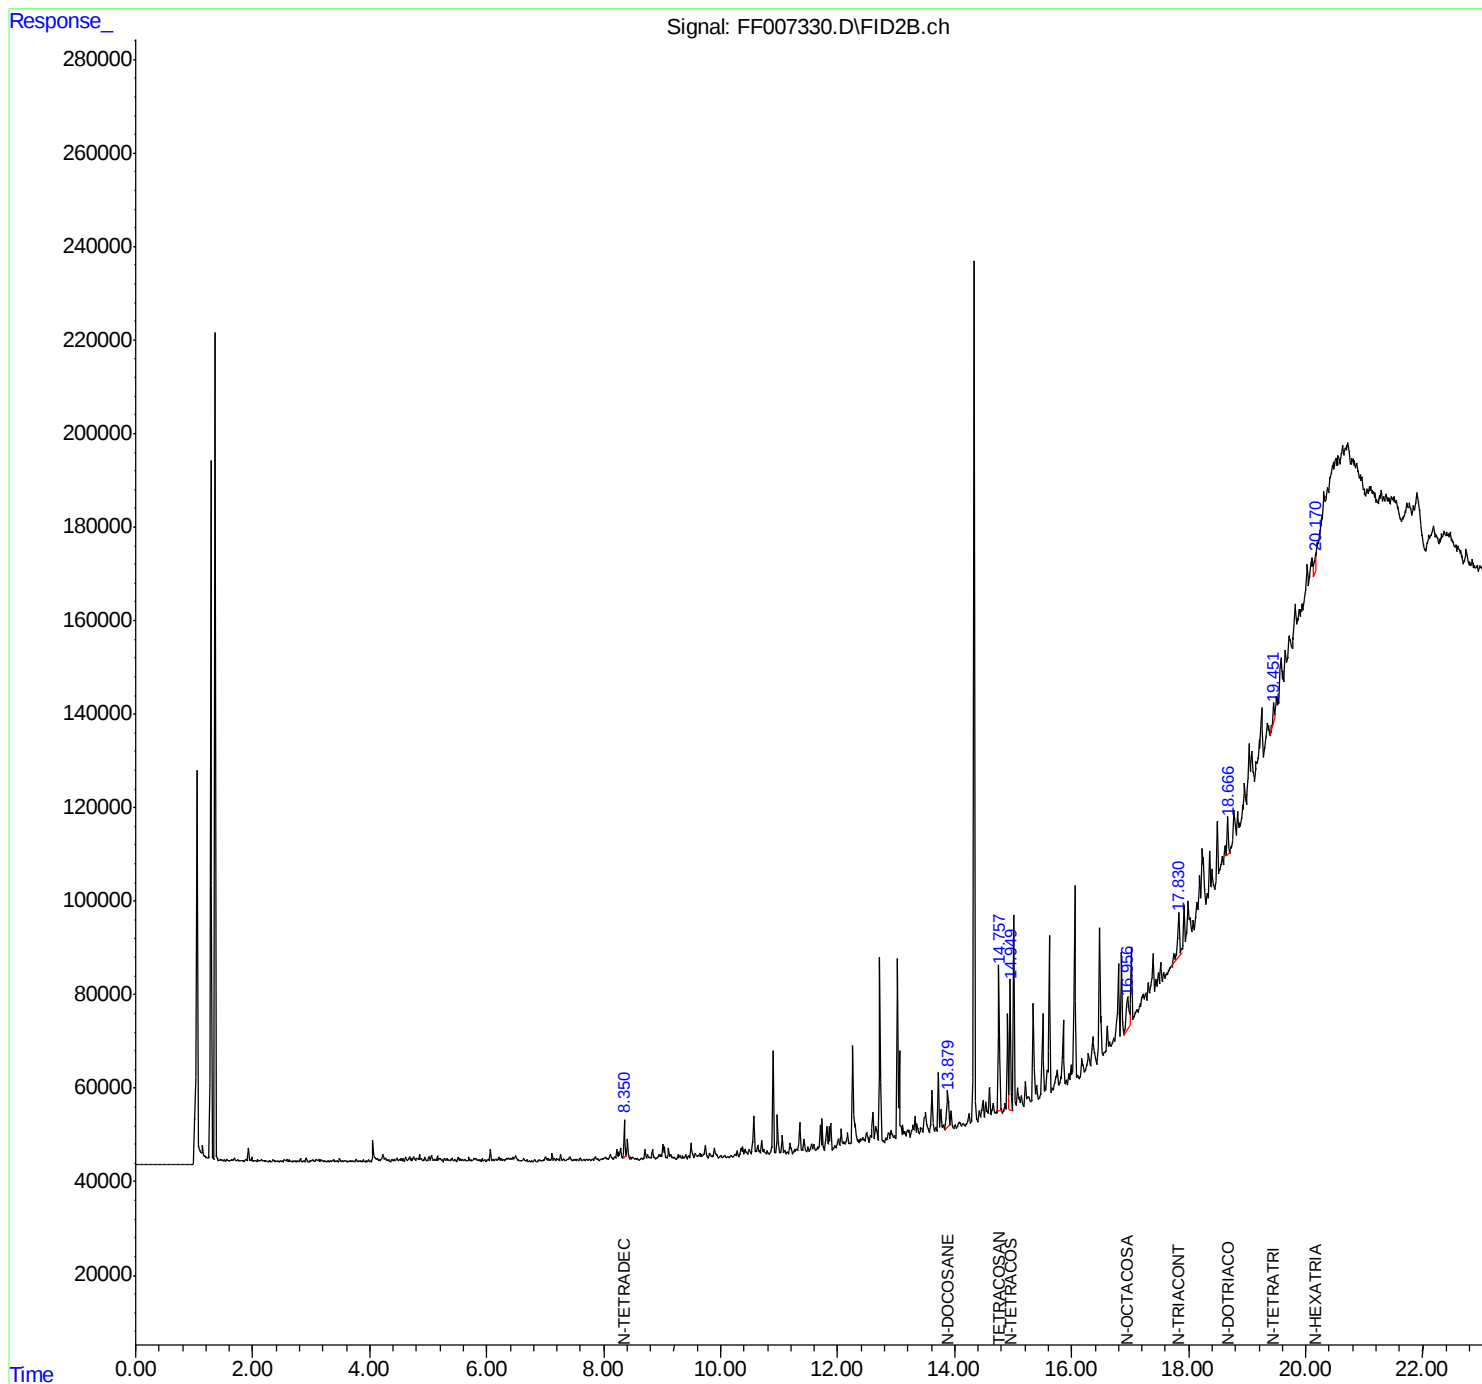


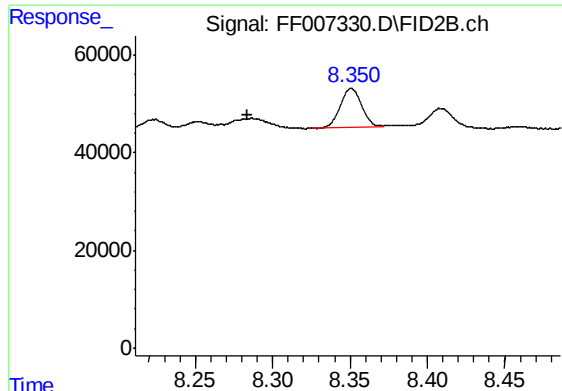

#4 N-TETRADECANE


R.T.: 8.351 min
Delta R.T.: 0.067 min
Response: 75249
Conc: 0.52 ug/ml

Instrument :
FID_F
ClientSampleId :
CAR-WASH-AREA-TPH-1

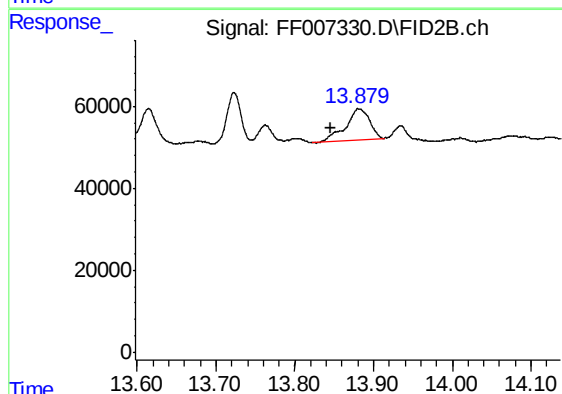


#8 N-DOCOSANE

R.T.: 13.882 min
Delta R.T.: 0.036 min
Response: 157477
Conc: 1.01 ug/ml

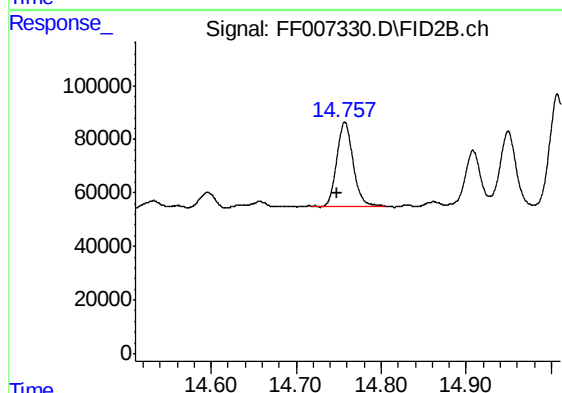


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.757 min
Delta R.T.: 0.010 min
Response: 412346
Conc: 3.02 ug/ml

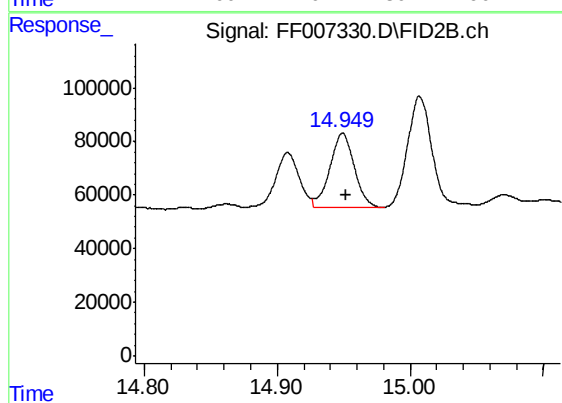

#10 N-TETRACOSANE


R.T.: 14.949 min
Delta R.T.: -0.002 min
Response: 355106
Conc: 2.25 ug/ml

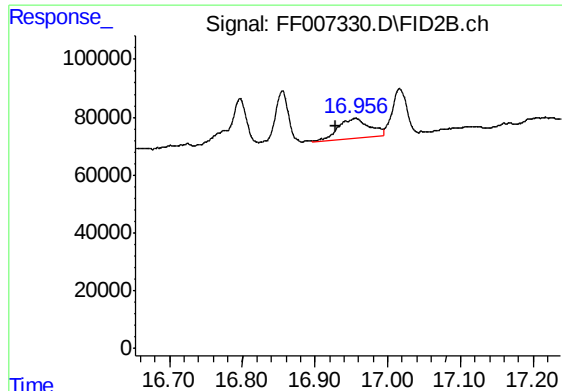

#12 N-OCTACOSANE


R.T.: 16.956 min
Delta R.T.: 0.027 min
Response: 208503
Conc: 1.33 ug/ml

Instrument :
FID_F
ClientSampleId :
CAR-WASH-AREA-TPH-1

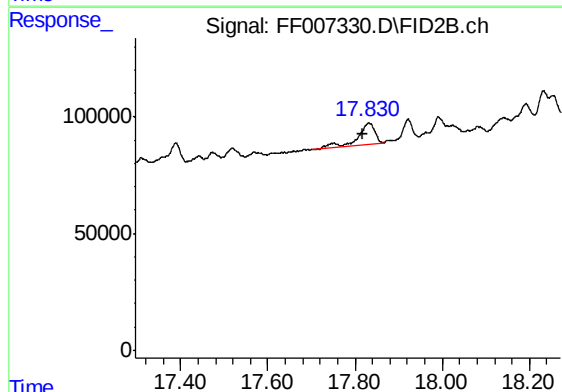


#13 N-TRIACONTANE

R.T.: 17.831 min
Delta R.T.: 0.013 min
Response: 246068
Conc: 1.57 ug/ml

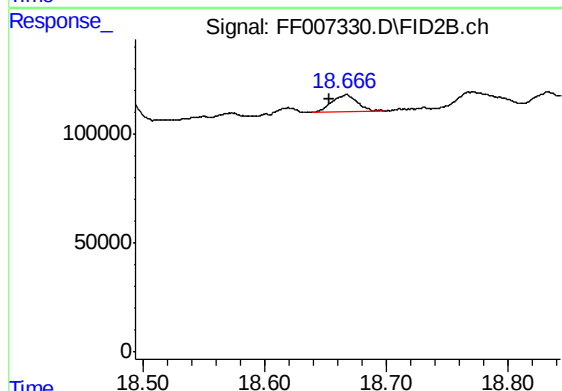


#14 N-DOTRIACONTANE

R.T.: 18.667 min
Delta R.T.: 0.014 min
Response: 116541
Conc: 0.79 ug/ml

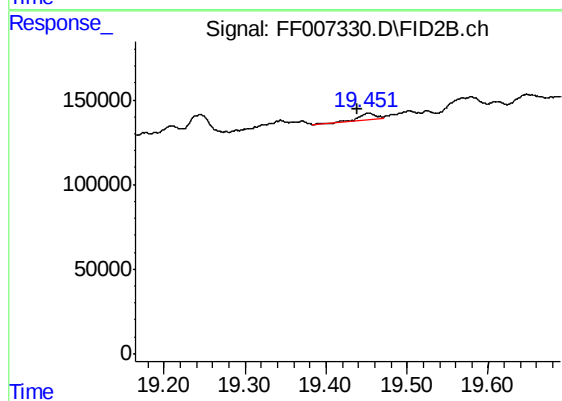

#15 N-TETRATRIACONTANE

R.T.: 19.452 min
Delta R.T.: 0.013 min
Response: 49307
Conc: 0.41 ug/ml

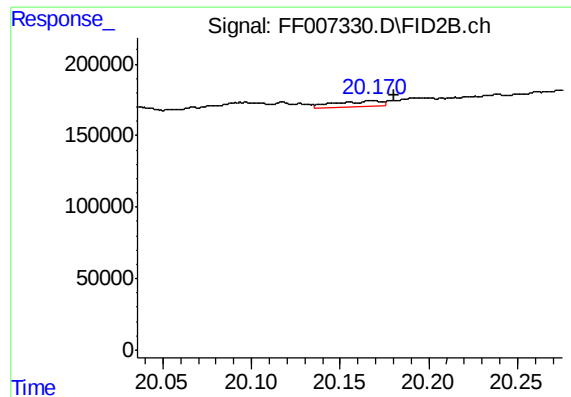

#16 N-HEXATRIACONTANE

R.T.: 20.168 min
Delta R.T.: -0.013 min
Response: 73418
Conc: 0.79 ug/ml

Instrument :
FID_F
ClientSampleId :
CAR-WASH-AREA-TPH-1