

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF081120\
Data File : FF007331.D
Signal(s) : FID2B.ch
Acq On : 11 Aug 2020 20:23
Operator : DD\AJ
Sample : L3637-10 10X
Misc :
ALS Vial : 62 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :
CAR-WASH-AREA-TPH-2

Integration File: autoint1.e
Quant Time: Aug 13 01:39:09 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF072820.M
Quant Title :
QLast Update : Wed Jul 29 09:33:32 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.757	205139	1.503 ug/ml
Target Compounds			
7) N-EICOSANE	12.606	112223	0.725 ug/ml
8) N-DOCOSANE	13.893	131636	0.843 ug/ml
10) N-TETRACOSANE	14.949	445989	2.824 ug/ml
12) N-OCTACOSANE	16.956	141164	0.899 ug/ml
13) N-TRIACONTANE	17.833	147343	0.939 ug/ml
14) N-DOTRIACONTANE	18.666	88416	0.597 ug/ml
15) N-TETRATRIACONTANE	19.502f	532574	4.404 ug/ml
16) N-HEXATRIACONTANE	20.120f	209285	2.263 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF081120\
Data File : FF07331.D
Signal(s) : FID2B.ch
Acq On : 11 Aug 2020 20:23
Operator : DD\AJ
Sample : L3637-10 10X
Misc :
ALS Vial : 62 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :
CAR-WASH-AREA-TPH-2

Integration File: autoint1.e
Quant Time: Aug 13 01:39:09 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF072820.M
Quant Title :
QLast Update : Wed Jul 29 09:33:32 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

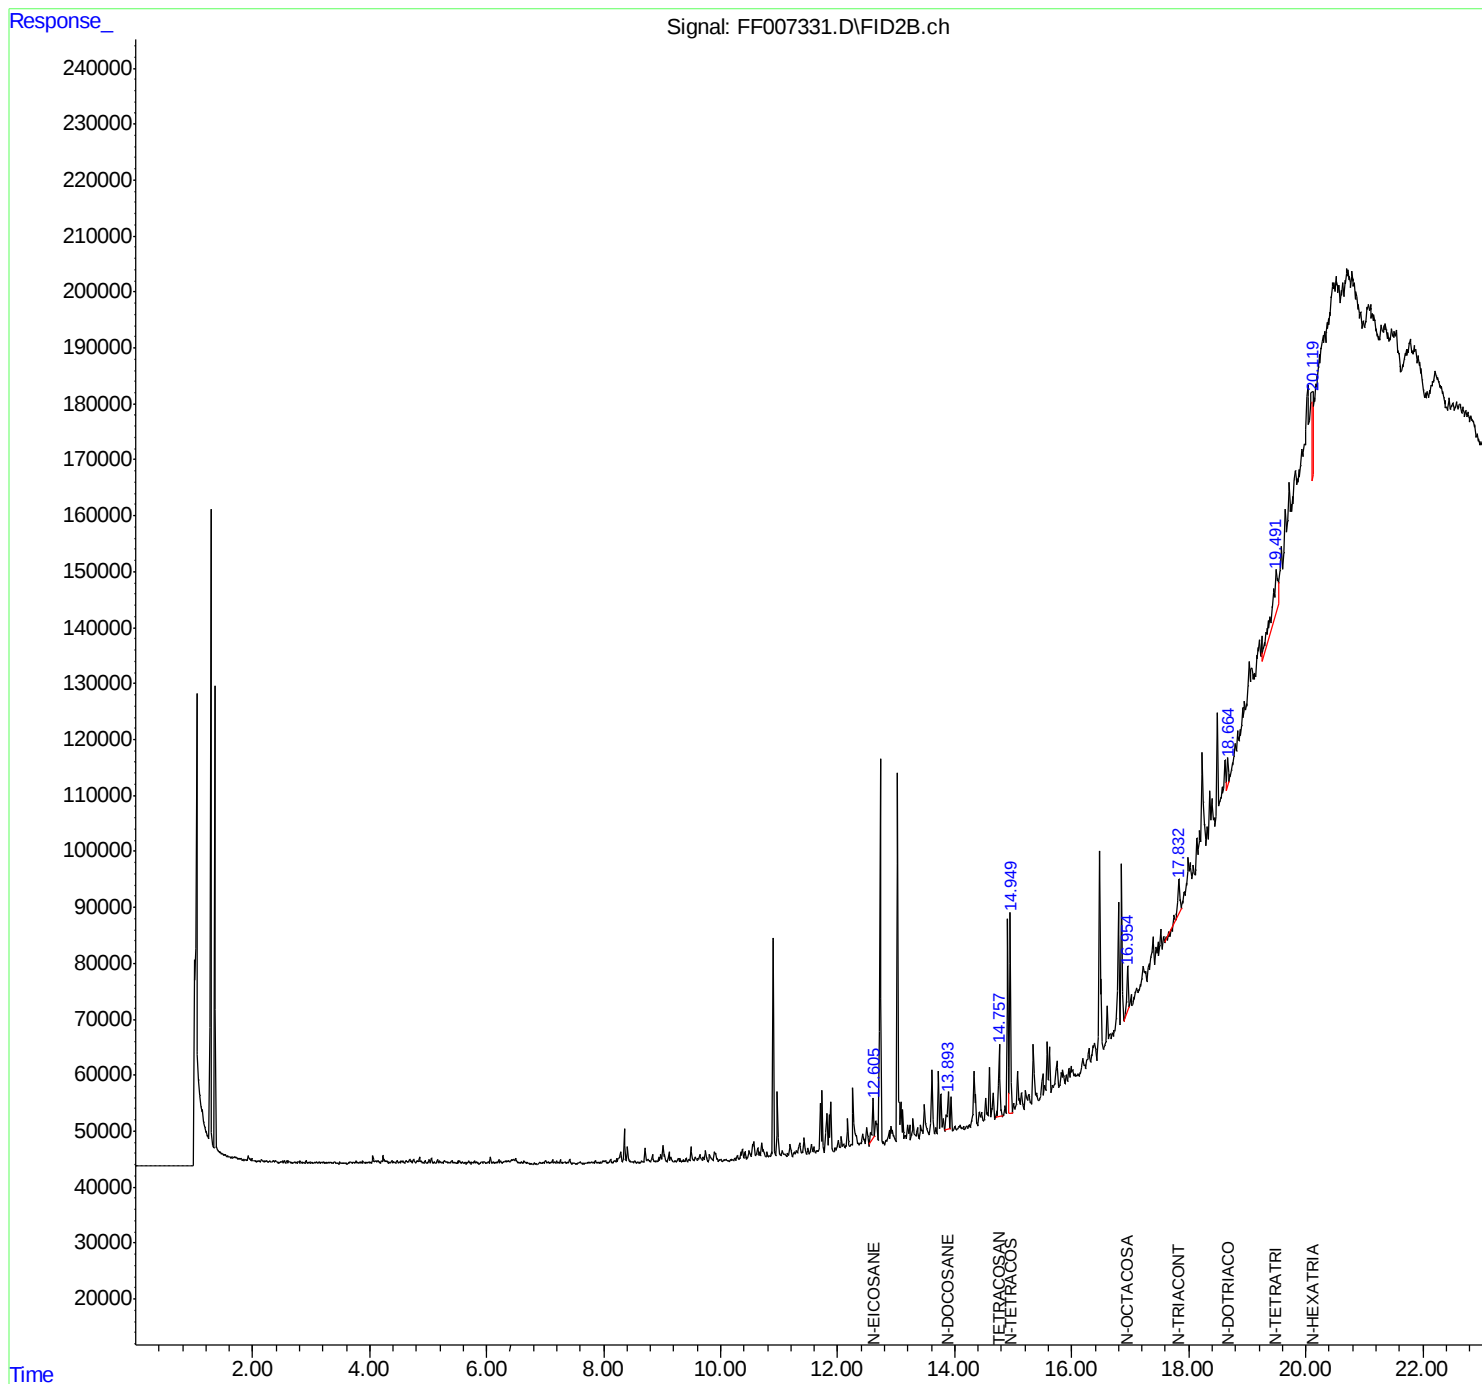


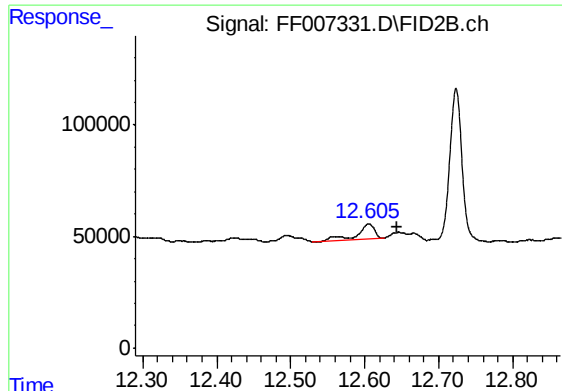

#7 N-EICOSANE


R.T.: 12.606 min
Delta R.T.: -0.038 min
Response: 112223
Conc: 0.73 ug/ml

Instrument :
FID_F
ClientSampleId :
CAR-WASH-AREA-TPH-2

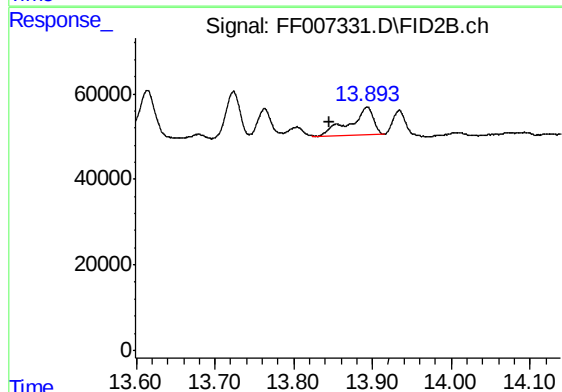


#8 N-DOCOSANE

R.T.: 13.893 min
Delta R.T.: 0.048 min
Response: 131636
Conc: 0.84 ug/ml

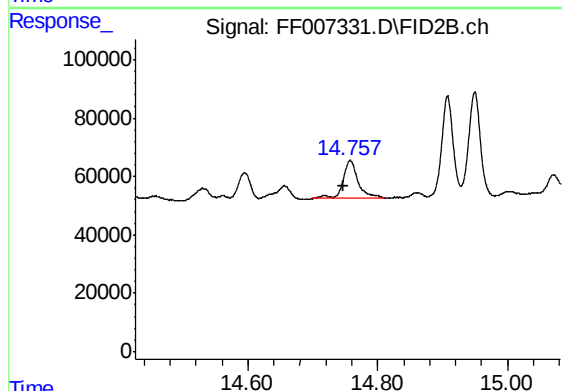


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.757 min
Delta R.T.: 0.010 min
Response: 205139
Conc: 1.50 ug/ml

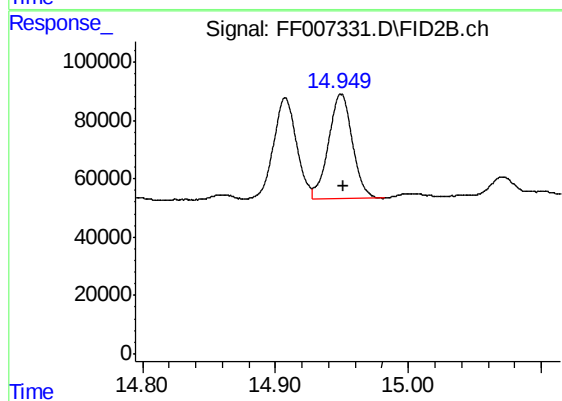

#10 N-TETRACOSANE


R.T.: 14.949 min
Delta R.T.: -0.002 min
Response: 445989
Conc: 2.82 ug/ml

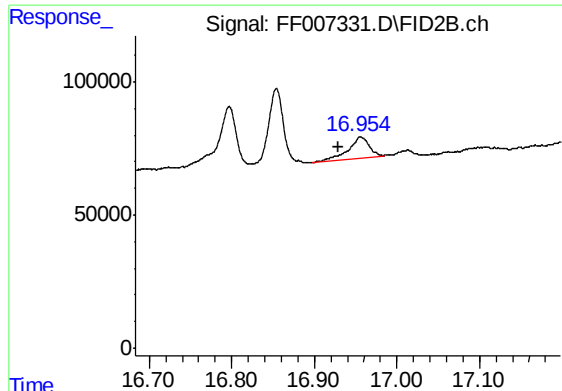

#12 N-OCTACOSANE


R.T.: 16.956 min
Delta R.T.: 0.028 min
Response: 141164
Conc: 0.90 ug/ml

Instrument :
FID_F
ClientSampleId :
CAR-WASH-AREA-TPH-2

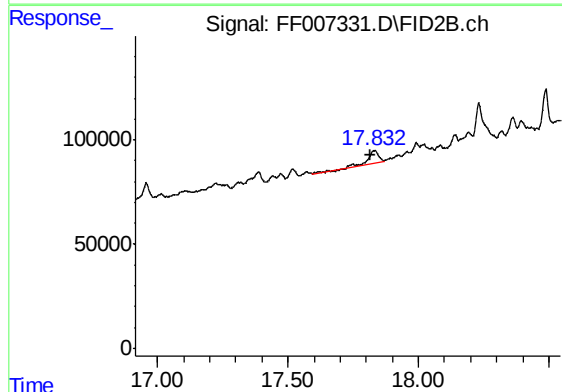


#13 N-TRIACONTANE

R.T.: 17.833 min
Delta R.T.: 0.015 min
Response: 147343
Conc: 0.94 ug/ml

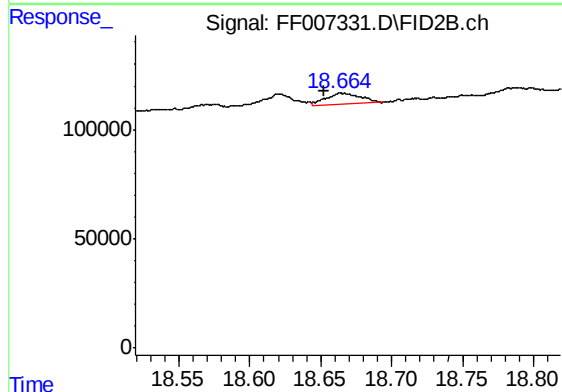


#14 N-DOTRIACONTANE

R.T.: 18.666 min
Delta R.T.: 0.013 min
Response: 88416
Conc: 0.60 ug/ml

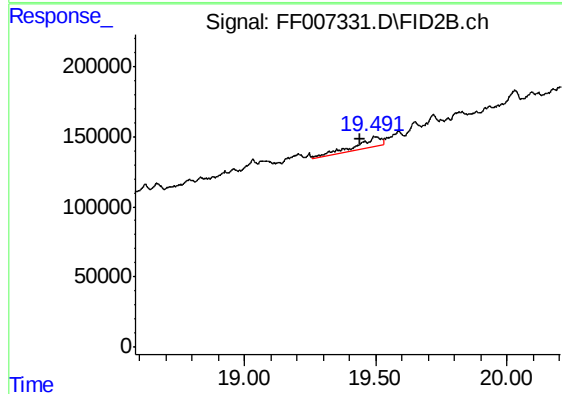

#15 N-TETRATRIACONTANE

R.T.: 19.502 min
Delta R.T.: 0.063 min
Response: 532574
Conc: 4.40 ug/ml

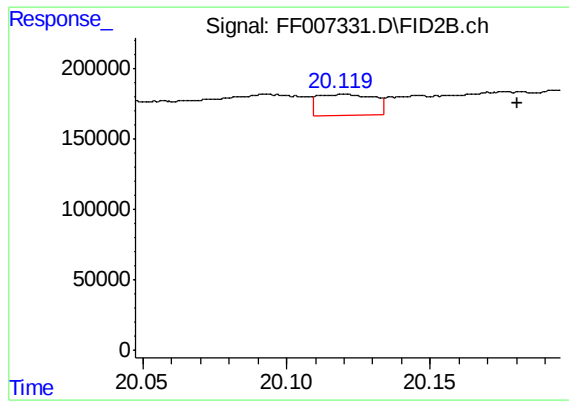

#16 N-HEXATRIACONTANE

R.T.: 20.120 min
Delta R.T.: -0.061 min
Response: 209285
Conc: 2.26 ug/ml

Instrument :
FID_F
ClientSampleId :
CAR-WASH-AREA-TPH-2