

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF081120\
 Data File : FF007332.D
 Signal(s) : FID2B.ch
 Acq On : 11 Aug 2020 20:54
 Operator : DD\AJ
 Sample : L3637-11 5X
 Misc :
 ALS Vial : 63 Sample Multiplier: 1

Instrument :
 FID_F
 ClientSampleId :
 CAR-WASH-AREA-TPH-3

Integration File: autoint1.e
 Quant Time: Aug 13 01:39:22 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF072820.M
 Quant Title :
 QLast Update : Wed Jul 29 09:33:32 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.756	438141	3.210 ug/ml
Target Compounds			
4) N-TETRADECANE	8.351f	62747	0.431 ug/ml
10) N-TETRACOSANE	14.948	296010	1.874 ug/ml
12) N-OCTACOSANE	16.957	116262	0.741 ug/ml
13) N-TRIACONTANE	17.834	277471	1.769 ug/ml
14) N-DOTRIACONTANE	18.663	135418	0.914 ug/ml
15) N-TETRATRIACONTANE	19.455	91265	0.755 ug/ml
16) N-HEXATRIACONTANE	20.132	82850	0.896 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF081120\
Data File : FF007332.D
Signal(s) : FID2B.ch
Acq On : 11 Aug 2020 20:54
Operator : DD\AJ
Sample : L3637-11 5X
Misc :
ALS Vial : 63 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :
CAR-WASH-AREA-TPH-3

Integration File: autoint1.e
Quant Time: Aug 13 01:39:22 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF072820.M
Quant Title :
QLast Update : Wed Jul 29 09:33:32 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

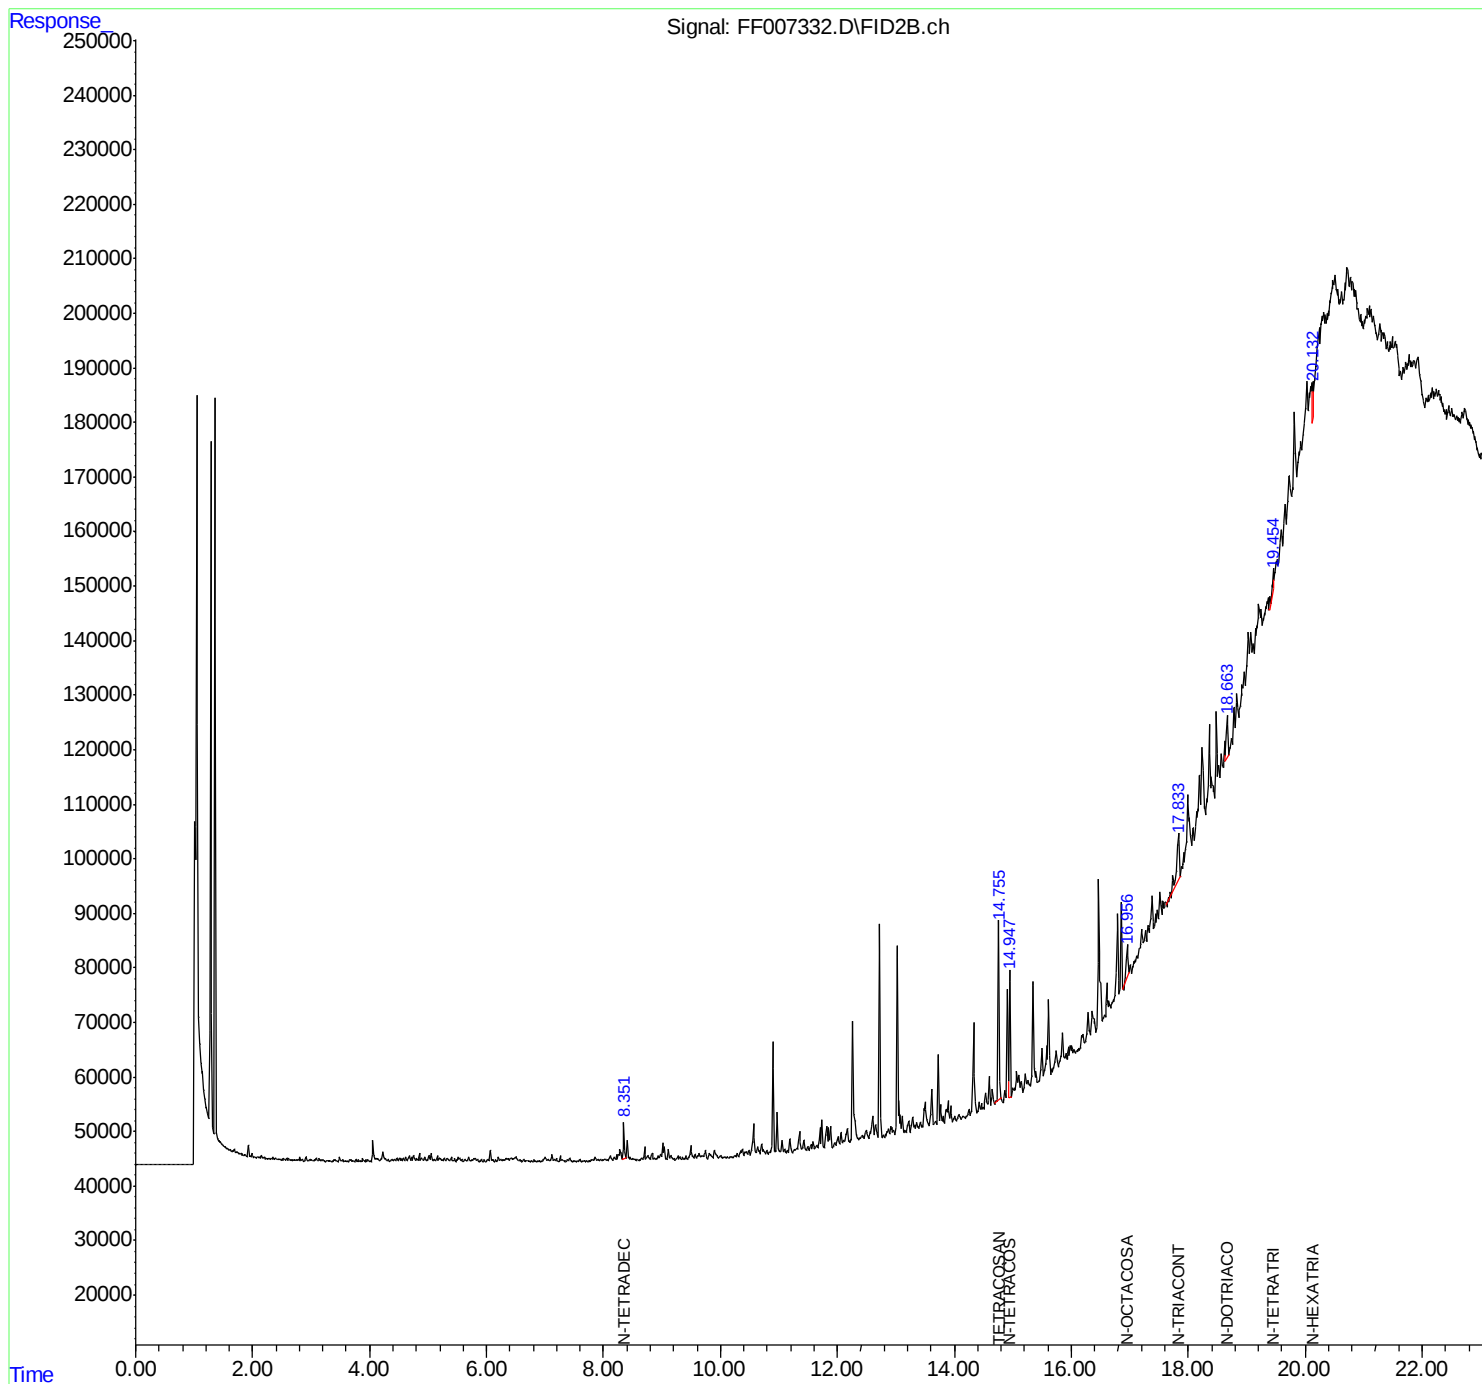


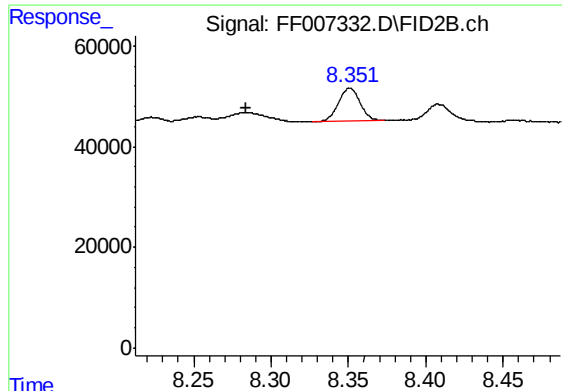

#4 N-TETRADECANE


R.T.: 8.351 min
Delta R.T.: 0.067 min
Response: 62747
Conc: 0.43 ug/ml

Instrument :
FID_F
ClientSampleId :
CAR-WASH-AREA-TPH-3

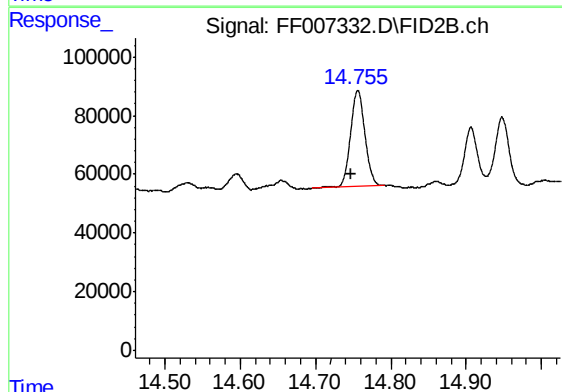


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.756 min
Delta R.T.: 0.008 min
Response: 438141
Conc: 3.21 ug/ml

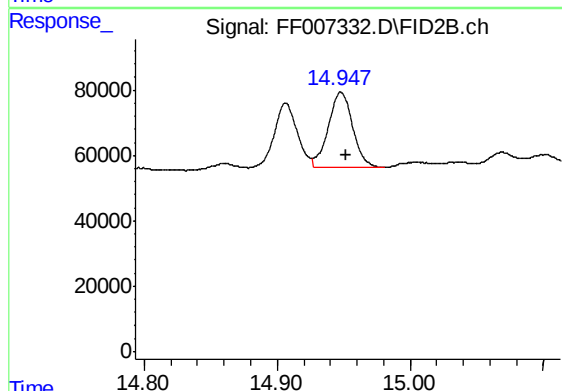


#10 N-TETRACOSANE

R.T.: 14.948 min
Delta R.T.: -0.004 min
Response: 296010
Conc: 1.87 ug/ml

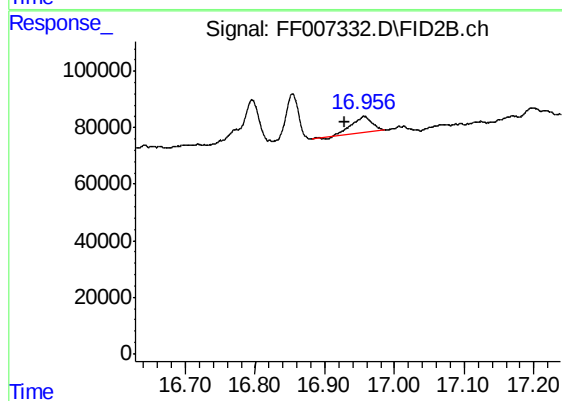

#12 N-OCTACOSANE


R.T.: 16.957 min
Delta R.T.: 0.029 min
Response: 116262
Conc: 0.74 ug/ml

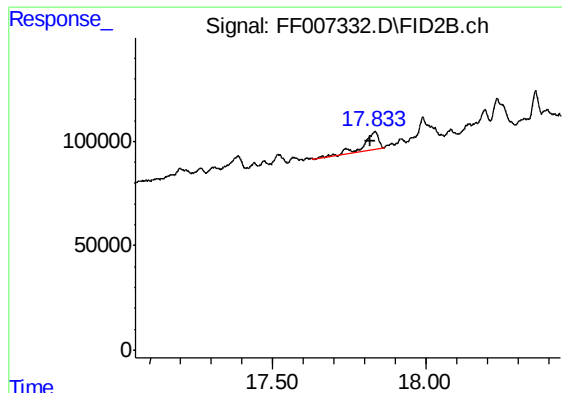

#13 N-TRIACONTANE


R.T.: 17.834 min
Delta R.T.: 0.016 min
Response: 277471
Conc: 1.77 ug/ml

Instrument :
FID_F
ClientSampleId :
CAR-WASH-AREA-TPH-3

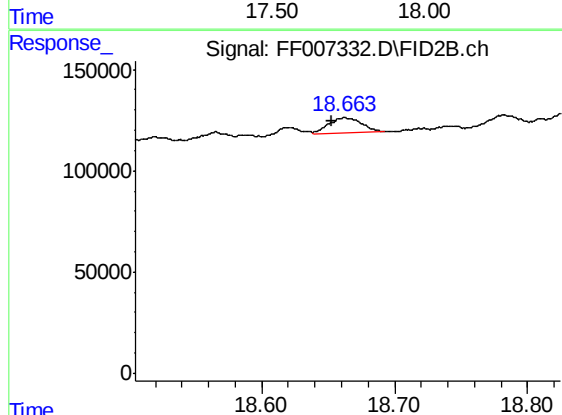


#14 N-DOTRIACONTANE

R.T.: 18.663 min
Delta R.T.: 0.010 min
Response: 135418
Conc: 0.91 ug/ml

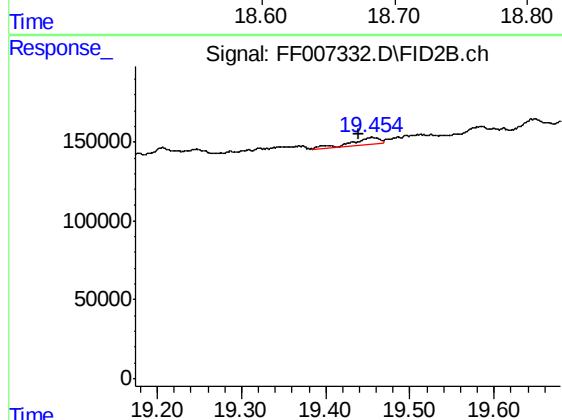

#15 N-TETRATRIACONTANE

R.T.: 19.455 min
Delta R.T.: 0.017 min
Response: 91265
Conc: 0.75 ug/ml

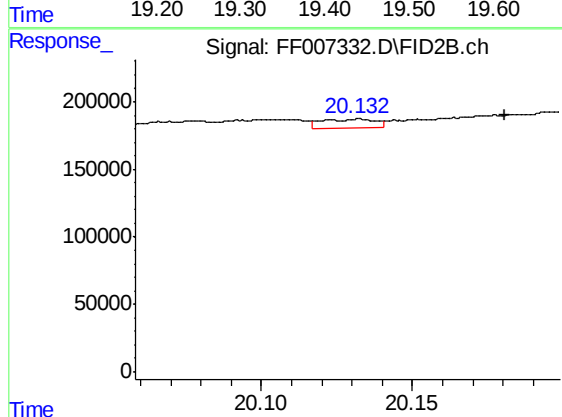

#16 N-HEXATRIACONTANE

R.T.: 20.132 min
Delta R.T.: -0.048 min
Response: 82850
Conc: 0.90 ug/ml