

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF081120\
Data File : FF007336.D
Signal(s) : FID2B.ch
Acq On : 11 Aug 2020 22:59
Operator : DD\AJ
Sample : L3637-17 5X
Misc :
ALS Vial : 67 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :
CAR-WASH-AREA-2-TPH-3

Integration File: autoint1.e
Quant Time: Aug 13 01:40:14 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF072820.M
Quant Title :
QLast Update : Wed Jul 29 09:33:32 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.757	488203	3.577 ug/ml
Target Compounds			
4) N-TETRADECANE	8.351f	99597	0.684 ug/ml
10) N-TETRACOSANE	14.948	219860	1.392 ug/ml
11) N-HEXACOSANE	15.999	309777	1.976 ug/ml
13) N-TRIACONTANE	17.830	191910	1.224 ug/ml
14) N-DOTRIACONTANE	18.665	114680	0.774 ug/ml
16) N-HEXATRIACONTANE	20.223	639103	6.909 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF081120\
Data File : FF007336.D
Signal(s) : FID2B.ch
Acq On : 11 Aug 2020 22:59
Operator : DD\AJ
Sample : L3637-17 5X
Misc :
ALS Vial : 67 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :
CAR-WASH-AREA-2-TPH-3

Integration File: autoint1.e
Quant Time: Aug 13 01:40:14 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF072820.M
Quant Title :
QLast Update : Wed Jul 29 09:33:32 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rx1-1ms
Signal Info : 20mx0.18mmx0.18um

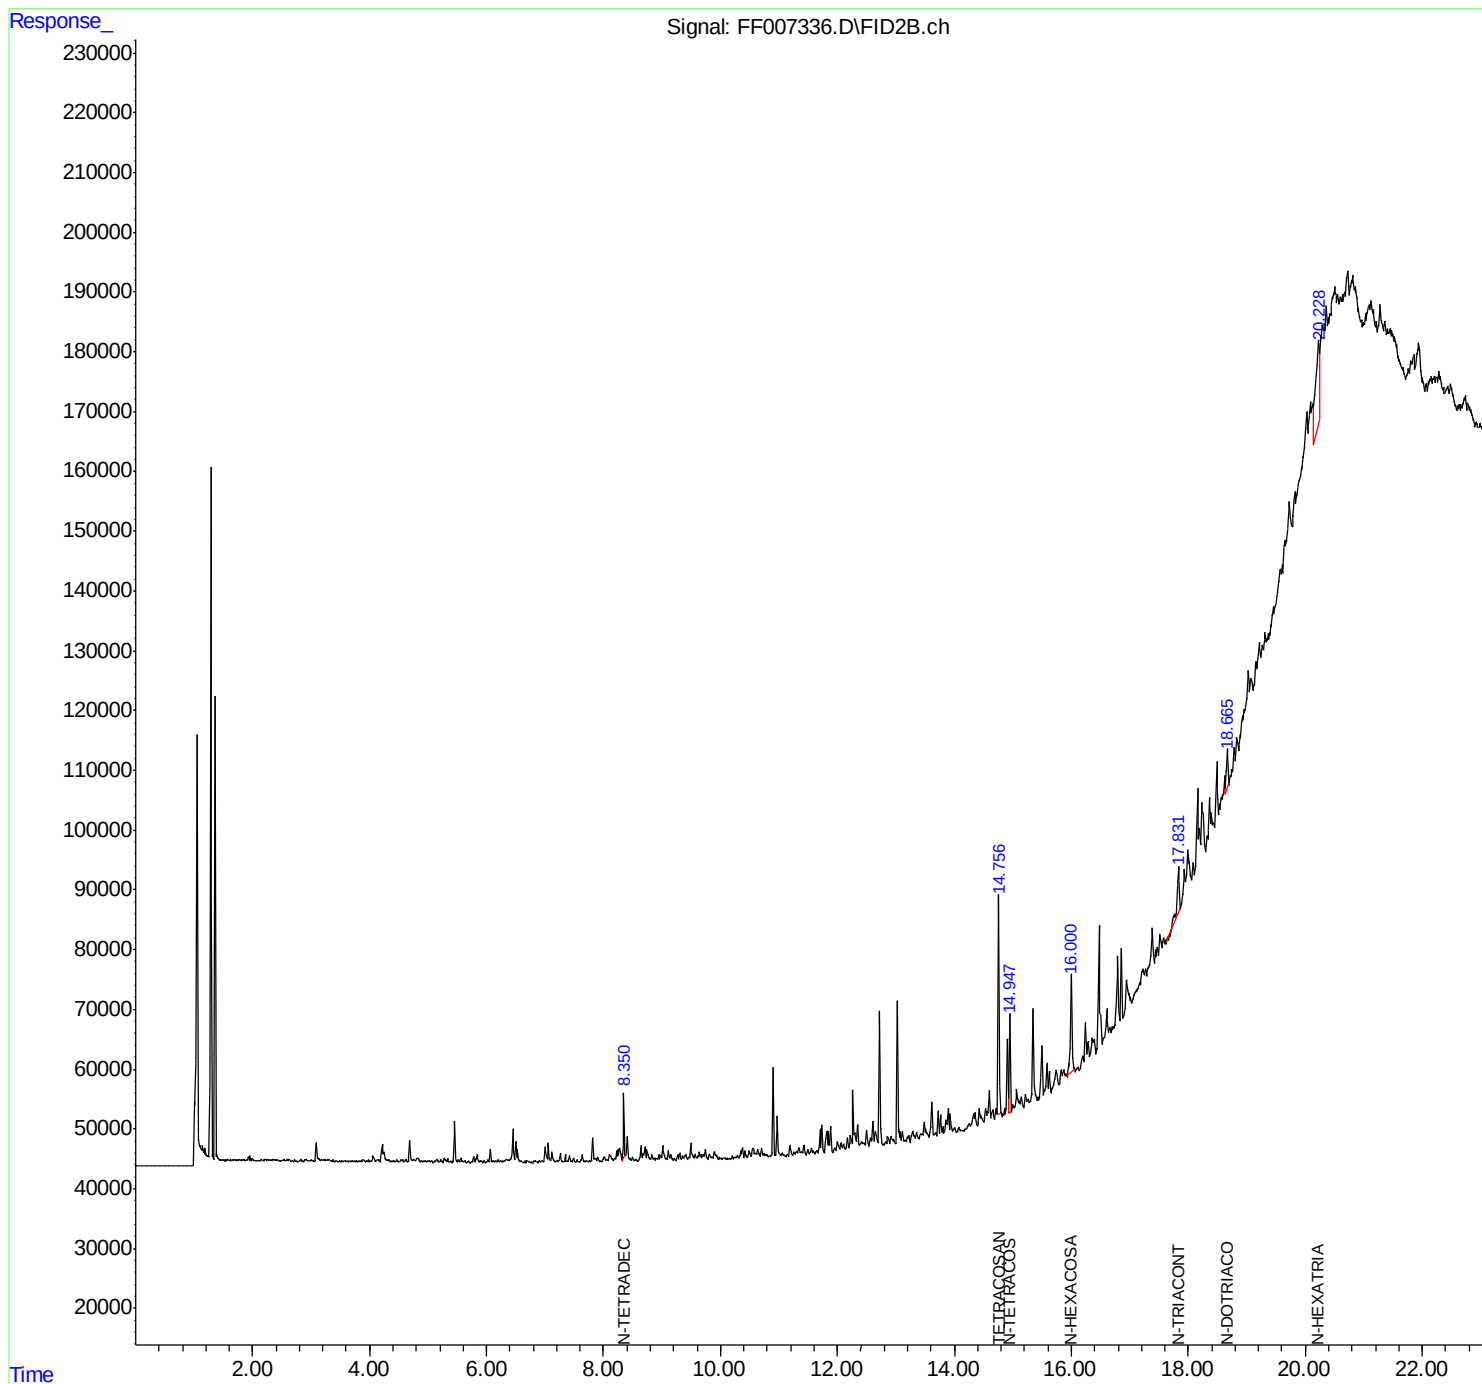


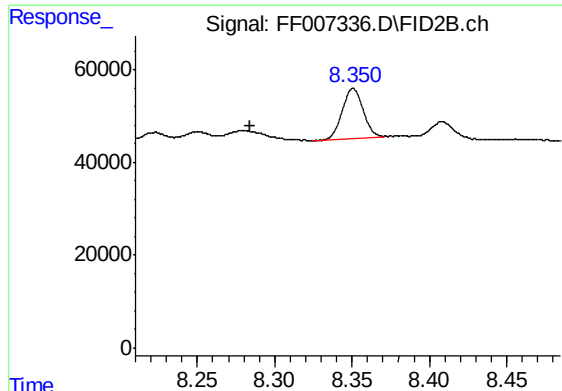

#4 N-TETRADECANE


R.T.: 8.351 min
Delta R.T.: 0.067 min
Response: 99597
Conc: 0.68 ug/ml

Instrument :
FID_F
ClientSampleId :
CAR-WASH-AREA-2-TPH-3

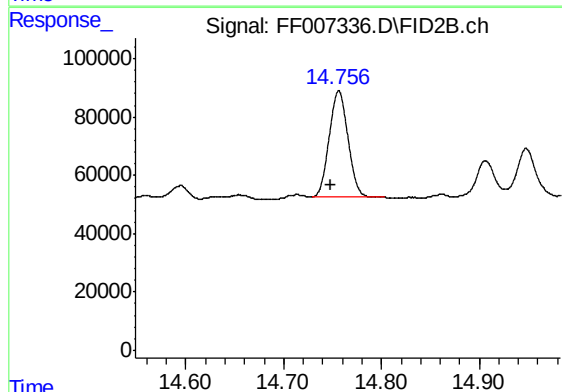


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.757 min
Delta R.T.: 0.009 min
Response: 488203
Conc: 3.58 ug/ml

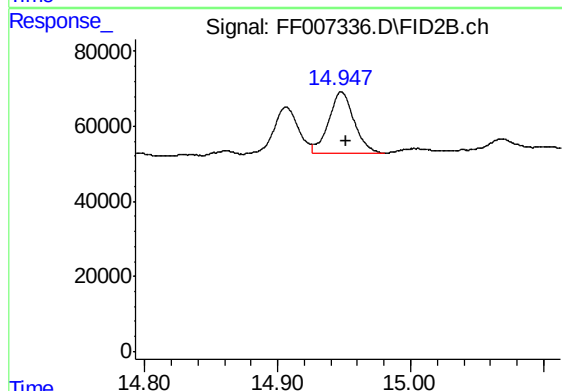


#10 N-TETRACOSANE

R.T.: 14.948 min
Delta R.T.: -0.004 min
Response: 219860
Conc: 1.39 ug/ml

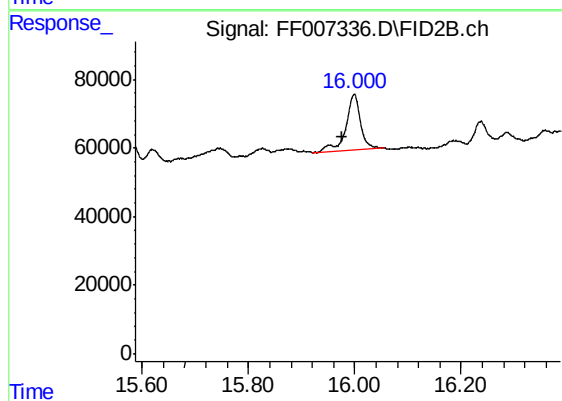

#11 N-HEXACOSANE


R.T.: 15.999 min
Delta R.T.: 0.024 min
Response: 309777
Conc: 1.98 ug/ml

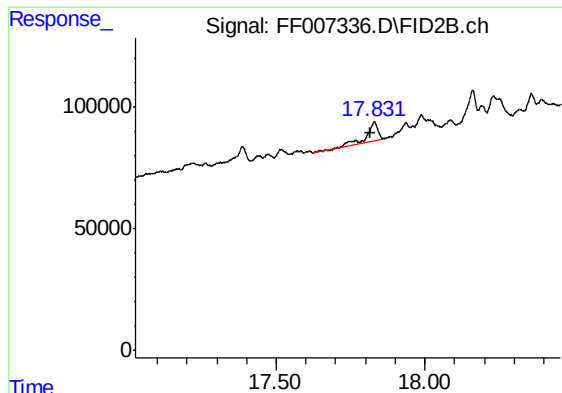

#13 N-TRIACONTANE


R.T.: 17.830 min
Delta R.T.: 0.013 min
Response: 191910
Conc: 1.22 ug/ml

Instrument :
FID_F
ClientSampleId :
CAR-WASH-AREA-2-TPH-3

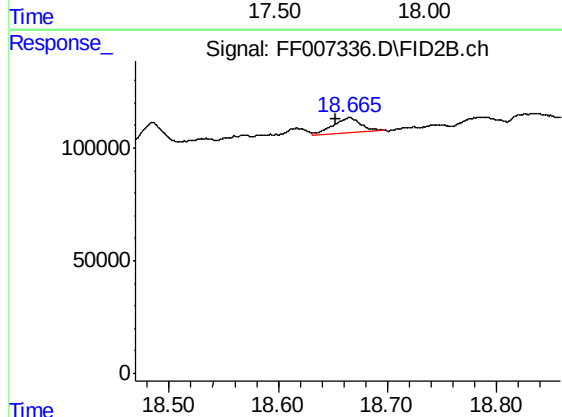

#14 N-DOTRIACONTANE

R.T.: 18.665 min
Delta R.T.: 0.013 min
Response: 114680
Conc: 0.77 ug/ml

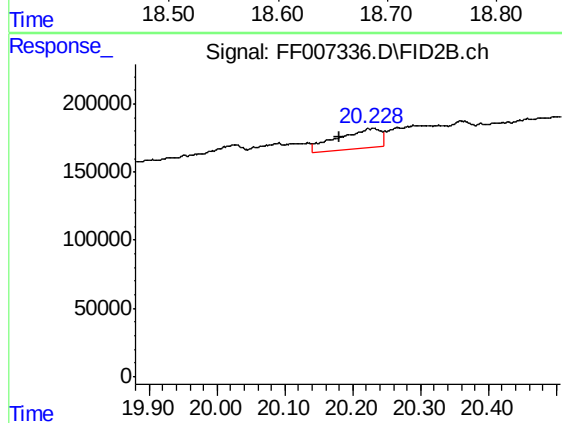

#16 N-HEXATRIACONTANE

R.T.: 20.223 min
Delta R.T.: 0.042 min
Response: 639103
Conc: 6.91 ug/ml