

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF081120\
 Data File : FF007337.D
 Signal(s) : FID2B.ch
 Acq On : 11 Aug 2020 23:30
 Operator : DD\AJ
 Sample : L3637-18 5X
 Misc :
 ALS Vial : 68 Sample Multiplier: 1

Instrument :
 FID_F
 ClientSampleId :
 CAR-WASH-AREA-2-TPH-4

Integration File: autoint1.e
 Quant Time: Aug 13 01:40:26 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF072820.M
 Quant Title :
 QLast Update : Wed Jul 29 09:33:32 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.755	463838	3.398 ug/ml
Target Compounds			
4) N-TETRADECANE	8.350f	93850	0.645 ug/ml
10) N-TETRACOSANE	14.948	353260	2.237 ug/ml
12) N-OCTACOSANE	16.953	146872	0.936 ug/ml
13) N-TRIACONTANE	17.828	183401	1.169 ug/ml
14) N-DOTRIACONTANE	18.664	125944	0.850 ug/ml
15) N-TETRATRIACONTANE	19.449	24879	0.206 ug/ml
16) N-HEXATRIACONTANE	20.227	294236	3.181 ug/ml
18) N-TETRACONTANE	21.917	912303	13.641 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF081120\
Data File : FF007337.D
Signal(s) : FID2B.ch
Acq On : 11 Aug 2020 23:30
Operator : DD\AJ
Sample : L3637-18 5X
Misc :
ALS Vial : 68 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :
CAR-WASH-AREA-2-TPH-4

Integration File: autoint1.e
Quant Time: Aug 13 01:40:26 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF072820.M
Quant Title :
QLast Update : Wed Jul 29 09:33:32 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rx1-1ms
Signal Info : 20mx0.18mmx0.18um

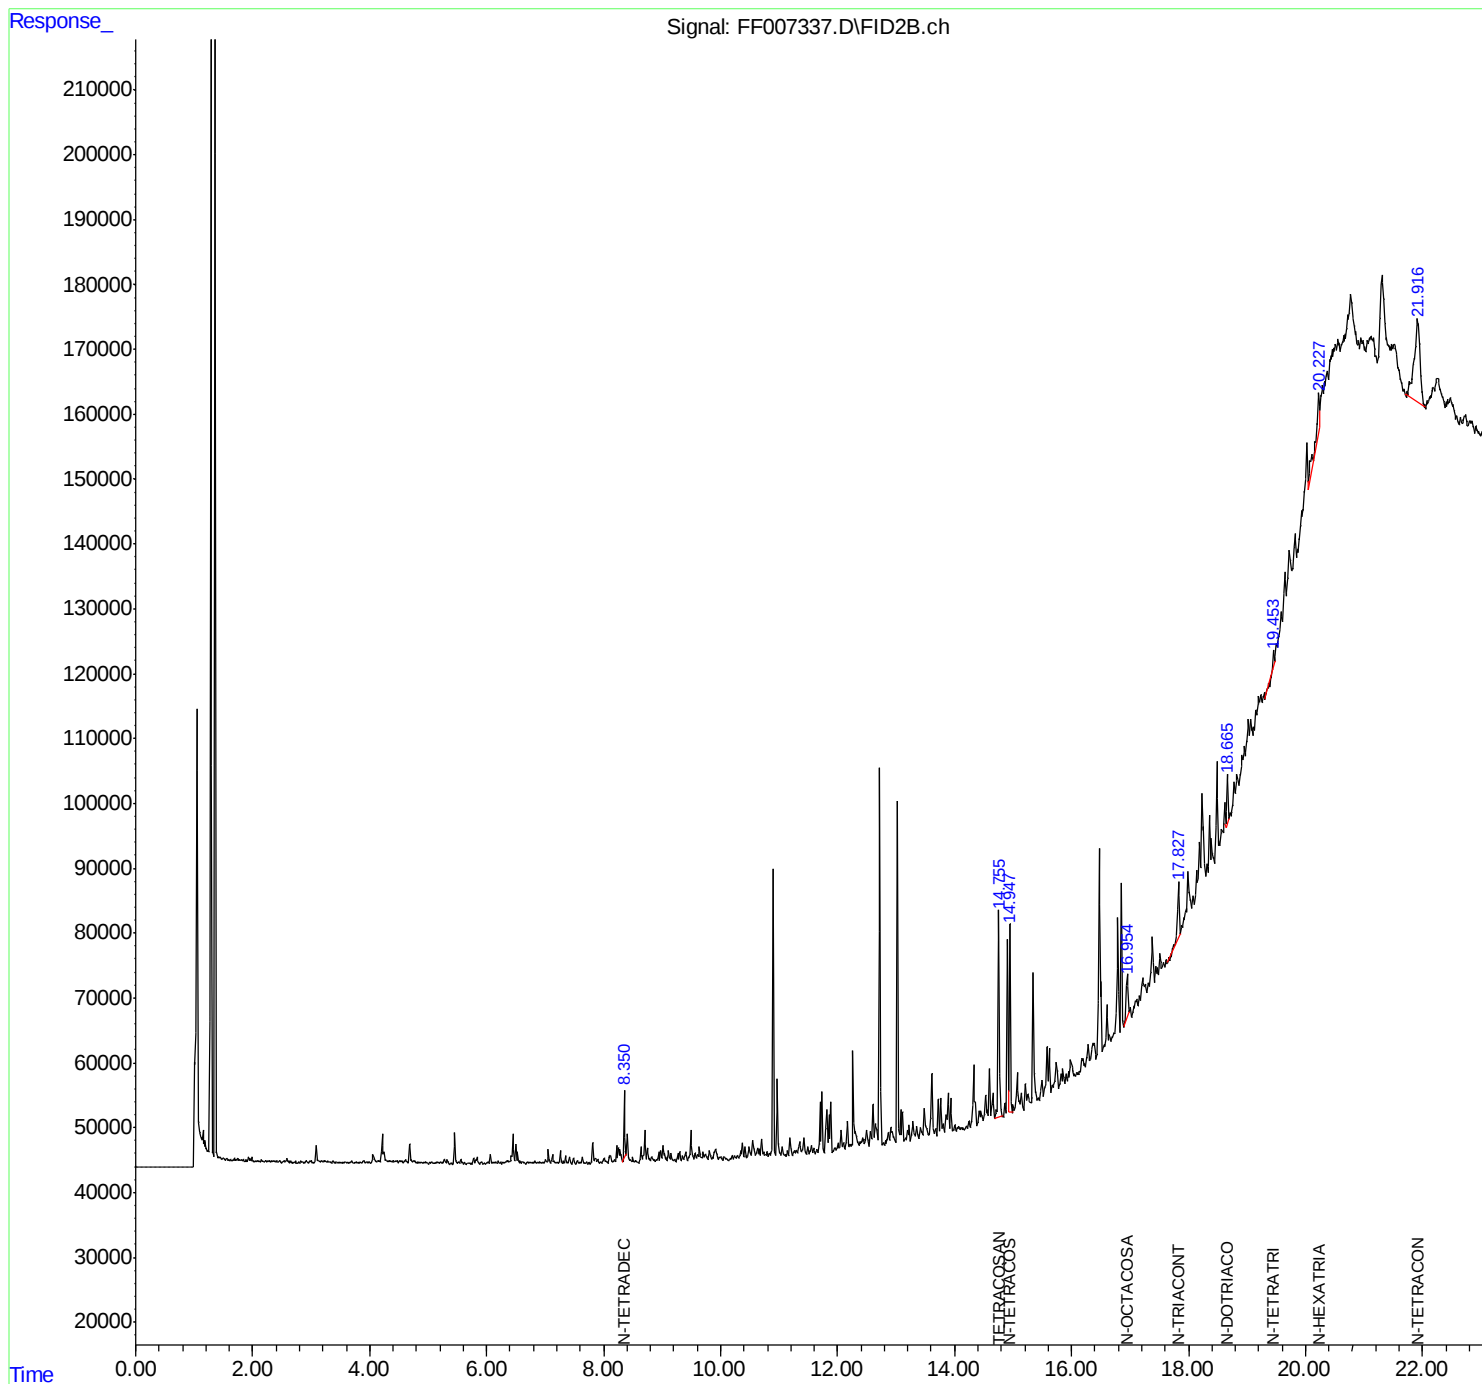


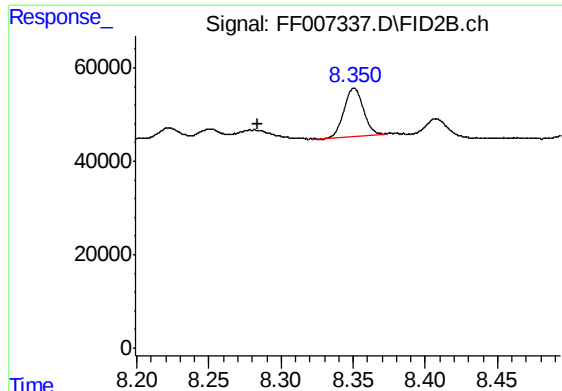

#4 N-TETRADECANE


R.T.: 8.350 min
Delta R.T.: 0.066 min
Response: 93850
Conc: 0.64 ug/ml

Instrument :
FID_F
ClientSampleId :
CAR-WASH-AREA-2-TPH-4

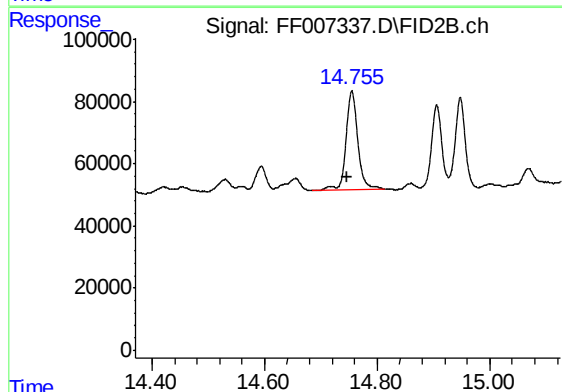


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.755 min
Delta R.T.: 0.007 min
Response: 463838
Conc: 3.40 ug/ml

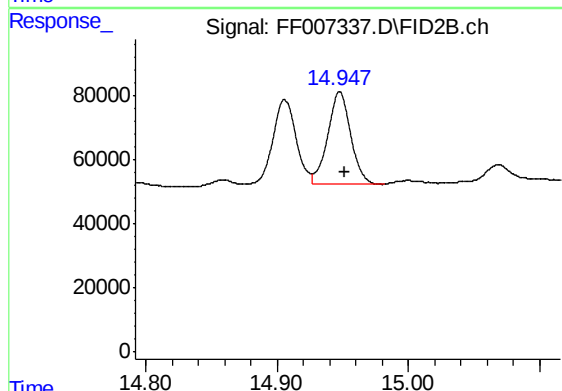


#10 N-TETRACOSANE

R.T.: 14.948 min
Delta R.T.: -0.004 min
Response: 353260
Conc: 2.24 ug/ml

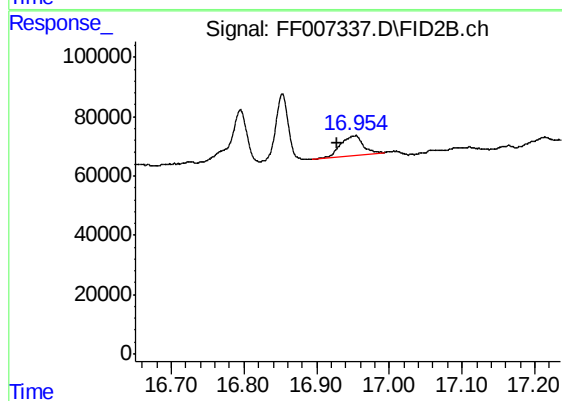

#12 N-OCTACOSANE


R.T.: 16.953 min
Delta R.T.: 0.025 min
Response: 146872
Conc: 0.94 ug/ml

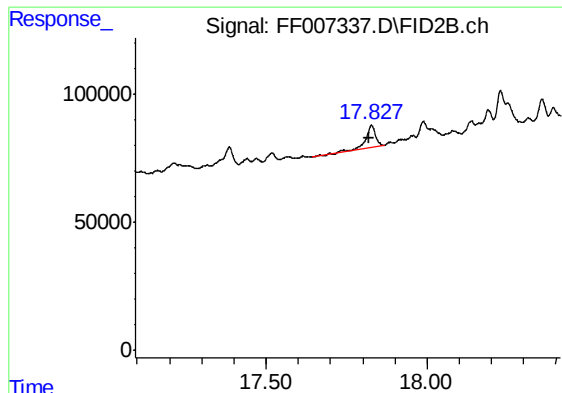

#13 N-TRIACONTANE


R.T.: 17.828 min
Delta R.T.: 0.010 min
Response: 183401
Conc: 1.17 ug/ml

Instrument :
FID_F
ClientSampleId :
CAR-WASH-AREA-2-TPH-4

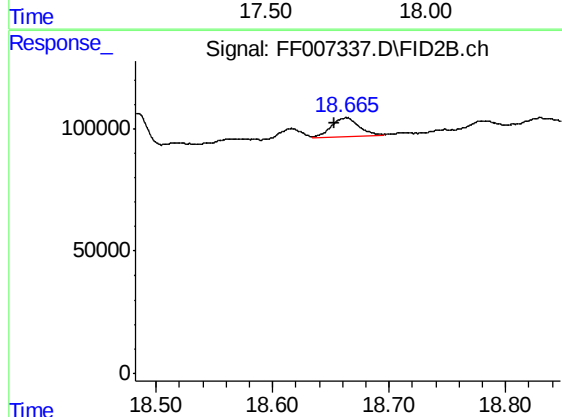


#14 N-DOTRIACONTANE

R.T.: 18.664 min
Delta R.T.: 0.011 min
Response: 125944
Conc: 0.85 ug/ml

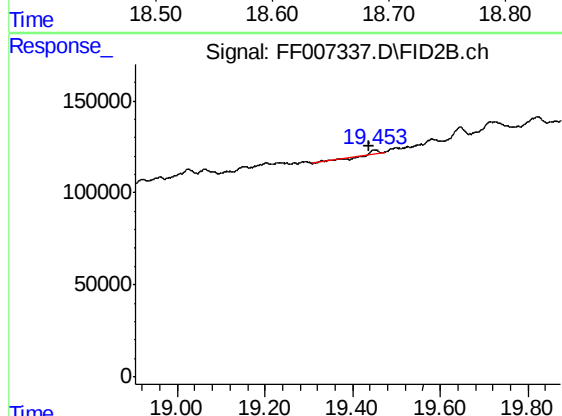


#15 N-TETRATRIACONTANE

R.T.: 19.449 min
Delta R.T.: 0.011 min
Response: 24879
Conc: 0.21 ug/ml

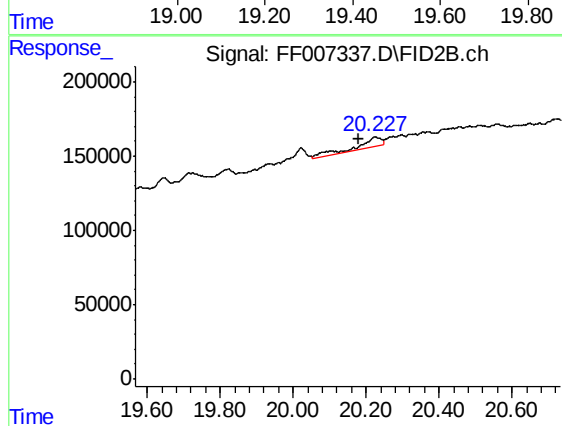

#16 N-HEXATRIACONTANE

R.T.: 20.227 min
Delta R.T.: 0.046 min
Response: 294236
Conc: 3.18 ug/ml

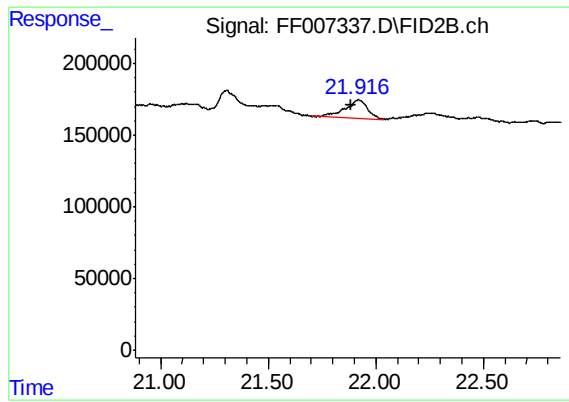

#18 N-TETRACONTANE

R.T.: 21.917 min
Delta R.T.: 0.030 min
Response: 912303
Conc: 13.64 ug/ml

Instrument :
FID_F
ClientSampleId :
CAR-WASH-AREA-2-TPH-4