

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF081120\
 Data File : FF007338.D
 Signal(s) : FID2B.ch
 Acq On : 12 Aug 2020 00:01
 Operator : DD\AJ
 Sample : L3637-21 5X
 Misc :
 ALS Vial : 69 Sample Multiplier: 1

Instrument :
 FID_F
 ClientSampleId :
 CAR-WASH-AREA-3-TPH-1

Integration File: autoint1.e
 Quant Time: Aug 13 01:40:39 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF072820.M
 Quant Title :
 QLast Update : Wed Jul 29 09:33:32 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.754	512371	3.754 ug/ml
Target Compounds			
4) N-TETRADECANE	8.222f	65480	0.450 ug/ml
7) N-EICOSANE	12.642	35850	0.232 ug/ml
8) N-DOCOSANE	13.891	233247	1.494 ug/ml
10) N-TETRACOSANE	14.947	627889	3.975 ug/ml
12) N-OCTACOSANE	16.956	329843	2.102 ug/ml
13) N-TRIACONTANE	17.829	343596	2.191 ug/ml
14) N-DOTRIACONTANE	18.664	148347	1.001 ug/ml
15) N-TETRATRIACONTANE	19.450	74438	0.615 ug/ml
16) N-HEXATRIACONTANE	20.174	40580	0.439 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF081120\
Data File : FF07338.D
Signal(s) : FID2B.ch
Acq On : 12 Aug 2020 00:01
Operator : DD\AJ
Sample : L3637-21 5X
Misc :
ALS Vial : 69 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :
CAR-WASH-AREA-3-TPH-1

Integration File: autoint1.e
Quant Time: Aug 13 01:40:39 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF072820.M
Quant Title :
QLast Update : Wed Jul 29 09:33:32 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

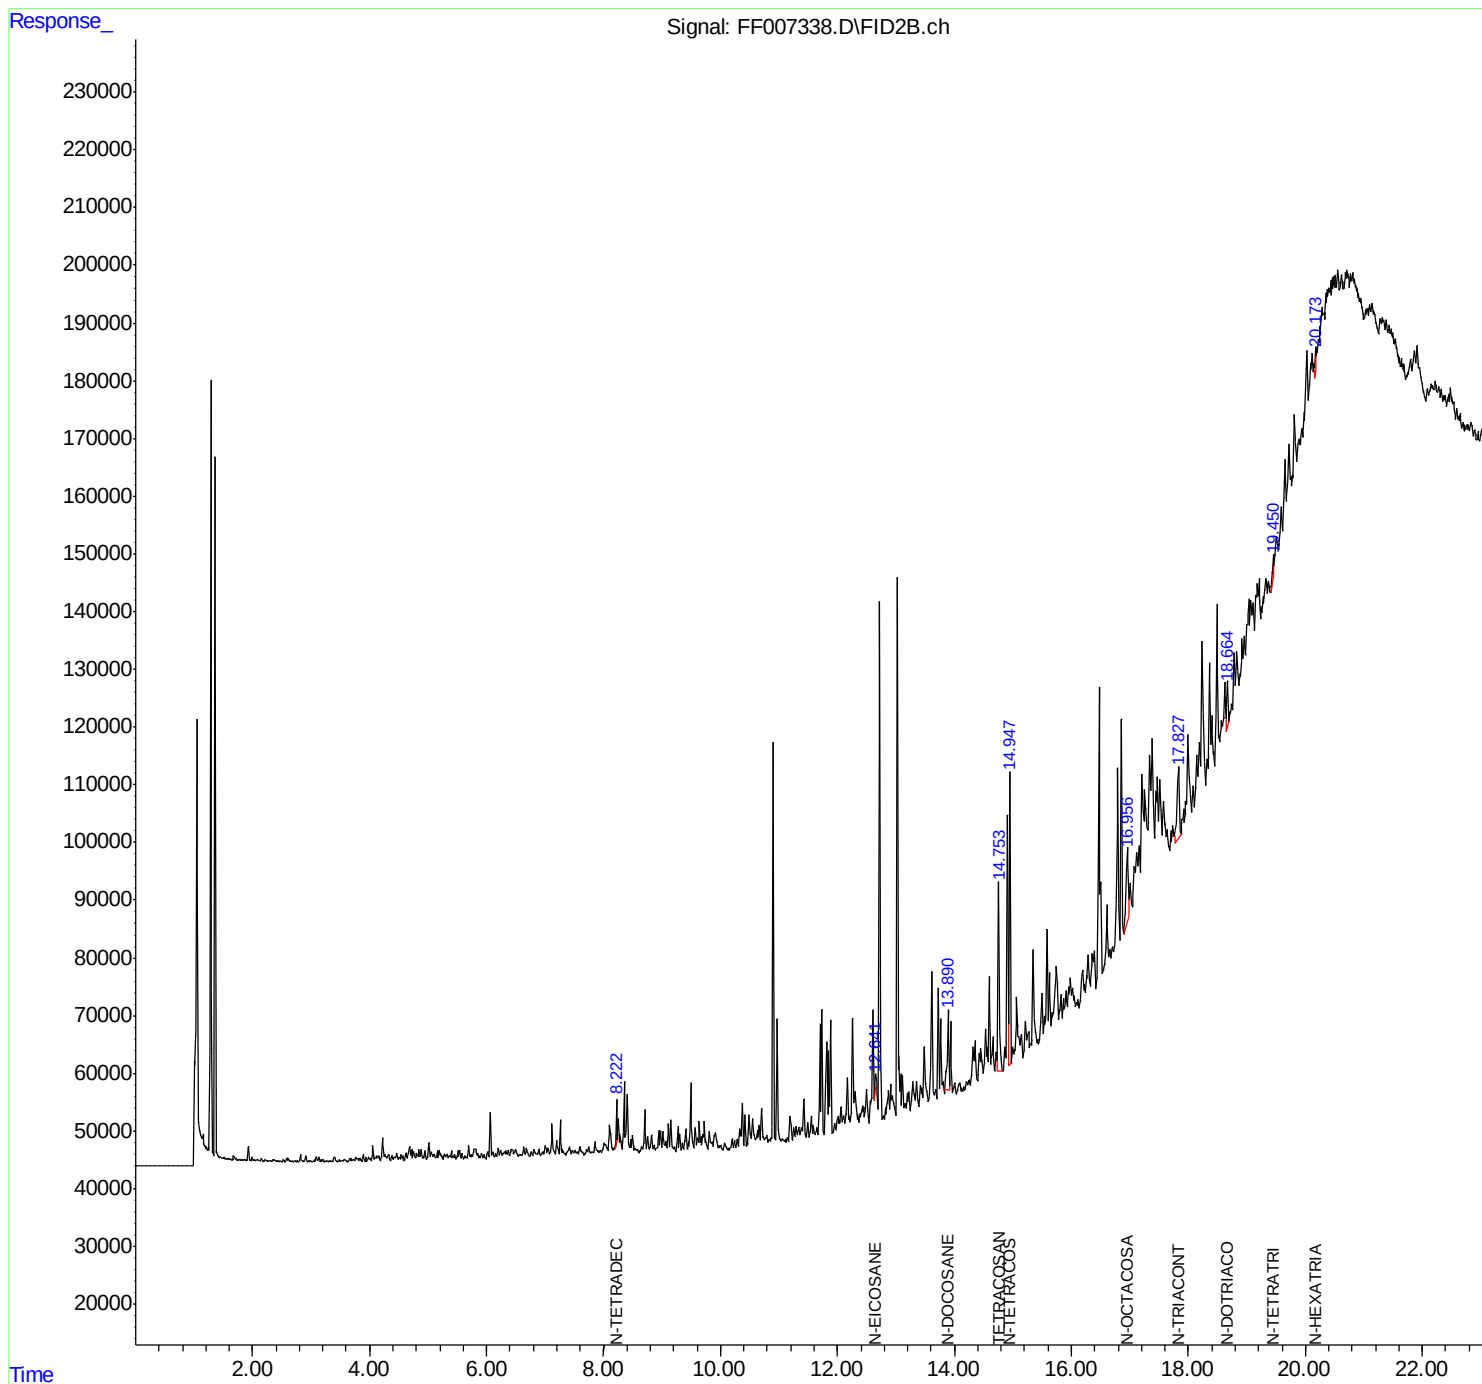


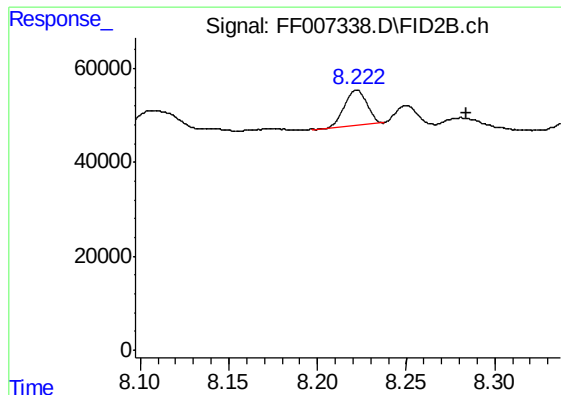

#4 N-TETRADECANE


R.T.: 8.222 min
Delta R.T.: -0.062 min
Response: 65480
Conc: 0.45 ug/ml

Instrument :
FID_F
ClientSampleId :
CAR-WASH-AREA-3-TPH-1

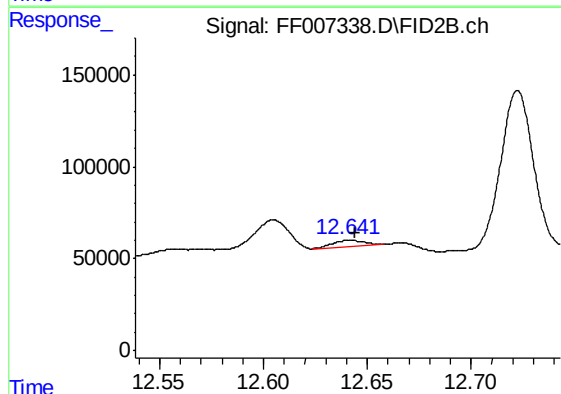


#7 N-EICOSANE

R.T.: 12.642 min
Delta R.T.: -0.002 min
Response: 35850
Conc: 0.23 ug/ml

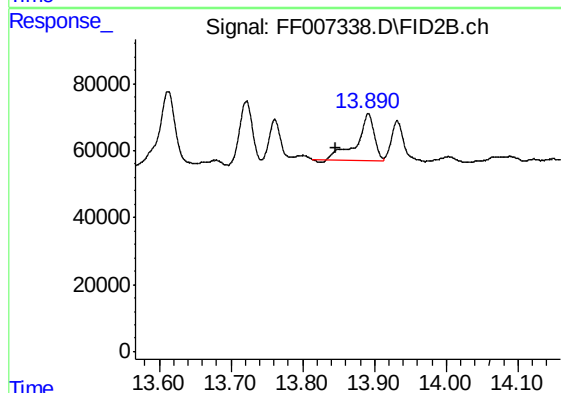


#8 N-DOCOSANE

R.T.: 13.891 min
Delta R.T.: 0.046 min
Response: 233247
Conc: 1.49 ug/ml

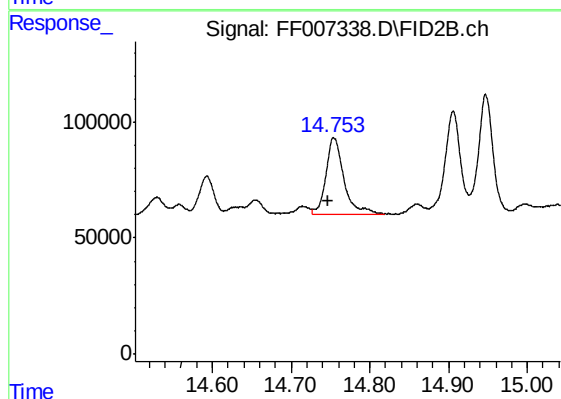

#9 TETRACOSANE-d50 (SURROGATE)


R.T.: 14.754 min
Delta R.T.: 0.007 min
Response: 512371
Conc: 3.75 ug/ml

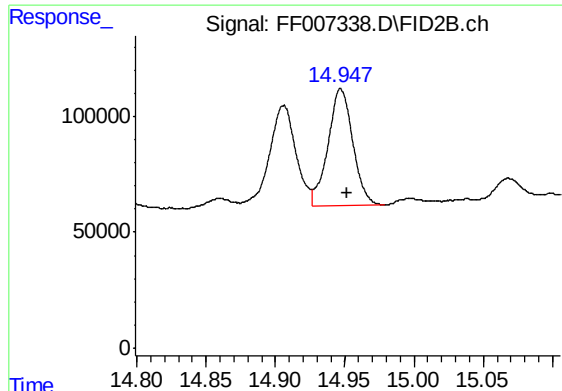

#10 N-TETRACOSANE


R.T.: 14.947 min
Delta R.T.: -0.004 min
Response: 627889
Conc: 3.98 ug/ml

Instrument :
FID_F
ClientSampleId :
CAR-WASH-AREA-3-TPH-1

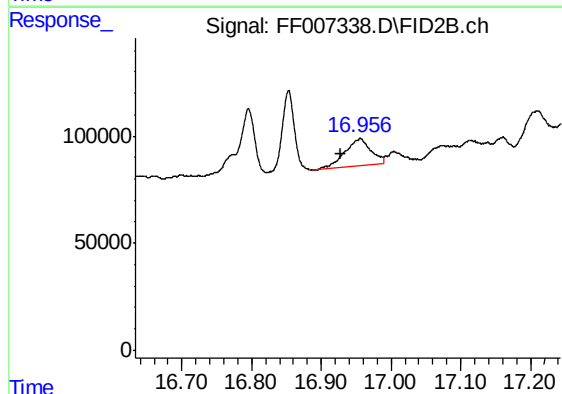


#12 N-OCTACOSANE

R.T.: 16.956 min
Delta R.T.: 0.028 min
Response: 329843
Conc: 2.10 ug/ml

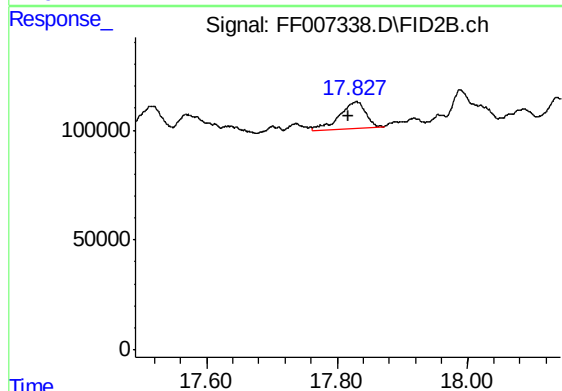


#13 N-TRIACONTANE

R.T.: 17.829 min
Delta R.T.: 0.011 min
Response: 343596
Conc: 2.19 ug/ml

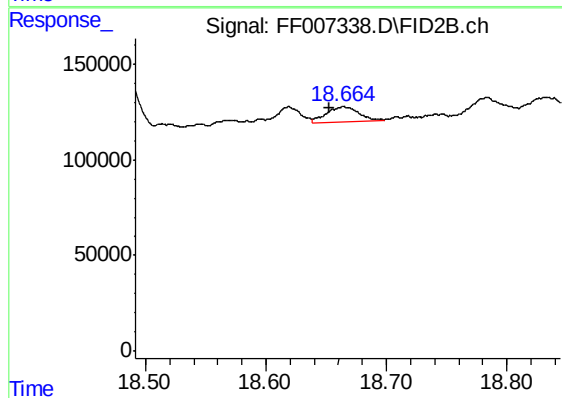

#14 N-DOTRIACONTANE


R.T.: 18.664 min
Delta R.T.: 0.012 min
Response: 148347
Conc: 1.00 ug/ml

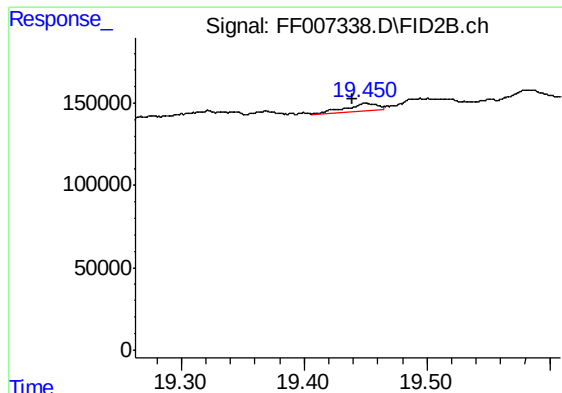

#15 N-TETRATRIACONTANE

R.T.: 19.450 min
Delta R.T.: 0.011 min
Response: 74438
Conc: 0.62 ug/ml

Instrument :
FID_F
ClientSampleId :
CAR-WASH-AREA-3-TPH-1

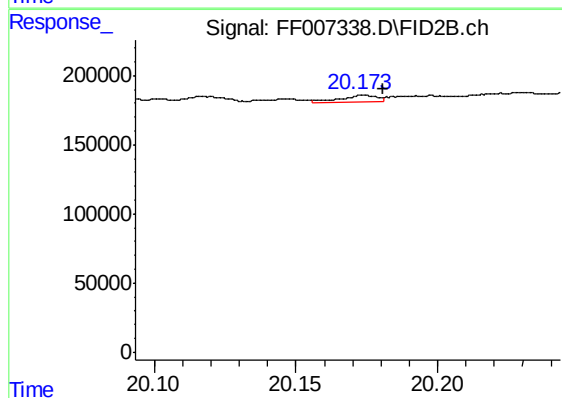

#16 N-HEXATRIACONTANE

R.T.: 20.174 min
Delta R.T.: -0.007 min
Response: 40580
Conc: 0.44 ug/ml