

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF081120\
 Data File : FF007339.D
 Signal(s) : FID2B.ch
 Acq On : 12 Aug 2020 00:32
 Operator : DD\AJ
 Sample : L3637-22 5X
 Misc :
 ALS Vial : 70 Sample Multiplier: 1

Instrument :
 FID_F
 ClientSampleId :
 CAR-WASH-AREA-3-TPH-2

Integration File: autoint1.e
 Quant Time: Aug 13 01:40:53 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF072820.M
 Quant Title :
 QLast Update : Wed Jul 29 09:33:32 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.756	480408	3.519 ug/ml
Target Compounds			
4) N-TETRADECANE	8.350f	138919	0.955 ug/ml
7) N-EICOSANE	12.605	191620	1.238 ug/ml
8) N-DOCOSANE	13.892	308329	1.975 ug/ml
10) N-TETRACOSANE	14.949	961907	6.090 ug/ml
12) N-OCTACOSANE	16.957	352572	2.246 ug/ml
13) N-TRIACONTANE	17.834	364979	2.327 ug/ml
14) N-DOTRIACONTANE	18.666	124933	0.843 ug/ml
15) N-TETRATRIACONTANE	19.500f	265885	2.198 ug/ml
16) N-HEXATRIACONTANE	20.174	118971	1.286 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF081120\
Data File : FF07339.D
Signal(s) : FID2B.ch
Acq On : 12 Aug 2020 00:32
Operator : DD\AJ
Sample : L3637-22 5X
Misc :
ALS Vial : 70 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :
CAR-WASH-AREA-3-TPH-2

Integration File: autoint1.e
Quant Time: Aug 13 01:40:53 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF072820.M
Quant Title :
QLast Update : Wed Jul 29 09:33:32 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

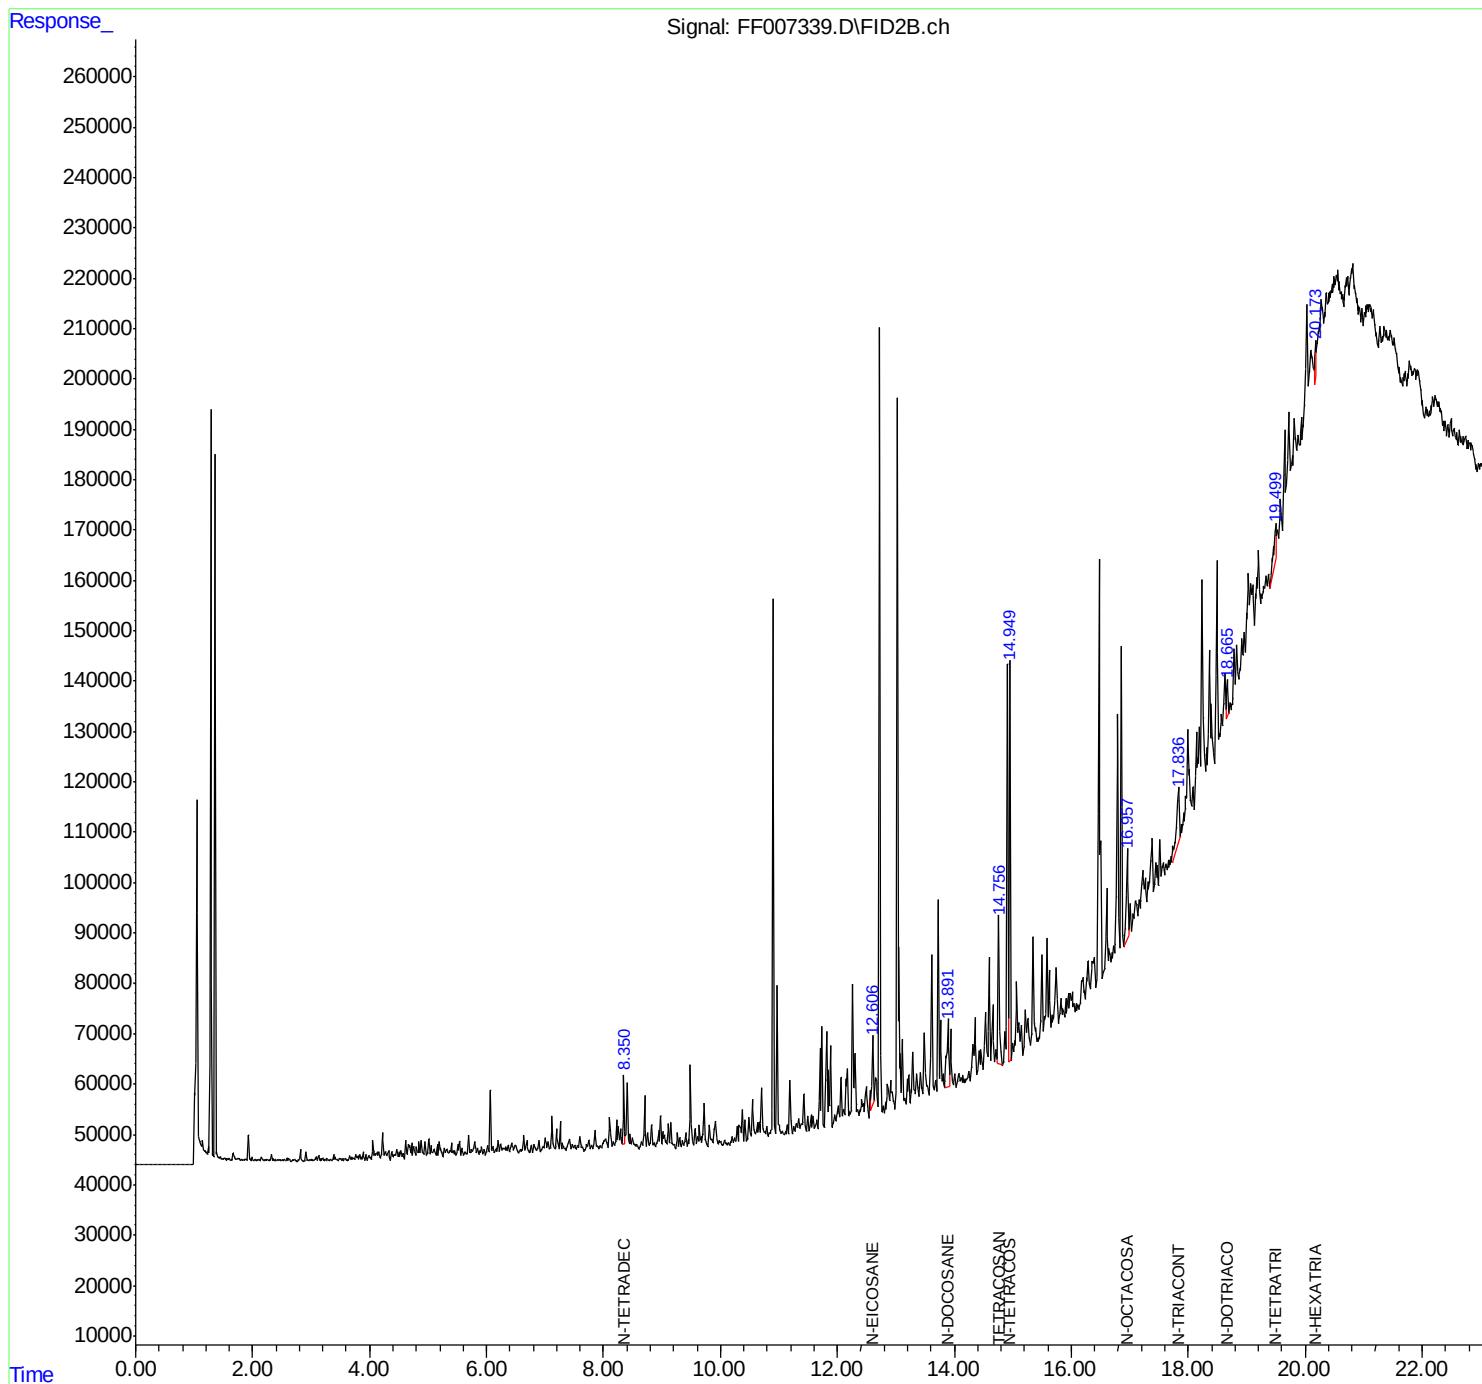


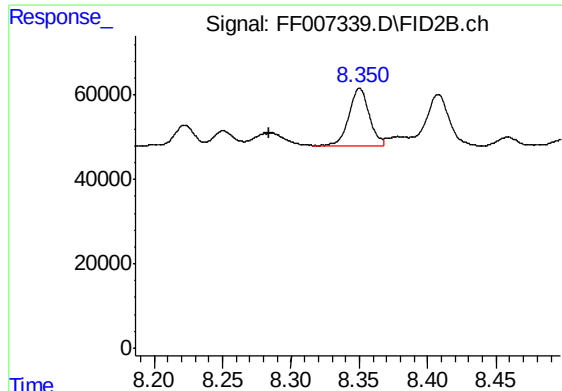

#4 N-TETRADECANE


R.T.: 8.350 min
Delta R.T.: 0.066 min
Response: 138919
Conc: 0.95 ug/ml

Instrument :
FID_F
ClientSampleId :
CAR-WASH-AREA-3-TPH-2

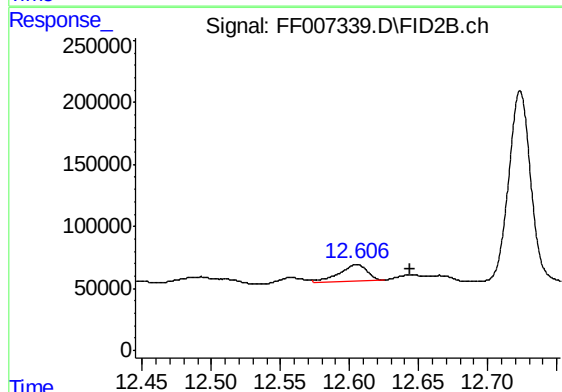


#7 N-EICOSANE

R.T.: 12.605 min
Delta R.T.: -0.039 min
Response: 191620
Conc: 1.24 ug/ml

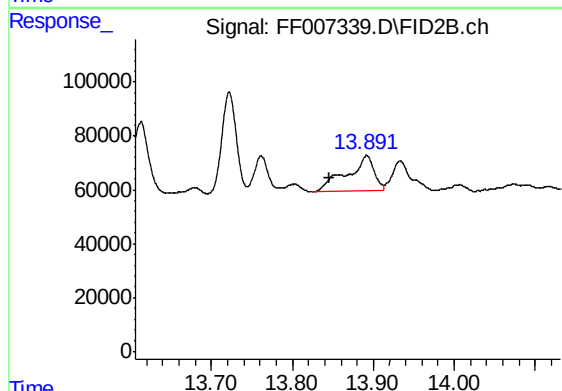


#8 N-DOCOSANE

R.T.: 13.892 min
Delta R.T.: 0.047 min
Response: 308329
Conc: 1.98 ug/ml

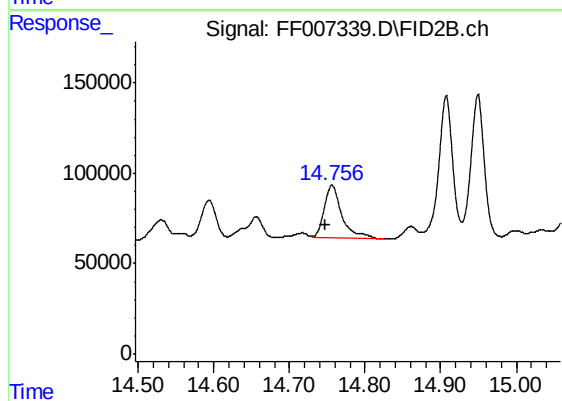

#9 TETRACOSANE-d50 (SURROGATE)


R.T.: 14.756 min
Delta R.T.: 0.008 min
Response: 480408
Conc: 3.52 ug/ml

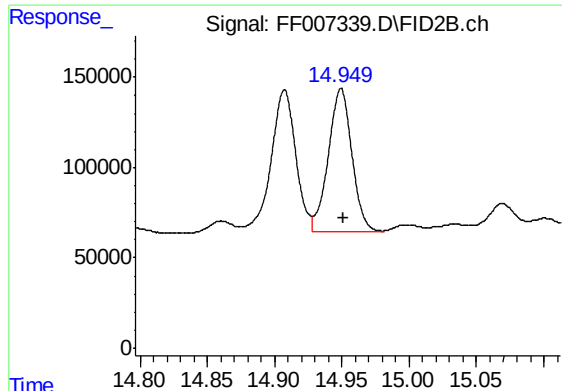

#10 N-TETRACOSANE


R.T.: 14.949 min
Delta R.T.: -0.002 min
Response: 961907
Conc: 6.09 ug/ml

Instrument :
FID_F
ClientSampleId :
CAR-WASH-AREA-3-TPH-2

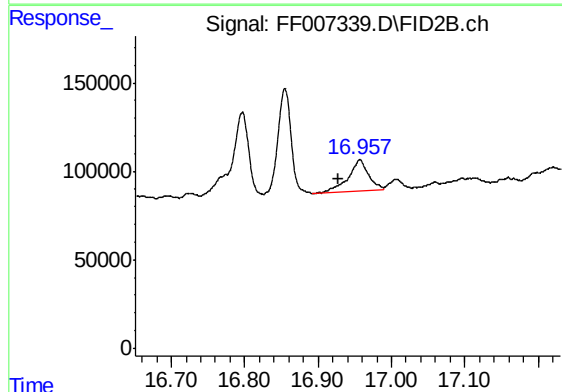


#12 N-OCTACOSANE

R.T.: 16.957 min
Delta R.T.: 0.029 min
Response: 352572
Conc: 2.25 ug/ml

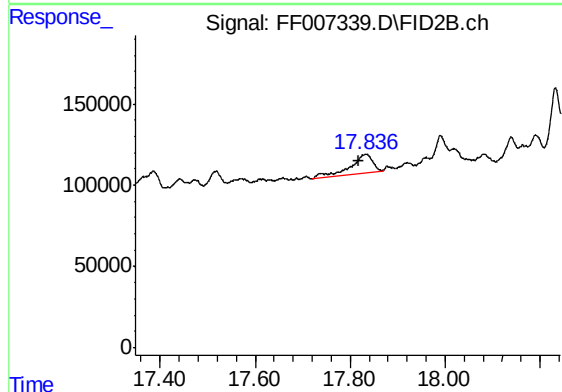


#13 N-TRIACONTANE

R.T.: 17.834 min
Delta R.T.: 0.016 min
Response: 364979
Conc: 2.33 ug/ml

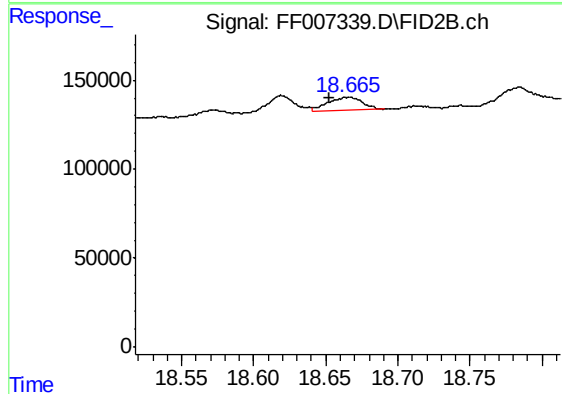

#14 N-DOTRIACONTANE


R.T.: 18.666 min
Delta R.T.: 0.014 min
Response: 124933
Conc: 0.84 ug/ml

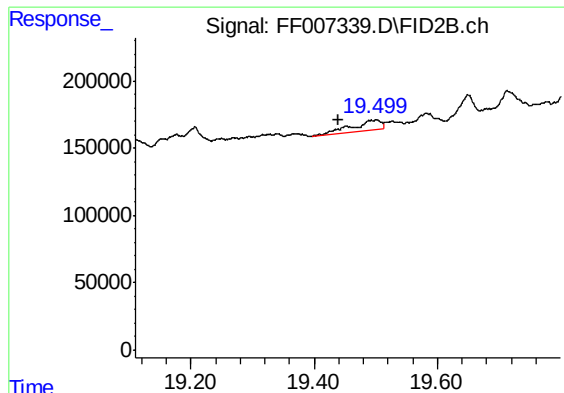

#15 N-TETRATRIACONTANE

R.T.: 19.500 min
Delta R.T.: 0.062 min
Response: 265885
Conc: 2.20 ug/ml

Instrument :
FID_F
ClientSampleId :
CAR-WASH-AREA-3-TPH-2

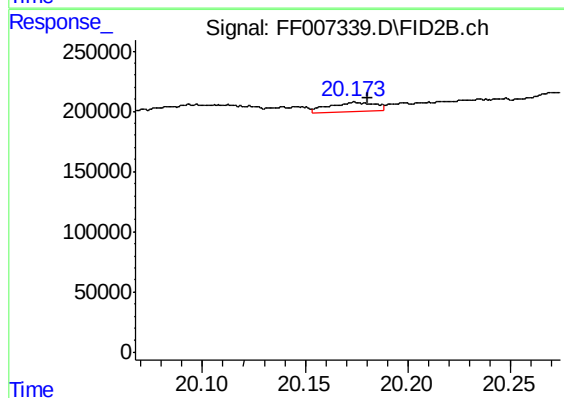

#16 N-HEXATRIACONTANE

R.T.: 20.174 min
Delta R.T.: -0.006 min
Response: 118971
Conc: 1.29 ug/ml