

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF081120\
 Data File : FF007320.D
 Signal(s) : FID2B.ch
 Acq On : 11 Aug 2020 14:06
 Operator : DD\AJ
 Sample : PB130880BS
 Misc :
 ALS Vial : 56 Sample Multiplier: 1

Instrument :
 FID_F
 ClientSampleId :
 PB130880BS

Integration File: autoint1.e
 Quant Time: Aug 11 15:27:21 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF072820.M
 Quant Title :
 QLast Update : Wed Jul 29 09:33:32 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.753	2180630	15.975 ug/ml
Target Compounds			
2) N-DECANE	4.461	2758277	19.763 ug/ml
3) N-DODECANE	6.488	2764955	19.439 ug/ml
4) N-TETRADECANE	8.286	2741179	18.837 ug/ml
5) N-HEXADECANE	9.890	2709058	18.228 ug/ml
6) N-OCTADECANE	11.335	2707619	17.658 ug/ml
7) N-EICOSANE	12.647	2636824	17.036 ug/ml
8) N-DOCOSANE	13.850	2568704	16.456 ug/ml
10) N-TETRACOSANE	14.957	2512647	15.909 ug/ml
11) N-HEXACOSANE	15.981	2422987	15.455 ug/ml
12) N-OCTACOSANE	16.934	2394449	15.256 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF081120\
Data File : FF007320.D
Signal(s) : FID2B.ch
Acq On : 11 Aug 2020 14:06
Operator : DD\AJ
Sample : PB130880BS
Misc :
ALS Vial : 56 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :
PB130880BS

Integration File: autoint1.e
Quant Time: Aug 11 15:27:21 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF072820.M
Quant Title :
QLast Update : Wed Jul 29 09:33:32 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

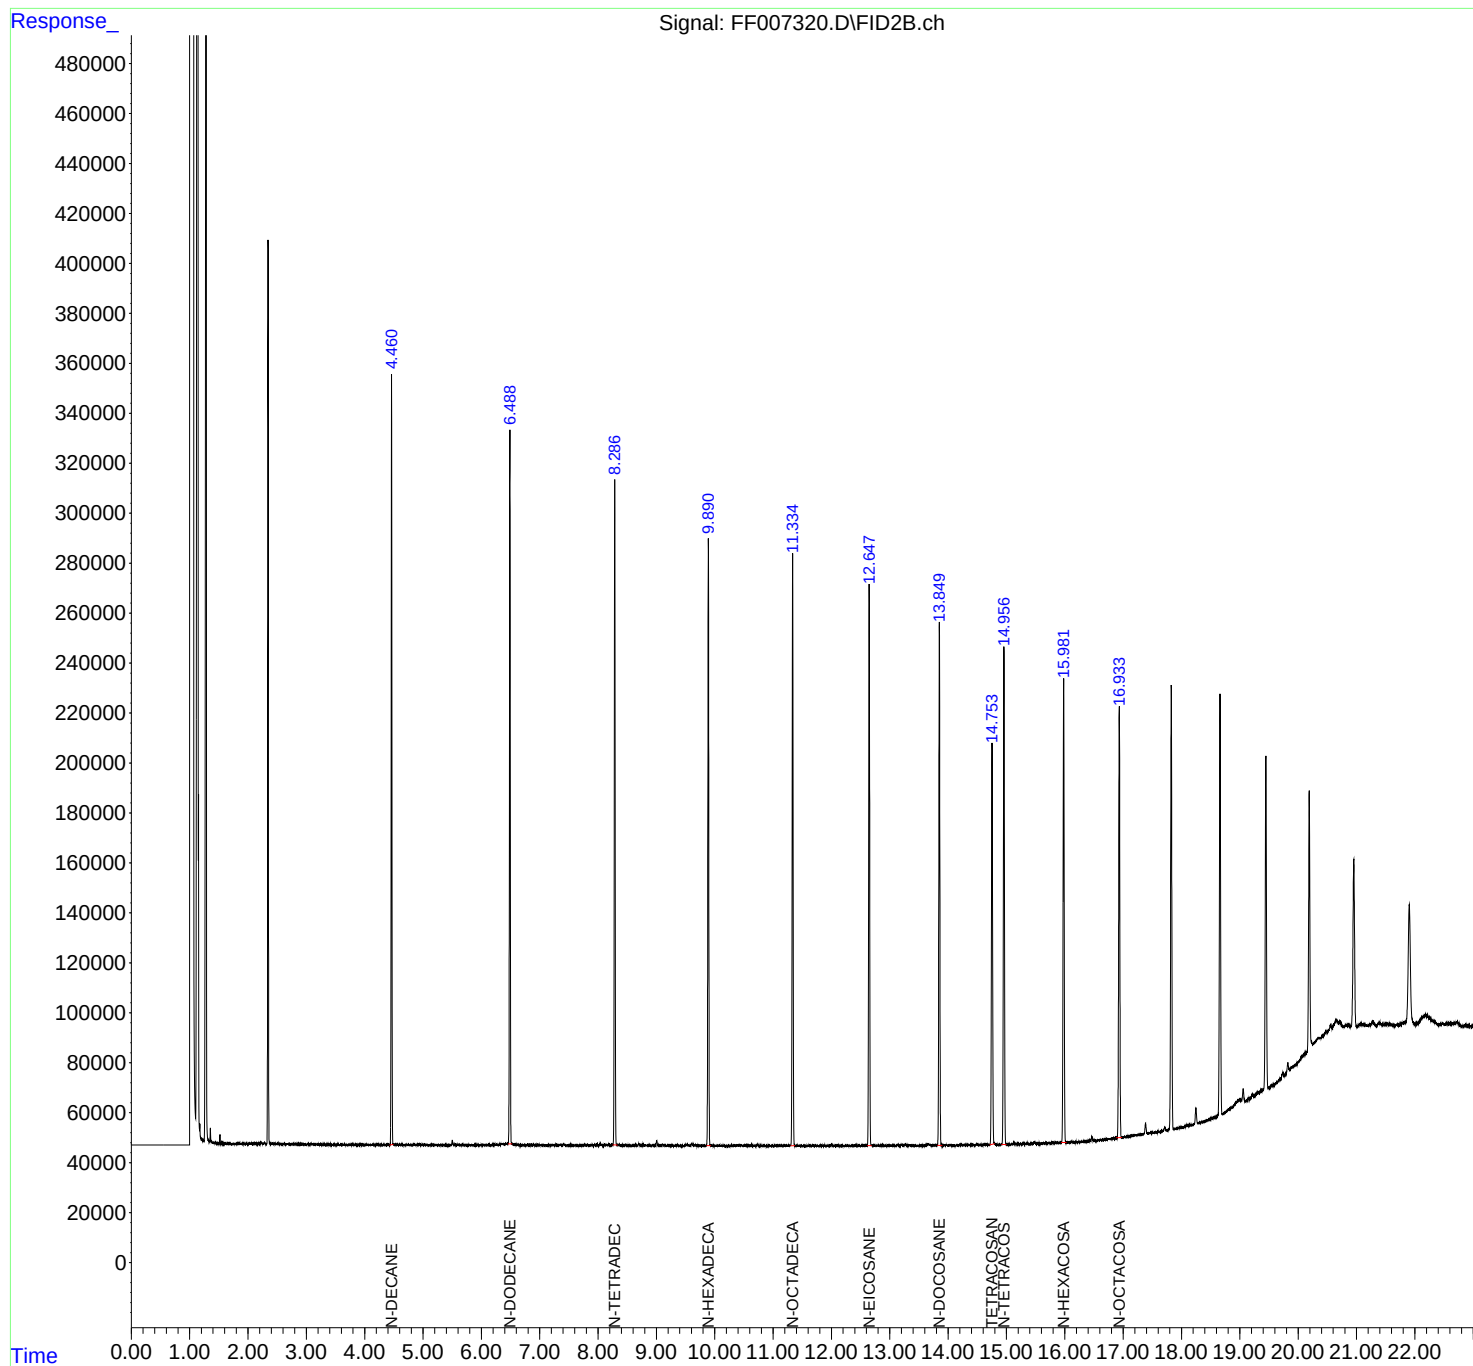


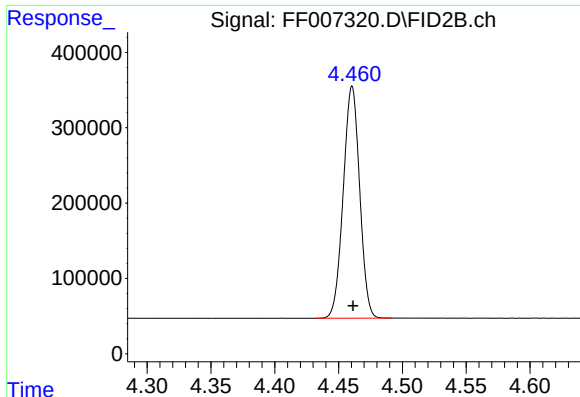

#2 N-DECANE


R.T.: 4.461 min
Delta R.T.: 0.000 min
Response: 2758277
Conc: 19.76 ug/ml

Instrument :
FID_F
ClientSampleId :
PB130880BS

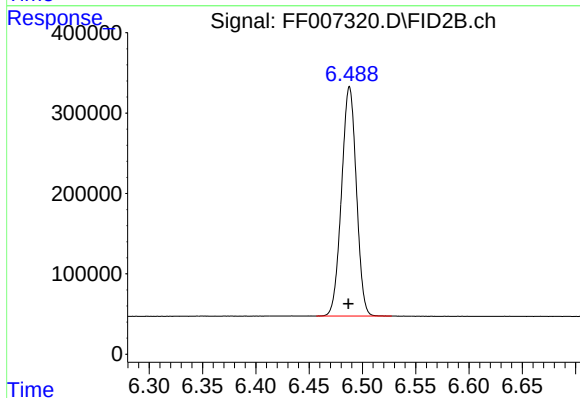


#3 N-DODECANE

R.T.: 6.488 min
Delta R.T.: 0.001 min
Response: 2764955
Conc: 19.44 ug/ml

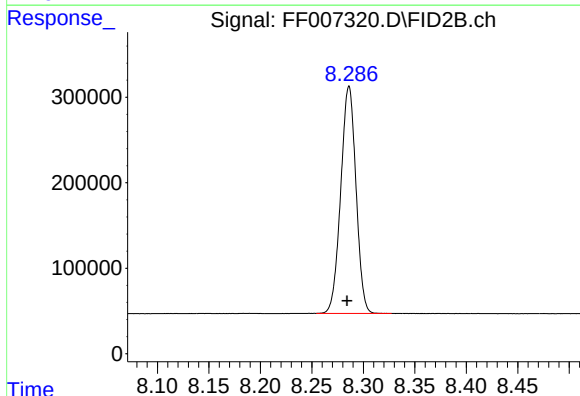


#4 N-TETRADECANE

R.T.: 8.286 min
Delta R.T.: 0.002 min
Response: 2741179
Conc: 18.84 ug/ml

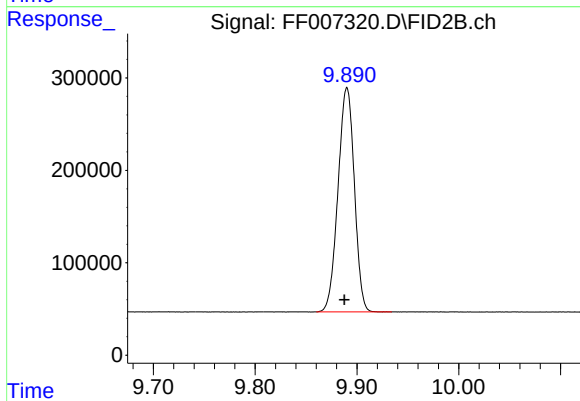

#5 N-HEXADECANE


R.T.: 9.890 min
Delta R.T.: 0.003 min
Response: 2709058
Conc: 18.23 ug/ml

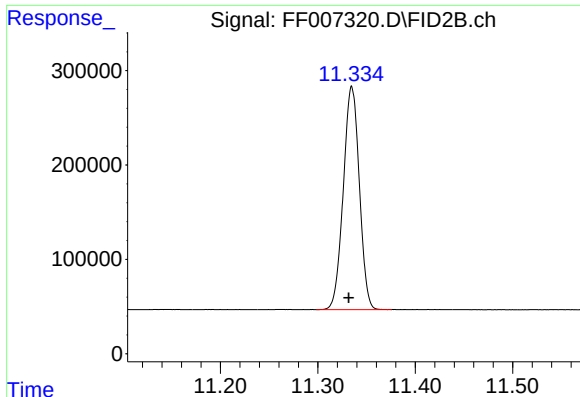

#6 N-OCTADECANE


R.T.: 11.335 min
Delta R.T.: 0.003 min
Response: 2707619
Conc: 17.66 ug/ml

Instrument :
FID_F
ClientSampleId :
PB130880BS

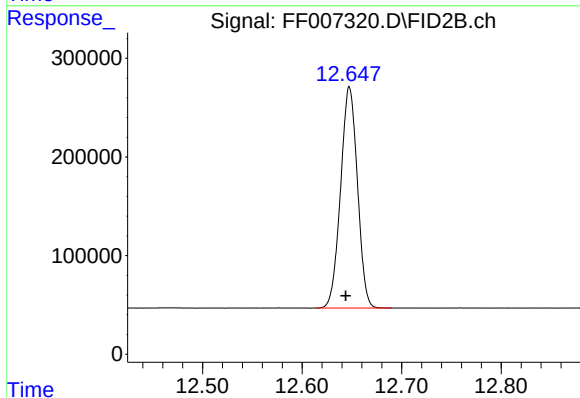


#7 N-EICOSANE

R.T.: 12.647 min
Delta R.T.: 0.003 min
Response: 2636824
Conc: 17.04 ug/ml

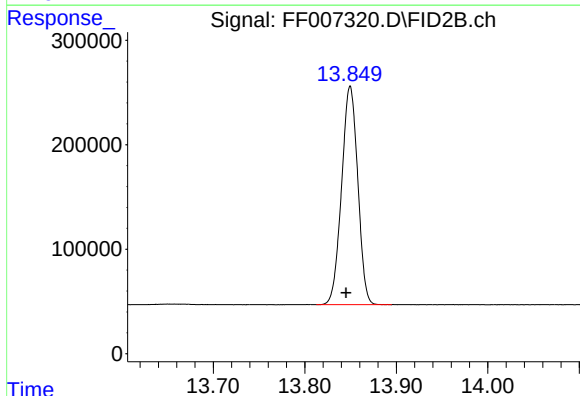


#8 N-DOCOSANE

R.T.: 13.850 min
Delta R.T.: 0.004 min
Response: 2568704
Conc: 16.46 ug/ml

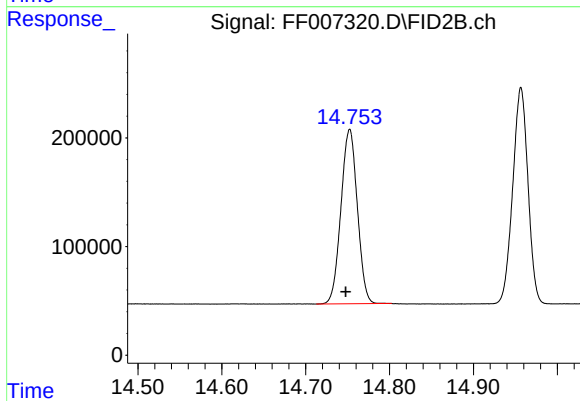

#9 TETRACOSANE-d50 (SURROGATE)


R.T.: 14.753 min
Delta R.T.: 0.005 min
Response: 2180630
Conc: 15.98 ug/ml

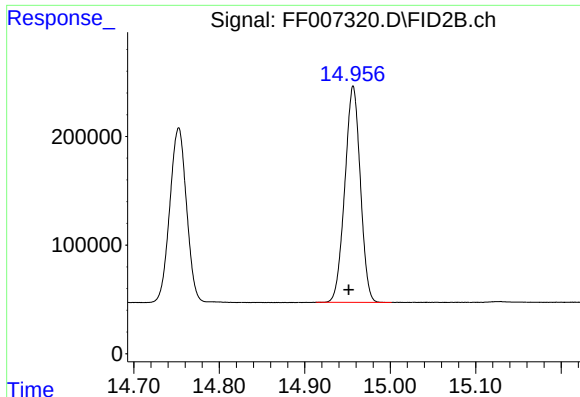

#10 N-TETRACOSANE


R.T.: 14.957 min
Delta R.T.: 0.005 min
Response: 2512647
Conc: 15.91 ug/ml

Instrument :
FID_F
ClientSampleId :
PB130880BS

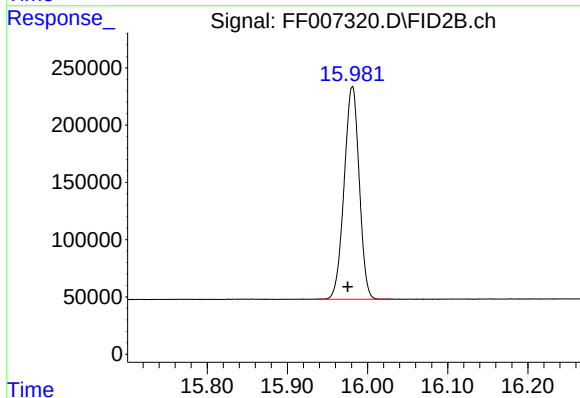

#11 N-HEXACOSANE

R.T.: 15.981 min
Delta R.T.: 0.006 min
Response: 2422987
Conc: 15.45 ug/ml

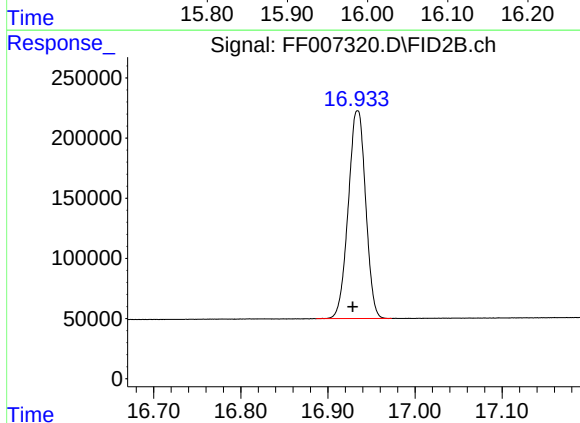

#12 N-OCTACOSANE

R.T.: 16.934 min
Delta R.T.: 0.006 min
Response: 2394449
Conc: 15.26 ug/ml