

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF081120\
Data File : FF007322.D
Signal(s) : FID2B.ch
Acq On : 11 Aug 2020 15:09
Operator : DD\AJ
Sample : L3506-01 2X
Misc :
ALS Vial : 58 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :
OR-02-080720

Integration File: autoint1.e
Quant Time: Aug 11 15:27:34 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF072820.M
Quant Title :
QLast Update : Wed Jul 29 09:33:32 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.758	818243	5.994 ug/ml
Target Compounds			

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF081120\
Data File : FF007322.D
Signal(s) : FID2B.ch
Acq On : 11 Aug 2020 15:09
Operator : DD\AJ
Sample : L3506-01 2X
Misc :
ALS Vial : 58 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :
OR-02-080720

Integration File: autoint1.e
Quant Time: Aug 11 15:27:34 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF072820.M
Quant Title :
QLast Update : Wed Jul 29 09:33:32 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

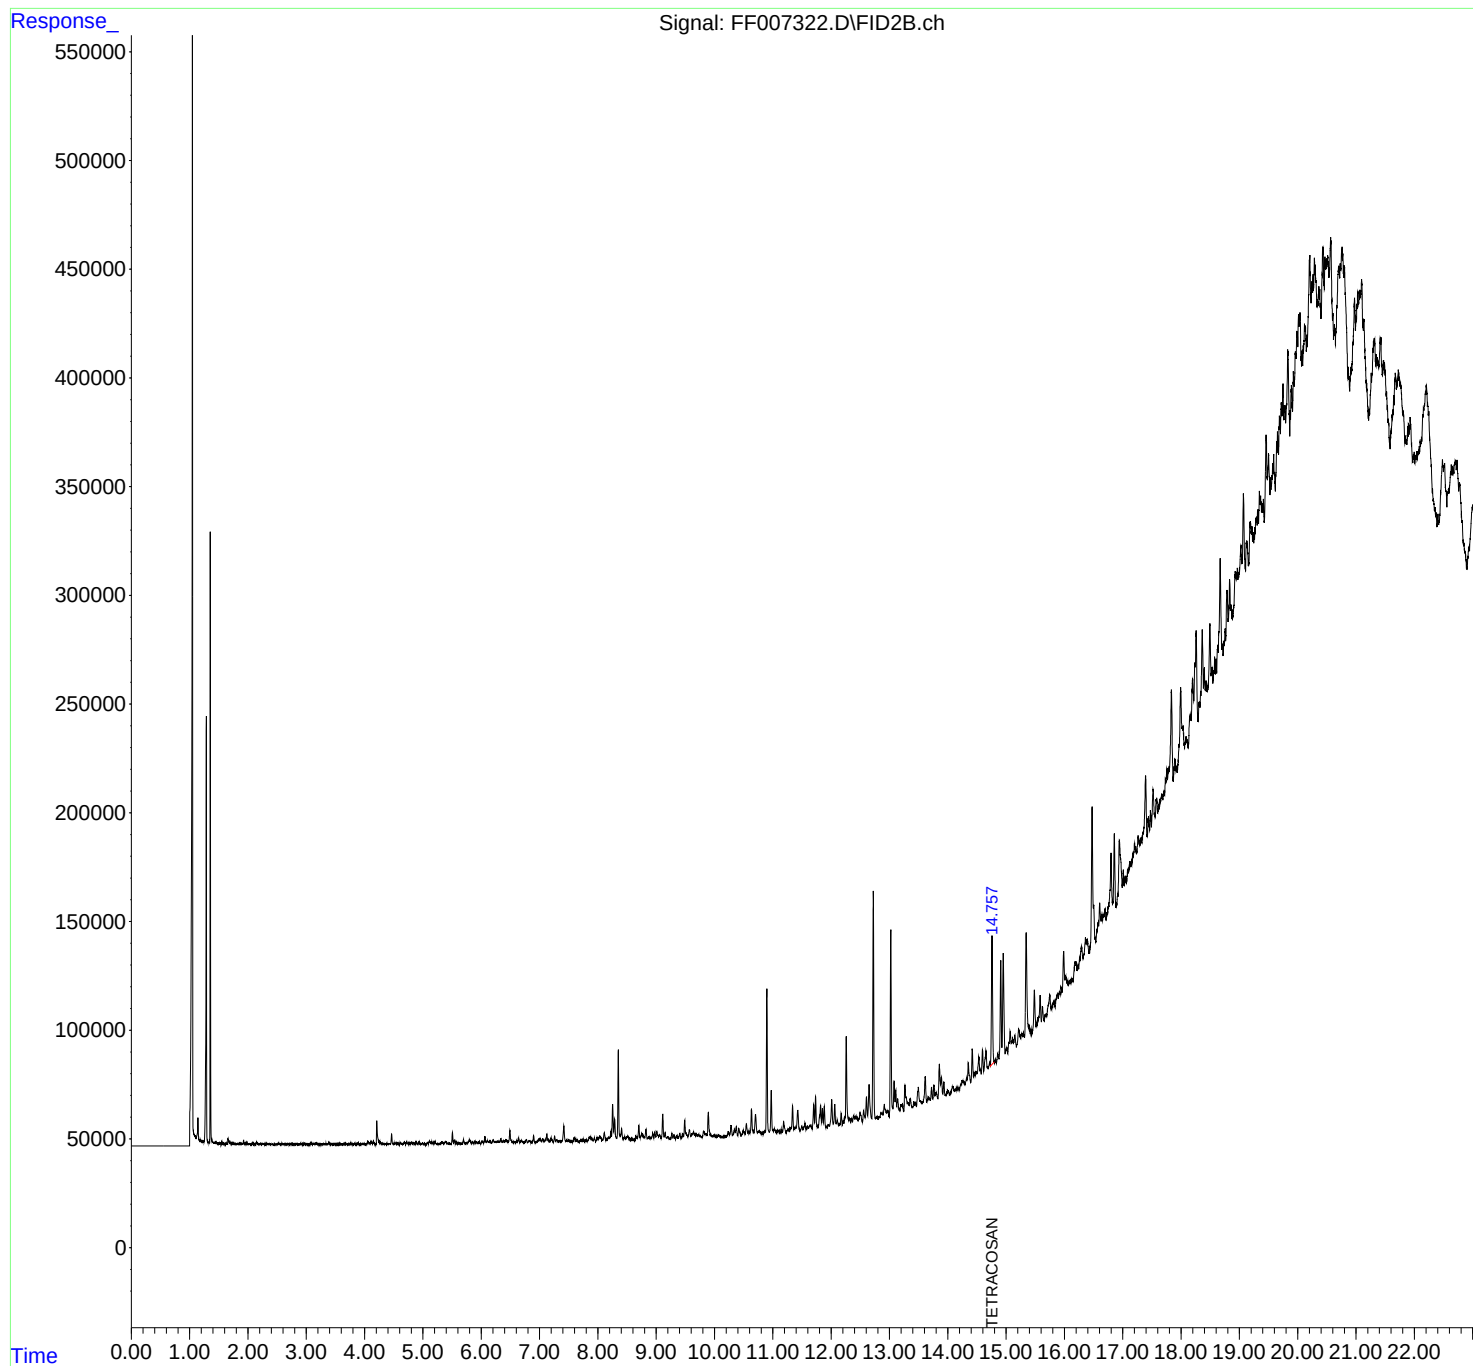

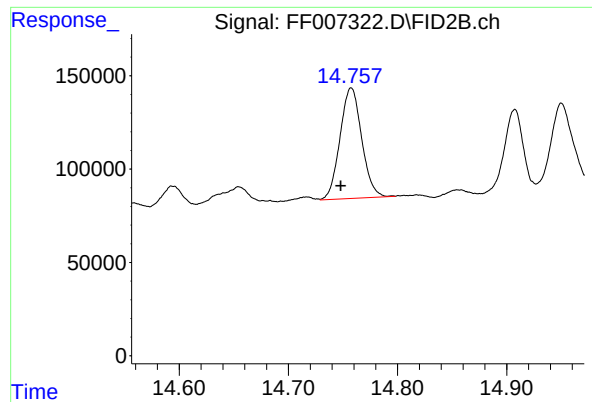

#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.758 min
Delta R.T.: 0.010 min
Response: 818243
Conc: 5.99 ug/ml

Instrument :
FID_F
ClientSampleId :
OR-02-080720