

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF081222\
Data File : FF011235.D
Signal(s) : FID2B.ch
Acq On : 12 Aug 2022 15:44
Operator : YP\AJ
Sample : RT MARKER
Misc :
ALS Vial : 54 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Aug 14 21:26:51 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF072822.M
Quant Title :
QLast Update : Thu Jul 28 14:46:22 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units
----------	------	----------	------------

System Monitoring Compounds

Target Compounds

3)	N-DODECANE	6.527	2198028	17.461 ug/ml
12)	N-OCTACOSANE	16.968	2189671	18.139 ug/ml
13)	N-TRIACONTANE	17.851	285036	2.386 ug/ml
14)	N-DOTRIACONTANE	18.681	400941	3.394 ug/ml
15)	N-TETRATRIACONTANE	19.463	352100	3.155 ug/ml
16)	N-HEXATRIACONTANE	20.201	237549	2.336 ug/ml
17)	N-OCTATRIACONTANE	20.908	161076	1.610 ug/ml
18)	N-TETRACONTANE	21.729	103385	0.943 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF081222\
Data File : FF011235.D
Signal(s) : FID2B.ch
Acq On : 12 Aug 2022 15:44
Operator : YP\AJ
Sample : RT MARKER
Misc :
ALS Vial : 54 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Aug 14 21:26:51 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF072822.M
Quant Title :
QLast Update : Thu Jul 28 14:46:22 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

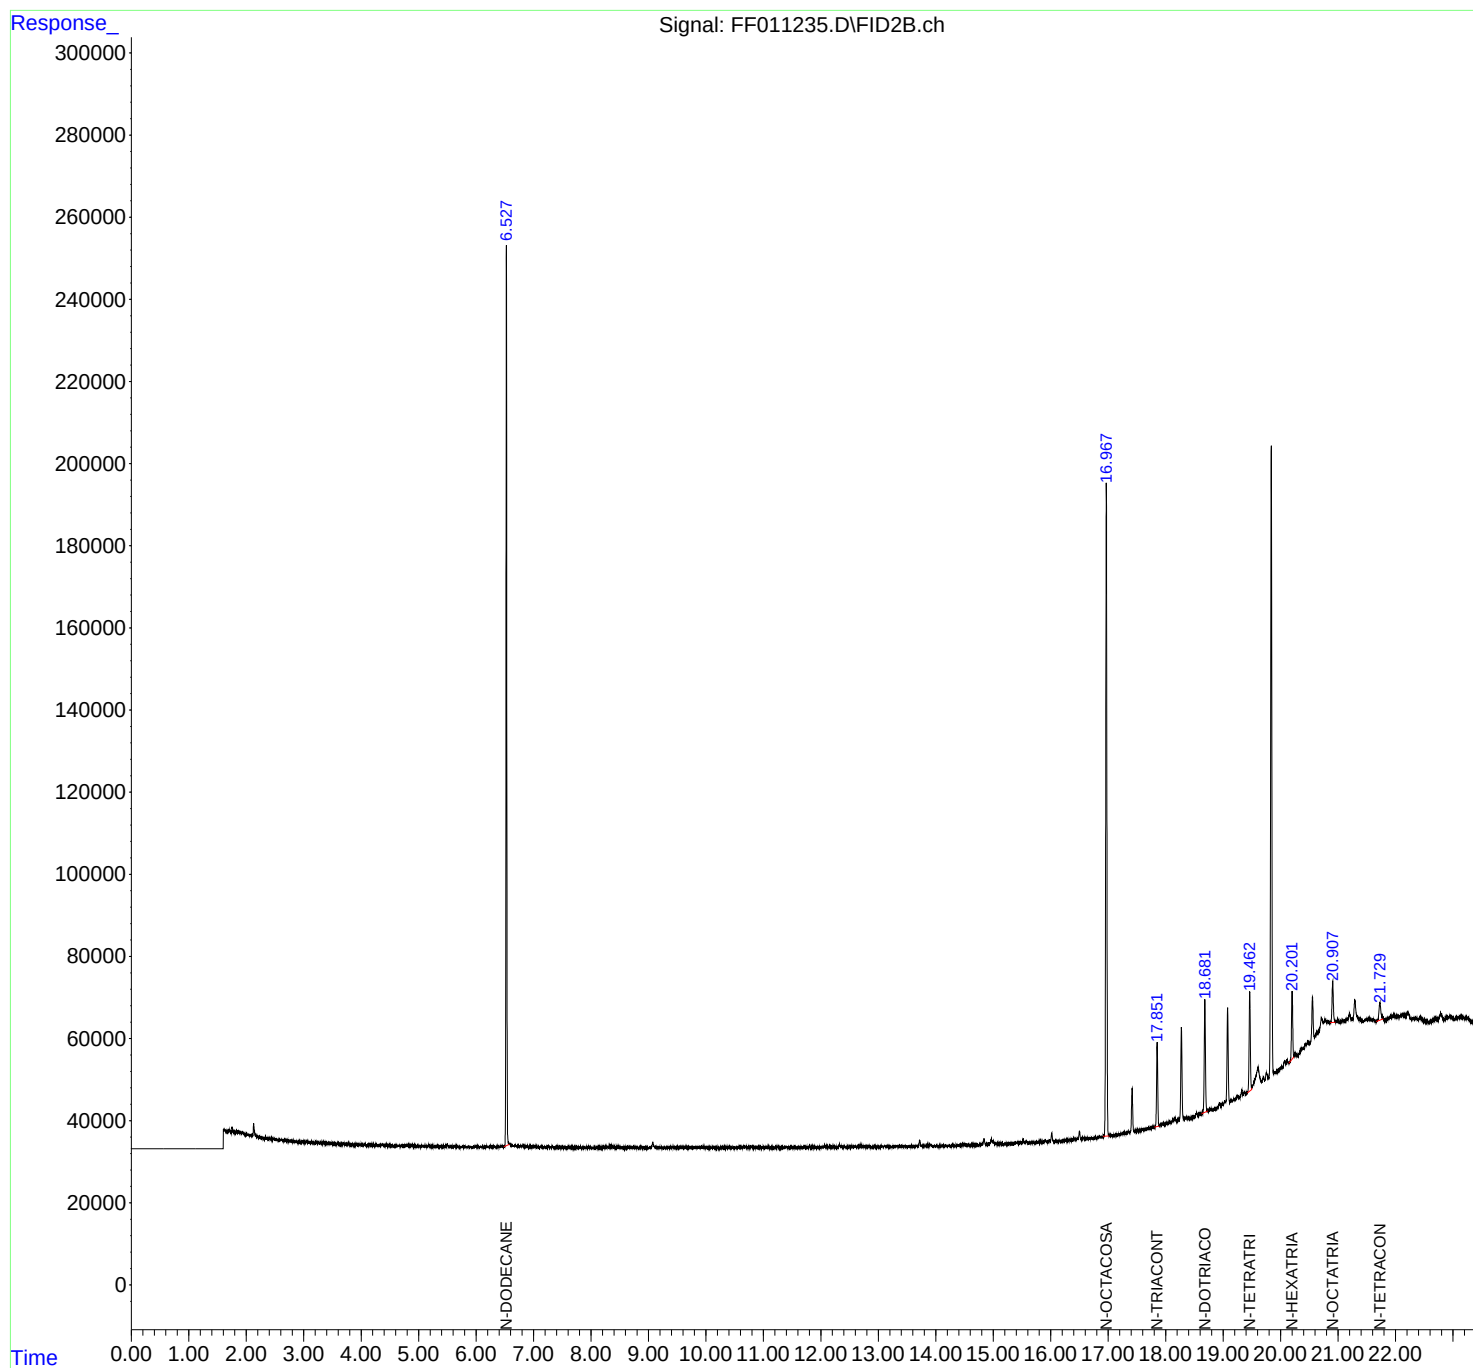


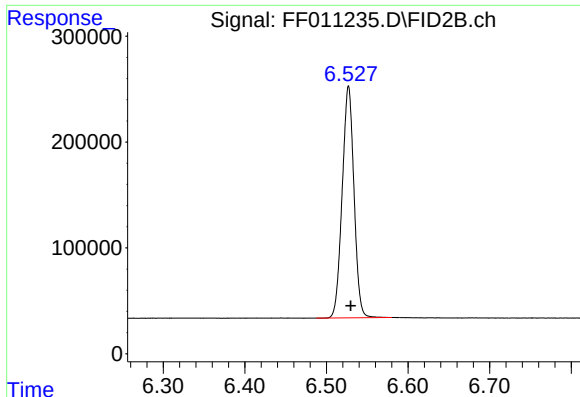

#3 N-DODECANE


R.T.: 6.527 min
Delta R.T.: -0.003 min
Response: 2198028
Conc: 17.46 ug/ml

Instrument :
FID_F
ClientSampleId :

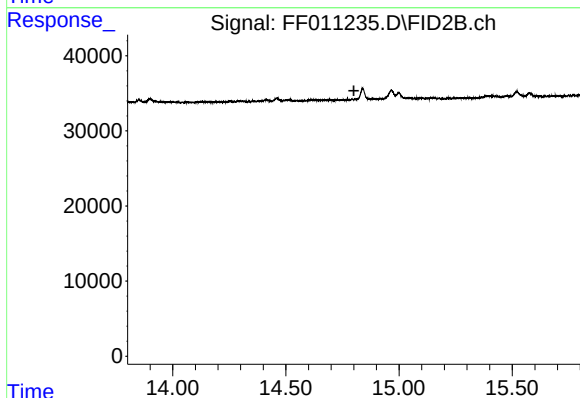


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 0.000 min
Exp R.T. : 14.801 min
Response: 0
Conc: N.D.

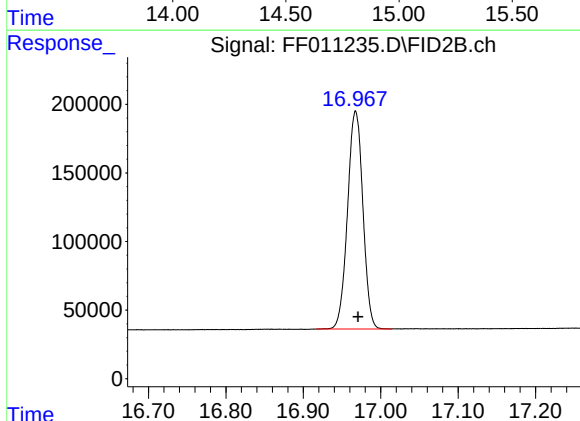


#12 N-OCTACOSANE

R.T.: 16.968 min
Delta R.T.: -0.003 min
Response: 2189671
Conc: 18.14 ug/ml

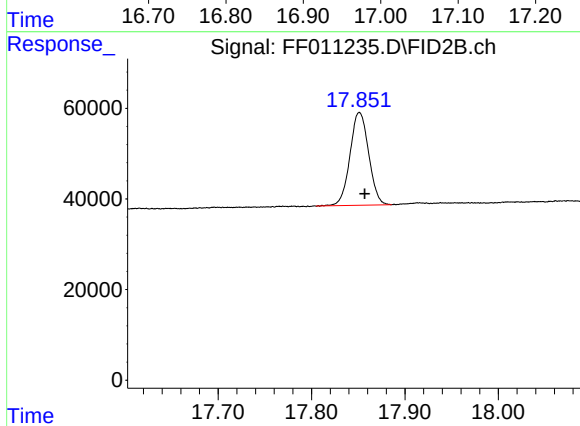

#13 N-TRIACONTANE


R.T.: 17.851 min
Delta R.T.: -0.006 min
Response: 285036
Conc: 2.39 ug/ml

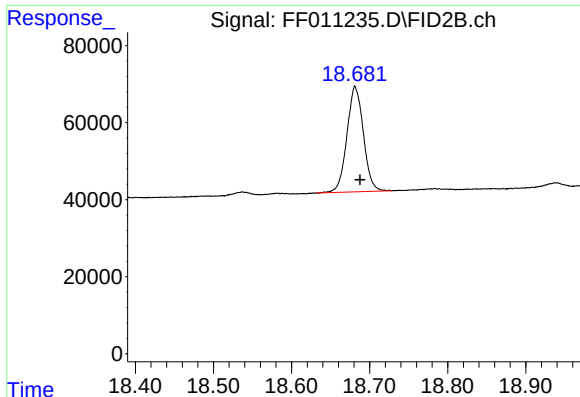

#14 N-DOTRIACONTANE


R.T.: 18.681 min
Delta R.T.: -0.006 min
Response: 400941
Conc: 3.39 ug/ml

Instrument :
FID_F
ClientSampleId :

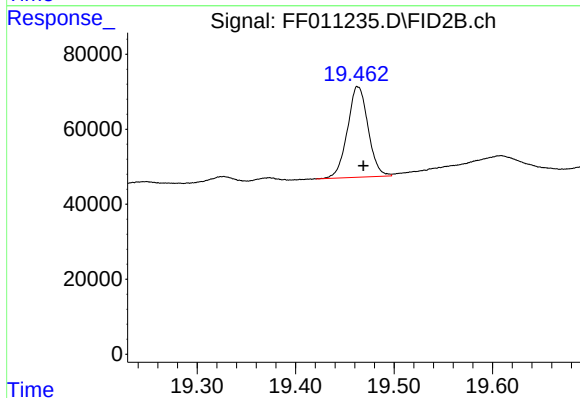


#15 N-TETRATRIACONTANE

R.T.: 19.463 min
Delta R.T.: -0.006 min
Response: 352100
Conc: 3.16 ug/ml

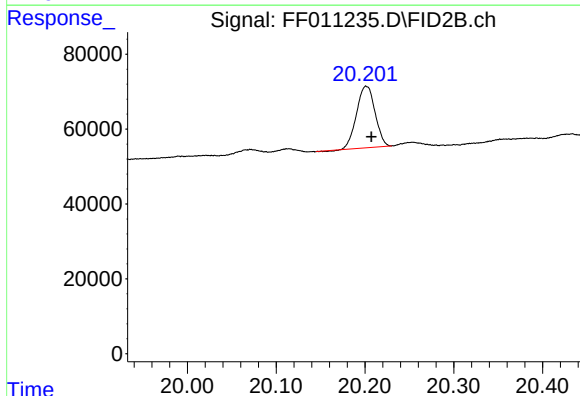


#16 N-HEXATRIACONTANE

R.T.: 20.201 min
Delta R.T.: -0.006 min
Response: 237549
Conc: 2.34 ug/ml

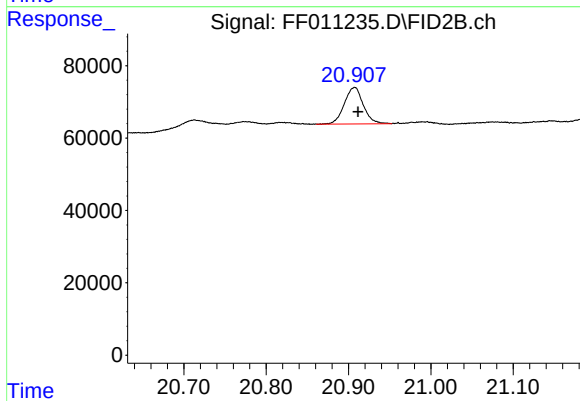

#17 N-OCTATRIACONTANE

R.T.: 20.908 min
Delta R.T.: -0.004 min
Response: 161076
Conc: 1.61 ug/ml

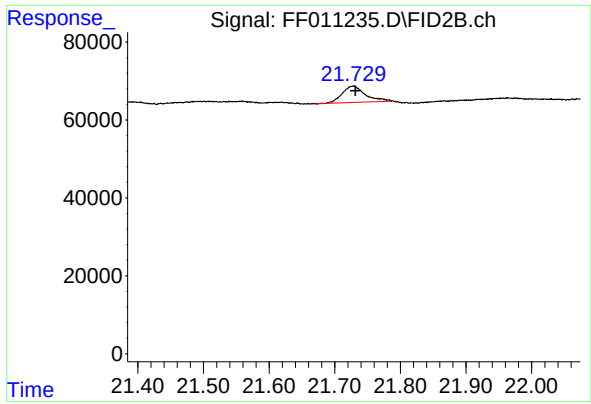

#18 N-TETRACONTANE

R.T.: 21.729 min
Delta R.T.: -0.003 min
Response: 103385
Conc: 0.94 ug/ml

Instrument :

FID_F

ClientSampleId :