

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF081222\
 Data File : FF011230.D
 Signal(s) : FID2B.ch
 Acq On : 12 Aug 2022 13:16
 Operator : YP\AJ
 Sample : N4130-07 2X
 Misc :
 ALS Vial : 61 Sample Multiplier: 1

Instrument :
 FID_F
 ClientSampleId :
 SB06

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 08/15/2022
 Supervised By :Ankita Jodhani 08/15/2022

Integration File: Sample.e
 Quant Time: Aug 12 13:40:11 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF072822.M
 Quant Title :
 QLast Update : Thu Jul 28 14:46:22 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.797	951777	8.757 ug/mlm
Target Compounds			

(f)=RT Delta > 1/2 Window

(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF081222\
Data File : FF011230.D
Signal(s) : FID2B.ch
Acq On : 12 Aug 2022 13:16
Operator : YP\AJ
Sample : N4130-07 2X
Misc :
ALS Vial : 61 Sample Multiplier: 1


Instrument :
FID_F
ClientSampleId :
SB06


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 08/15/2022
Supervised By :Ankita Jodhani 08/15/2022

Integration File: Sample.e
Quant Time: Aug 12 13:40:11 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF072822.M
Quant Title :
QLast Update : Thu Jul 28 14:46:22 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

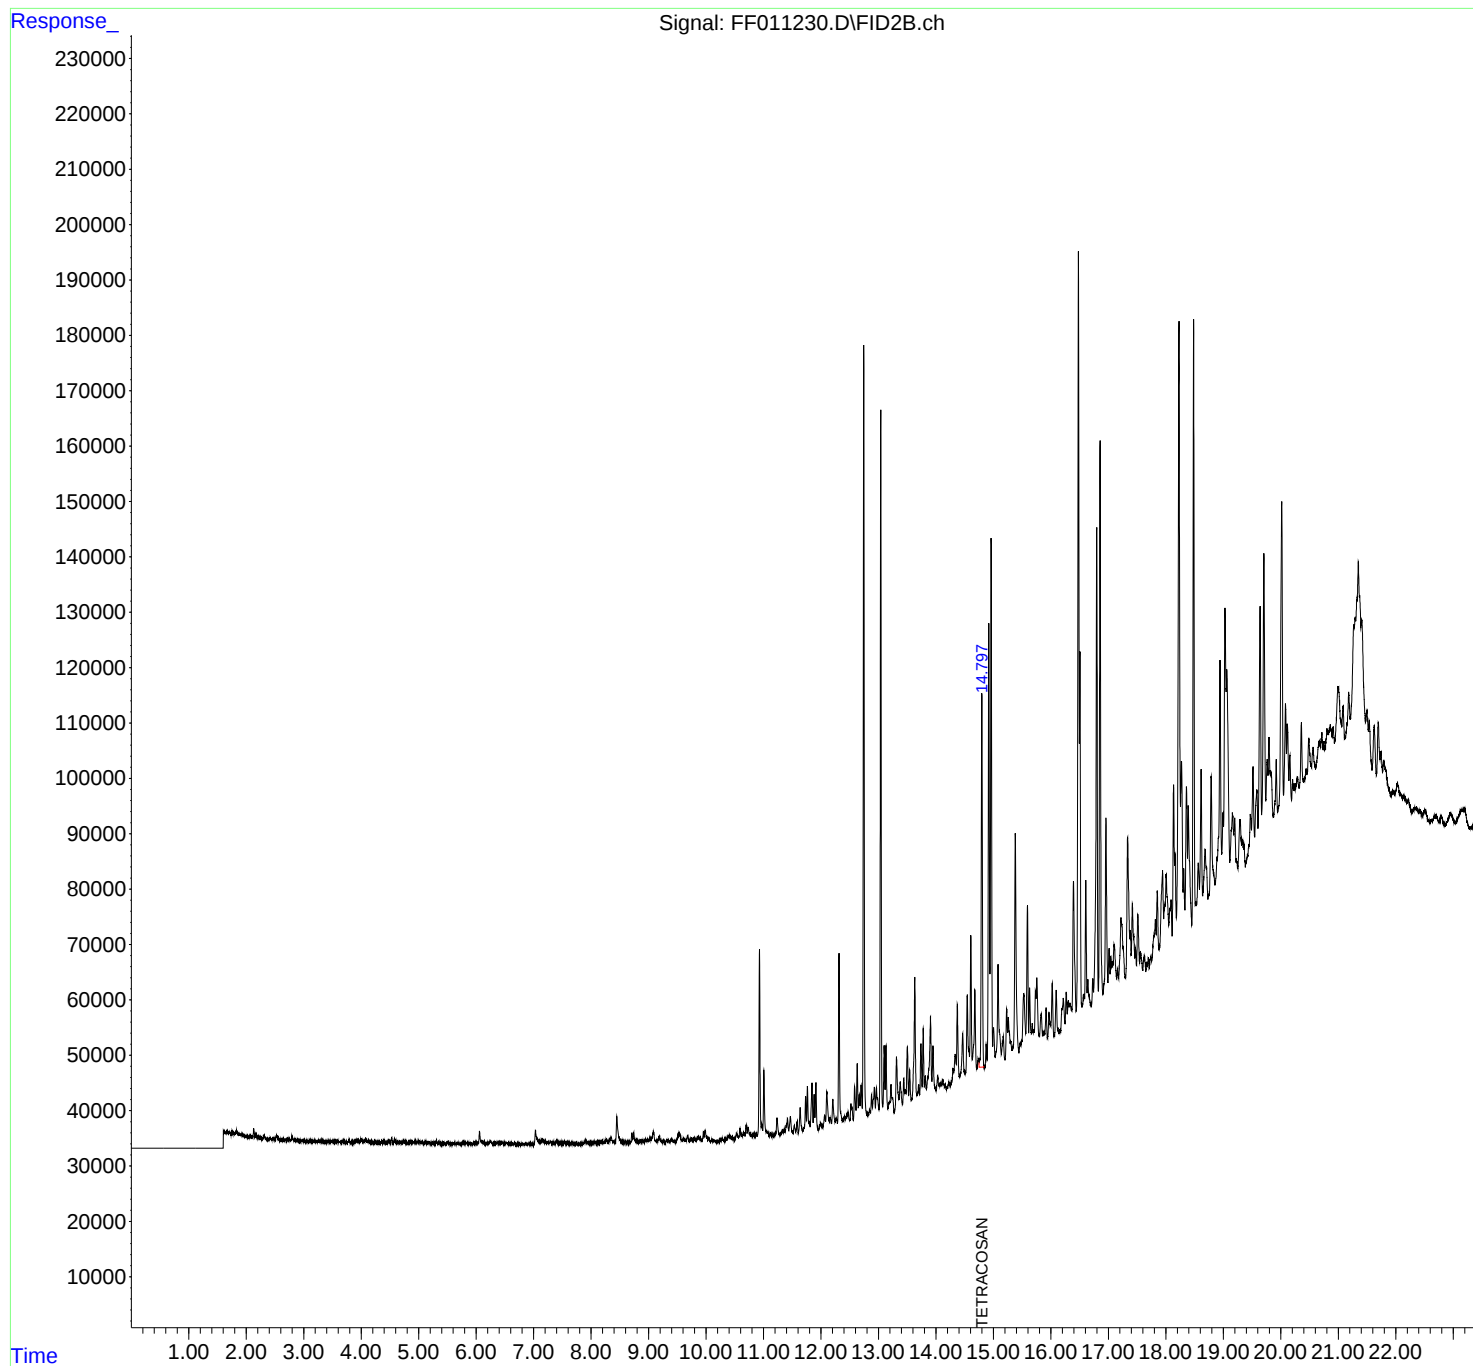

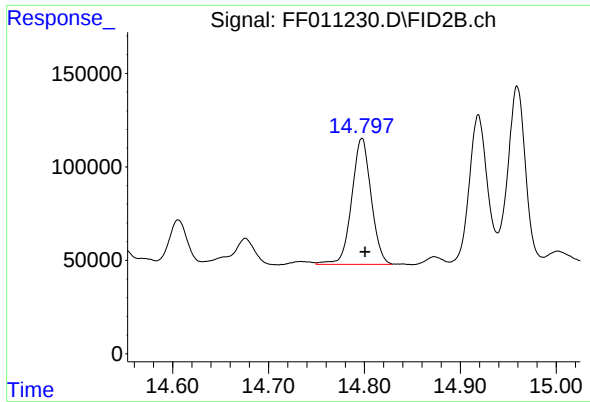

#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.797 min
Delta R.T.: -0.003 min
Response: 951777
Conc: 8.76 ug/ml

Instrument :
FID_F
ClientSampleId :
SB06

Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 08/15/2022
Supervised By :Ankita Jodhani 08/15/2022