

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF081318\
 Data File : FF001854.D
 Signal(s) : FID2B.ch
 Acq On : 13 Aug 2018 09:33
 Operator : AJ\SJ
 Sample : MECL2
 Misc :
 ALS Vial : 51 Sample Multiplier: 1

Instrument :
 FID_F
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Aug 14 02:02:16 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF073018.M
 Quant Title :
 QLast Update : Fri Aug 03 12:00:27 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
Target Compounds			
7) N-EICOSANE	12.198	545277	3.658 ug/ml
8) N-DOCOSANE	13.406	407585	2.790 ug/ml
10) N-TETRACOSANE	14.482	23138525	162.203 ug/ml
11) N-HEXACOSANE	15.529	210413	1.494 ug/ml
12) N-OCTACOSANE	16.478	308383	2.199 ug/ml
13) N-TRIACONTANE	17.362	233387	1.686 ug/ml
14) N-DOTRIACONTANE	18.192	518052	3.971 ug/ml
15) N-TETRATRIACONTANE	18.977	199685	1.652 ug/ml
16) N-HEXATRIACONTANE	19.722	110256	0.991 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF081318\
Data File : FF001854.D
Signal(s) : FID2B.ch
Acq On : 13 Aug 2018 09:33
Operator : AJ\SJ
Sample : MECL2
Misc :
ALS Vial : 51 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Aug 14 02:02:16 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF073018.M
Quant Title :
QLast Update : Fri Aug 03 12:00:27 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

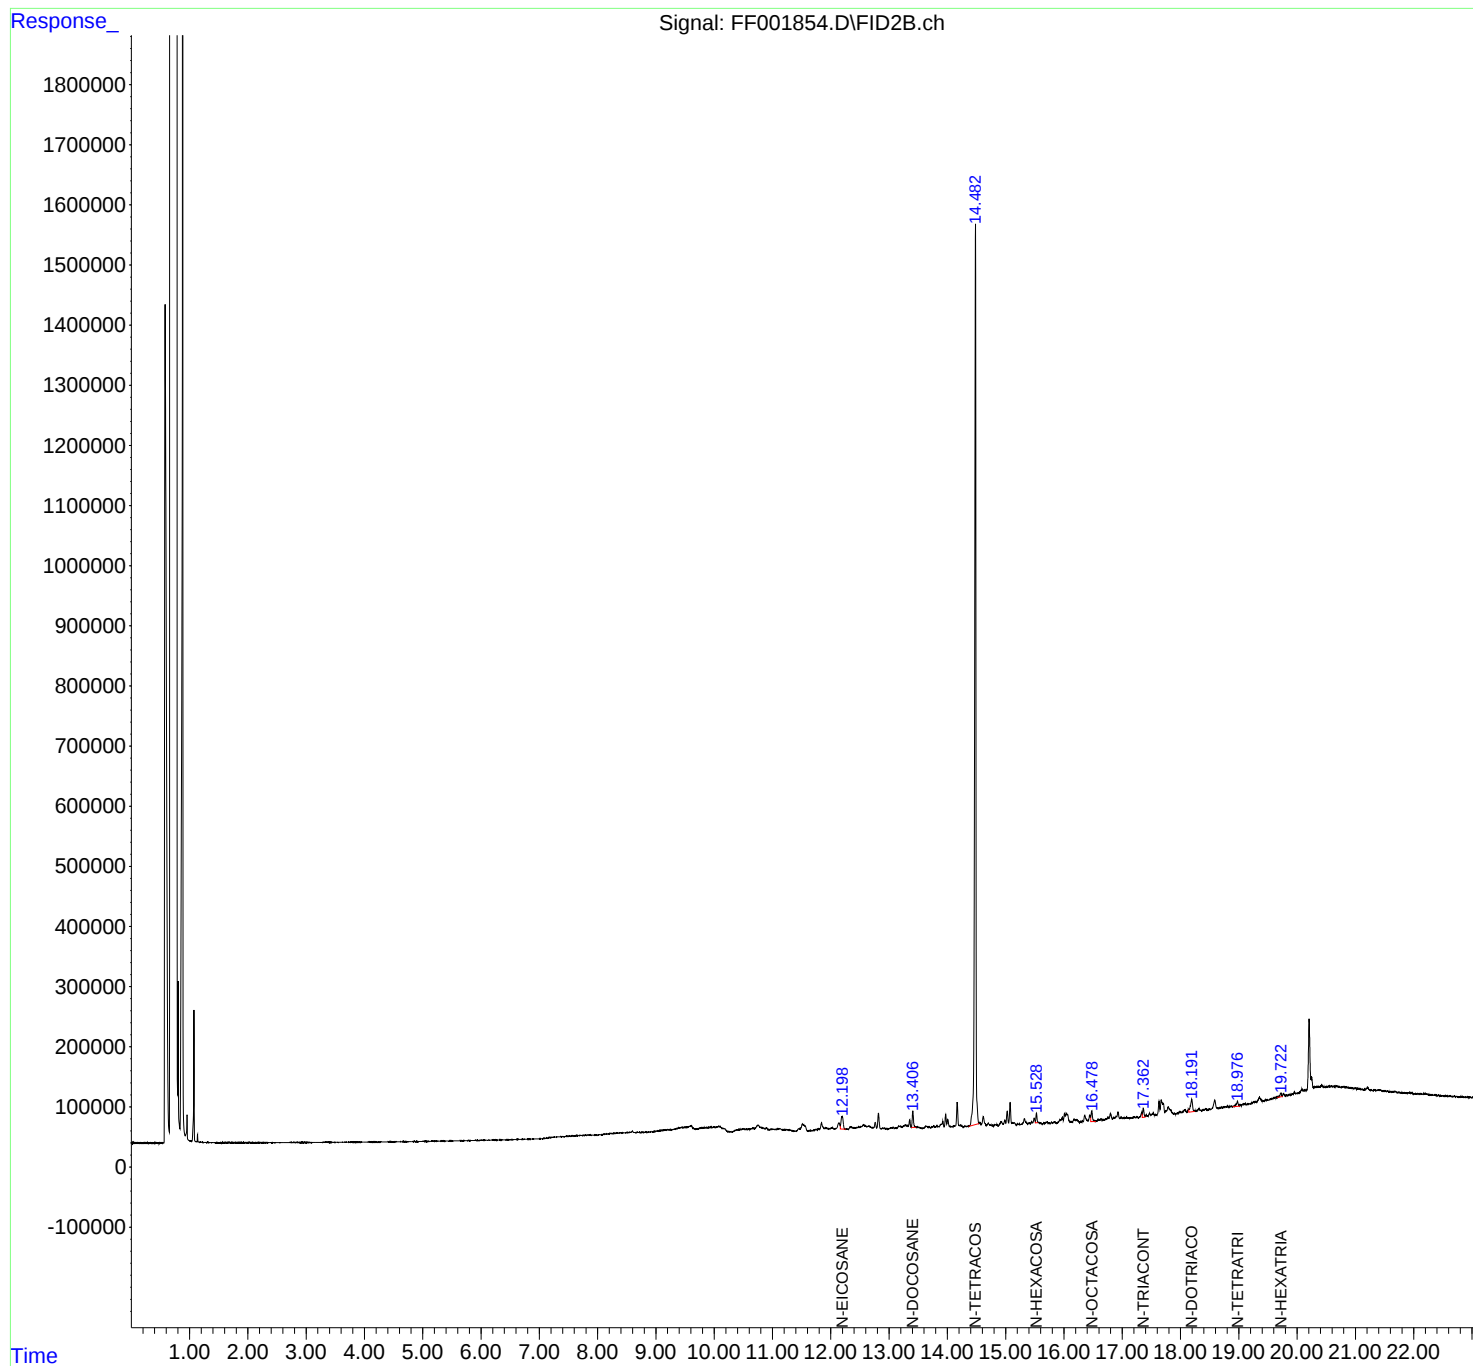


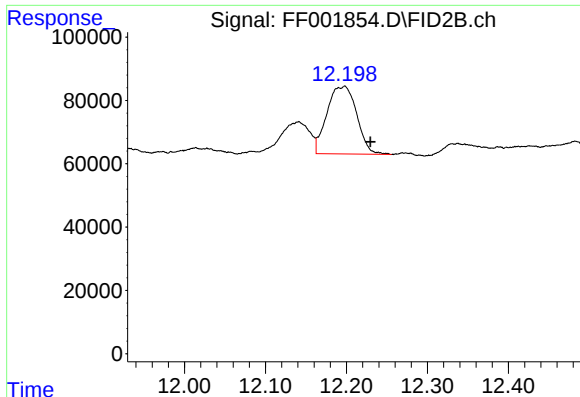

#7 N-EICOSANE


R.T.: 12.198 min
Delta R.T.: -0.032 min
Response: 545277
Conc: 3.66 ug/ml

Instrument :
FID_F
ClientSampleId :

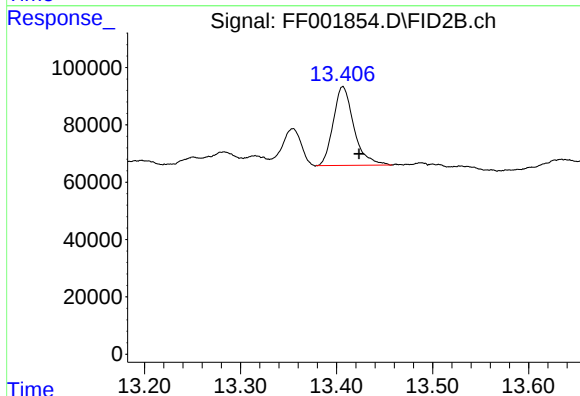


#8 N-DOCOSANE

R.T.: 13.406 min
Delta R.T.: -0.017 min
Response: 407585
Conc: 2.79 ug/ml

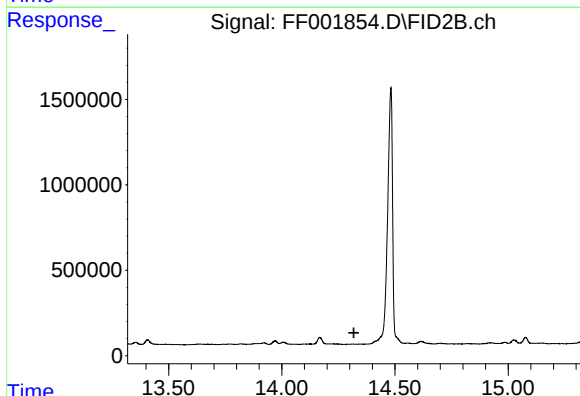


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 0.000 min
Exp R.T. : 14.318 min
Response: 0
Conc: N.D.

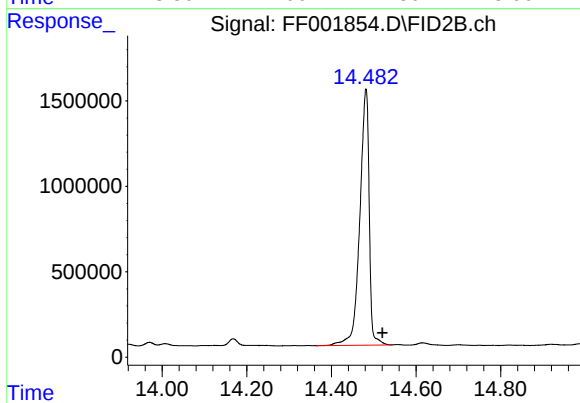

#10 N-TETRACOSANE


R.T.: 14.482 min
Delta R.T.: -0.039 min
Response: 23138525
Conc: 162.20 ug/ml

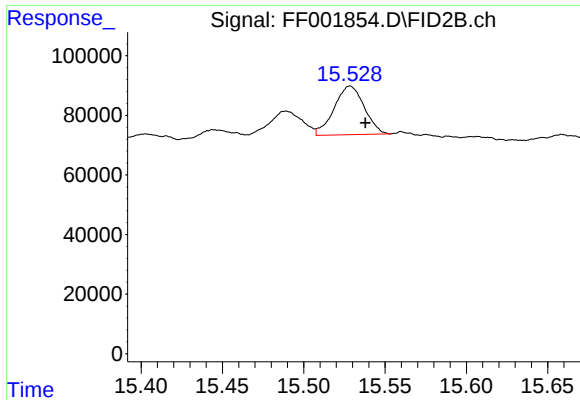

#11 N-HEXACOSANE


R.T.: 15.529 min
Delta R.T.: -0.009 min
Response: 210413
Conc: 1.49 ug/ml

Instrument :
FID_F
ClientSampleId :

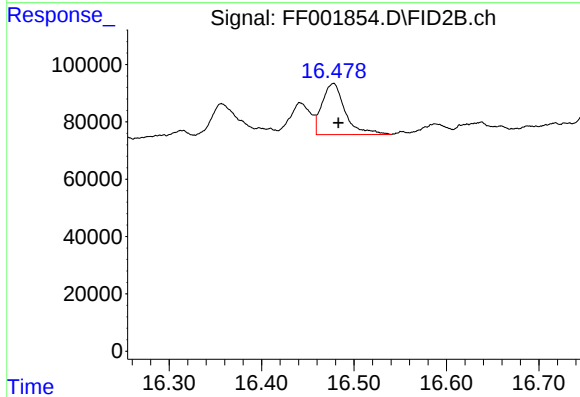


#12 N-OCTACOSANE

R.T.: 16.478 min
Delta R.T.: -0.005 min
Response: 308383
Conc: 2.20 ug/ml

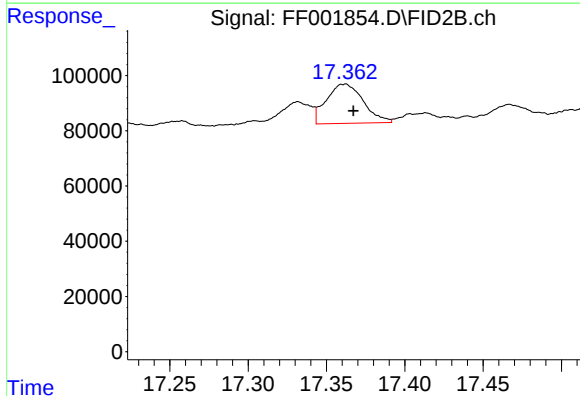


#13 N-TRIACONTANE

R.T.: 17.362 min
Delta R.T.: -0.006 min
Response: 233387
Conc: 1.69 ug/ml

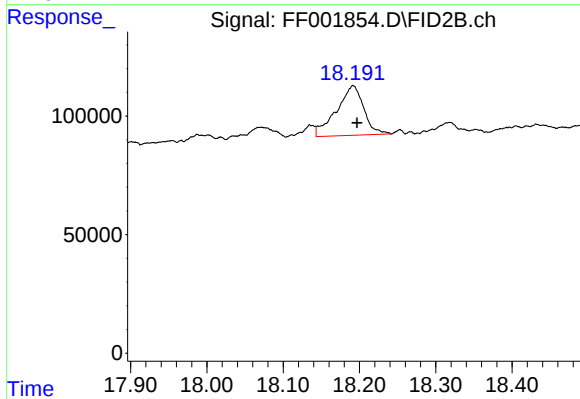

#14 N-DOTRIACONTANE


R.T.: 18.192 min
Delta R.T.: -0.005 min
Response: 518052
Conc: 3.97 ug/ml

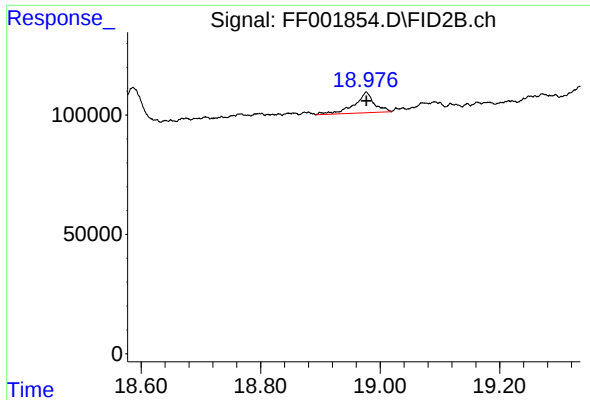

#15 N-TETRATRIACONTANE

R.T.: 18.977 min
Delta R.T.: 0.000 min
Response: 199685
Conc: 1.65 ug/ml

Instrument :
FID_F
ClientSampleId :

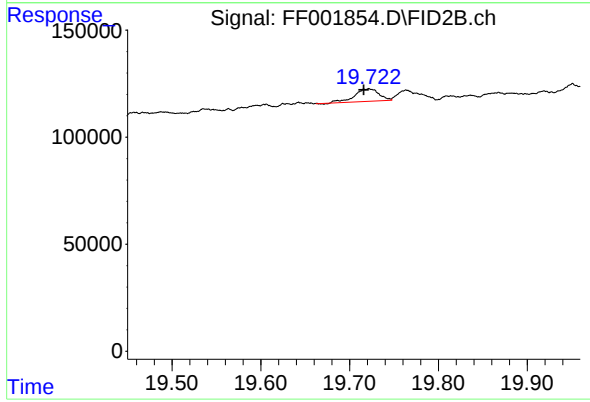

#16 N-HEXATRIACONTANE

R.T.: 19.722 min
Delta R.T.: 0.006 min
Response: 110256
Conc: 0.99 ug/ml