

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF081318\
 Data File : FF001857.D
 Signal(s) : FID2B.ch
 Acq On : 13 Aug 2018 11:05
 Operator : AJ\SJ
 Sample : RT MARKER
 Misc :
 ALS Vial : 54 Sample Multiplier: 1

Instrument :
 FID_F
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Aug 14 02:02:44 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF073018.M
 Quant Title :
 QLast Update : Fri Aug 03 12:00:27 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units
----------	------	----------	------------

System Monitoring Compounds

Target Compounds			
3) N-DODECANE	6.105	2888762	19.380 ug/ml
10) N-TETRACOSANE	14.479	268704	1.884 ug/ml
12) N-OCTACOSANE	16.484	2649569	18.896 ug/ml
13) N-TRIACONTANE	17.368	108066	0.781 ug/ml
14) N-DOTRIACONTANE	18.199	137467	1.054 ug/ml
15) N-TETRATRIACONTANE	18.981	116301	0.962 ug/ml
16) N-HEXATRIACONTANE	19.722	106425	0.956 ug/ml
17) N-OCTATRIACONTANE	20.426	137117	1.376 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF081318\
Data File : FF001857.D
Signal(s) : FID2B.ch
Acq On : 13 Aug 2018 11:05
Operator : AJ\SJ
Sample : RT MARKER
Misc :
ALS Vial : 54 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Aug 14 02:02:44 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF073018.M
Quant Title :
QLast Update : Fri Aug 03 12:00:27 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

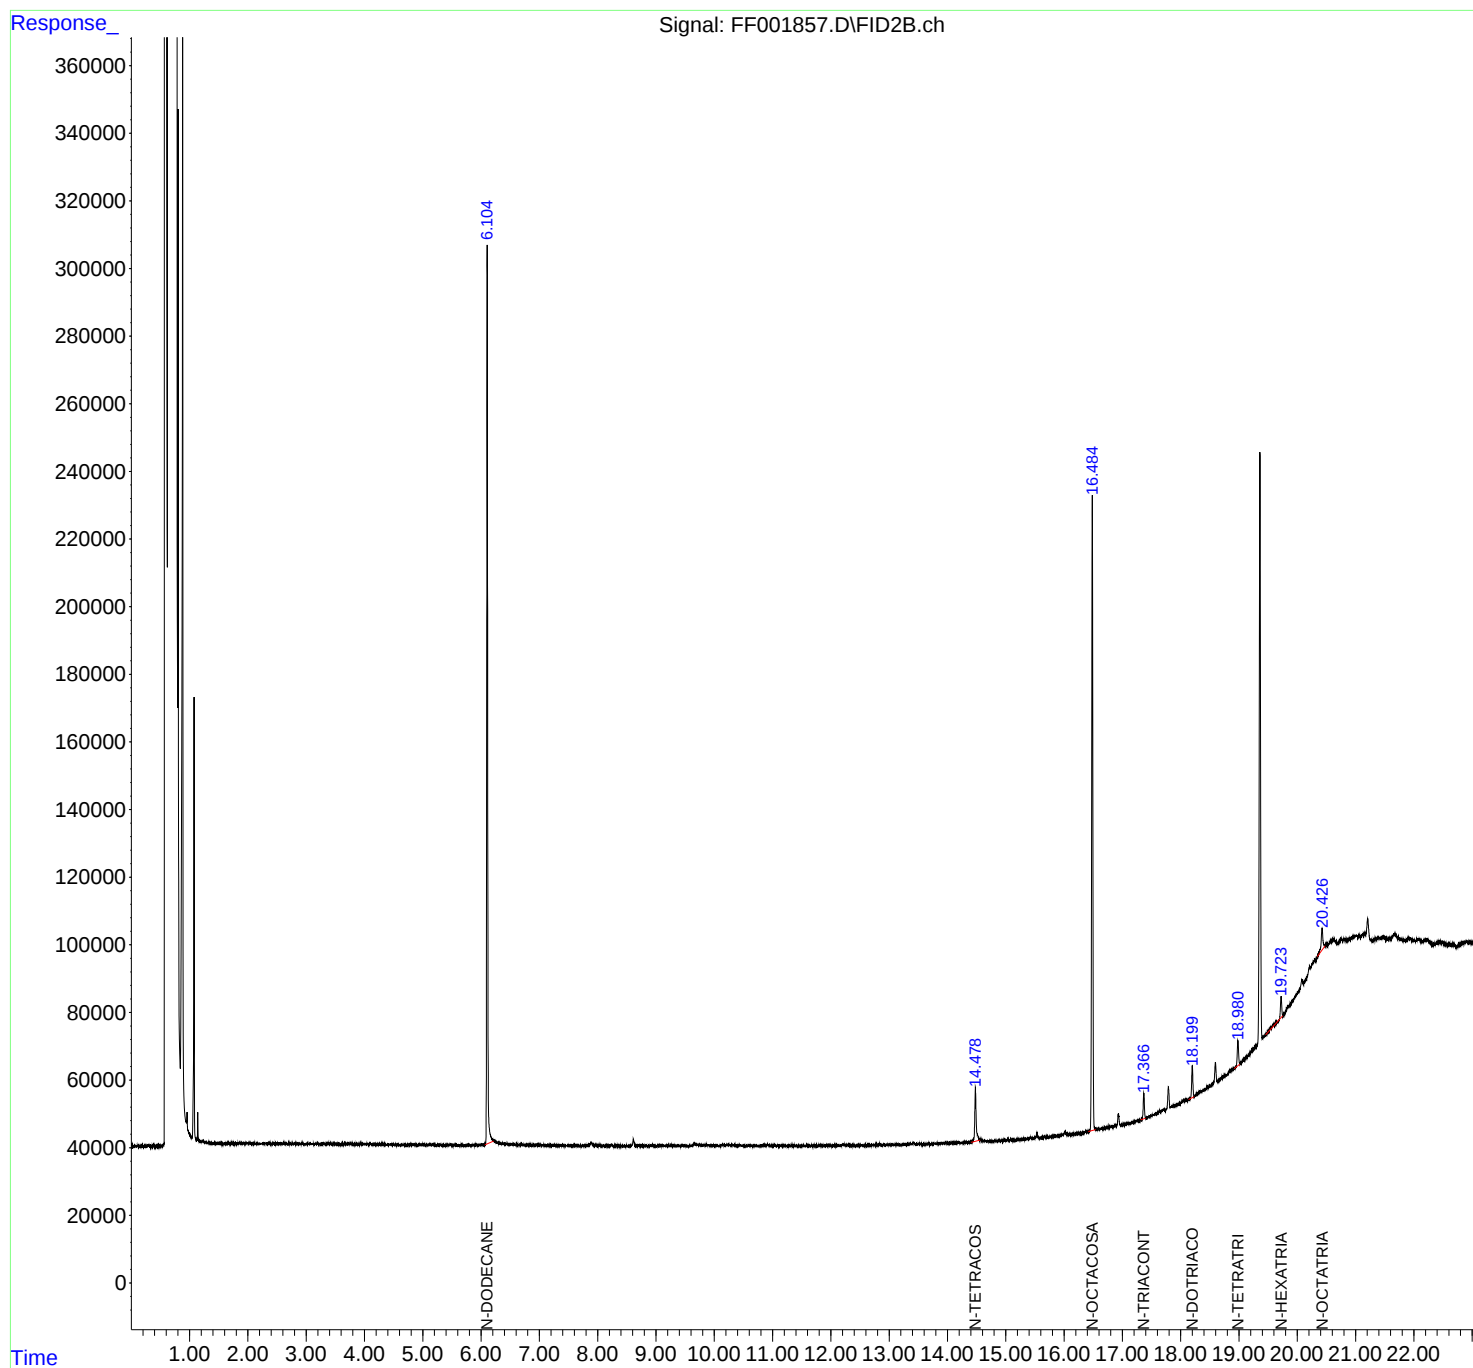


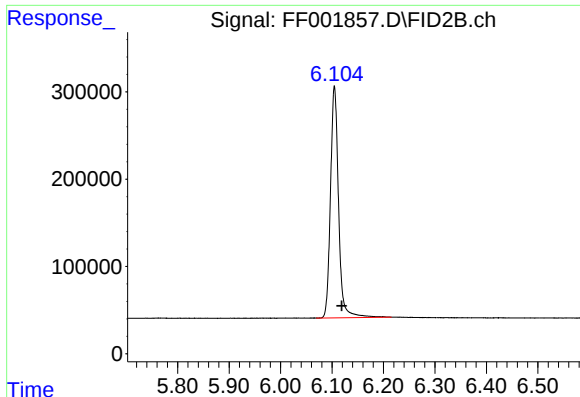

#3 N-DODECANE


R.T.: 6.105 min
Delta R.T.: -0.014 min
Response: 2888762
Conc: 19.38 ug/ml

Instrument :
FID_F
ClientSampleId :

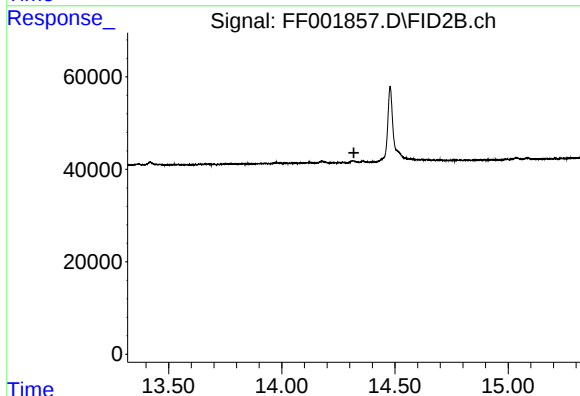


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 0.000 min
Exp R.T. : 14.318 min
Response: 0
Conc: N.D.

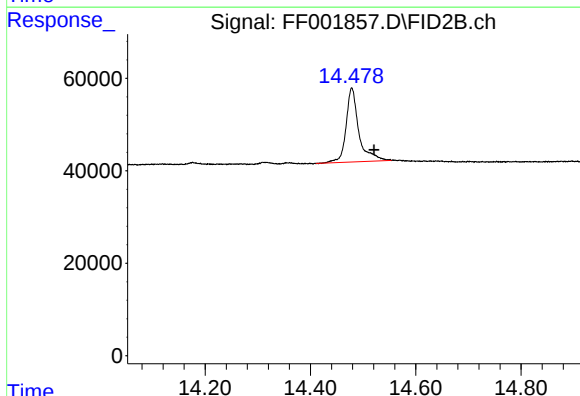


#10 N-TETRACOSANE

R.T.: 14.479 min
Delta R.T.: -0.042 min
Response: 268704
Conc: 1.88 ug/ml

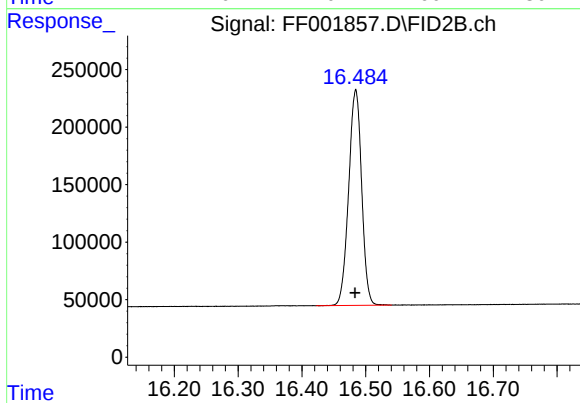

#12 N-OCTACOSANE


R.T.: 16.484 min
Delta R.T.: 0.001 min
Response: 2649569
Conc: 18.90 ug/ml

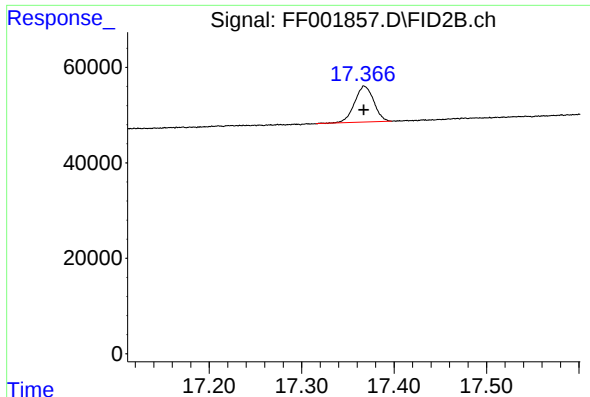

#13 N-TRIACONTANE


R.T.: 17.368 min
Delta R.T.: 0.000 min
Response: 108066
Conc: 0.78 ug/ml

Instrument :
FID_F
ClientSampleId :

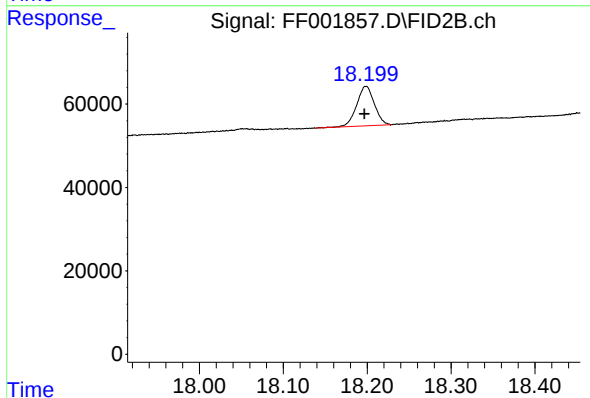


#14 N-DOTRIACONTANE

R.T.: 18.199 min
Delta R.T.: 0.002 min
Response: 137467
Conc: 1.05 ug/ml

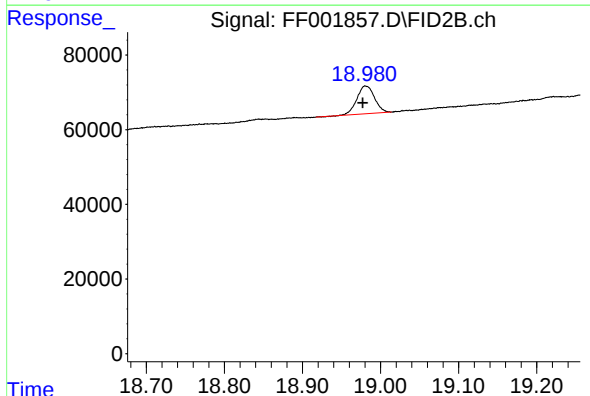


#15 N-TETRATRIACONTANE

R.T.: 18.981 min
Delta R.T.: 0.004 min
Response: 116301
Conc: 0.96 ug/ml

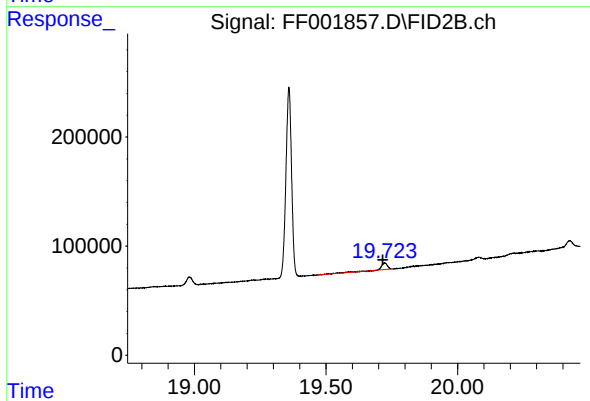

#16 N-HEXATRIACONTANE

R.T.: 19.722 min
Delta R.T.: 0.006 min
Response: 106425
Conc: 0.96 ug/ml

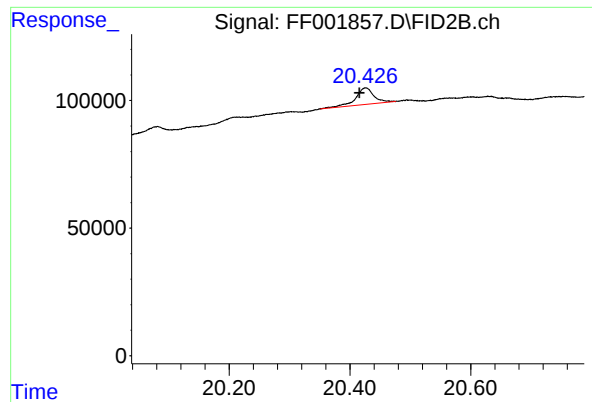

#17 N-OCTATRIACONTANE

R.T.: 20.426 min
Delta R.T.: 0.011 min
Response: 137117
Conc: 1.38 ug/ml

Instrument :
FID_F
ClientSampleId :