

Data Path : Z:\pestpcbsrv\HPCHEM1\FID\_F\Data\FF081320\  
 Data File : FF007349.D  
 Signal(s) : FID2B.ch  
 Acq On : 13 Aug 2020 08:36  
 Operator : DD\AJ  
 Sample : I.BLK  
 Misc :  
 ALS Vial : 52 Sample Multiplier: 1

Instrument :  
 FID\_F  
 ClientSampleId :

Integration File: autoint1.e  
 Quant Time: Aug 13 15:15:59 2020  
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID\_F\Method\FF072820.M  
 Quant Title :  
 QLast Update : Wed Jul 29 09:33:32 2020  
 Response via : Initial Calibration  
 Integrator: ChemStation

Volume Inj. : 1uL  
 Signal Phase : Rxi-1ms  
 Signal Info : 20mx0.18mmx0.18um

| Compound                      | R.T.    | Response | Conc Units   |
|-------------------------------|---------|----------|--------------|
| -----                         |         |          |              |
| System Monitoring Compounds   |         |          |              |
| 9) S TETRACOSANE-d50 (SURR... | 14.754  | 2015598  | 14.766 ug/ml |
| Target Compounds              |         |          |              |
| 16) N-HEXATRIACONTANE         | 20.224  | 120869   | 1.307 ug/ml  |
| 18) N-TETRACONTANE            | 21.942f | 119206   | 1.782 ug/ml  |
| -----                         |         |          |              |

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID\_F\Data\FF081320\  
Data File : FF007349.D  
Signal(s) : FID2B.ch  
Acq On : 13 Aug 2020 08:36  
Operator : DD\AJ  
Sample : I.BLK  
Misc :  
ALS Vial : 52 Sample Multiplier: 1

Instrument :  
FID\_F  
ClientSampleId :

Integration File: autoint1.e  
Quant Time: Aug 13 15:15:59 2020  
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID\_F\Method\FF072820.M  
Quant Title :  
QLast Update : Wed Jul 29 09:33:32 2020  
Response via : Initial Calibration  
Integrator: ChemStation

Volume Inj. : 1uL  
Signal Phase : Rxi-1ms  
Signal Info : 20mx0.18mmx0.18um

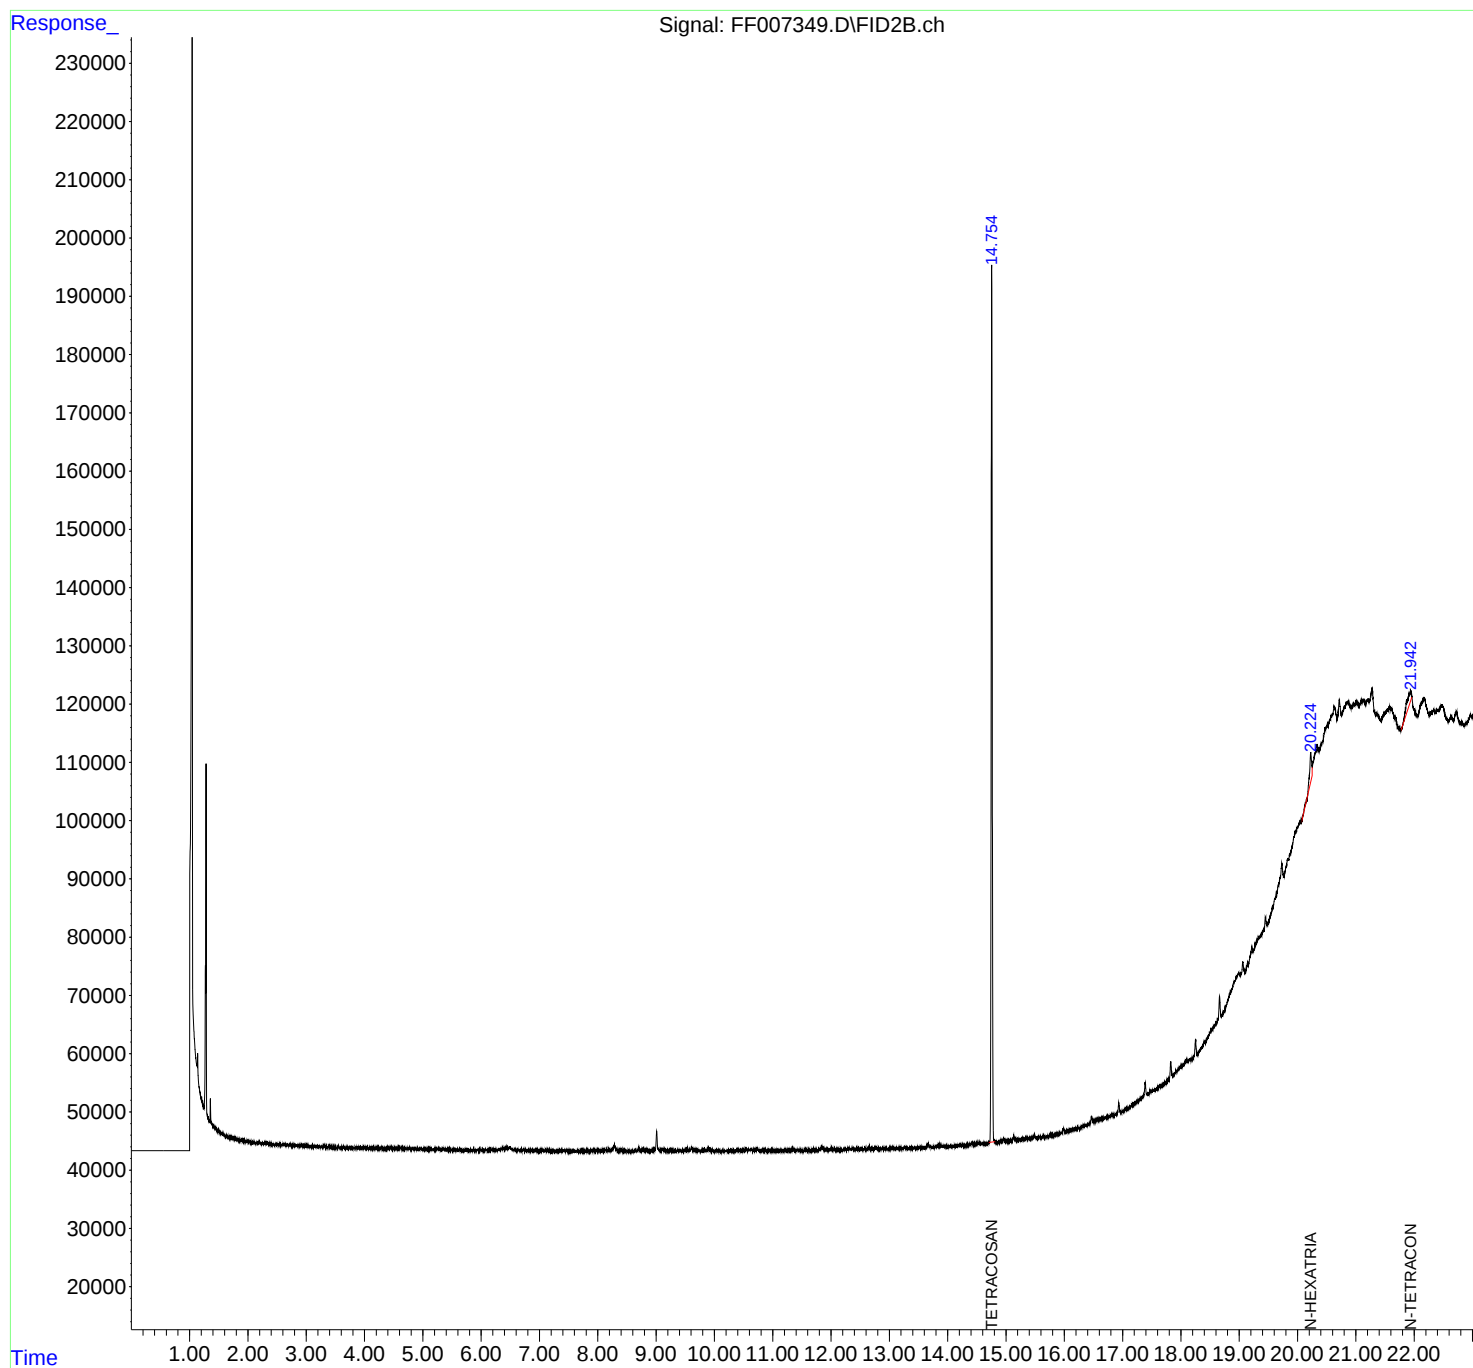


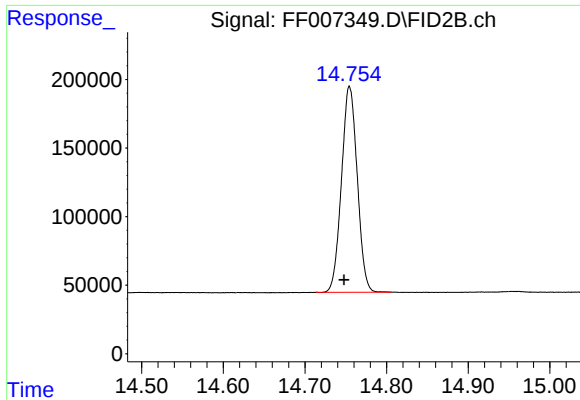

#9 TETRACOSANE-d50 (SURROGATE)


R.T.: 14.754 min  
Delta R.T.: 0.007 min  
Response: 2015598  
Conc: 14.77 ug/ml

Instrument :  
FID\_F  
ClientSampleId :

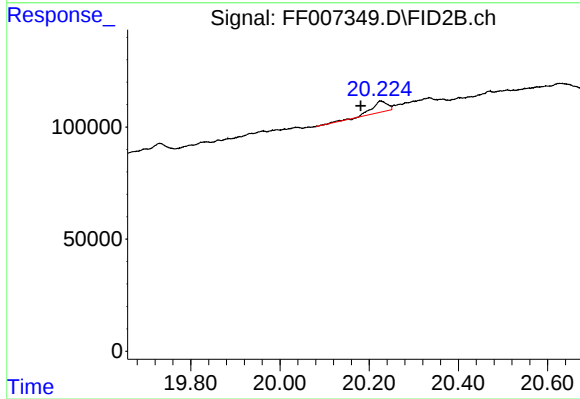

#16 N-HEXATRIACONTANE

R.T.: 20.224 min  
Delta R.T.: 0.044 min  
Response: 120869  
Conc: 1.31 ug/ml

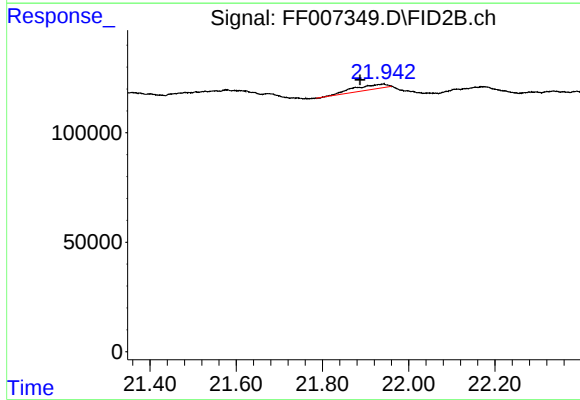

#18 N-TETRACONTANE

R.T.: 21.942 min  
Delta R.T.: 0.055 min  
Response: 119206  
Conc: 1.78 ug/ml