

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF081320\
 Data File : FF007352.D
 Signal(s) : FID2B.ch
 Acq On : 13 Aug 2020 10:21
 Operator : DD\AJ
 Sample : L3637-09 10X
 Misc :
 ALS Vial : 55 Sample Multiplier: 1

Instrument :
 FID_F
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Aug 13 15:16:16 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF072820.M
 Quant Title :
 QLast Update : Wed Jul 29 09:33:32 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

	Compound	R.T.	Response	Conc Units

System Monitoring Compounds				
9) S	TETRACOSANE-d50 (SURR...	14.754	202749	1.485 ug/ml
Target Compounds				
10)	N-TETRACOSANE	14.946	195392	1.237 ug/ml
13)	N-TRIACONTANE	17.827	174029	1.110 ug/ml
14)	N-DOTRIACONTANE	18.663	132128	0.892 ug/ml
16)	N-HEXATRIACONTANE	20.200	71804	0.776 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF081320\
Data File : FF007352.D
Signal(s) : FID2B.ch
Acq On : 13 Aug 2020 10:21
Operator : DD\AJ
Sample : L3637-09 10X
Misc :
ALS Vial : 55 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Aug 13 15:16:16 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF072820.M
Quant Title :
QLast Update : Wed Jul 29 09:33:32 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

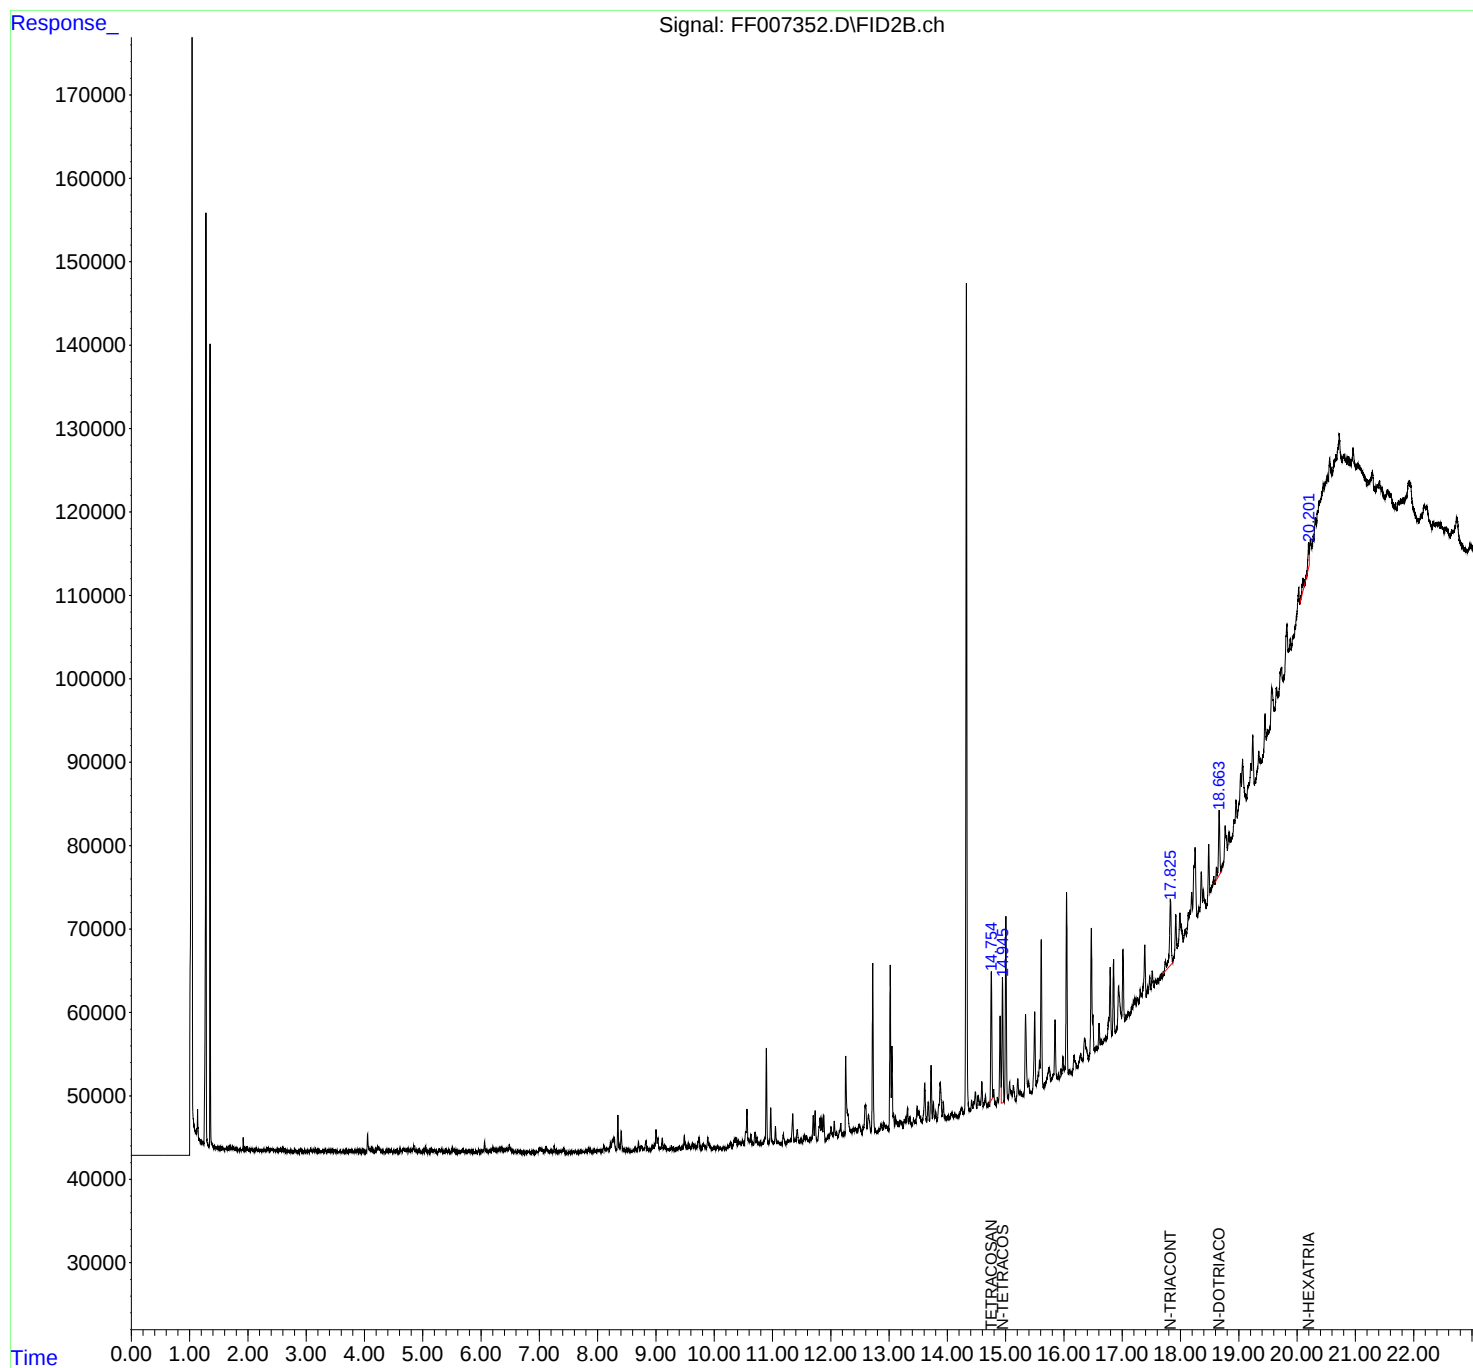


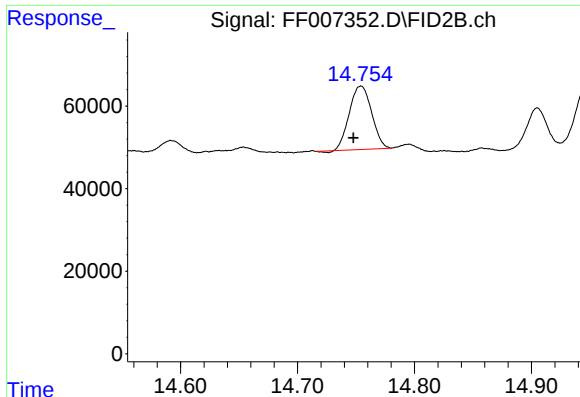

#9 TETRACOSANE-d50 (SURROGATE)


R.T.: 14.754 min
Delta R.T.: 0.007 min
Response: 202749
Conc: 1.49 ug/ml

Instrument :
FID_F
ClientSampleId :

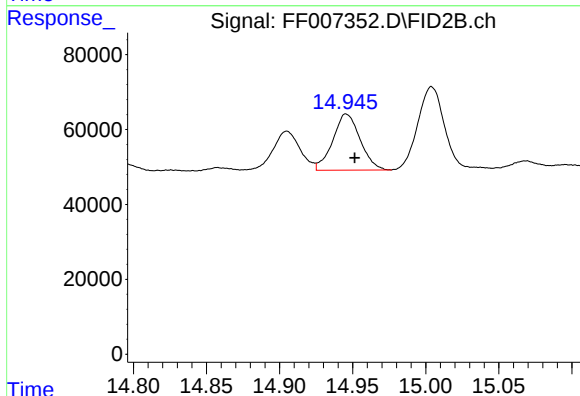


#10 N-TETRACOSANE

R.T.: 14.946 min
Delta R.T.: -0.006 min
Response: 195392
Conc: 1.24 ug/ml

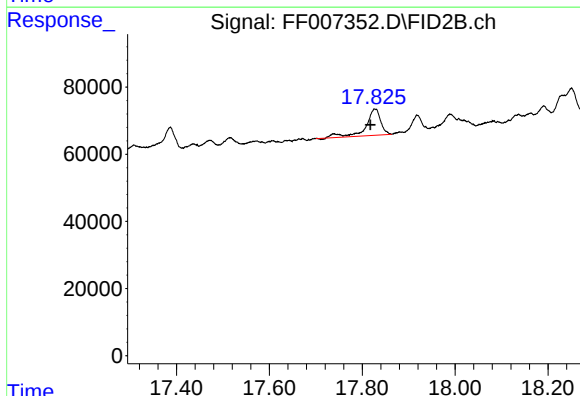


#13 N-TRIACONTANE

R.T.: 17.827 min
Delta R.T.: 0.009 min
Response: 174029
Conc: 1.11 ug/ml

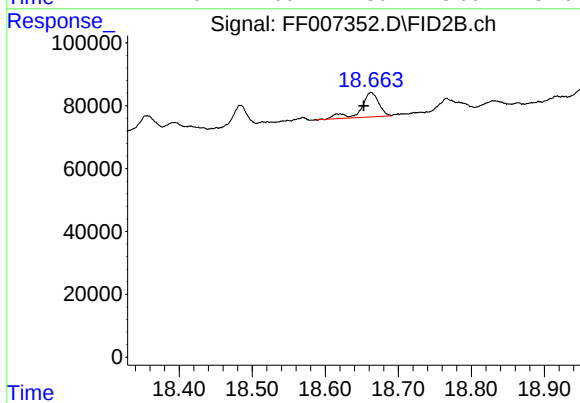

#14 N-DOTRIACONTANE

R.T.: 18.663 min
Delta R.T.: 0.010 min
Response: 132128
Conc: 0.89 ug/ml

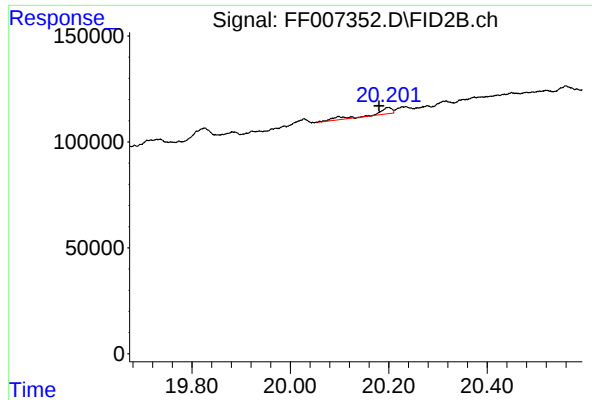

#16 N-HEXATRIACONTANE

R.T.: 20.200 min
Delta R.T.: 0.019 min
Response: 71804
Conc: 0.78 ug/ml

Instrument :
FID_F
ClientSampleId :