

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF081320\
 Data File : FF007353.D
 Signal(s) : FID2B.ch
 Acq On : 13 Aug 2020 10:53
 Operator : DD\AJ
 Sample : L3637-10 20X
 Misc :
 ALS Vial : 56 Sample Multiplier: 1

Instrument :
 FID_F
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Aug 13 15:16:21 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF072820.M
 Quant Title :
 QLast Update : Wed Jul 29 09:33:32 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

	Compound	R.T.	Response	Conc Units

System Monitoring Compounds				
9) S	TETRACOSANE-d50 (SURR...	14.754	97137	0.712 ug/ml
Target Compounds				
10)	N-TETRACOSANE	14.946	276182	1.749 ug/ml
13)	N-TRIACONTANE	17.826	133329	0.850 ug/ml
14)	N-DOTRIACONTANE	18.662	77345	0.522 ug/ml
16)	N-HEXATRIACONTANE	20.227	96158	1.040 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF081320\
Data File : FF007353.D
Signal(s) : FID2B.ch
Acq On : 13 Aug 2020 10:53
Operator : DD\AJ
Sample : L3637-10 20X
Misc :
ALS Vial : 56 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Aug 13 15:16:21 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF072820.M
Quant Title :
QLast Update : Wed Jul 29 09:33:32 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

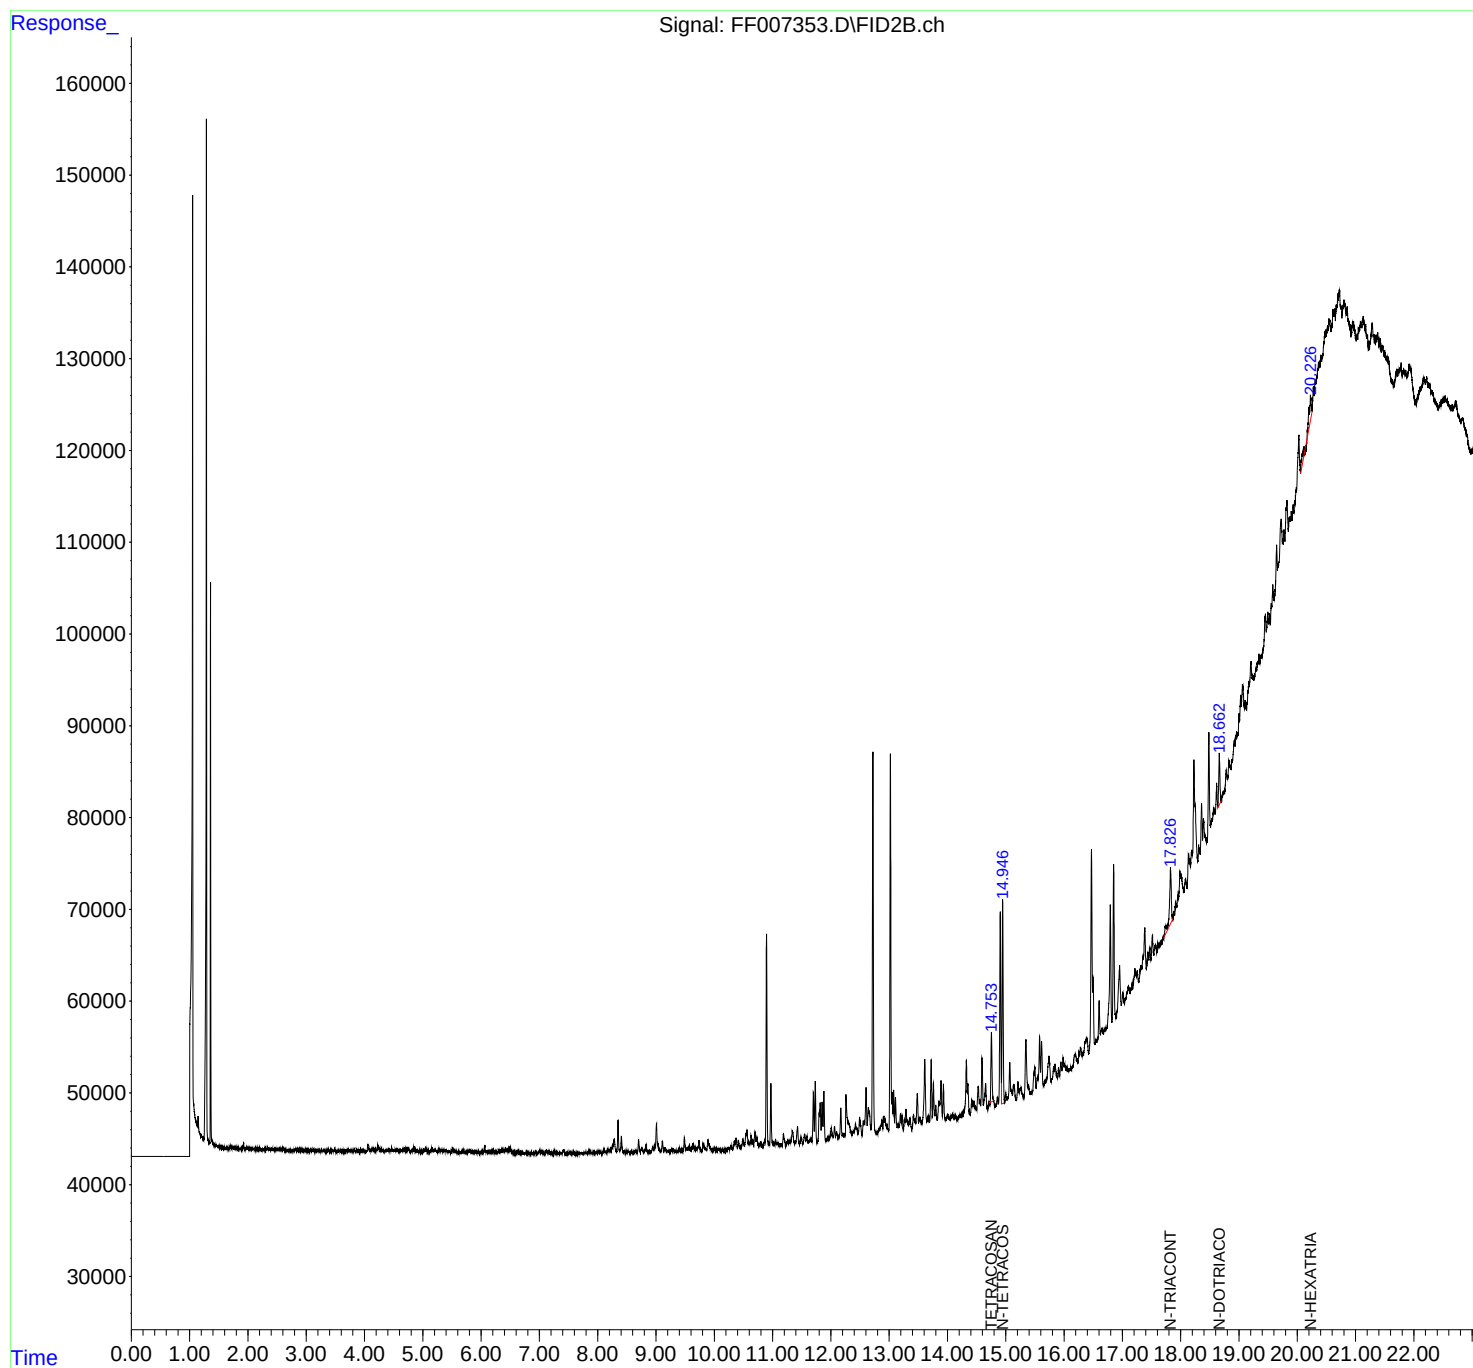


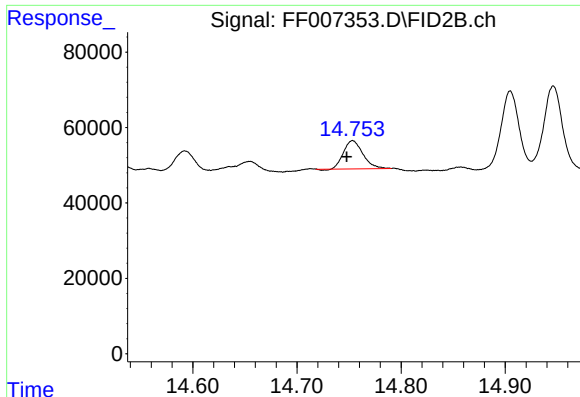

#9 TETRACOSANE-d50 (SURROGATE)


R.T.: 14.754 min
Delta R.T.: 0.006 min
Response: 97137
Conc: 0.71 ug/ml

Instrument :
FID_F
ClientSampleId :

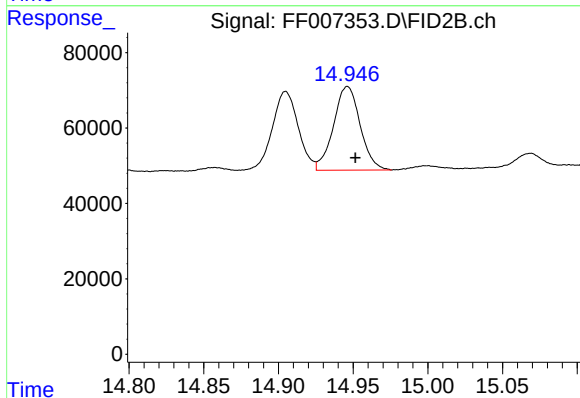


#10 N-TETRACOSANE

R.T.: 14.946 min
Delta R.T.: -0.005 min
Response: 276182
Conc: 1.75 ug/ml

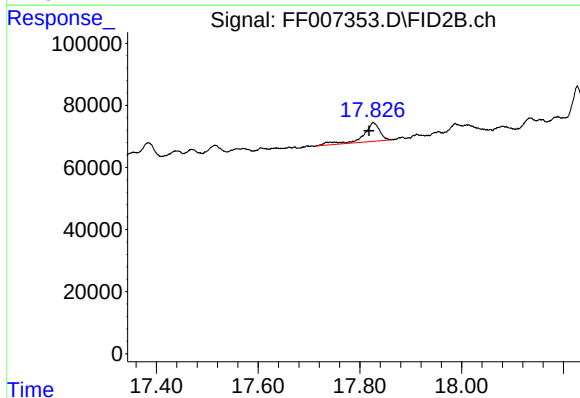


#13 N-TRIACONTANE

R.T.: 17.826 min
Delta R.T.: 0.008 min
Response: 133329
Conc: 0.85 ug/ml

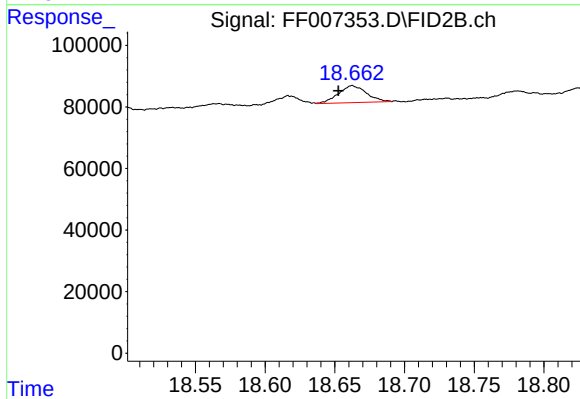

#14 N-DOTRIACONTANE

R.T.: 18.662 min
Delta R.T.: 0.010 min
Response: 77345
Conc: 0.52 ug/ml

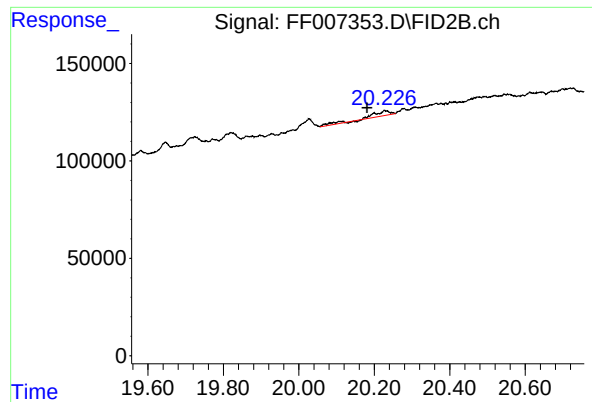

#16 N-HEXATRIACONTANE

R.T.: 20.227 min
Delta R.T.: 0.046 min
Response: 96158
Conc: 1.04 ug/ml

Instrument :
FID_F
ClientSampleId :